

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU012920\
 Data File : VU036597.D
 Acq On : 29 Jan 2020 16:58
 Operator : JC/MD
 Sample : VIBLK22
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK22

Quant Time: Jan 30 04:30:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 30 02:48:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	277029	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	256045	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	120842	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	80302	38.70	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.40%
7) Chloroethane-d5	1.93	69	77551	43.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.12%
11) 1,1-Dichloroethene-d2	2.59	63	107997	32.19	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.38%
21) 2-Butanone-d5	4.68	46	147261	119.57	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	119.57%
24) Chloroform-d	5.11	84	156097	45.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.88%
26) 1,2-Dichloroethane-d4	5.75	65	105609	49.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.74%
32) Benzene-d6	5.77	84	352895	49.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.73	67	115121	51.29	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.58%
41) Toluene-d8	7.93	98	326122	47.07	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.14%
43) trans-1,3-Dichloropropene-	8.21	79	53743	50.35	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.70%
47) 2-Hexanone-d5	8.67	63	128906	123.85	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	123.85%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	169918	51.49	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	102.98%
64) 1,2-Dichlorobenzene-d4	12.21	152	127201	49.05	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.10%


Target Compounds					Ovalue
13) Acetone	2.66	43	2072	1.738 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU012920\
Data File : VU036597.D
Acq On : 29 Jan 2020 16:58
Operator : JC/MD
Sample : VIBLK22
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK22

Quant Time: Jan 30 04:30:04 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 30 02:48:11 2020
Response via : Initial Calibration

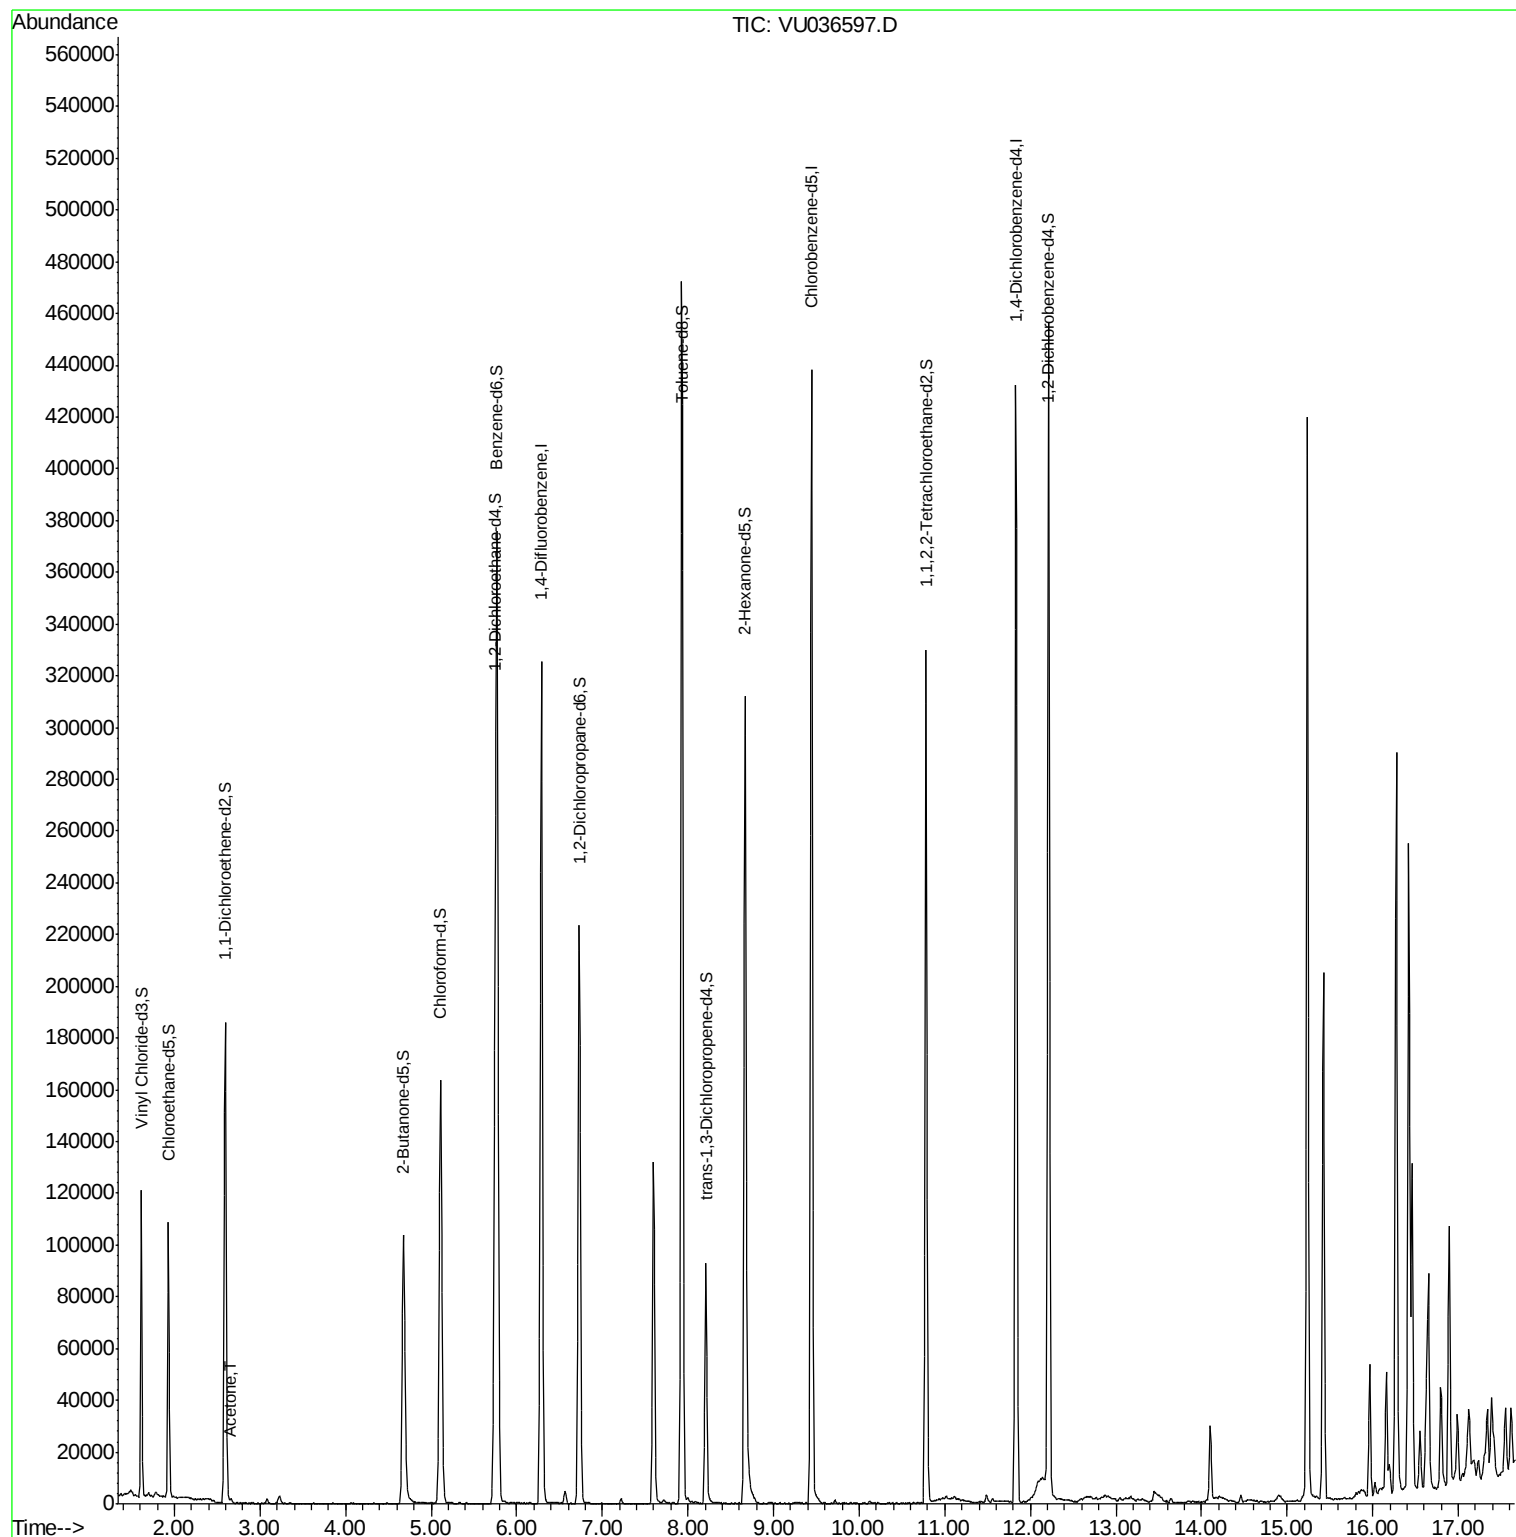

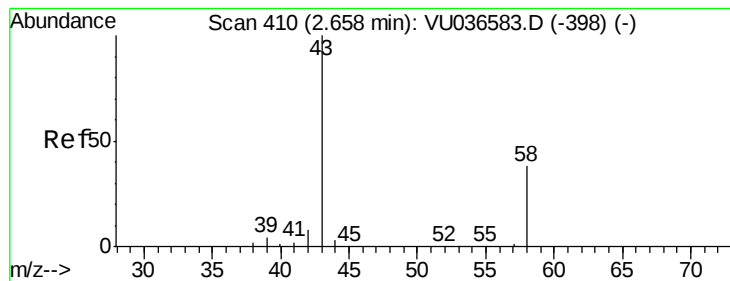

#13
 Acetone
 Concen: 1.738 ug/L
 RT: 2.66 min Scan# 410
 Delta R.T. 0.00 min
 Lab File: VU036597.D
 Acq: 29 Jan 2020 16:58

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK22

Tot Ion: 43 Resp: 2072
 Ion Ratio Lower Upper
 43 100
 58 31.0 0.0 75.4

