

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU012920\
 Data File : VU036605.D
 Acq On : 29 Jan 2020 20:09
 Operator : JC/MD
 Sample : L1271-03MSD
 Misc : 5.06g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GASZ4MSD

Quant Time: Jan 30 05:57:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 30 02:48:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	296725	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	295822	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	162565	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	86130	38.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.50%
7) Chloroethane-d5	1.89	69	21010	11.02	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	22.04%#
11) 1,1-Dichloroethene-d2	2.56	63	151480	42.15	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.30%
21) 2-Butanone-d5	4.69	46	122438	92.81	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.81%
24) Chloroform-d	5.11	84	151197	41.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.10%
26) 1,2-Dichloroethane-d4	5.74	65	98098	43.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.50%
32) Benzene-d6	5.76	84	353903	42.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.06%
36) 1,2-Dichloropropane-d6	6.73	67	111034	42.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.64%
41) Toluene-d8	7.93	98	349708	43.68	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.36%
43) trans-1,3-Dichloropropene-	8.21	79	53731	43.57	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.14%
47) 2-Hexanone-d5	8.68	63	143312	119.18	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	119.18%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	180838	47.43	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.86%
64) 1,2-Dichlorobenzene-d4	12.21	152	153090	43.89	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.78%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
12) 1,1-Dichloroethene	2.57	96	89166	48.348	ug/L	97
13) Acetone	2.68	43	2833	2.219	ug/L	91
15) Methyl Acetate	2.99	43	2144	1.074	ug/L	97
16) Methylene chloride	3.06	84	2516	1.125	ug/L	96
33) Benzene	5.81	78	1184793	133.959	ug/L	100
34) Trichloroethene	6.57	95	104802	46.036	ug/L	98
42) Toluene	8.00	91	2022728	210.406	ug/L	98
51) Chlorobenzene	9.48	112	314832	50.185	ug/L	99
52) Ethylbenzene	9.60	91	1091591	103.655	ug/L	100
53) m,p-Xylene	9.72	106	2798858	681.409	ug/L	98
54) o-xylene	10.13	106	1248752	304.789	ug/L	99
56) Isopropylbenzene	10.51	105	37882	3.637	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU012920\
Data File : VU036605.D
Acq On : 29 Jan 2020 20:09
Operator : JC/MD
Sample : L1271-03MSD
Misc : 5.06µ/5.0mL/100µL/5.0mL/MSVOA_U/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GASZ4MSD

Quant Time: Jan 30 05:57:45 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 30 02:48:11 2020
Response via : Initial Calibration




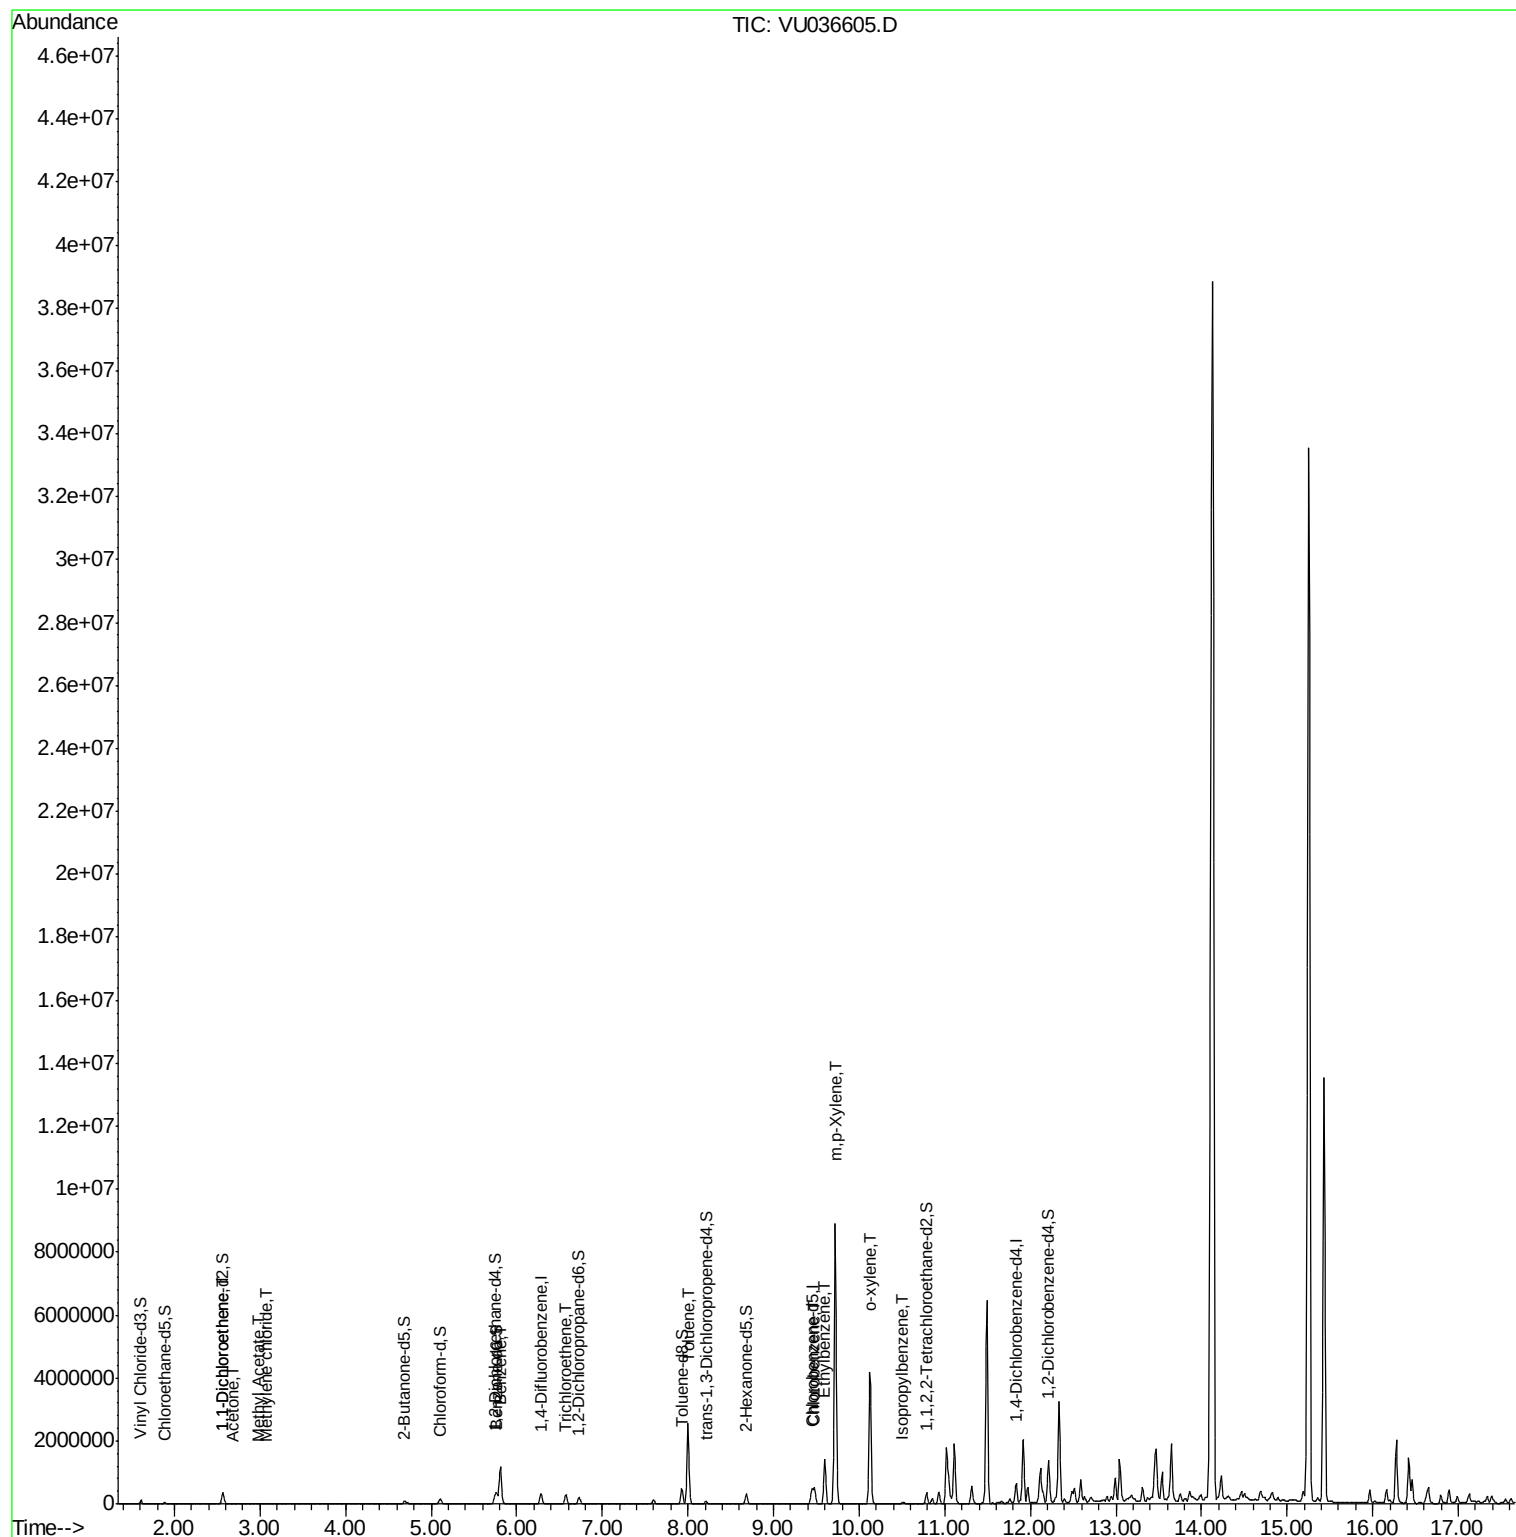


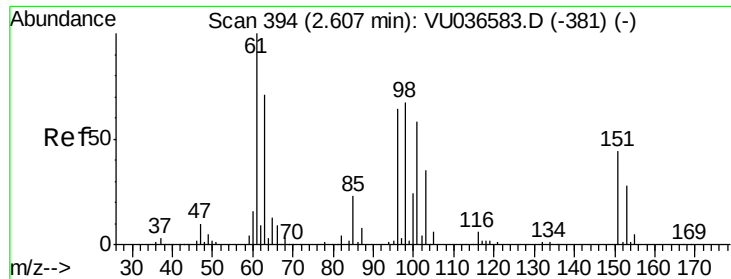

#12
 1,1-Dichloroethene
 Concen: 48.348 ug/L
 RT: 2.57 min Scan# 383
 Delta R.T. -0.03 min
 Lab File: VU036605.D
 Acq: 29 Jan 2020 20:09




Instrument :
 MSVOA_U
 ClientSampleId :
 GASZ4MSD


Tot Ion: 96 Resp: 89166
 Ion Ratio Lower Upper
 96 100
 61 152.8 108.6 201.8
 63 111.6 75.0 139.2

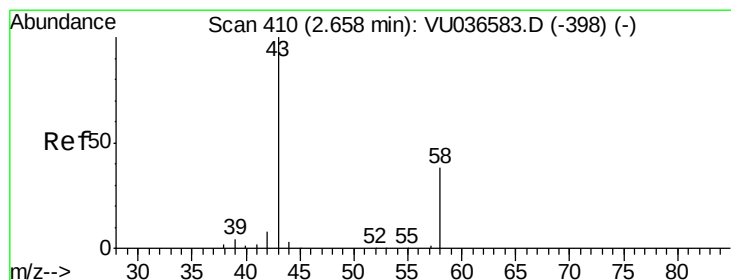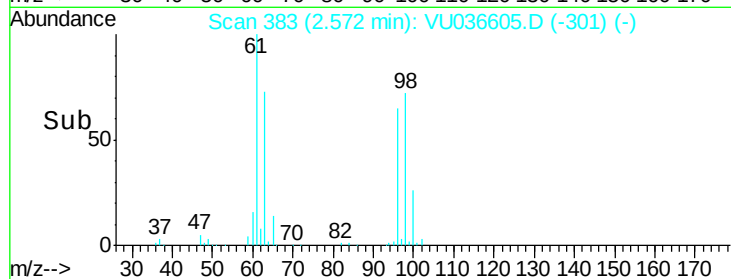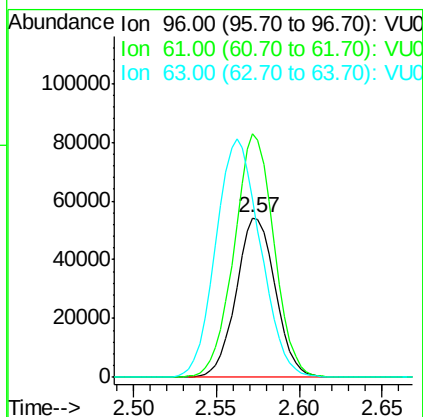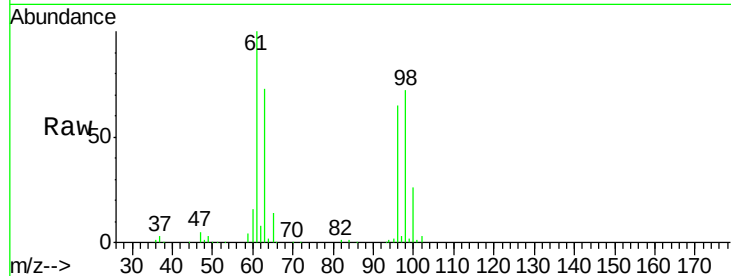

#13
 Acetone
 Concen: 2.219 ug/L
 RT: 2.68 min Scan# 416
 Delta R.T. 0.02 min
 Lab File: VU036605.D
 Acq: 29 Jan 2020 20:09

Tgt Ion: 43 Resp: 2833
 Ion Ratio Lower Upper
 43 100
 58 32.6 0.0 75.4


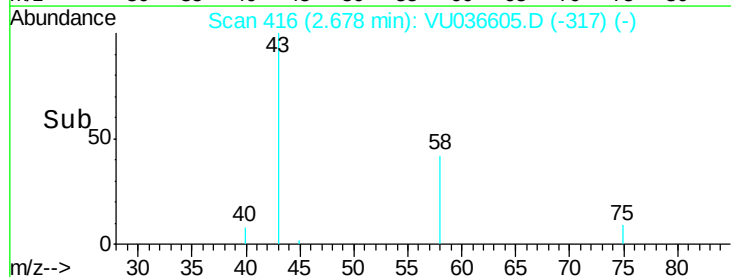
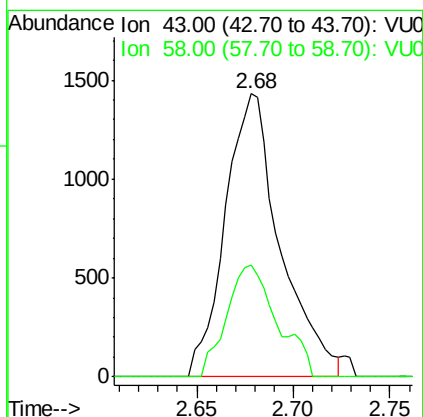
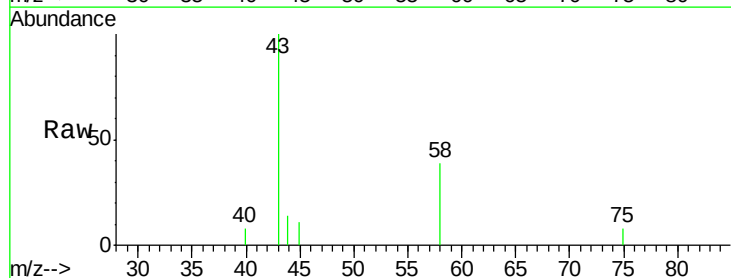


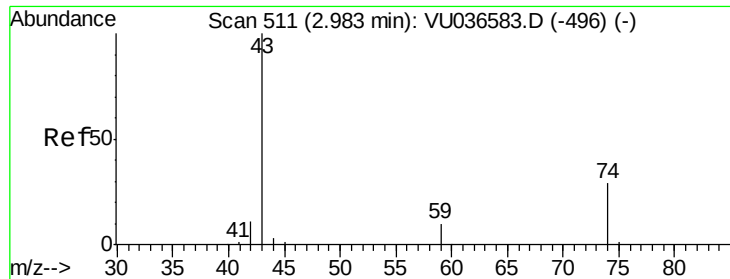

#15
Methvl Acetate
Concen: 1.074 ug/L
RT: 2.99 min Scan# 513
Delta R.T. 0.01 min
Lab File: VU036605.D
Acq: 29 Jan 2020 20:09




Instrument :
MSVOA_U
ClientSampleId :
GASZ4MSD


Tot Ion: 43 Resp: 2144
Ion Ratio Lower Upper
43 100
74 30.5 23.3 34.9

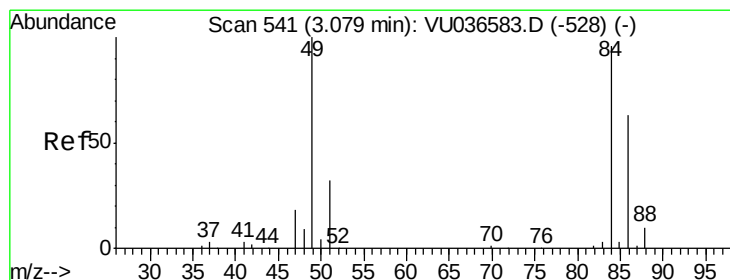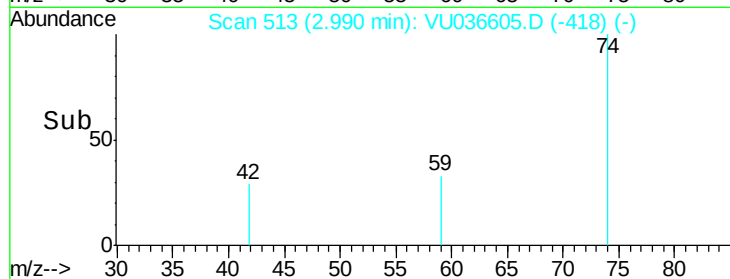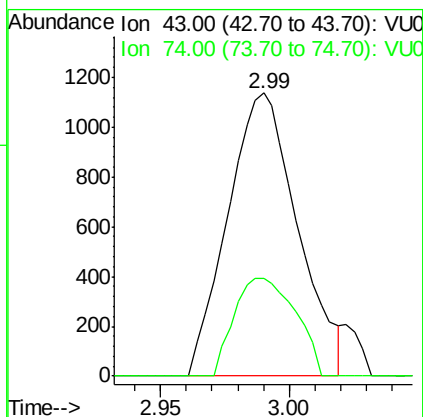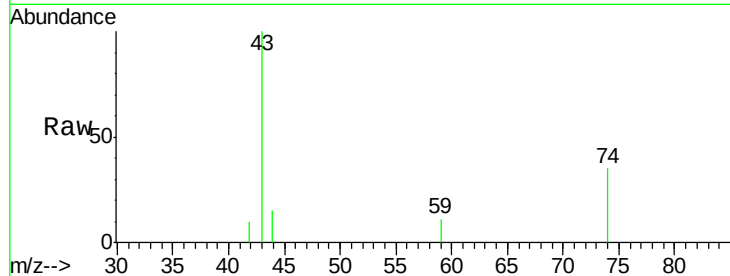

#16
Methylene chloride
Concen: 1.125 ug/L
RT: 3.06 min Scan# 536
Delta R.T. -0.02 min
Lab File: VU036605.D
Acq: 29 Jan 2020 20:09

Tgt Ion: 84 Resp: 2516
Ion Ratio Lower Upper
84 100
86 64.5 44.1 81.9
49 109.6 73.3 136.1

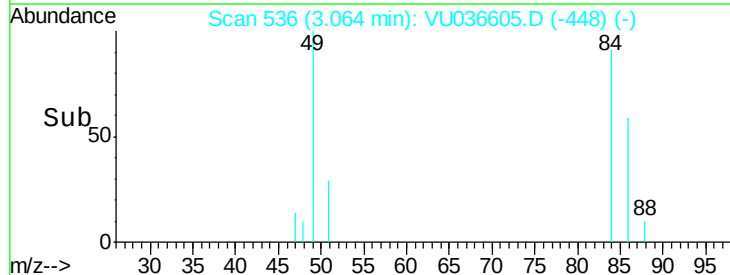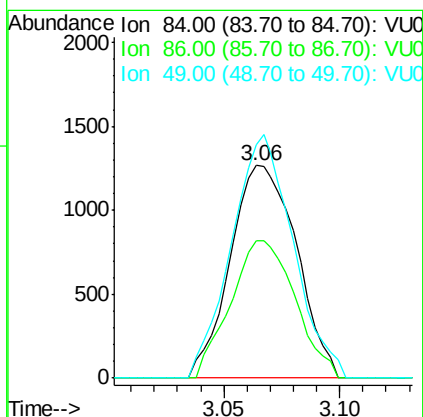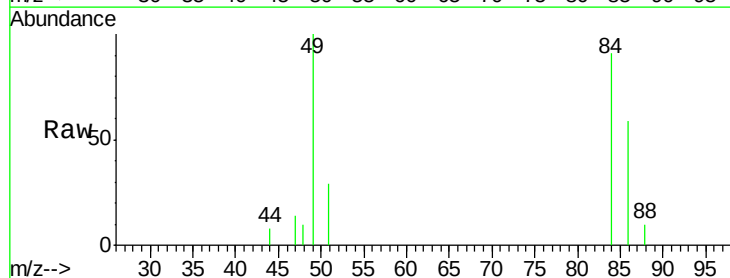

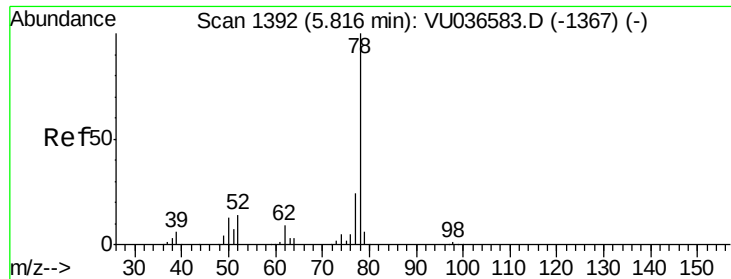

#33

Benzene

Concen: 133.959 ug/L

RT: 5.81 min Scan# 1390

Delta R.T. -0.01 min

Lab File: VU036605.D

Acq: 29 Jan 2020 20:09


Instrument :

MSVOA_U

ClientSampleId :

GASZ4MSD

Tgt Ion: 78 Resp: 1184793

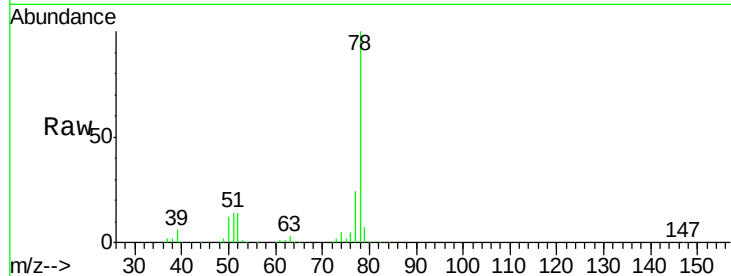

Abundance Ion 78.00 (77.70 to 78.70): VU0

5.81



600000

400000

200000

0

Time-->

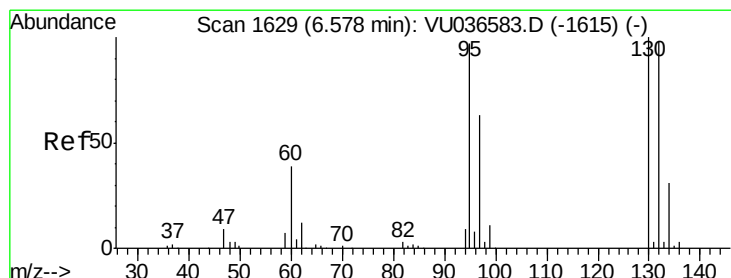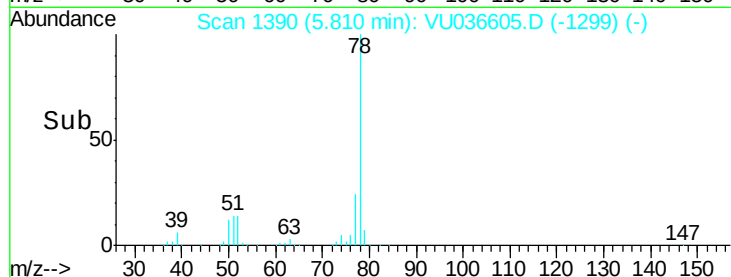

#34

Trichloroethene

Concen: 46.036 ug/L

RT: 6.57 min Scan# 1628

Delta R.T. -0.00 min

Lab File: VU036605.D

Acq: 29 Jan 2020 20:09

Tgt Ion: 95 Resp: 104802


Ion Ratio Lower Upper

95 100

97 65.1 45.5 84.5

132 103.4 70.9 131.7

130 107.2 72.9 135.3

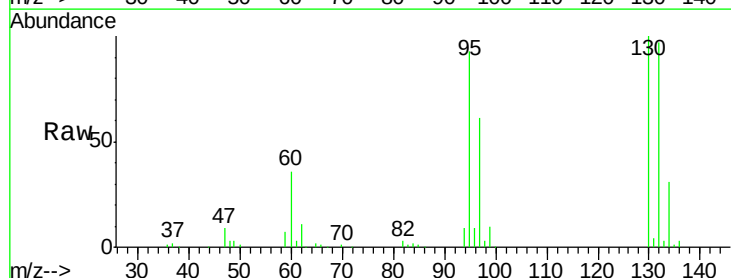

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

Ion 132.00 (131.70 to 132.70): V

Ion 130.00 (129.70 to 130.70): V

6.57

80000


60000


40000

20000

0

Time-->

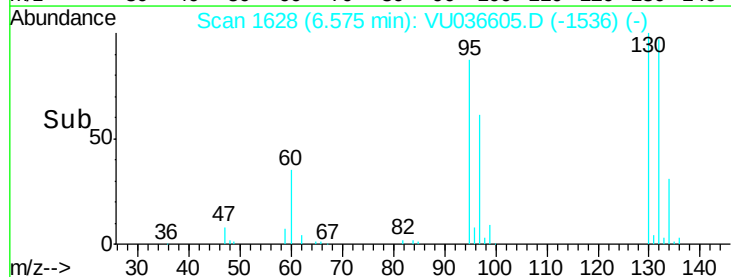

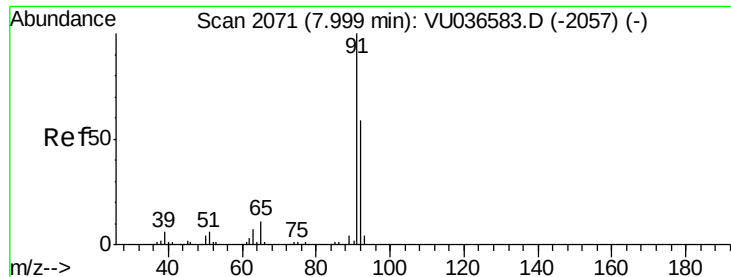

#42

Toluene

Concen: 210.406 ug/L

RT: 8.00 min Scan# 2071

Delta R.T. 0.00 min

Lab File: VU036605.D

Acq: 29 Jan 2020 20:09

Instrument :

MSVOA_U

ClientSampleId :





GASZ4MSD

Tot Ion: 91 Resp: 2022728

Ion Ratio Lower Upper

91 100

92 58.3 39.9 74.1

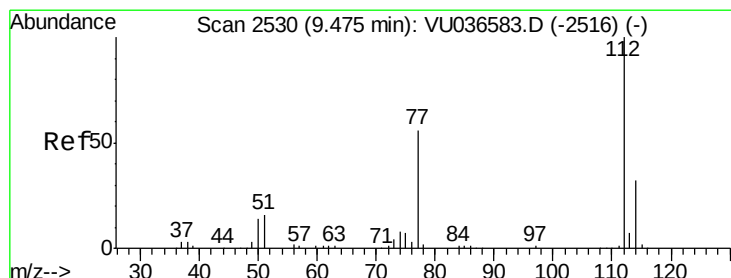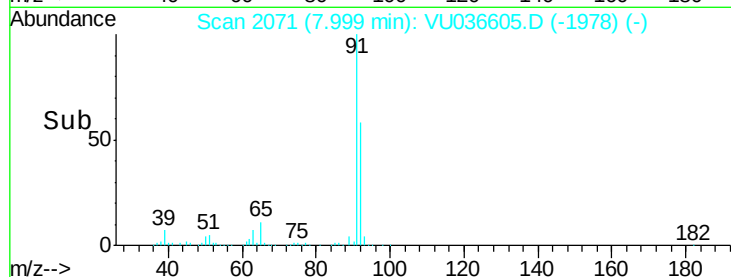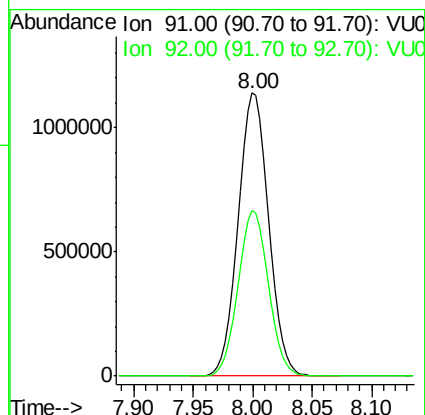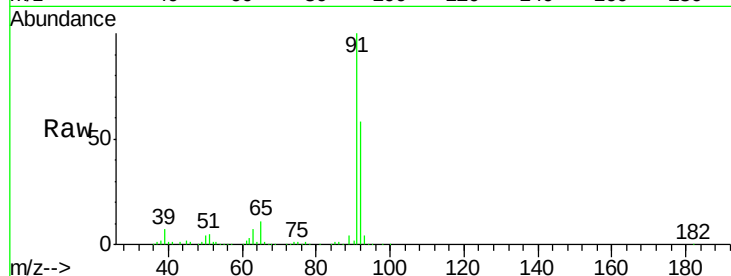

#51

Chlorobenzene

Concen: 50.185 ug/L

RT: 9.48 min Scan# 2531

Delta R.T. 0.00 min

Lab File: VU036605.D

Acq: 29 Jan 2020 20:09




Tgt Ion: 112 Resp: 314832


Ion Ratio Lower Upper

112 100

114 32.0 22.3 41.5

77 56.1 45.7 68.5

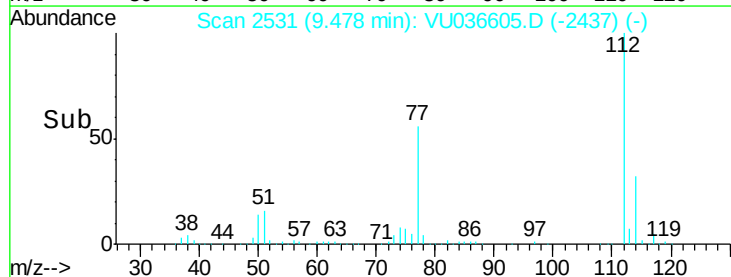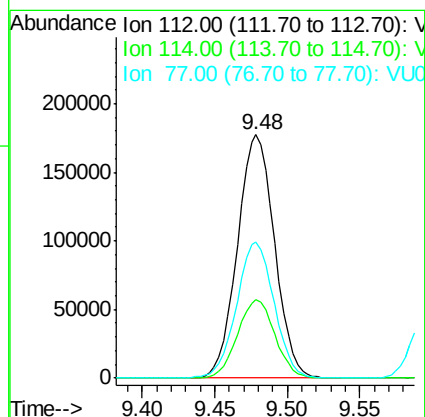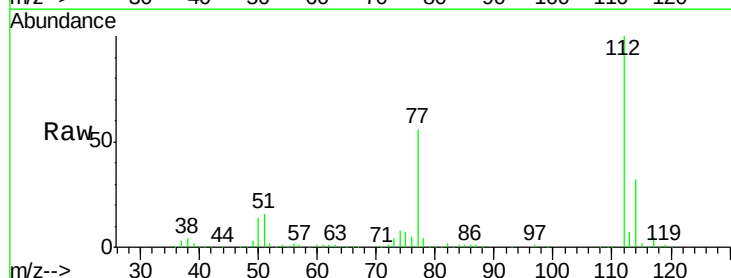

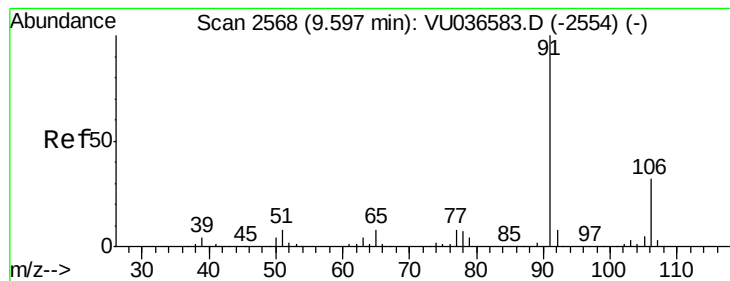

#52

Ethylbenzene

Concen: 103.655 ug/L

RT: 9.60 min Scan# 2568

Delta R.T. 0.00 min

Lab File: VU036605.D

Acq: 29 Jan 2020 20:09

Instrument :

MSVOA_U

ClientSampleId :


GASZ4MSD

Tot Ion: 91 Resp: 1091591

Ion Ratio Lower Upper




91 100

106 32.4 22.6 42.0

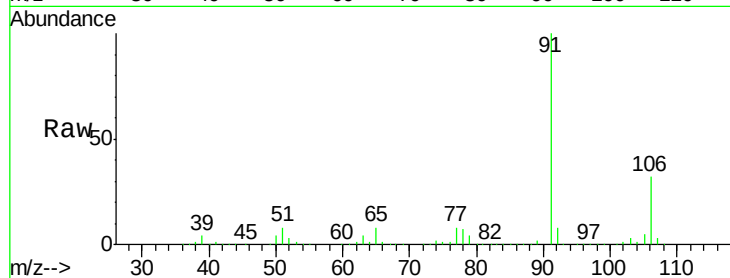

Abundance Ion 91.00 (90.70 to 91.70): VU036583.D (-2554) (-)

Ion 106.00 (105.70 to 106.70): VU036583.D (-2554) (-)

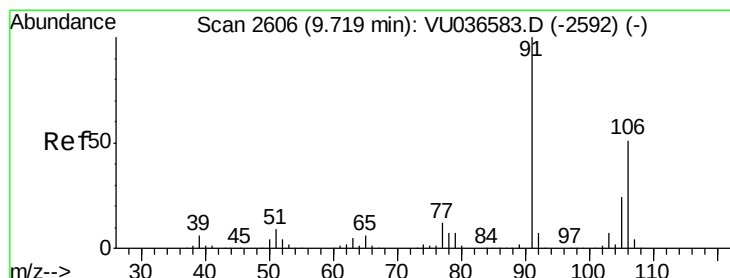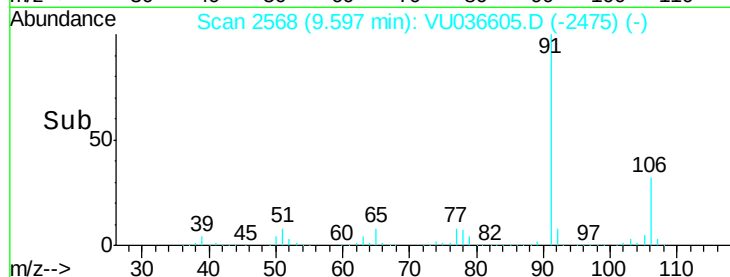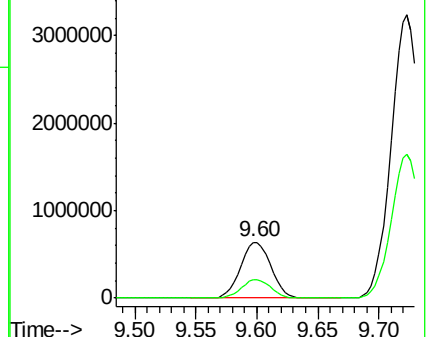

#53

m,p-Xylene

Concen: 681.409 ug/L

RT: 9.72 min Scan# 2607

Delta R.T. 0.00 min

Lab File: VU036605.D


Acq: 29 Jan 2020 20:09

Tgt Ion: 106 Resp: 2798858

Ion Ratio Lower Upper



106 100


91 196.2 139.4 259.0

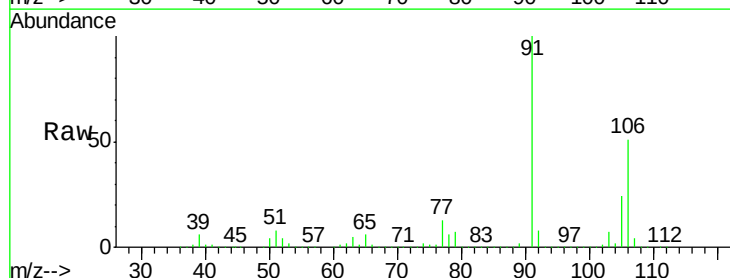

Abundance Ion 106.00 (105.70 to 106.70): VU036583.D (-2592) (-)

Ion 91.00 (90.70 to 91.70): VU036583.D (-2592) (-)

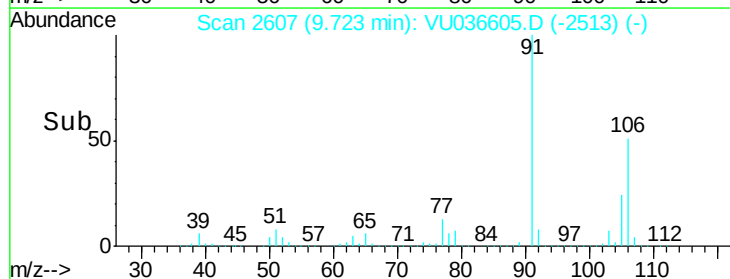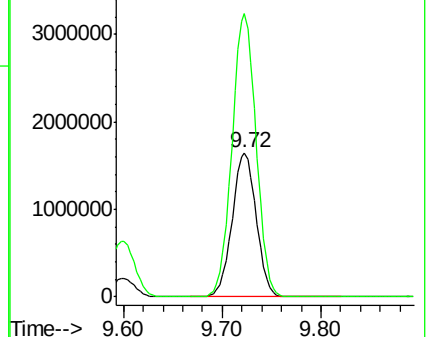

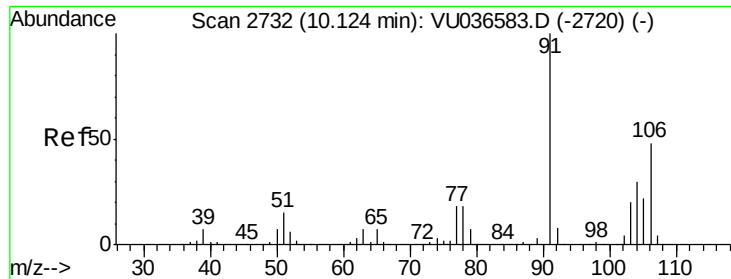

#54

o-xylene

Concen: 304.789 ug/L

RT: 10.13 min Scan# 2733

Delta R.T. 0.00 min

Lab File: VU036605.D

Acq: 29 Jan 2020 20:09

Instrument :

MSVOA_U

ClientSampleId :


GASZ4MSD

Tot Ion:106 Resp: 1248752

Ion Ratio Lower Upper




106 100

91 207.0 145.9 271.1

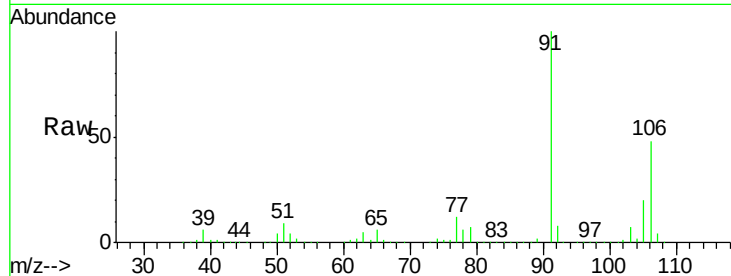

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VU0

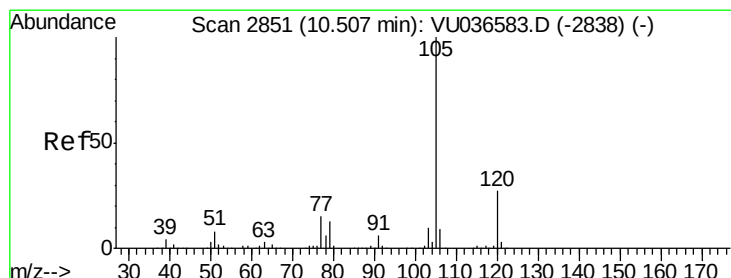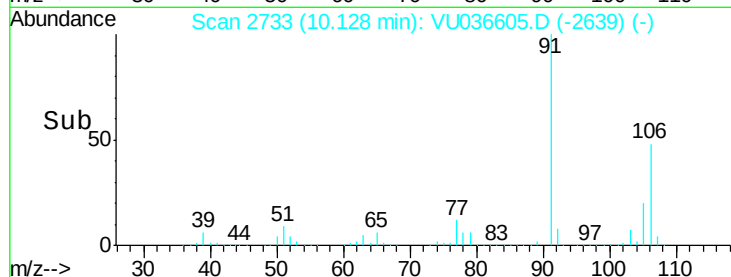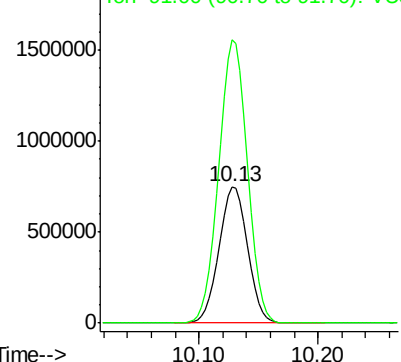

#56

Isopropylbenzene

Concen: 3.637 ug/L

RT: 10.51 min Scan# 2852

Delta R.T. 0.00 min

Lab File: VU036605.D

Acq: 29 Jan 2020 20:09


Tgt Ion:105 Resp: 37882

Ion Ratio Lower Upper

105 100

120 27.7 21.6 32.4

77 15.7 11.8 17.8

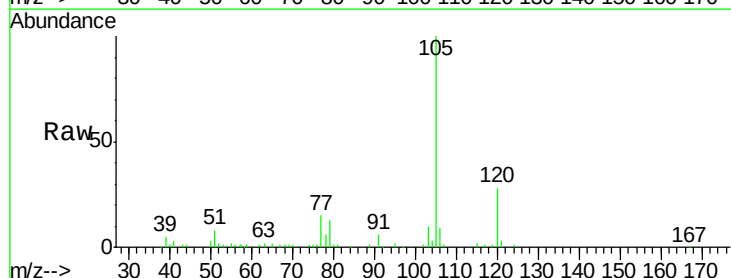

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

Ion 77.00 (76.70 to 77.70): VU0

