


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU012920\
 Data File : VU036582.D
 Acq On : 29 Jan 2020 10:05
 Operator : JC/MD
 Sample : BFB44
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB44

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis
 Last Update : Thu Jan 30 02:48:11 2020

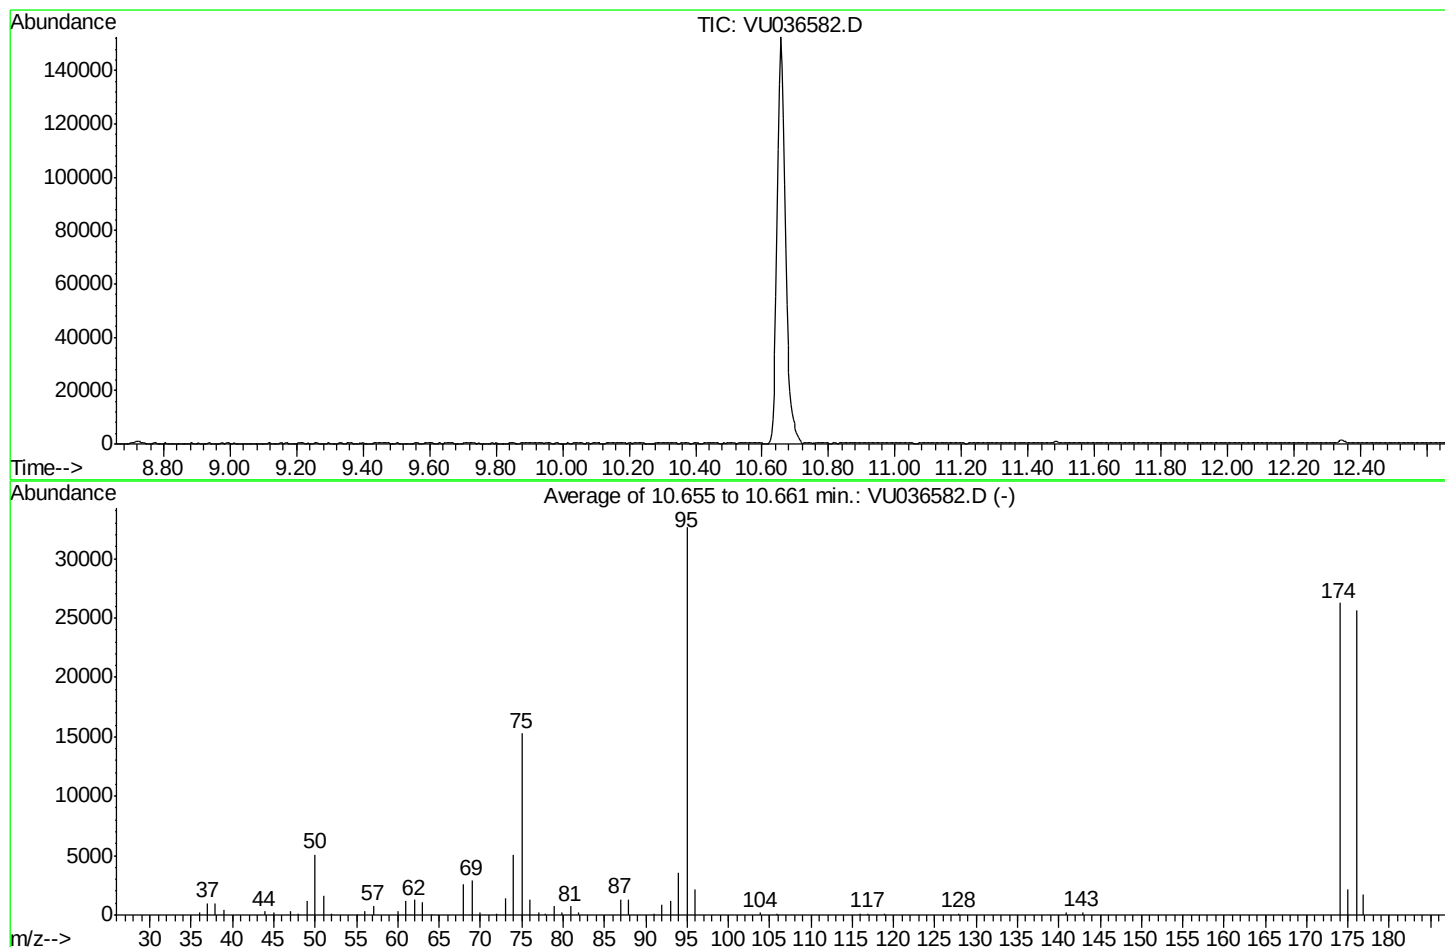

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	5121	PASS
75	95	30	80	46.8	15263	PASS
95	95	100	100	100.0	32629	PASS
96	95	5	9	6.5	2128	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.5	26253	PASS
175	174	5	9	8.1	2129	PASS
176	174	95	101	97.8	25685	PASS
177	176	5	9	6.9	1776	PASS

m/z	Abundance
35.90	221.0
37.00	1018.0
38.00	1032.0
38.90	399.0
43.90	503.0
44.90	282.0
47.00	384.0
47.90	145.0
49.00	1156.0
50.00	5328.0
51.00	1560.0
52.00	110.0
56.00	367.0
57.00	752.0
60.00	254.0
61.00	1212.0
62.00	1307.0
63.00	1085.0
68.00	2588.0
69.00	2795.0
70.00	236.0
71.90	165.0
73.00	1478.0
74.00	5360.0
75.00	15719.0
76.00	1438.0
77.00	229.0
77.90	140.0
78.90	746.0
79.80	222.0
80.90	766.0
81.90	205.0
87.00	1372.0
87.90	1329.0
90.90	114.0
92.00	912.0
93.00	1250.0
94.00	3460.0
95.00	33456.0
96.00	2217.0
103.90	173.0
105.90	177.0
117.00	140.0
118.80	119.0
127.90	145.0
140.90	183.0
142.90	280.0
174.00	26160.0
175.00	2228.0
176.00	25416.0
176.90	1795.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
35.90	240.0
37.00	990.0
37.90	980.0
39.00	399.0
43.90	515.0
44.90	283.0
47.00	366.0
47.90	117.0
49.00	1247.0
50.00	5296.0
51.00	1621.0
52.00	116.0
56.00	383.0
57.10	799.0
60.00	295.0
61.00	1235.0
62.00	1311.0
63.00	1139.0
64.00	112.0
68.00	2666.0
69.00	2931.0
70.00	218.0
71.80	171.0
73.00	1488.0
74.00	5282.0
75.00	15687.0
76.00	1339.0
77.00	210.0
77.80	139.0
78.90	737.0
79.90	214.0
80.90	771.0
81.90	201.0
87.00	1341.0
88.00	1287.0
91.00	114.0
92.00	895.0
92.90	1220.0
94.00	3647.0
95.00	33608.0
96.00	2187.0
103.90	185.0
105.90	155.0
115.90	109.0
116.90	131.0
118.80	121.0
128.00	138.0
140.90	233.0
142.90	275.0
174.00	26960.0
175.00	2191.0
176.00	26464.0
176.90	1838.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	229.0
37.00	934.0
37.90	862.0
39.00	358.0
43.90	523.0
45.00	225.0
47.00	317.0
47.90	106.0
49.00	1210.0
50.00	4741.0
51.00	1534.0
55.00	108.0
56.00	385.0
57.10	744.0
60.00	283.0
61.00	1205.0
62.00	1262.0
63.00	1000.0
68.00	2558.0
69.00	2860.0
69.90	180.0
72.00	156.0
73.00	1332.0
74.00	4680.0
75.00	14385.0
76.00	1138.0
77.00	171.0
77.90	137.0
78.90	678.0
79.90	181.0
80.90	701.0
81.90	175.0
86.90	1266.0
88.00	1211.0
91.00	112.0
92.00	853.0
92.90	1098.0
94.00	3557.0
95.00	30824.0
96.00	1982.0
103.90	151.0
105.90	109.0
116.00	128.0
116.80	135.0
118.90	107.0
128.00	142.0
140.90	284.0
142.90	234.0
174.00	25640.0
175.00	1968.0
176.00	25176.0
176.90	1697.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
44.00	227.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44