

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012921\
 Data File : VU042217.D
 Acq On : 29 Jan 2021 10:07
 Operator : SY/MD
 Sample : VU0129WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0129WBL01

Quant Time: Jan 30 00:46:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012821DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Jan 29 09:59:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.125	96	13134	1.00	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	5167	1.01	ug/l	0.00
Spiked Amount 1.000			Recovery	=	101.00%	
68) 1,2-Dichlorobenzene-d4	12.205	152	5117	0.99	ug/l	0.00
Spiked Amount 1.000			Recovery	=	99.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012921\
Data File : VU042217.D
Acq On : 29 Jan 2021 10:07
Operator : SY/MD
Sample : VU0129WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0129WBL01

Quant Time: Jan 30 00:46:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012821DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Jan 29 09:59:59 2021
Response via : Initial Calibration

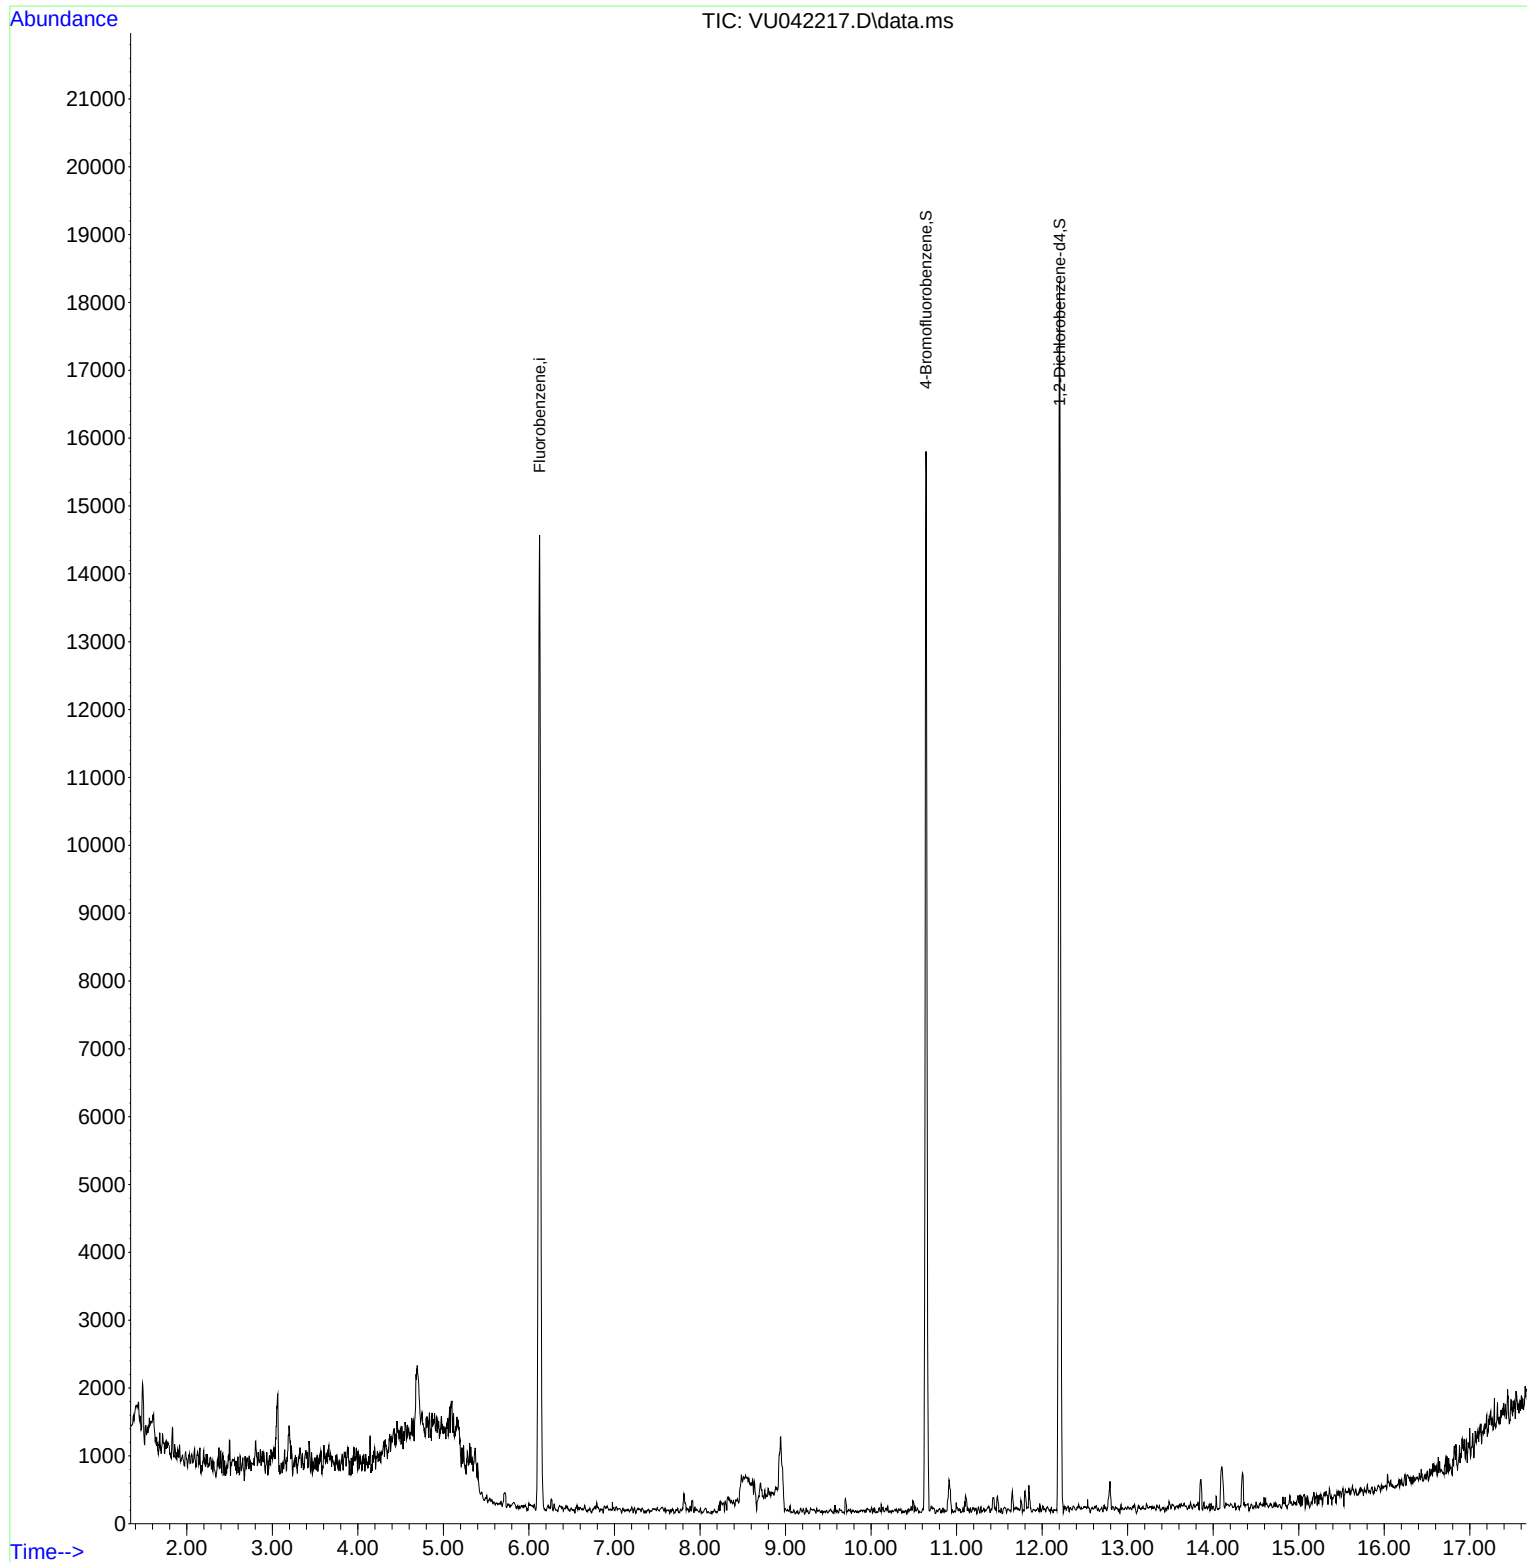




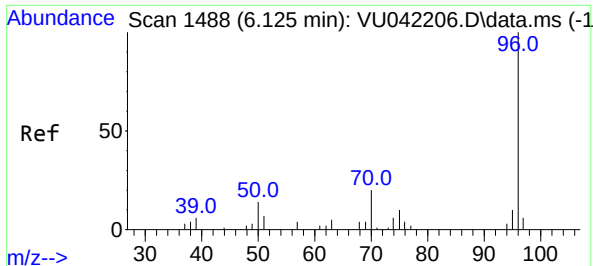


#1
Fluorobenzene
Concen: 1.00 ug/l
RT: 6.125 min Scan# 1488
Delta R.T. -0.000 min
Lab File: VU042217.D
Acq: 29 Jan 2021 10:07

Instrument :
MSVOA_U
ClientSampleId :
VU0129WBL01

Tgt Ion: 96 Resp: 13134




Ion	Ratio	Lower	Upper
96	100		
70	20.4	16.3	24.5
95	9.4	7.6	11.4
97	6.2	0.0	0.0

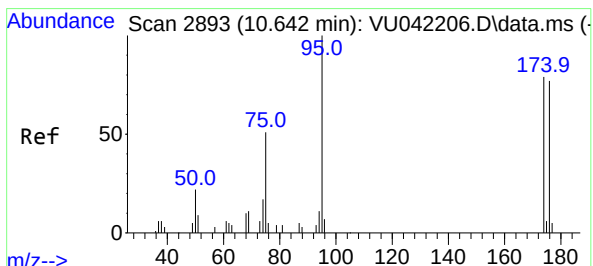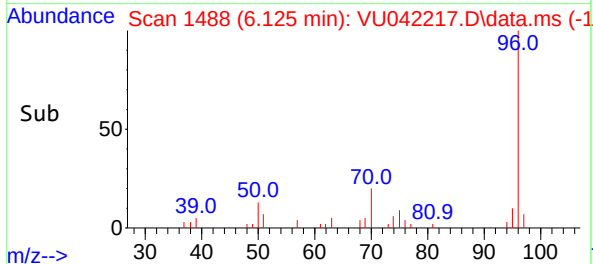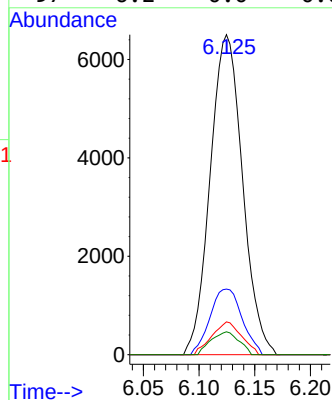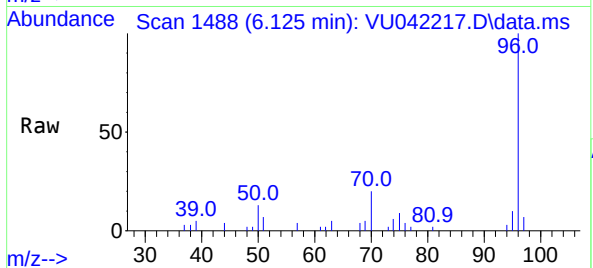


#57
4-Bromofluorobenzene
Concen: 1.01 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.000 min
Lab File: VU042217.D
Acq: 29 Jan 2021 10:07

Tgt Ion: 95 Resp: 5167


Ion	Ratio	Lower	Upper
95	100		
174	81.3	69.6	104.4
176	78.5	65.5	98.3

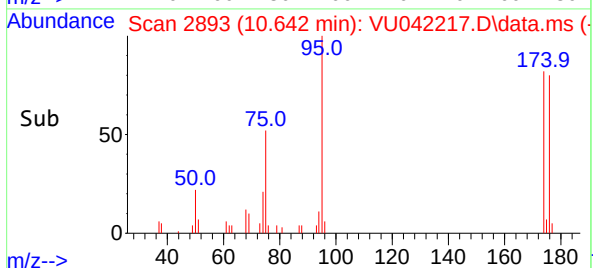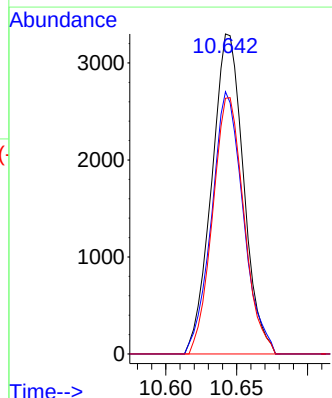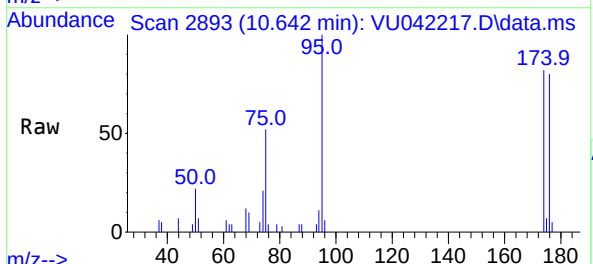

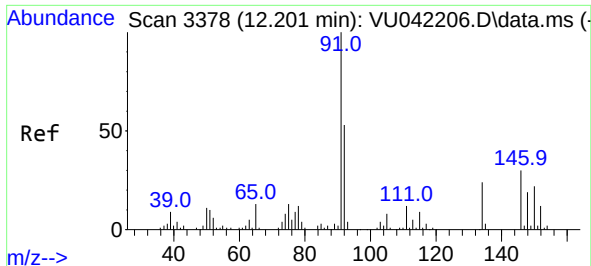

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.99 ug/l
 RT: 12.205 min Scan# 3379
 Delta R.T. 0.004 min
 Lab File: VU042217.D
 Acq: 29 Jan 2021 10:07

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0129WBL01

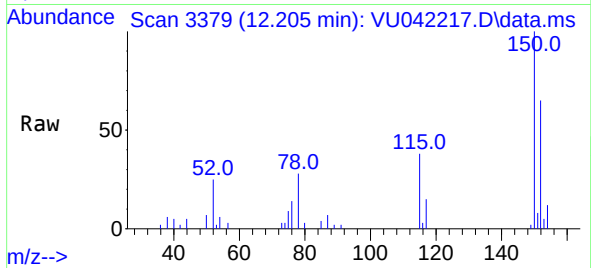

Tgt Ion:	152	Resp:	5117
Ion Ratio	Lower	Upper	
152	100		
115	57.8	0.0	243.2
150	154.4	0.0	642.6

