

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012921\
 Data File : VU042218.D
 Acq On : 29 Jan 2021 10:42
 Operator : SY/MD
 Sample : M1126-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-EDBCP-WS

Quant Time: Jan 30 00:47:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012821DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Jan 29 09:59:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.125	96	13413	1.00	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	5037	0.97	ug/l	0.00
Spiked Amount 1.000			Recovery	=	97.00%	
68) 1,2-Dichlorobenzene-d4	12.205	152	5189	0.98	ug/l	0.00
Spiked Amount 1.000			Recovery	=	98.00%	
Target Compounds						
56) 1,2-Dibromoethane	8.935	107	3863	1.34	ug/l	99
71) 1,2,3-Trichloropropane	10.832	75	1108	0.37	ug/l	71
86) 1,2-Dibromo-3-Chloropr...	13.009	75	1185	1.52	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012921\
Data File : VU042218.D
Acq On : 29 Jan 2021 10:42
Operator : SY/MD
Sample : M1126-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS

Quant Time: Jan 30 00:47:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012821DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Jan 29 09:59:59 2021
Response via : Initial Calibration




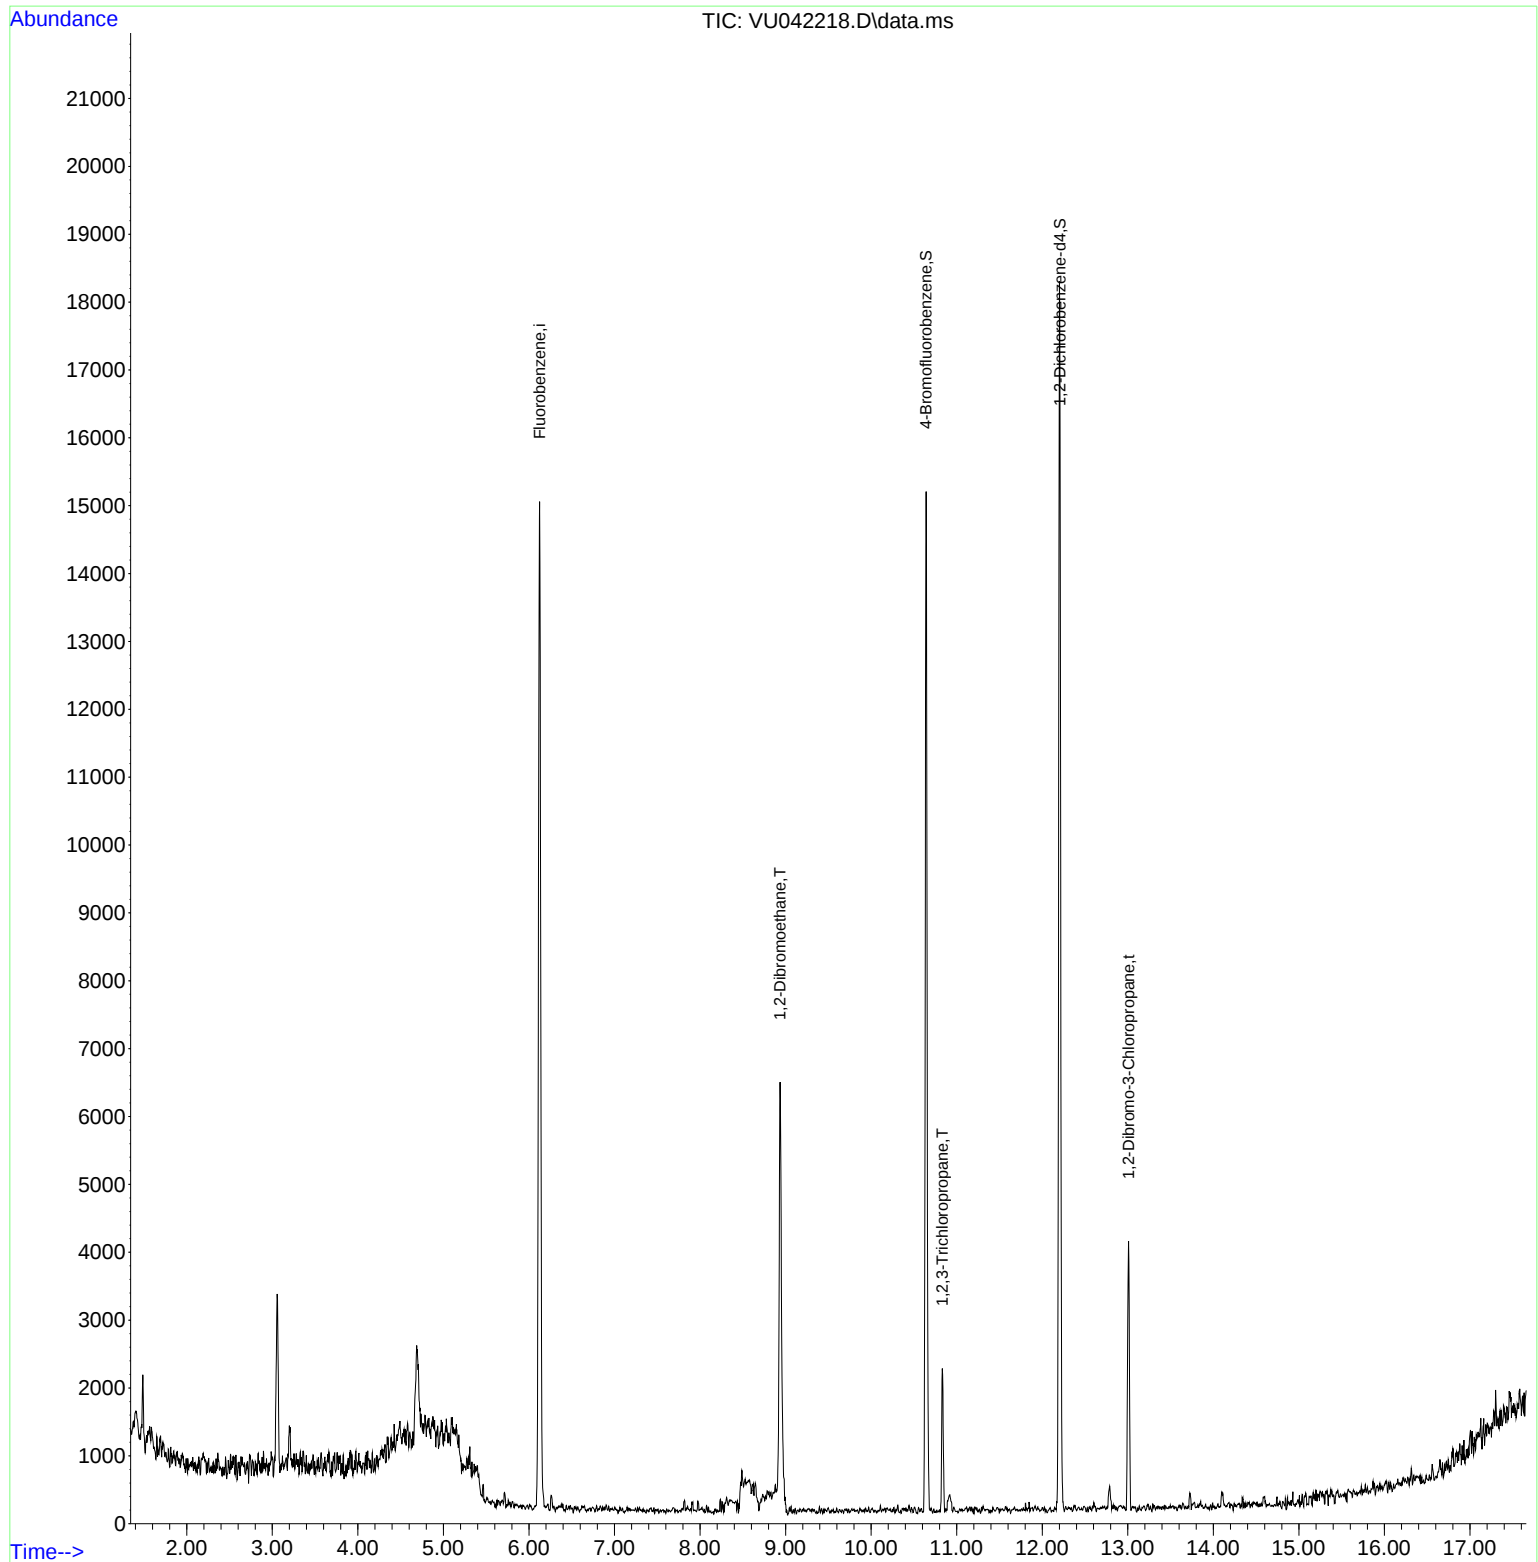


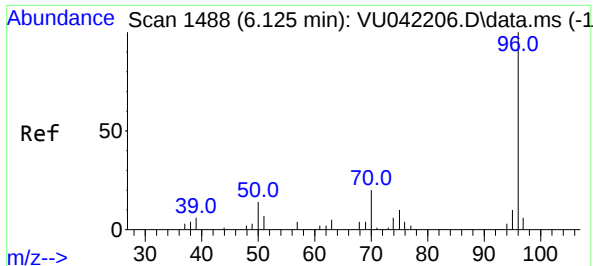

#1
Fluorobenzene
Concen: 1.00 ug/l
RT: 6.125 min Scan# 1488
Delta R.T. -0.000 min
Lab File: VU042218.D
Acq: 29 Jan 2021 10:42




Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS


Tgt Ion: 96	Resp: 13413
Ion Ratio	Lower Upper
96 100	
70 22.0	16.3 24.5
95 8.4	7.6 11.4
97 6.4	0.0 0.0#

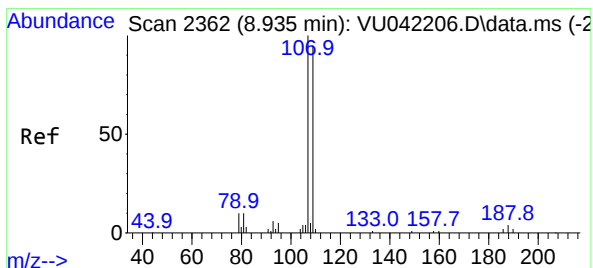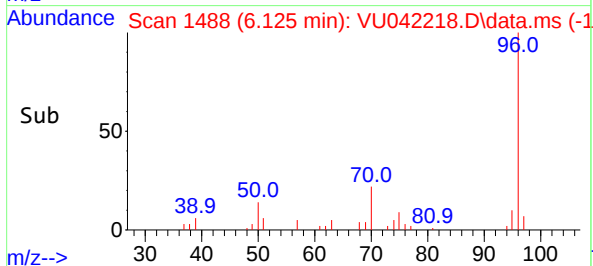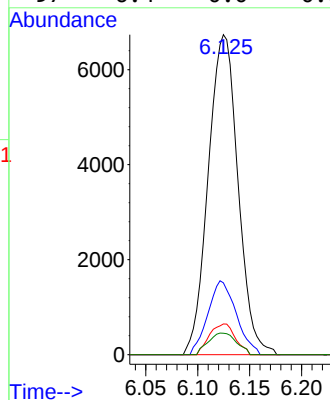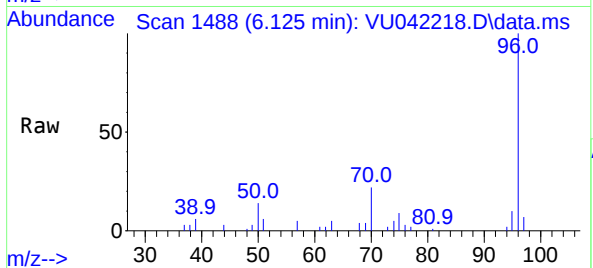

#56
1,2-Dibromoethane
Concen: 1.34 ug/l
RT: 8.935 min Scan# 2362
Delta R.T. -0.000 min
Lab File: VU042218.D
Acq: 29 Jan 2021 10:42

Tgt Ion:107	Resp:	3863	
Ion	Ratio	Lower	Upper
107	100		
109	92.5	0.0	187.2


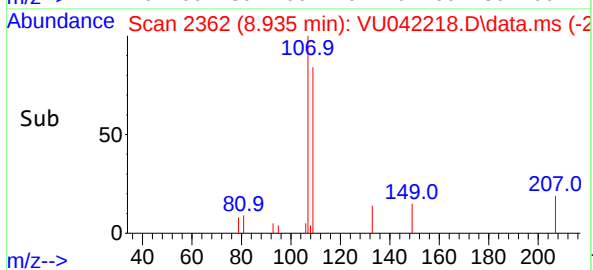
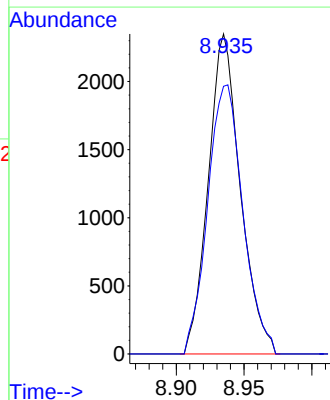
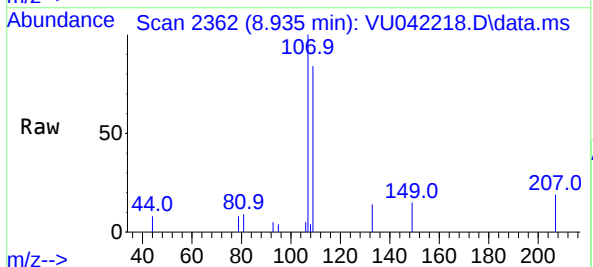


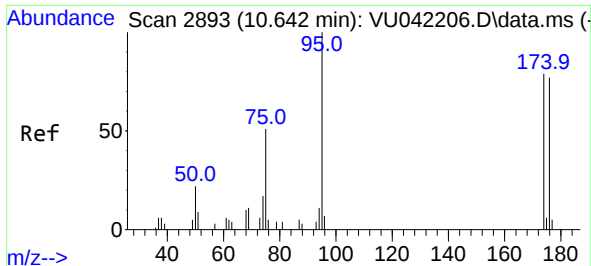

#57
4-Bromofluorobenzene
Concen: 0.97 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.000 min
Lab File: VU042218.D
Acq: 29 Jan 2021 10:42




Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS


Tgt Ion: 95 Resp: 5037
Ion Ratio Lower Upper
95 100
174 83.3 69.6 104.4
176 79.3 65.5 98.3

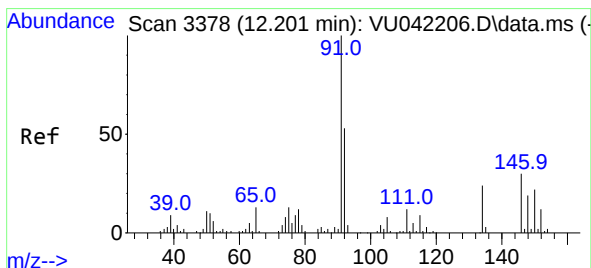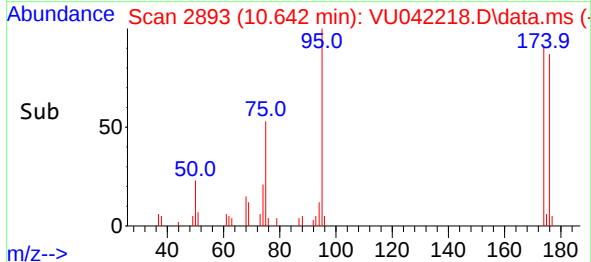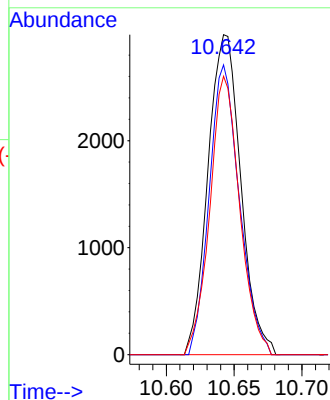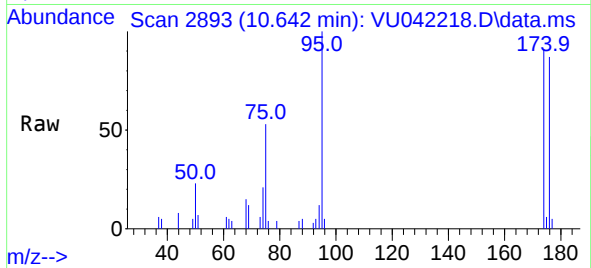

#68
1,2-Dichlorobenzene-d4
Concen: 0.98 ug/l
RT: 12.205 min Scan# 3379
Delta R.T. 0.004 min
Lab File: VU042218.D
Acq: 29 Jan 2021 10:42

Tgt Ion:152 Resp: 5189
Ion Ratio Lower Upper
152 100
115 58.5 0.0 243.2
150 160.9 0.0 642.6


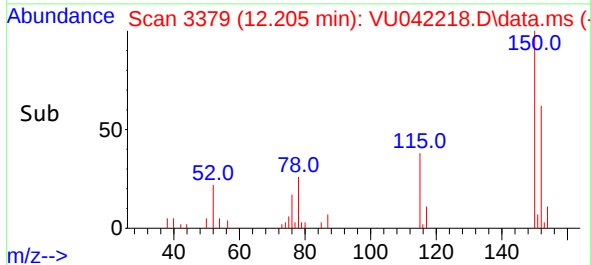
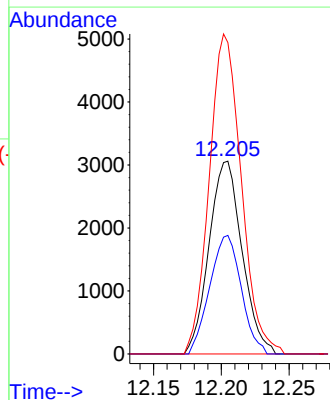
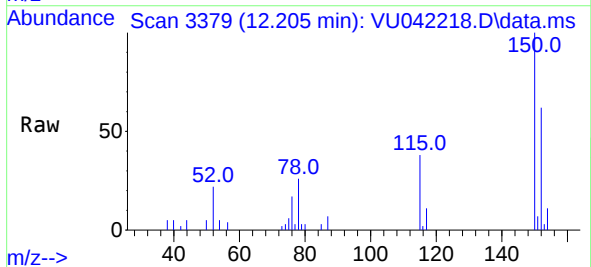


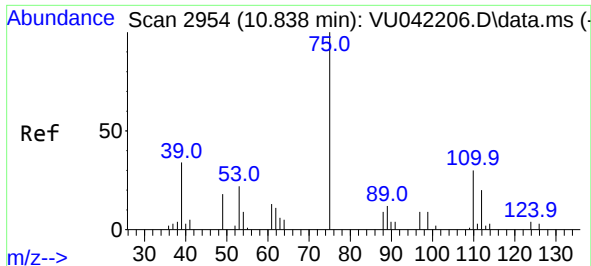

#71
1,2,3-Trichloropropane
Concen: 0.37 ug/l
RT: 10.832 min Scan# 2952
Delta R.T. -0.006 min
Lab File: VU042218.D
Acq: 29 Jan 2021 10:42

Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS

Tgt Ion: 75	Resp:	1108	
Ion	Ratio	Lower	Upper
75	100		
77	21.5	0.0	107.2
110	28.3	0.0	69.0
97	11.4	0.0	36.6

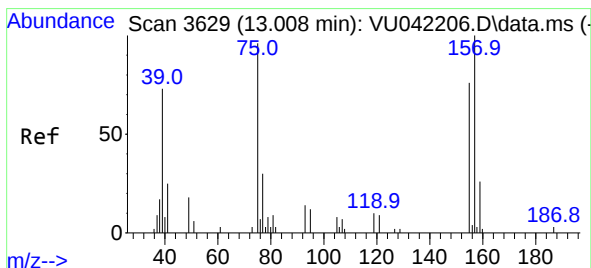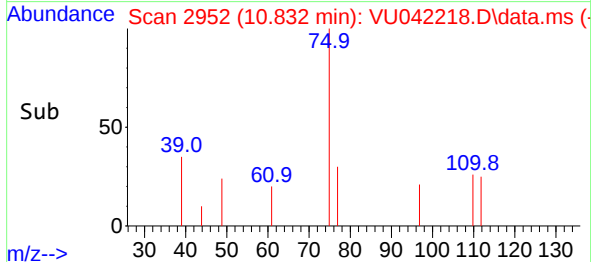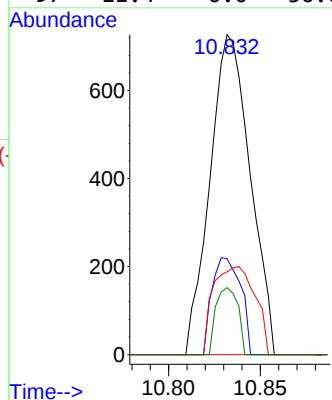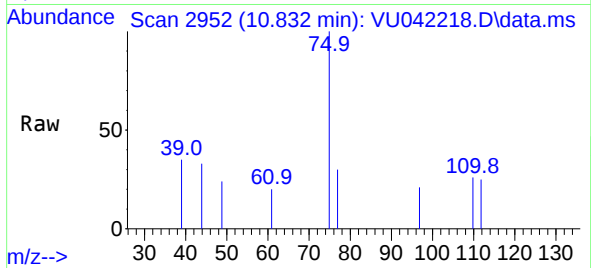

#86
1,2-Dibromo-3-Chloropropane
Concen: 1.52 ug/l
RT: 13.009 min Scan# 3629
Delta R.T. 0.001 min
Lab File: VU042218.D
Acq: 29 Jan 2021 10:42

Tgt Ion: 75	Resp:	1185	
Ion	Ratio	Lower	Upper
75	100		
155	75.9	65.4	98.0
157	104.2	83.3	124.9

