


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012921\
 Data File : VU042215.D
 Acq On : 29 Jan 2021 09:00
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012821DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Jan 29 09:59:59 2021

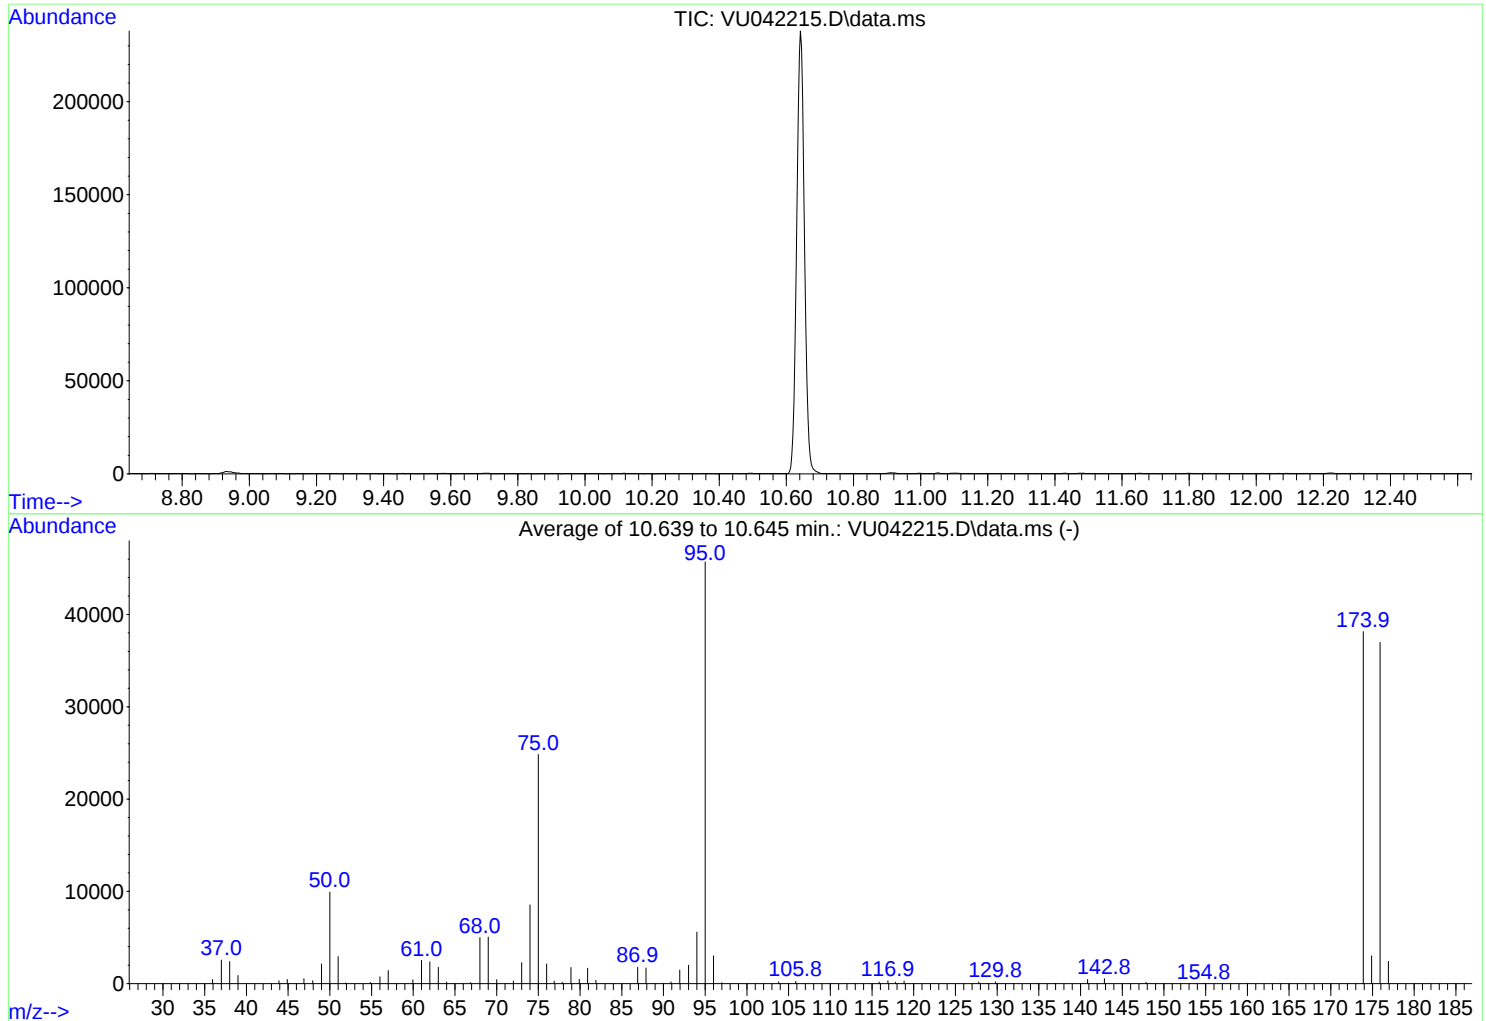

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	9918	PASS
75	95	30	60	54.3	24827	PASS
95	95	100	100	100.0	45709	PASS
96	95	5	9	6.6	3025	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.5	38149	PASS
175	174	5	9	7.9	3019	PASS
176	174	95	101	97.0	36987	PASS
177	176	5	9	6.5	2405	PASS