

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012924\
 Data File : VU057709.D
 Acq On : 29 Jan 2024 12:05
 Operator : MD/SY
 Sample : P1239-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 30 00:32:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 30 00:30:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	61831	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	56456	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	25369	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	11634	3.415	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.400%
7) Chloroethane-d5	1.911	69	10517	3.684	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.600%
11) 1,1-Dichloroethene-d2	2.563	65	5875	3.668	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.400%
20) 2-Butanone-d5	4.631	46	33496	52.120	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.240%
24) Chloroform-d	5.055	84	28903	4.180	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.600%
26) 1,2-Dichloroethane-d4	5.695	65	14651	4.662	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
32) Benzene-d6	5.721	84	54730	4.133	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.600%
36) 1,2-Dichloropropane-d6	6.682	67	17615	4.410	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.200%
41) Toluene-d8	7.894	98	50001	3.978	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.600%
43) trans-1,3-Dichloroprop...	8.177	79	4882	3.067	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	61.400%
46) 2-Hexanone-d5	8.631	63	23938	47.130	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.260%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	12256	4.578	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	16536	4.645	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.800%
Target Compounds						Qvalue
3) Chloromethane	1.515	50	722	0.138	ug/L	97
5) Vinyl chloride	1.602	62	18988	3.403	ug/L	98
12) 1,1-Dichloroethene	2.576	96	4936	1.098	ug/L #	49
18) trans-1,2-Dichloroethene	3.351	96	938	0.198	ug/L	94
19) 1,1-Dichloroethane	3.862	63	22122	2.531	ug/L	98
22) cis-1,2-Dichloroethene	4.656	96	1115583	219.245	ug/L	100
34) Trichloroethene	6.541	95	2053	0.385	ug/L	95
35) Methylcyclohexane	6.685	83	4008	0.465	ug/L #	20
37) 1,2-Dichloropropane	6.682	63	2056	0.424	ug/L #	89
61) 1,2,3-Trichloropropane	11.807	75	3215	1.263	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012924\
Data File : VU057709.D
Acq On : 29 Jan 2024 12:05
Operator : MD/SY
Sample : P1239-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jan 30 00:32:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 30 00:30:52 2024
Response via : Initial Calibration




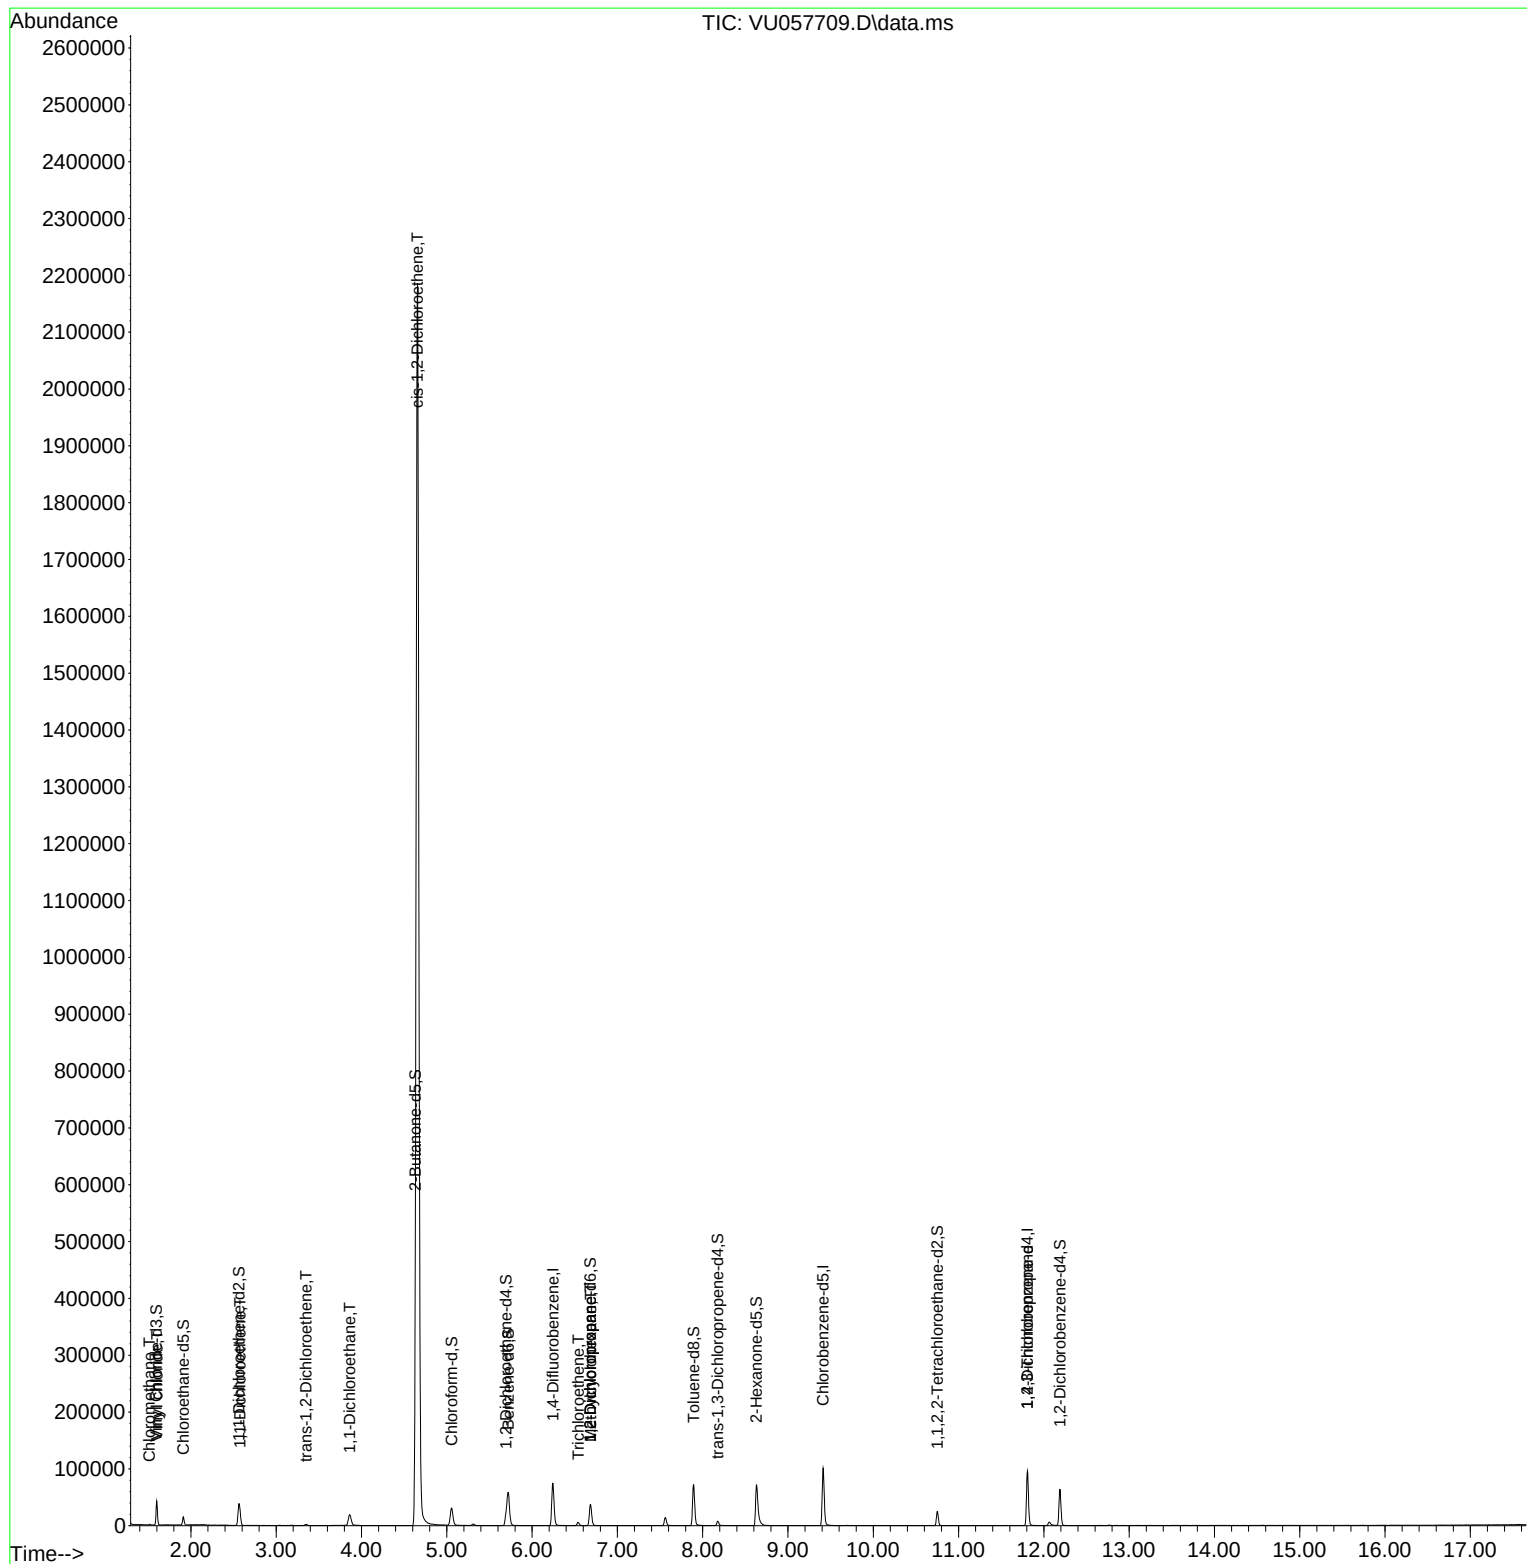


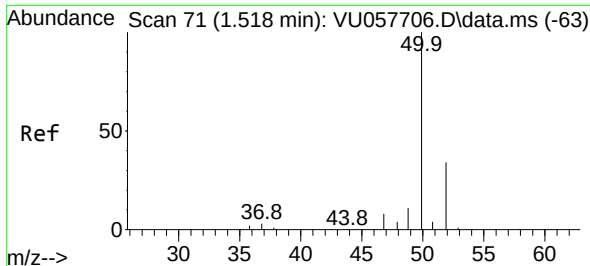

#3
Chloromethane
Concen: 0.138 ug/L
RT: 1.515 min Scan# 71
Delta R.T. -0.003 min
Lab File: VU057709.D
Acq: 29 Jan 2024 12:05




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 50 Resp: 722
Ion Ratio Lower Upper
50 100
52 35.6 23.7 43.9

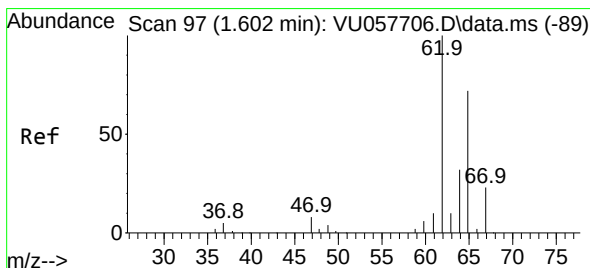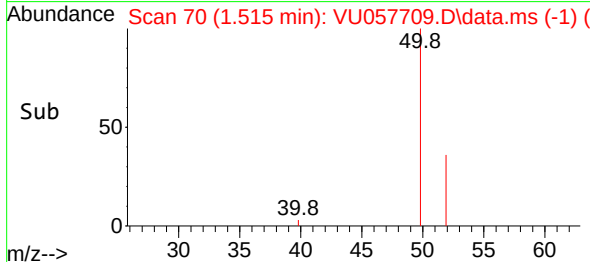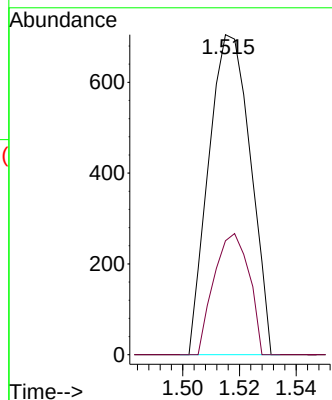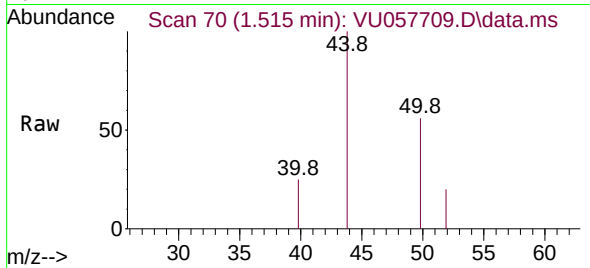

#5
Vinyl chloride
Concen: 3.403 ug/L
RT: 1.602 min Scan# 97
Delta R.T. 0.000 min
Lab File: VU057709.D
Acq: 29 Jan 2024 12:05

Tgt Ion: 62 Resp: 18988
Ion Ratio Lower Upper
62 100
64 33.7 22.8 42.4


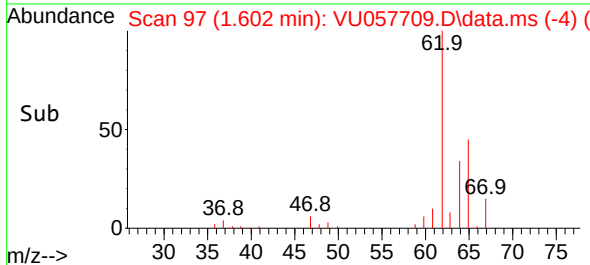
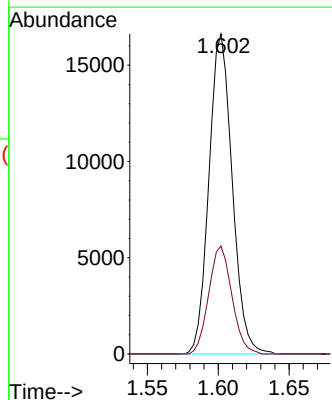
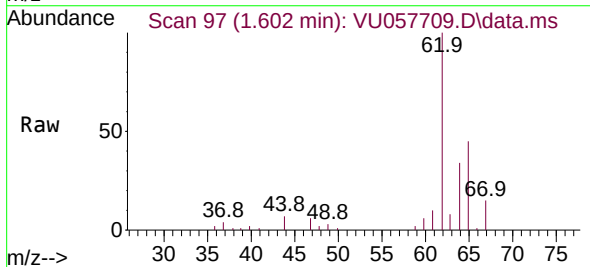


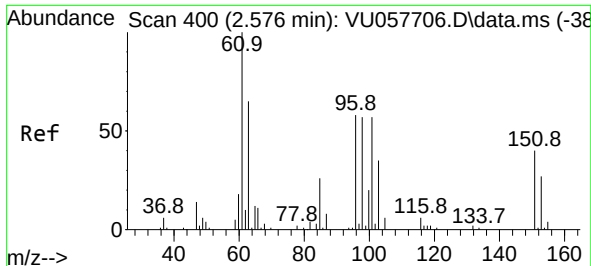

#12
1,1-Dichloroethene
Concen: 1.098 ug/L
RT: 2.576 min Scan# 400
Delta R.T. 0.000 min
Lab File: VU057709.D
Acq: 29 Jan 2024 12:05




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 96 Resp: 4936
Ion Ratio Lower Upper
96 100
61 196.7 120.7 224.1
63 213.5 72.5 134.7#

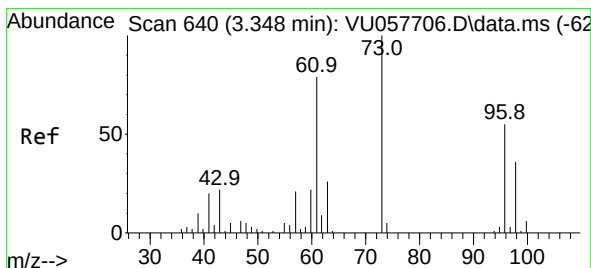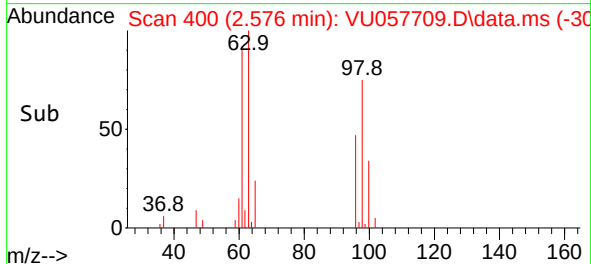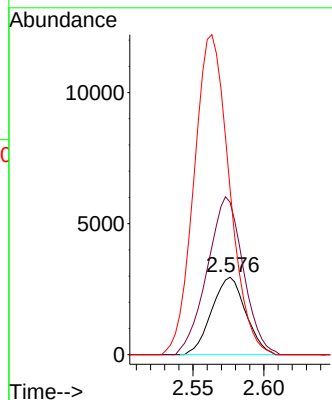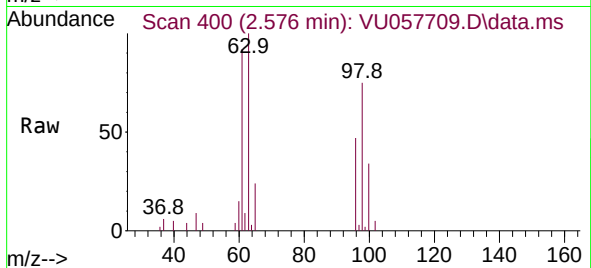

#18
trans-1,2-Dichloroethene
Concen: 0.198 ug/L
RT: 3.351 min Scan# 641
Delta R.T. 0.003 min
Lab File: VU057709.D
Acq: 29 Jan 2024 12:05

Tgt Ion: 96 Resp: 938
Ion Ratio Lower Upper
96 100
61 136.6 99.3 184.5
98 57.0 44.5 82.7


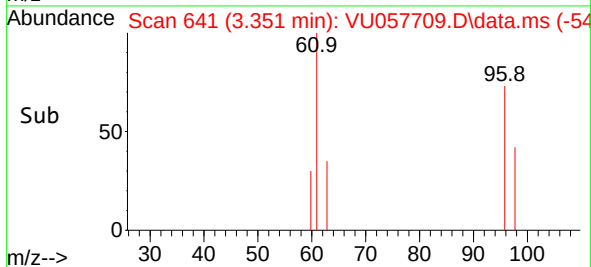
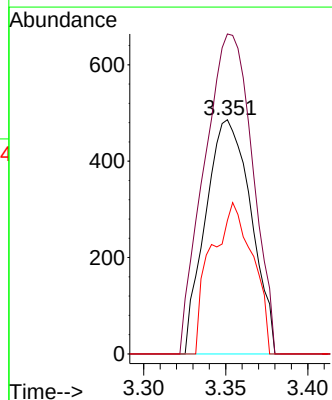
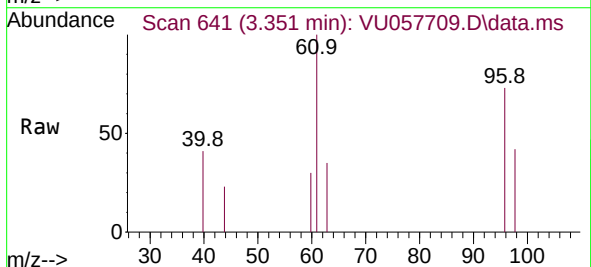


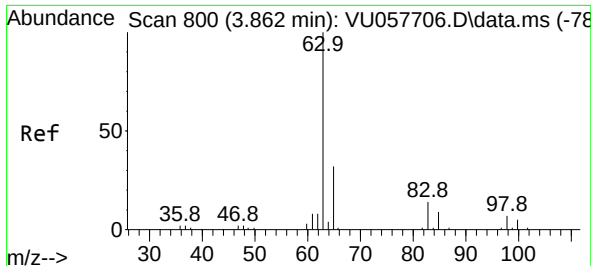

#19
1,1-Dichloroethane
Concen: 2.531 ug/L
RT: 3.862 min Scan# 800
Delta R.T. 0.000 min
Lab File: VU057709.D
Acq: 29 Jan 2024 12:05




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 63 Resp: 22122
Ion Ratio Lower Upper
63 100
65 32.0 23.0 42.8
83 13.1 9.7 17.9

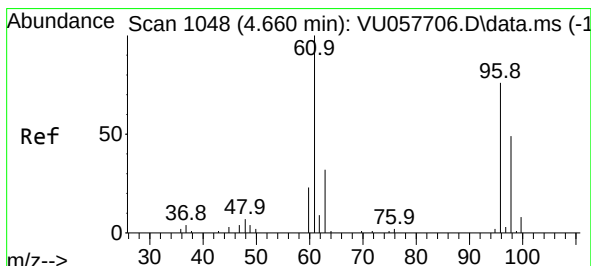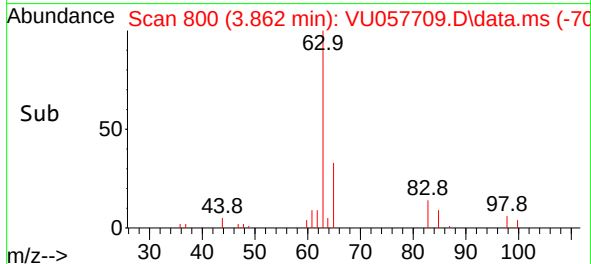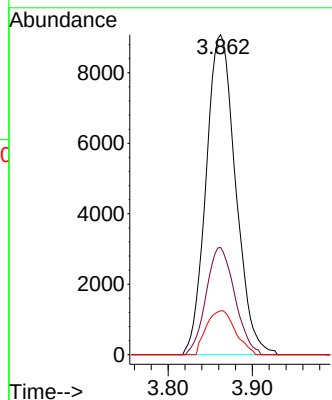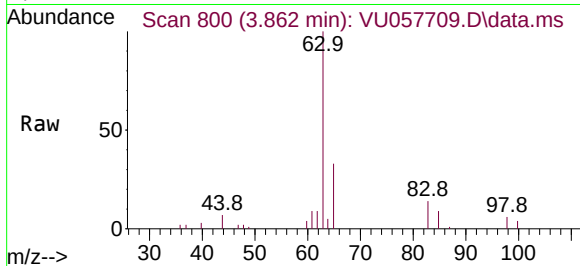

#22
cis-1,2-Dichloroethene
Concen: 219.245 ug/L
RT: 4.656 min Scan# 1047
Delta R.T. -0.003 min
Lab File: VU057709.D
Acq: 29 Jan 2024 12:05

Tgt Ion: 96 Resp: 1115583
Ion Ratio Lower Upper
96 100
61 132.9 92.7 172.1
98 64.5 44.9 83.5

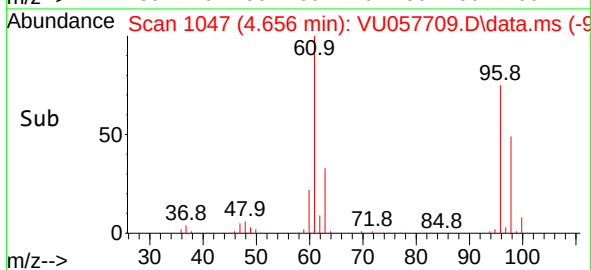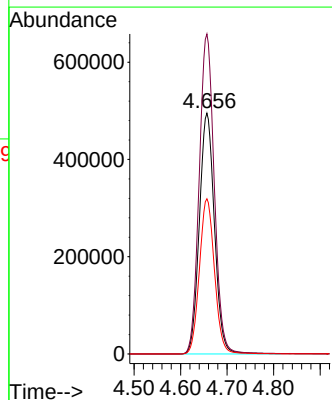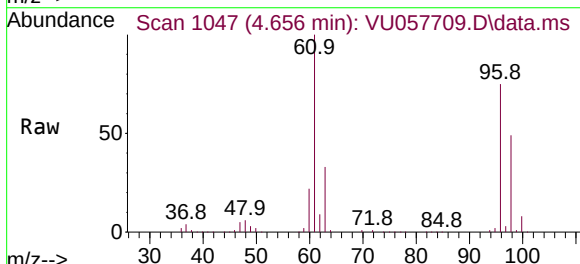




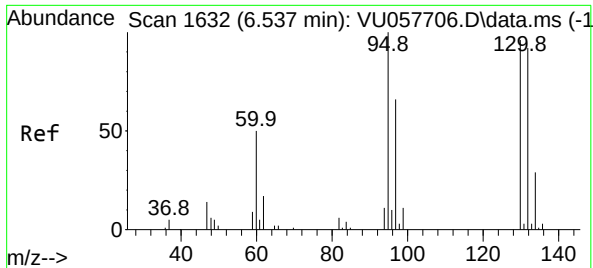


#34
Trichloroethene
Concen: 0.385 ug/L
RT: 6.541 min Scan# 1633
Delta R.T. 0.003 min
Lab File: VU057709.D
Acq: 29 Jan 2024 12:05

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 95 Resp: 2053




Ion	Ratio	Lower	Upper
95	100		
97	68.1	46.1	85.5
132	92.2	66.1	122.8
130	89.8	68.7	127.5

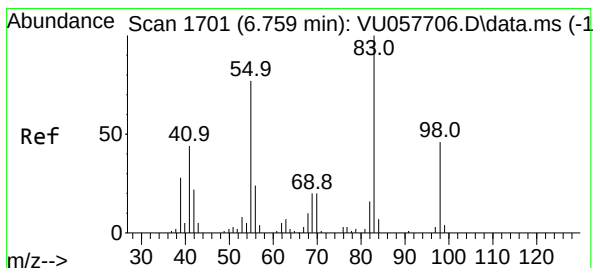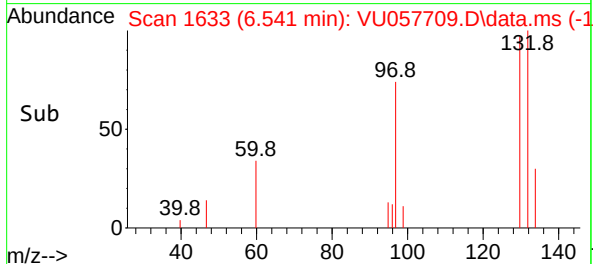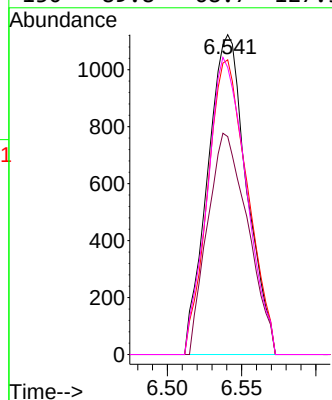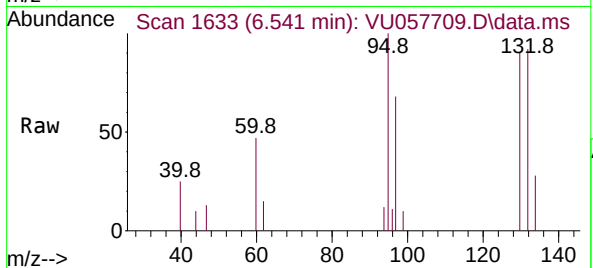


#35
Methylcyclohexane
Concen: 0.465 ug/L
RT: 6.685 min Scan# 1678
Delta R.T. -0.074 min
Lab File: VU057709.D
Acq: 29 Jan 2024 12:05

Tgt Ion: 83 Resp: 4008

Ion	Ratio	Lower	Upper
83	100		
55	0.0	61.4	92.0#
98	2.7	38.2	57.4#

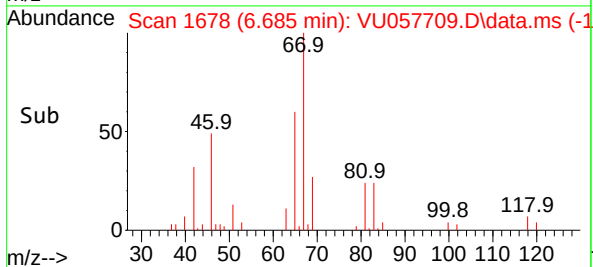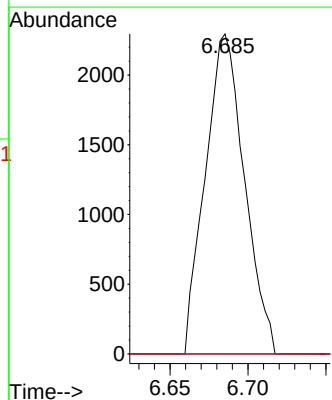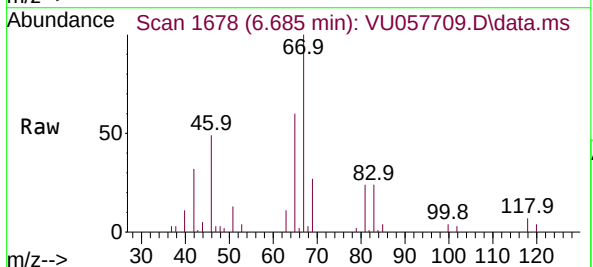

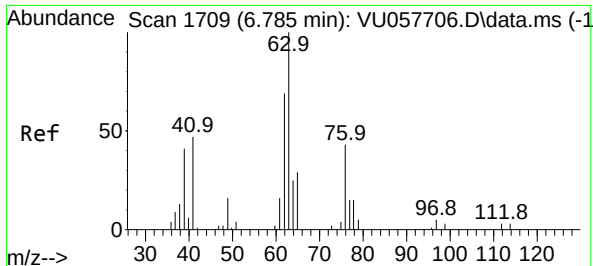

#37

1,2-Dichloropropane

Concen: 0.424 ug/L

RT: 6.682 min Scan# 1

Delta R.T. -0.103 min

Lab File: VU057709.D

Acq: 29 Jan 2024 12:05

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 63 Resp: 2056

Ion Ratio Lower Upper

63 100

112 0.0 3.0 4.4#

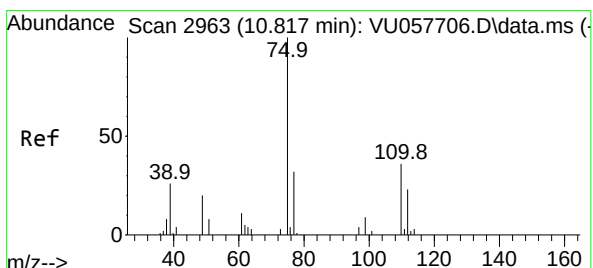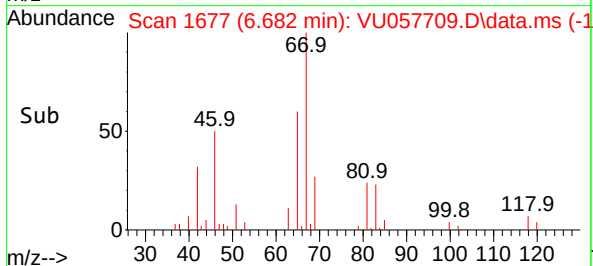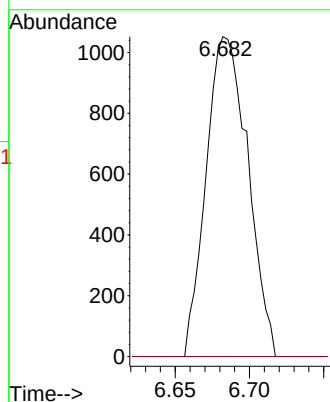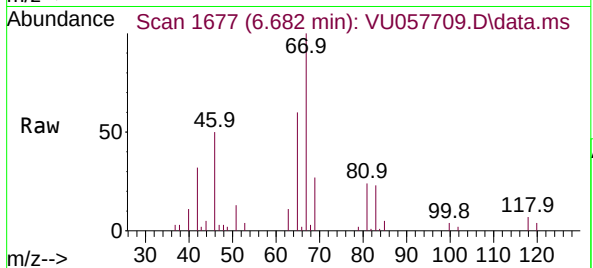

#61

1,2,3-Trichloropropane

Concen: 1.263 ug/L

RT: 11.807 min Scan# 3271

Delta R.T. 0.990 min

Lab File: VU057709.D

Acq: 29 Jan 2024 12:05

Tgt Ion: 75 Resp: 3215

Ion Ratio Lower Upper

75 100

110 0.0 30.1 45.1#

77 31.4 25.5 38.3

