

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012924\
 Data File : VU057719.D
 Acq On : 29 Jan 2024 16:07
 Operator : MD/SY
 Sample : P1239-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FD0

Quant Time: Jan 30 00:34:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 30 00:30:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	66826	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	61932	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	28423	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	19847	5.390	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.800%
7) Chloroethane-d5	1.911	69	16764	5.434	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.600%
11) 1,1-Dichloroethene-d2	2.563	65	9036	5.219	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	104.400%
20) 2-Butanone-d5	4.634	46	38062	54.798	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.600%
24) Chloroform-d	5.055	84	36760	4.919	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
26) 1,2-Dichloroethane-d4	5.695	65	18567	5.467	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.400%
32) Benzene-d6	5.721	84	76085	5.237	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.800%
36) 1,2-Dichloropropane-d6	6.682	67	22402	5.113	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.200%
41) Toluene-d8	7.891	98	69632	5.049	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.000%
43) trans-1,3-Dichloroprop...	8.177	79	8338	4.775	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.400%
46) 2-Hexanone-d5	8.631	63	29499	52.943	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.880%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	14786	5.034	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.600%
66) 1,2-Dichlorobenzene-d4	12.190	152	21887	5.487	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.800%
Target Compounds						
					Qvalue	
13) Acetone	2.650	43	3922	5.942	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012924\
Data File : VU057719.D
Acq On : 29 Jan 2024 16:07
Operator : MD/SY
Sample : P1239-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FD0

Quant Time: Jan 30 00:34:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 30 00:30:52 2024
Response via : Initial Calibration

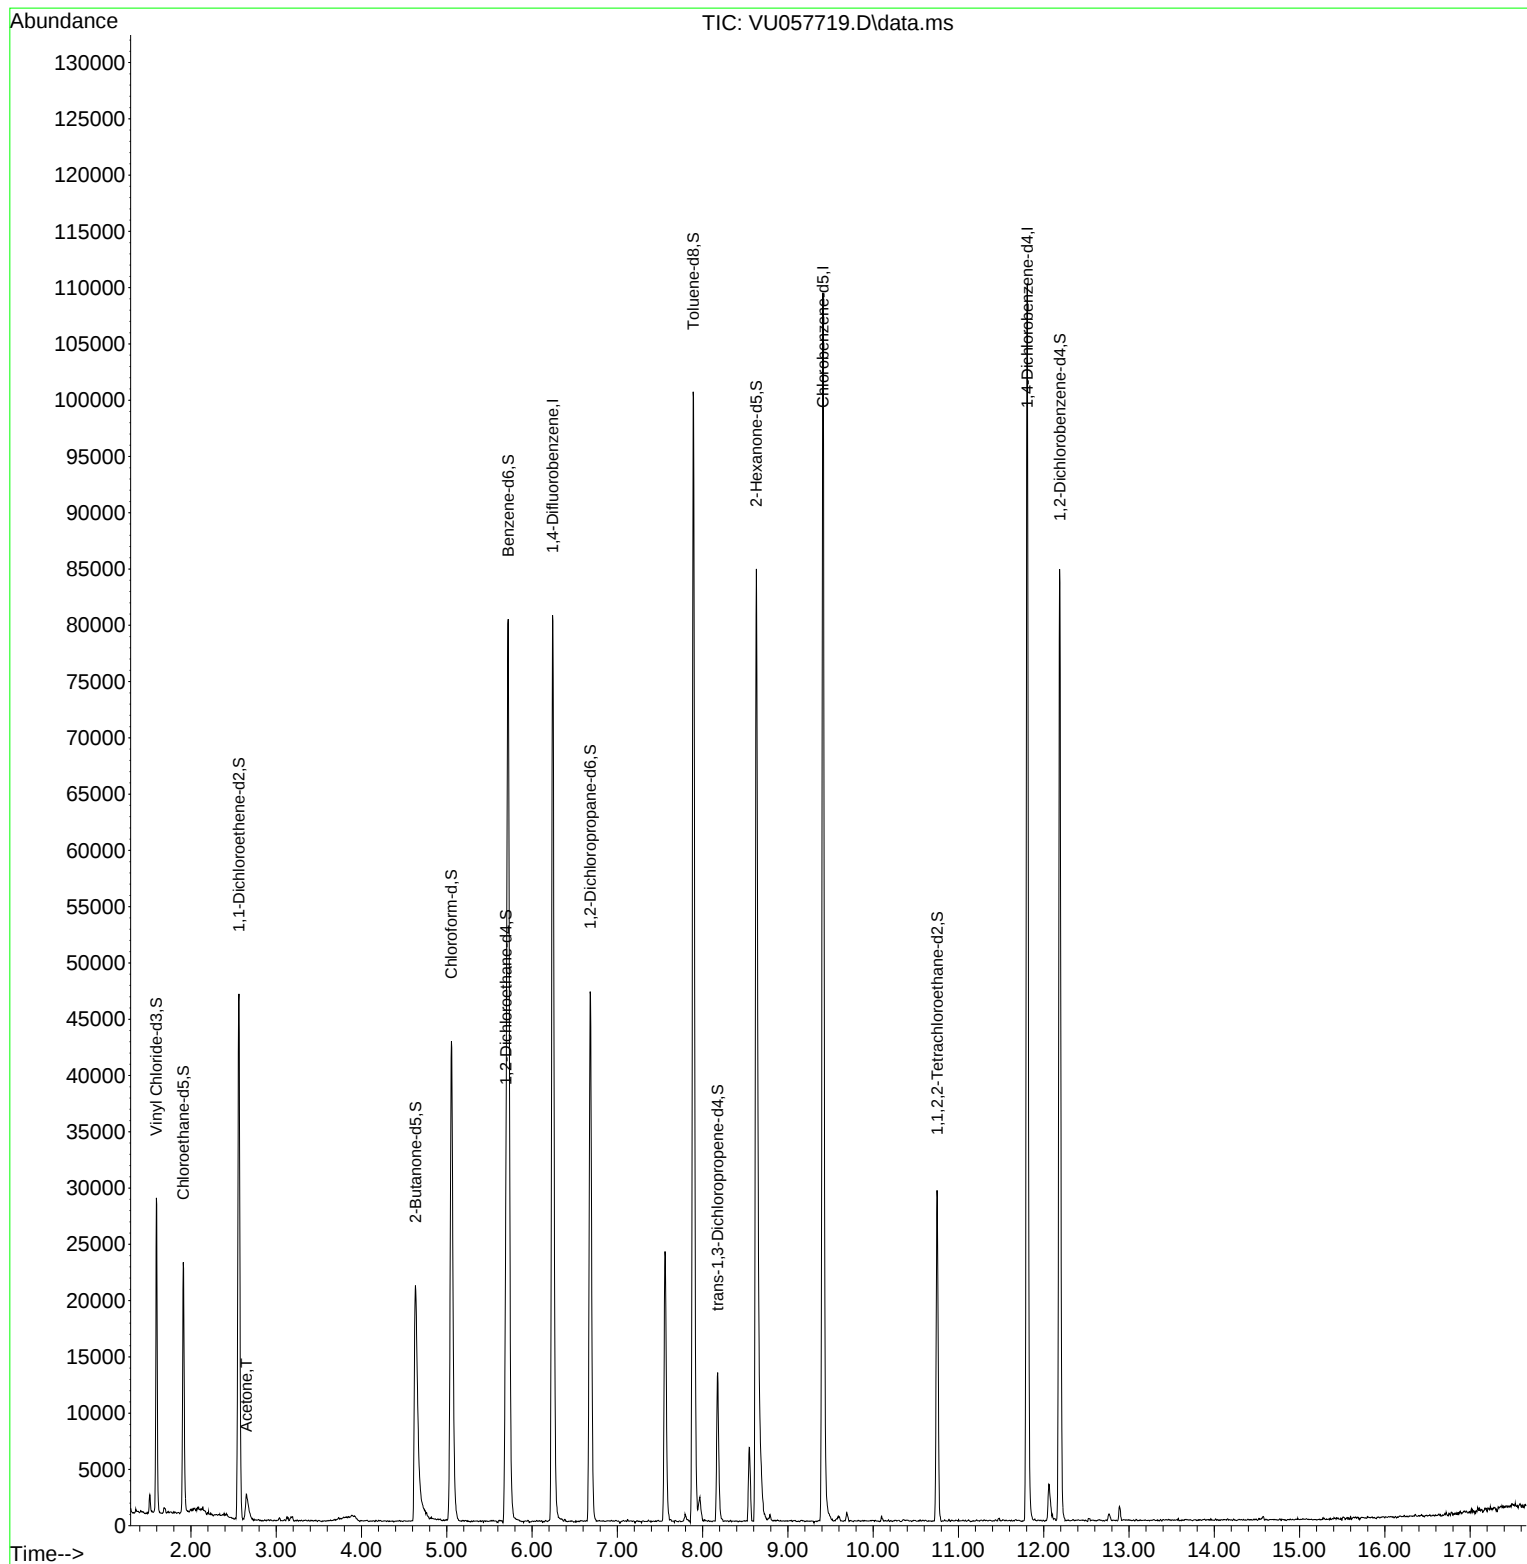

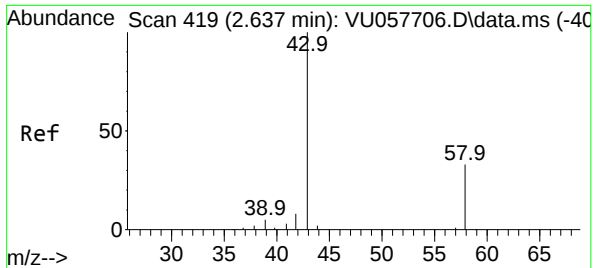

#13
 Acetone
 Concen: 5.942 ug/L
 RT: 2.650 min Scan# 41
 Delta R.T. 0.013 min
 Lab File: VU057719.D
 Acq: 29 Jan 2024 16:07

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FD0

Tgt Ion: 43 Resp: 3922
 Ion Ratio Lower Upper
 43 100
 58 29.3 0.0 61.4

