

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012924\
 Data File : VU057720.D
 Acq On : 29 Jan 2024 16:32
 Operator : MD/SY
 Sample : P1239-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FD1

Quant Time: Jan 30 00:34:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 30 00:30:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	64937	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	59267	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	27485	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	19932	5.571	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.400%
7) Chloroethane-d5	1.911	69	16258	5.423	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.400%
11) 1,1-Dichloroethene-d2	2.560	65	9279	5.516	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	110.400%
20) 2-Butanone-d5	4.634	46	39666	58.768	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.540%
24) Chloroform-d	5.055	84	37429	5.154	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.000%
26) 1,2-Dichloroethane-d4	5.695	65	19018	5.763	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.200%
32) Benzene-d6	5.721	84	77339	5.563	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.200%
36) 1,2-Dichloropropane-d6	6.685	67	23473	5.598	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.000%
41) Toluene-d8	7.894	98	69749	5.285	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.800%
43) trans-1,3-Dichloroprop...	8.174	79	8514	5.095	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.800%
46) 2-Hexanone-d5	8.631	63	30385	56.985	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.980%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	14701	5.230	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	22794	5.910	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.200%
Target Compounds					Qvalue	
13) Acetone	2.657	43	4027	6.279	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012924\
Data File : VU057720.D
Acq On : 29 Jan 2024 16:32
Operator : MD/SY
Sample : P1239-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FD1

Quant Time: Jan 30 00:34:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 30 00:30:52 2024
Response via : Initial Calibration

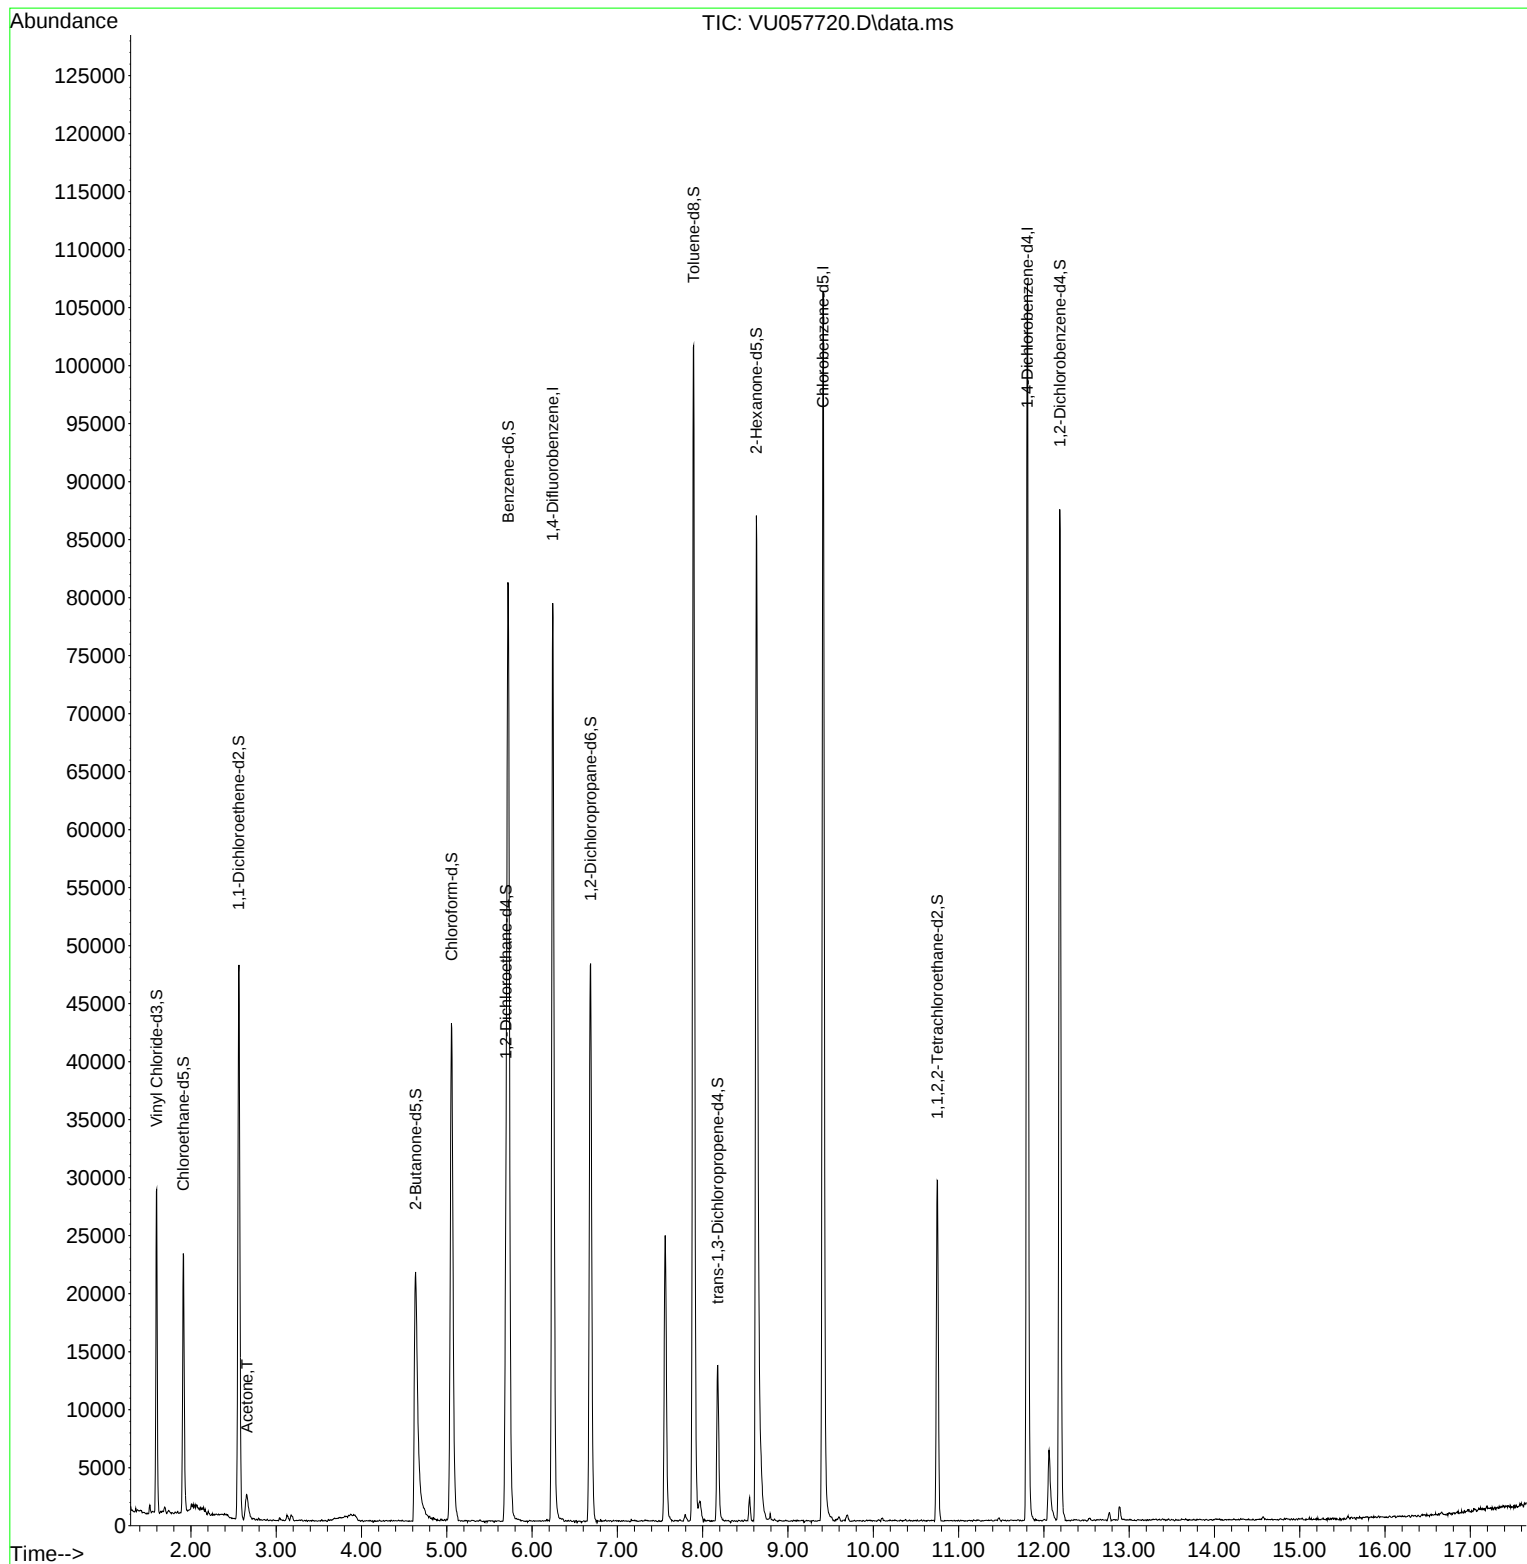

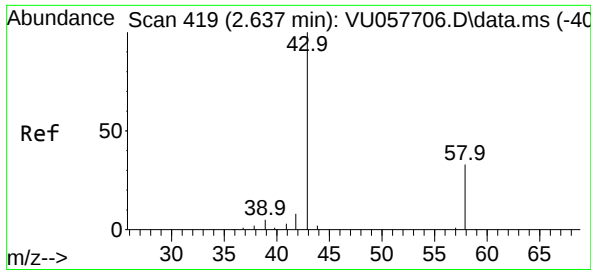

#13

Acetone

Concen: 6.279 ug/L

RT: 2.657 min Scan# 41

Delta R.T. 0.019 min

Lab File: VU057720.D


Acq: 29 Jan 2024 16:32

Instrument :

MSVOA_U

ClientSampleId :

C0FD1

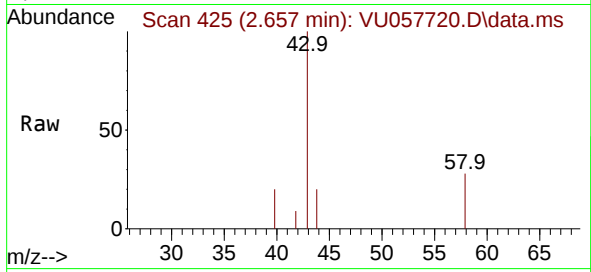

Tgt Ion: 43 Resp: 4027

Ion Ratio Lower Upper

43 100

58 28.5 0.0 61.4

