

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012924\
 Data File : VU057722.D
 Acq On : 29 Jan 2024 17:20
 Operator : MD/SY
 Sample : P1239-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FD2

Quant Time: Jan 30 00:35:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 30 00:30:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	64670	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	58767	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	27308	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	20262	5.687	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	113.800%
7) Chloroethane-d5	1.911	69	17317	5.800	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	116.000%
11) 1,1-Dichloroethene-d2	2.560	65	9116	5.441	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	108.800%
20) 2-Butanone-d5	4.627	46	39313	58.486	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.980%
24) Chloroform-d	5.055	84	38138	5.273	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.400%
26) 1,2-Dichloroethane-d4	5.695	65	19244	5.855	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	117.200%
32) Benzene-d6	5.721	84	77986	5.657	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.200%
36) 1,2-Dichloropropane-d6	6.685	67	23440	5.638	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.800%
41) Toluene-d8	7.894	98	71562	5.469	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.400%
43) trans-1,3-Dichloroprop...	8.177	79	8681	5.239	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	104.800%
46) 2-Hexanone-d5	8.631	63	30691	58.049	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	116.100%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	15370	5.515	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	22493	5.869	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.400%
Target Compounds						
					Qvalue	
13) Acetone	2.647	43	3943	6.173	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012924\
Data File : VU057722.D
Acq On : 29 Jan 2024 17:20
Operator : MD/SY
Sample : P1239-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FD2

Quant Time: Jan 30 00:35:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 30 00:30:52 2024
Response via : Initial Calibration

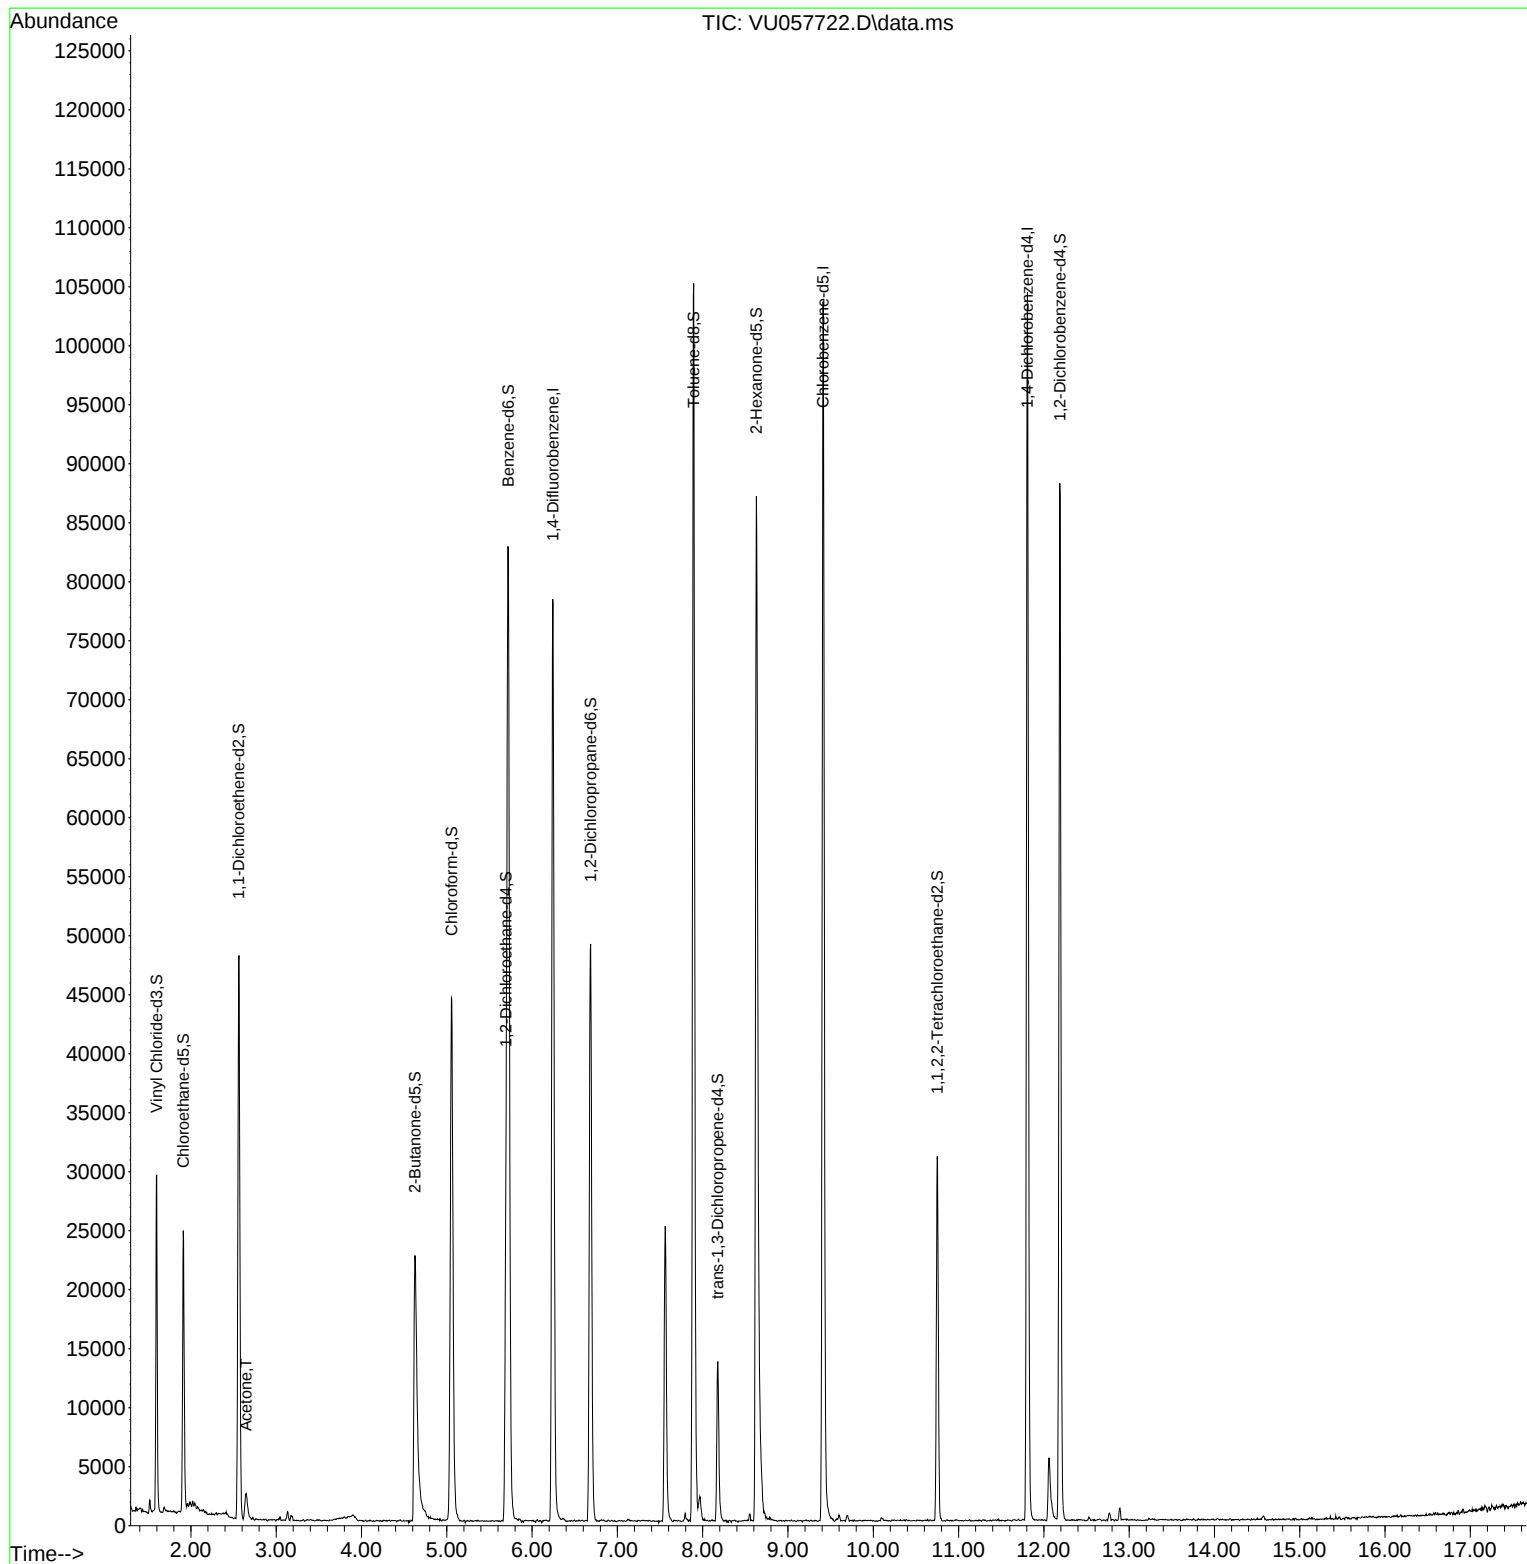

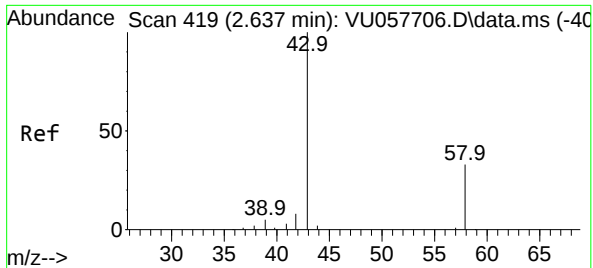

#13
 Acetone
 Concen: 6.173 ug/L
 RT: 2.647 min Scan# 41
 Delta R.T. 0.010 min
 Lab File: VU057722.D
 Acq: 29 Jan 2024 17:20

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FD2

Tgt Ion: 43 Resp: 3943
 Ion Ratio Lower Upper
 43 100
 58 27.7 0.0 61.4

