

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013020\
 Data File : VU036614.D
 Acq On : 30 Jan 2020 13:13
 Operator : JC/MD
 Sample : L1301-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFM06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	79	85	98	rVB	140212	147185	14.42%	1.810%
2	1.932	176	184	197	rVB	118068	149257	14.62%	1.836%
3	2.594	377	390	405	rBV	211592	346106	33.91%	4.257%
4	2.797	442	453	466	rBV2	2363	4427	0.43%	0.054%
5	3.086	537	543	547	rBV2	450	416	0.04%	0.005%
6	3.141	557	560	562	rBV	117	83	0.01%	0.001%
7	3.224	576	586	601	rVB2	1656	3593	0.35%	0.044%
8	3.620	705	709	710	rBV	86	55	0.01%	0.001%
9	3.633	710	713	716	rVB	188	117	0.01%	0.001%
10	3.842	775	778	780	rBV	76	56	0.01%	0.001%
11	3.916	798	801	804	rBV	71	48	0.00%	0.001%
12	3.980	818	821	830	rBV2	303	458	0.04%	0.006%
13	4.076	849	851	852	rBV2	133	59	0.01%	0.001%
14	4.112	858	862	867	rVB	171	197	0.02%	0.002%
15	4.137	867	870	872	rBV	131	110	0.01%	0.001%
16	4.170	876	880	882	rBV	124	125	0.01%	0.002%
17	4.215	892	894	898	rVB2	162	94	0.01%	0.001%
18	4.247	899	904	906	rBV2	197	203	0.02%	0.002%
19	4.292	915	918	920	rBV	112	69	0.01%	0.001%
20	4.305	920	922	924	rVV	126	76	0.01%	0.001%
21	4.424	956	959	961	rBV	102	64	0.01%	0.001%
22	4.504	982	984	988	rVB2	146	99	0.01%	0.001%
23	4.597	1009	1013	1015	rBV	86	74	0.01%	0.001%
24	4.613	1015	1018	1020	rBV	136	75	0.01%	0.001%
25	4.678	1022	1038	1071	rBV	101366	240451	23.56%	2.958%
26	5.054	1152	1155	1156	rBV2	148	83	0.01%	0.001%
27	5.108	1156	1172	1195	rVV	177374	383261	37.55%	4.714%
28	5.215	1204	1205	1208	rVB2	148	78	0.01%	0.001%
29	5.330	1236	1241	1251	rVB2	463	756	0.07%	0.009%
30	5.417	1262	1268	1276	rBV2	537	707	0.07%	0.009%
31	5.497	1289	1293	1296	rBV2	204	151	0.01%	0.002%
32	5.639	1335	1337	1338	rBV2	121	52	0.01%	0.001%
33	5.681	1347	1350	1354	rVB	151	96	0.01%	0.001%
34	5.768	1354	1377	1397	rBV2	393718	1020576	100.00%	12.553%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013020\
 Data File : VU036614.D
 Acq On : 30 Jan 2020 13:13
 Operator : JC/MD
 Sample : L1301-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFM06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis

35	6.047	1461	1464	1466	rBV2	186	86	0.01%	0.001%
36	6.063	1467	1469	1471	rBV2	199	106	0.01%	0.001%
37	6.288	1522	1539	1567	rBV	355896	667837	65.44%	8.215%
38	6.642	1646	1649	1654	rBV	207	202	0.02%	0.002%
39	6.674	1657	1659	1662	rBV	130	58	0.01%	0.001%
40	6.729	1662	1676	1694	rBV	234799	452628	44.35%	5.567%
41	6.835	1707	1709	1711	rBV	304	178	0.02%	0.002%
42	6.886	1722	1725	1727	rBV	212	97	0.01%	0.001%
43	6.906	1729	1731	1733	rVV	137	60	0.01%	0.001%
44	6.938	1737	1741	1743	rBV	72	65	0.01%	0.001%
45	7.054	1774	1777	1779	rBV	154	94	0.01%	0.001%
46	7.083	1784	1786	1789	rVB	142	67	0.01%	0.001%
47	7.214	1819	1827	1836	rVV3	1638	2696	0.26%	0.033%
48	7.311	1854	1857	1861	rVB	75	51	0.00%	0.001%
49	7.372	1873	1876	1880	rVV2	214	219	0.02%	0.003%
50	7.417	1884	1890	1892	rVB	86	76	0.01%	0.001%
51	7.468	1904	1906	1910	rVB	93	52	0.01%	0.001%
52	7.497	1913	1915	1920	rVB2	141	91	0.01%	0.001%
53	7.523	1920	1923	1926	rBV	113	76	0.01%	0.001%
54	7.600	1932	1947	1967	rBV	134969	238274	23.35%	2.931%
55	7.713	1977	1982	1986	rBV3	1236	1461	0.14%	0.018%
56	7.784	2000	2004	2009	rBV2	169	222	0.02%	0.003%
57	7.857	2024	2027	2028	rBV	144	57	0.01%	0.001%
58	7.867	2028	2030	2034	rBV	103	55	0.01%	0.001%
59	7.928	2034	2049	2069	rBV	514332	883608	86.58%	10.869%
60	8.150	2113	2118	2124	rBV	229	151	0.01%	0.002%
61	8.211	2124	2137	2160	rBV	91854	156599	15.34%	1.926%
62	8.433	2202	2206	2207	rBV	157	65	0.01%	0.001%
63	8.501	2219	2227	2236	rBV3	893	1397	0.14%	0.017%
64	8.542	2236	2240	2243	rBV	108	91	0.01%	0.001%
65	8.591	2254	2255	2258	rVB	182	65	0.01%	0.001%
66	8.610	2258	2261	2265	rBV	139	116	0.01%	0.001%
67	8.668	2265	2279	2323	rVV	293412	573224	56.17%	7.051%
68	9.066	2398	2403	2405	rBV	240	209	0.02%	0.003%
69	9.156	2428	2431	2437	rVB	202	146	0.01%	0.002%
70	9.185	2437	2440	2443	rBV	89	65	0.01%	0.001%
71	9.308	2476	2478	2481	rBV	138	61	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013020\
 Data File : VU036614.D
 Acq On : 30 Jan 2020 13:13
 Operator : JC/MD
 Sample : L1301-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFM06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis

72	9.324	2481	2483	2486	rVB	210	109	0.01%	0.001%
73	9.446	2507	2521	2558	rBV	479449	796084	78.00%	9.792%
74	9.591	2564	2566	2568	rBV	156	109	0.01%	0.001%
75	9.719	2600	2606	2617	rVB2	591	1003	0.10%	0.012%
76	9.764	2617	2620	2623	rBV	76	58	0.01%	0.001%
77	9.787	2624	2627	2628	rBV	111	69	0.01%	0.001%
78	9.812	2633	2635	2638	rVV	181	101	0.01%	0.001%
79	9.838	2639	2643	2647	rVB2	171	122	0.01%	0.002%
80	10.086	2717	2720	2725	rBV2	192	142	0.01%	0.002%
81	10.111	2725	2728	2730	rBV	284	169	0.02%	0.002%
82	10.189	2750	2752	2758	rVB	156	90	0.01%	0.001%
83	10.375	2804	2810	2813	rBV2	196	214	0.02%	0.003%
84	10.552	2862	2865	2868	rBV	124	97	0.01%	0.001%
85	10.587	2874	2876	2881	rVB	194	118	0.01%	0.001%
86	10.780	2923	2936	2957	rBV	337052	547844	53.68%	6.739%
87	11.111	3034	3039	3042	rBV3	347	303	0.03%	0.004%
88	11.127	3042	3044	3046	rBV	98	56	0.01%	0.001%
89	11.262	3084	3086	3090	rVB	166	55	0.01%	0.001%
90	11.311	3097	3101	3104	rBV	314	204	0.02%	0.003%
91	11.488	3152	3156	3163	rVB3	645	709	0.07%	0.009%
92	11.745	3234	3236	3239	rVB	270	113	0.01%	0.001%
93	11.835	3251	3264	3284	rVB	457153	740867	72.59%	9.113%
94	12.214	3369	3382	3397	rBV	459559	754520	73.93%	9.281%
95	12.285	3402	3404	3406	rVB	220	107	0.01%	0.001%
96	12.462	3457	3459	3461	rBV	157	56	0.01%	0.001%
97	12.648	3515	3517	3525	rVB	167	138	0.01%	0.002%
98	12.873	3583	3587	3593	rBV2	280	221	0.02%	0.003%
99	13.709	3845	3847	3851	rBV	274	168	0.02%	0.002%
100	14.105	3964	3970	3981	rVB	4479	6238	0.61%	0.077%


Sum of corrected areas: 8129946

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU013020\
Data File : VU036614.D
Acq On : 30 Jan 2020 13:13
Operator : JC/MD
Sample : L1301-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFM06

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

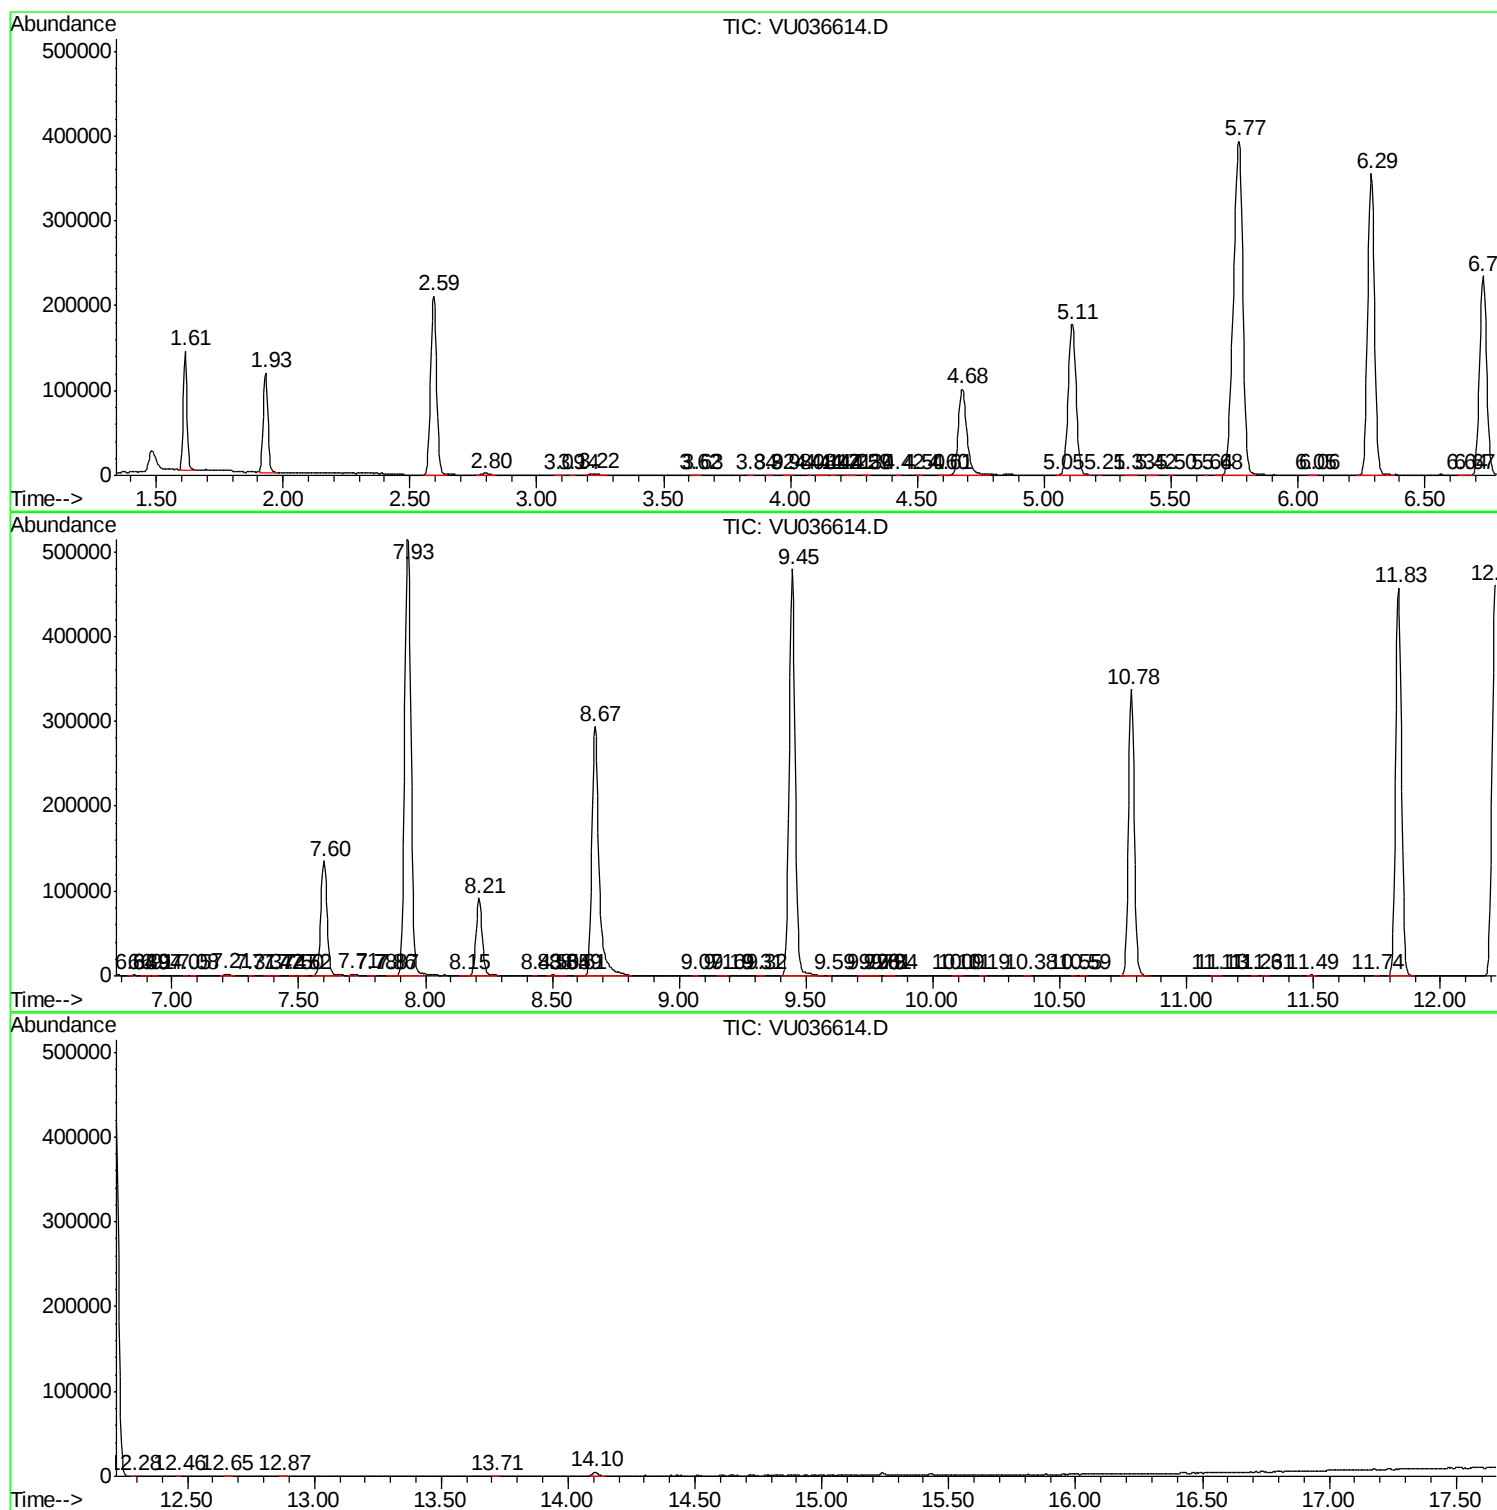

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU013020\
Data File : VU036614.D
Acq On : 30 Jan 2020 13:13
Operator : JC/MD
Sample : L1301-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFM06

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU013020\
Data File : VU036614.D
Acq On : 30 Jan 2020 13:13
Operator : JC/MD
Sample : L1301-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFM06

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc