

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013020\
 Data File : VU036618.D
 Acq On : 30 Jan 2020 14:49
 Operator : JC/MD
 Sample : L1301-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	79	85	97	rVB	130683	136277	13.69%	1.721%
2	1.932	176	184	195	rVB	108670	139571	14.02%	1.762%
3	2.594	377	390	405	rBV	200292	327482	32.90%	4.135%
4	2.822	459	461	463	rBV	263	71	0.01%	0.001%
5	2.970	504	507	512	rVB	226	167	0.02%	0.002%
6	3.018	520	522	525	rVB2	186	101	0.01%	0.001%
7	3.079	534	541	557	rVB4	1694	2915	0.29%	0.037%
8	3.227	575	587	599	rVB2	1604	3672	0.37%	0.046%
9	3.295	606	608	610	rVV	145	43	0.00%	0.001%
10	3.308	610	612	615	rVB	196	94	0.01%	0.001%
11	3.427	647	649	651	rVB	155	44	0.00%	0.001%
12	3.459	658	659	662	rVB	155	44	0.00%	0.001%
13	3.485	662	667	670	rBV	136	136	0.01%	0.002%
14	3.677	725	727	730	rVB	145	54	0.01%	0.001%
15	3.739	745	746	750	rVB	142	58	0.01%	0.001%
16	3.835	772	776	781	rBV	133	144	0.01%	0.002%
17	3.864	782	785	786	rBV	109	46	0.00%	0.001%
18	3.970	815	818	823	rVB	125	103	0.01%	0.001%
19	4.079	848	852	855	rBV2	163	129	0.01%	0.002%
20	4.231	896	899	902	rBV	204	120	0.01%	0.002%
21	4.407	951	954	957	rBV2	177	117	0.01%	0.001%
22	4.436	957	963	965	rBV	65	62	0.01%	0.001%
23	4.546	992	997	999	rBV	49	46	0.00%	0.001%
24	4.677	1021	1038	1067	rBV	100372	252767	25.40%	3.192%
25	4.999	1136	1138	1140	rBV	125	66	0.01%	0.001%
26	5.031	1146	1148	1150	rBV	130	73	0.01%	0.001%
27	5.112	1155	1173	1194	rBV	165100	372957	37.47%	4.709%
28	5.256	1216	1218	1219	rBV	117	46	0.00%	0.001%
29	5.292	1225	1229	1230	rBV	240	129	0.01%	0.002%
30	5.330	1235	1241	1244	rBV	482	584	0.06%	0.007%
31	5.372	1250	1254	1256	rBV	50	44	0.00%	0.001%
32	5.417	1261	1268	1272	rBV3	419	443	0.04%	0.006%
33	5.472	1284	1285	1288	rVB3	140	53	0.01%	0.001%
34	5.584	1313	1320	1323	rBV	105	99	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013020\
 Data File : VU036618.D
 Acq On : 30 Jan 2020 14:49
 Operator : JC/MD
 Sample : L1301-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis

35	5.607	1324	1327	1330	rVV	73	50	0.01%	0.001%
36	5.623	1330	1332	1335	rVB	94	50	0.01%	0.001%
37	5.645	1335	1339	1342	rBV	103	84	0.01%	0.001%
38	5.767	1354	1377	1398	rBV2	385707	995285	100.00%	12.567%
39	6.134	1488	1491	1492	rBV2	153	87	0.01%	0.001%
40	6.192	1508	1509	1513	rVB	229	96	0.01%	0.001%
41	6.214	1514	1516	1518	rBV	127	58	0.01%	0.001%
42	6.288	1524	1539	1570	rBV	337590	626019	62.90%	7.905%
43	6.562	1618	1624	1634	rVB3	2176	3336	0.34%	0.042%
44	6.729	1662	1676	1699	rBV	229278	445671	44.78%	5.627%
45	6.845	1707	1712	1717	rVB2	635	691	0.07%	0.009%
46	6.912	1731	1733	1735	rBV	91	46	0.00%	0.001%
47	6.970	1748	1751	1755	rBV	104	88	0.01%	0.001%
48	7.176	1813	1815	1817	rBV2	120	68	0.01%	0.001%
49	7.218	1819	1828	1837	rBV3	1787	2696	0.27%	0.034%
50	7.253	1837	1839	1842	rVB2	161	85	0.01%	0.001%
51	7.346	1866	1868	1870	rBV	156	59	0.01%	0.001%
52	7.356	1870	1871	1873	rVB	117	47	0.00%	0.001%
53	7.436	1894	1896	1900	rVB2	195	126	0.01%	0.002%
54	7.472	1904	1907	1910	rVV2	138	85	0.01%	0.001%
55	7.504	1915	1917	1919	rBV	71	40	0.00%	0.001%
56	7.600	1934	1947	1967	rBV	135368	233389	23.45%	2.947%
57	7.713	1977	1982	1991	rVB4	1172	1713	0.17%	0.022%
58	7.793	2004	2007	2011	rVB2	207	134	0.01%	0.002%
59	7.928	2035	2049	2065	rBV	494982	853114	85.72%	10.772%
60	8.211	2124	2137	2159	rBV	91617	156834	15.76%	1.980%
61	8.491	2221	2224	2225	rBV2	119	65	0.01%	0.001%
62	8.526	2232	2235	2239	rBV	96	69	0.01%	0.001%
63	8.590	2251	2255	2258	rBV	74	75	0.01%	0.001%
64	8.668	2265	2279	2324	rBV	309759	597088	59.99%	7.539%
65	8.851	2335	2336	2341	rVB	155	73	0.01%	0.001%
66	9.127	2419	2422	2423	rBV	77	47	0.00%	0.001%
67	9.163	2429	2433	2437	rBV	103	111	0.01%	0.001%
68	9.398	2502	2506	2507	rBV	61	42	0.00%	0.001%
69	9.446	2507	2521	2556	rVB	450306	758943	76.25%	9.583%
70	9.600	2565	2569	2574	rVB2	187	215	0.02%	0.003%
71	9.668	2588	2590	2594	rVB	240	122	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013020\
 Data File : VU036618.D
 Acq On : 30 Jan 2020 14:49
 Operator : JC/MD
 Sample : L1301-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis

72	9.719	2600	2606	2612	rVB2	651	749	0.08%	0.009%
73	9.832	2638	2641	2647	rBV	74	60	0.01%	0.001%
74	9.880	2652	2656	2662	rVB	94	103	0.01%	0.001%
75	9.909	2662	2665	2668	rBV	80	63	0.01%	0.001%
76	9.979	2685	2687	2691	rBV	154	51	0.01%	0.001%
77	10.066	2712	2714	2718	rBV	138	80	0.01%	0.001%
78	10.127	2728	2733	2743	rVV3	367	514	0.05%	0.006%
79	10.166	2743	2745	2748	rVB	100	55	0.01%	0.001%
80	10.323	2791	2794	2799	rBV	96	103	0.01%	0.001%
81	10.378	2805	2811	2815	rBV	117	154	0.02%	0.002%
82	10.465	2836	2838	2840	rBV	137	56	0.01%	0.001%
83	10.613	2882	2884	2886	rBV	145	53	0.01%	0.001%
84	10.780	2924	2936	2959	rBV	336698	546677	54.93%	6.903%
85	10.864	2959	2962	2966	rBV	199	132	0.01%	0.002%
86	10.983	2997	2999	3004	rBV	85	55	0.01%	0.001%
87	11.037	3011	3016	3022	rBV	158	212	0.02%	0.003%
88	11.295	3094	3096	3098	rBV	177	78	0.01%	0.001%
89	11.372	3117	3120	3124	rBV	159	136	0.01%	0.002%
90	11.584	3184	3186	3189	rBV	168	79	0.01%	0.001%
91	11.835	3250	3264	3280	rBV	435522	702810	70.61%	8.874%
92	12.008	3315	3318	3321	rBV	247	170	0.02%	0.002%
93	12.214	3369	3382	3401	rBV	454569	742560	74.61%	9.376%
94	12.703	3532	3534	3538	rBV	228	129	0.01%	0.002%
95	12.741	3543	3546	3549	rVB	271	142	0.01%	0.002%
96	12.761	3549	3552	3560	rBV2	283	289	0.03%	0.004%
97	13.471	3771	3773	3776	rBV	235	117	0.01%	0.001%
98	13.722	3849	3851	3853	rBV	186	85	0.01%	0.001%
99	14.108	3965	3971	3980	rVB	3718	5092	0.51%	0.064%
100	15.236	4315	4322	4334	rBV5	2044	3403	0.34%	0.043%


Sum of corrected areas: 7919765

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU013020\
Data File : VU036618.D
Acq On : 30 Jan 2020 14:49
Operator : JC/MD
Sample : L1301-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

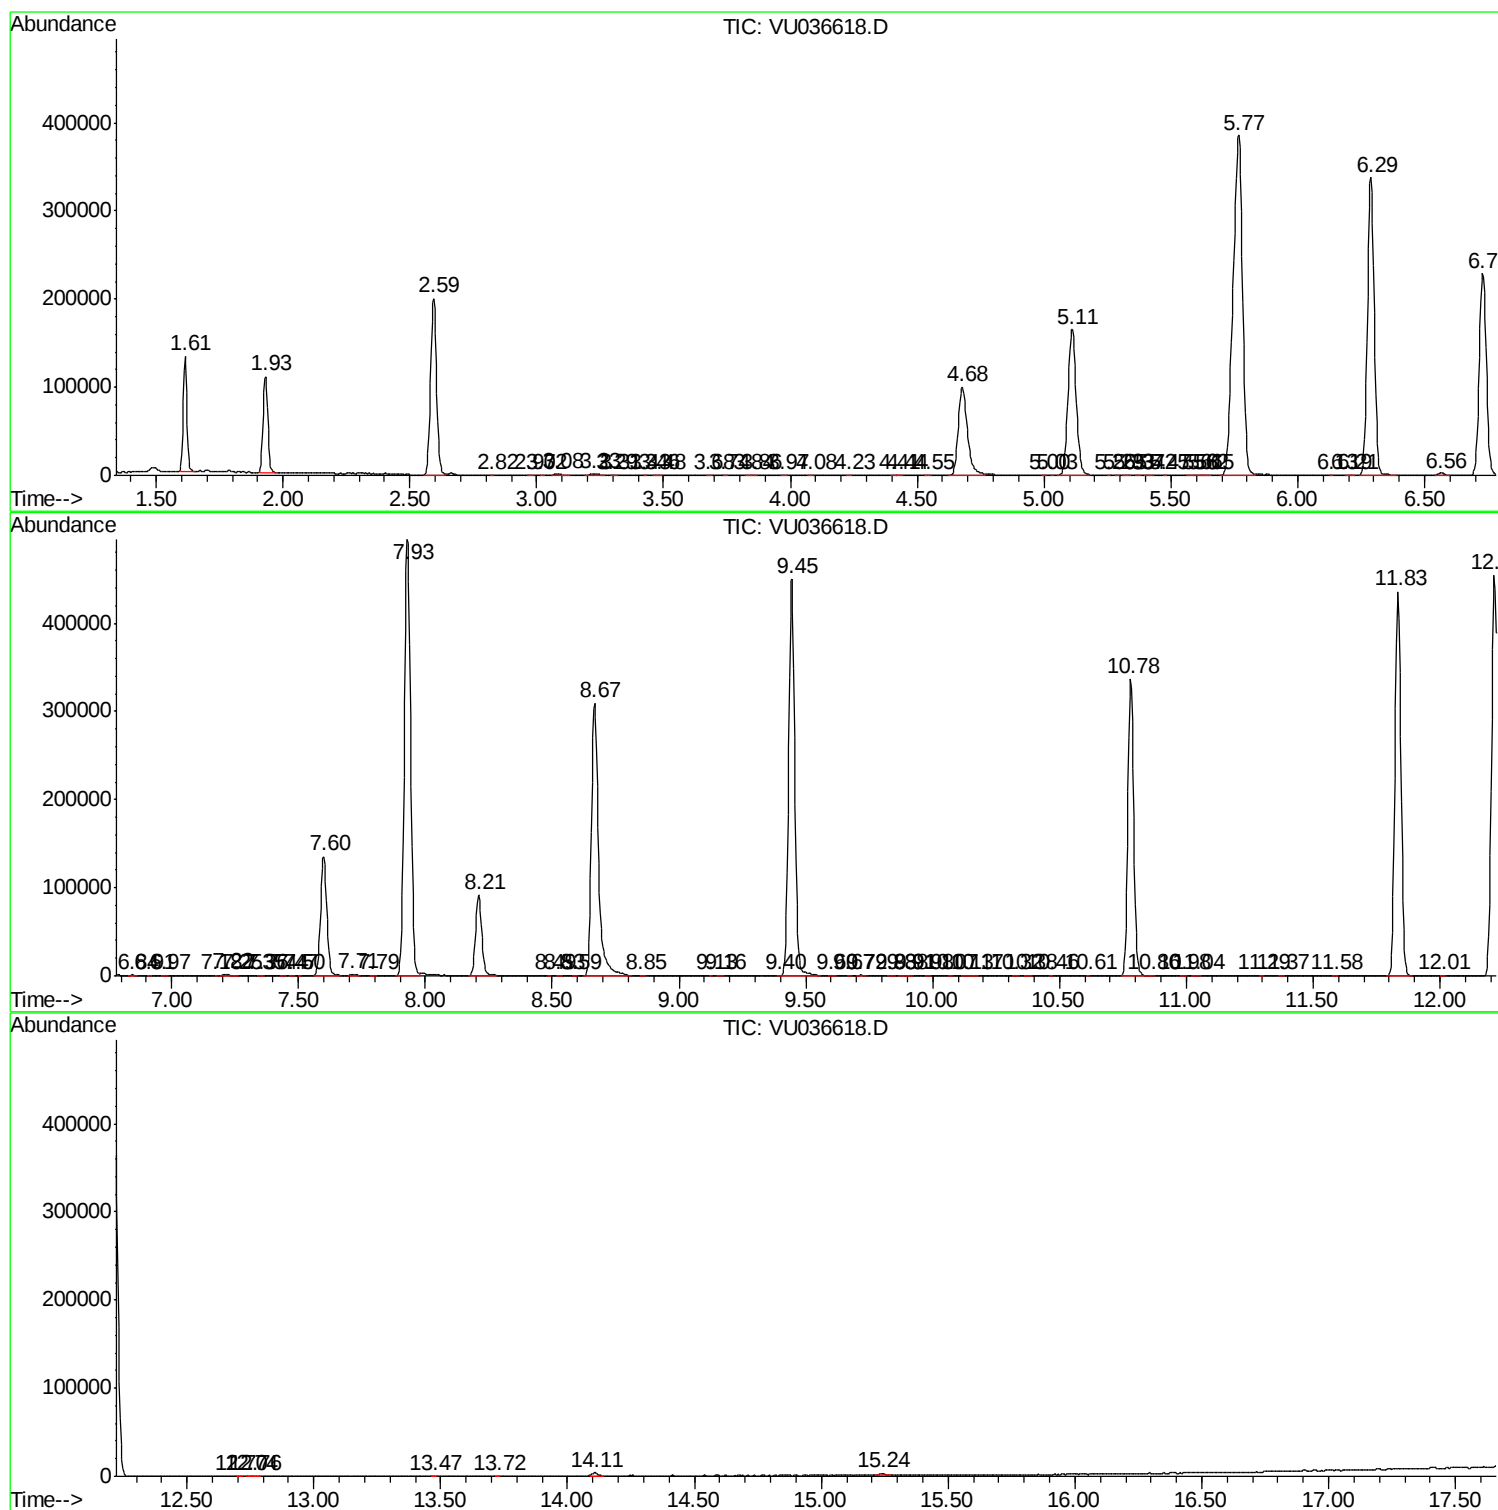

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU013020\
Data File : VU036618.D
Acq On : 30 Jan 2020 14:49
Operator : JC/MD
Sample : L1301-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU013020\
Data File : VU036618.D
Acq On : 30 Jan 2020 14:49
Operator : JC/MD
Sample : L1301-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc