

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013020\
 Data File : VU036619.D
 Acq On : 30 Jan 2020 15:13
 Operator : JC/MD
 Sample : L1322-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XR7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	94	rBV	135376	140922	14.08%	1.671%
2	1.929	176	183	197	rVB	111744	143200	14.31%	1.698%
3	2.594	377	390	406	rBV	204473	336264	33.60%	3.988%
4	2.755	437	440	443	rBV	174	88	0.01%	0.001%
5	2.797	443	453	469	rVV	4844	8907	0.89%	0.106%
6	3.125	553	555	559	rBV2	185	139	0.01%	0.002%
7	3.224	574	586	598	rBV	2487	5369	0.54%	0.064%
8	3.581	695	697	698	rBV	120	48	0.00%	0.001%
9	3.655	714	720	723	rBV	114	124	0.01%	0.001%
10	3.713	735	738	739	rBV	84	50	0.00%	0.001%
11	3.877	784	789	790	rBV	66	63	0.01%	0.001%
12	3.912	798	800	803	rVB	97	51	0.01%	0.001%
13	3.945	803	810	815	rBV	112	164	0.02%	0.002%
14	4.015	829	832	836	rVB	89	57	0.01%	0.001%
15	4.099	854	858	867	rBV2	326	339	0.03%	0.004%
16	4.215	891	894	897	rBV	82	50	0.00%	0.001%
17	4.305	920	922	929	rBV	163	123	0.01%	0.001%
18	4.375	941	944	946	rBV	87	63	0.01%	0.001%
19	4.449	965	967	968	rBV	146	66	0.01%	0.001%
20	4.501	982	983	986	rVB	179	84	0.01%	0.001%
21	4.523	986	990	995	rVB	78	73	0.01%	0.001%
22	4.555	995	1000	1001	rBV	146	128	0.01%	0.002%
23	4.581	1004	1008	1010	rBV	76	63	0.01%	0.001%
24	4.678	1022	1038	1071	rBV	98330	248528	24.84%	2.948%
25	5.002	1136	1139	1141	rBV	228	121	0.01%	0.001%
26	5.018	1141	1144	1151	rVB2	201	244	0.02%	0.003%
27	5.108	1156	1172	1199	rBV	164435	373874	37.36%	4.434%
28	5.240	1212	1213	1218	rVB	197	111	0.01%	0.001%
29	5.266	1218	1221	1223	rBV	180	102	0.01%	0.001%
30	5.327	1234	1240	1247	rBV3	569	770	0.08%	0.009%
31	5.382	1247	1257	1260	rVB	80	120	0.01%	0.001%
32	5.407	1262	1265	1268	rBV	193	159	0.02%	0.002%
33	5.488	1287	1290	1295	rVB	107	85	0.01%	0.001%
34	5.633	1334	1335	1337	rVV	128	54	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013020\
 Data File : VU036619.D
 Acq On : 30 Jan 2020 15:13
 Operator : JC/MD
 Sample : L1322-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XR7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis

35	5.768	1354	1377	1401	rBV2	386499	1000702	100.00%	11.869%
36	6.195	1508	1510	1513	rBV	229	102	0.01%	0.001%
37	6.215	1513	1516	1517	rBV	150	107	0.01%	0.001%
38	6.288	1523	1539	1562	rBV	358873	670256	66.98%	7.950%
39	6.578	1616	1629	1647	rVB	99597	187153	18.70%	2.220%
40	6.674	1654	1659	1662	rBV	116	113	0.01%	0.001%
41	6.729	1662	1676	1701	rVV	228813	441882	44.16%	5.241%
42	6.841	1707	1711	1717	rBV3	802	929	0.09%	0.011%
43	6.880	1720	1723	1724	rVV3	139	60	0.01%	0.001%
44	6.896	1727	1728	1732	rVB	211	90	0.01%	0.001%
45	6.915	1732	1734	1736	rBV	217	121	0.01%	0.001%
46	6.944	1741	1743	1745	rBV	231	91	0.01%	0.001%
47	6.983	1753	1755	1757	rBV	121	65	0.01%	0.001%
48	7.015	1763	1765	1771	rVB2	170	103	0.01%	0.001%
49	7.070	1780	1782	1786	rVB	188	96	0.01%	0.001%
50	7.089	1786	1788	1792	rVB	88	59	0.01%	0.001%
51	7.115	1792	1796	1798	rBV	68	59	0.01%	0.001%
52	7.166	1810	1812	1814	rBV	142	64	0.01%	0.001%
53	7.218	1819	1828	1837	rVB3	1686	2839	0.28%	0.034%
54	7.279	1843	1847	1849	rBV	128	98	0.01%	0.001%
55	7.382	1877	1879	1884	rVB	159	84	0.01%	0.001%
56	7.404	1884	1886	1888	rBV	153	66	0.01%	0.001%
57	7.600	1932	1947	1965	rBV	132525	233597	23.34%	2.771%
58	7.864	2026	2029	2034	rVB2	205	213	0.02%	0.003%
59	7.928	2034	2049	2065	rBV	505836	867241	86.66%	10.286%
60	8.211	2125	2137	2152	rBV	92653	154396	15.43%	1.831%
61	8.449	2209	2211	2214	rVB	151	75	0.01%	0.001%
62	8.494	2220	2225	2229	rBV2	343	439	0.04%	0.005%
63	8.581	2241	2252	2266	rBV	100536	165157	16.50%	1.959%
64	8.668	2266	2279	2322	rVB	306306	577210	57.68%	6.846%
65	8.854	2334	2337	2340	rBV	191	89	0.01%	0.001%
66	8.928	2356	2360	2362	rBV	168	120	0.01%	0.001%
67	9.005	2382	2384	2386	rBV	141	105	0.01%	0.001%
68	9.083	2406	2408	2412	rVB	205	133	0.01%	0.002%
69	9.166	2431	2434	2437	rBV	119	87	0.01%	0.001%
70	9.247	2455	2459	2462	rBV	111	102	0.01%	0.001%
71	9.259	2462	2463	2465	rVV	124	52	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013020\
 Data File : VU036619.D
 Acq On : 30 Jan 2020 15:13
 Operator : JC/MD
 Sample : L1322-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XR7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis

72	9.304	2476	2477	2481	rVB	159	86	0.01%	0.001%
73	9.443	2506	2520	2542	rBV	484341	804683	80.41%	9.544%
74	9.591	2563	2566	2567	rBV	248	165	0.02%	0.002%
75	9.716	2598	2605	2613	rVV3	609	749	0.07%	0.009%
76	10.018	2696	2699	2705	rVB2	193	159	0.02%	0.002%
77	10.047	2706	2708	2714	rVB	197	134	0.01%	0.002%
78	10.102	2722	2725	2727	rBV	126	82	0.01%	0.001%
79	10.118	2727	2730	2731	rBV	180	106	0.01%	0.001%
80	10.179	2746	2749	2751	rBV	106	79	0.01%	0.001%
81	10.298	2784	2786	2790	rVB	180	83	0.01%	0.001%
82	10.362	2804	2806	2810	rBV	134	95	0.01%	0.001%
83	10.407	2816	2820	2821	rBV	175	135	0.01%	0.002%
84	10.533	2857	2859	2862	rBV	171	67	0.01%	0.001%
85	10.549	2862	2864	2867	rVB	155	84	0.01%	0.001%
86	10.697	2906	2910	2911	rBV	105	78	0.01%	0.001%
87	10.780	2924	2936	2954	rVB	331005	537975	53.76%	6.381%
88	10.864	2960	2962	2964	rBV	199	98	0.01%	0.001%
89	11.002	3003	3005	3008	rBV	125	82	0.01%	0.001%
90	11.176	3057	3059	3064	rBV2	156	107	0.01%	0.001%
91	11.269	3085	3088	3090	rBV2	165	106	0.01%	0.001%
92	11.317	3101	3103	3105	rBV	181	84	0.01%	0.001%
93	11.459	3144	3147	3148	rBV	187	114	0.01%	0.001%
94	11.835	3250	3264	3280	rVV	468671	762118	76.16%	9.039%
95	12.050	3329	3331	3337	rBV2	140	141	0.01%	0.002%
96	12.214	3368	3382	3398	rBV	463880	753788	75.33%	8.941%
97	12.317	3412	3414	3416	rBV	131	54	0.01%	0.001%
98	12.497	3468	3470	3472	rBV	297	86	0.01%	0.001%
99	13.761	3861	3863	3865	rBV	186	90	0.01%	0.001%
100	14.105	3965	3970	3980	rVB	3761	4680	0.47%	0.056%


Sum of corrected areas: 8431066

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU013020\
Data File : VU036619.D
Acq On : 30 Jan 2020 15:13
Operator : JC/MD
Sample : L1322-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XR7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

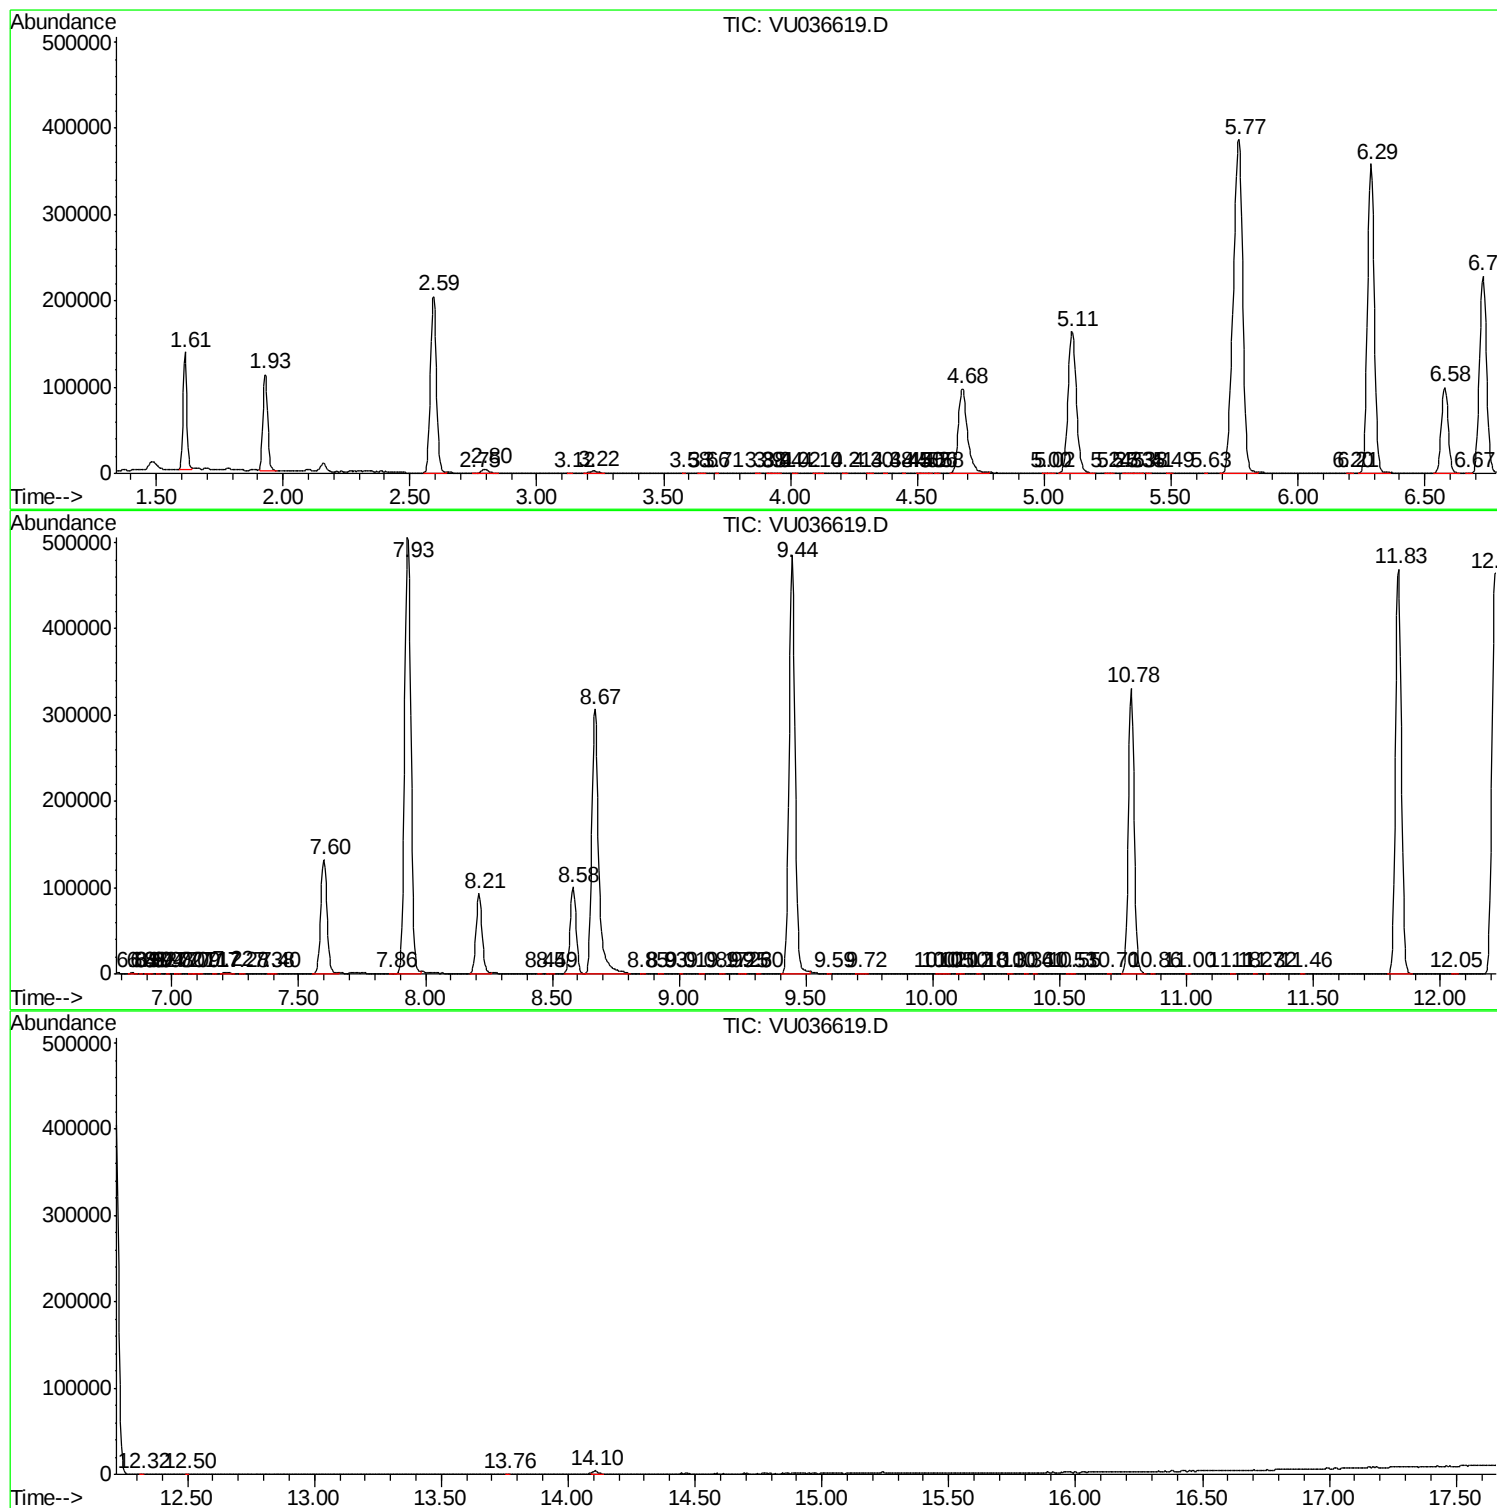

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU013020\
Data File : VU036619.D
Acq On : 30 Jan 2020 15:13
Operator : JC/MD
Sample : L1322-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XR7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU013020\
Data File : VU036619.D
Acq On : 30 Jan 2020 15:13
Operator : JC/MD
Sample : L1322-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XR7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc