

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013020\
 Data File : VU036629.D
 Acq On : 30 Jan 2020 19:36
 Operator : JC/MD
 Sample : L1326-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBCS7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	95	rBV	123107	129187	13.78%	1.673%
2	1.932	176	184	198	rVB	102505	130475	13.92%	1.689%
3	2.594	378	390	403	rBV	189717	306121	32.65%	3.964%
4	2.793	443	452	472	rVB3	6282	14568	1.55%	0.189%
5	2.903	484	486	489	rBV	157	61	0.01%	0.001%
6	2.964	502	505	508	rBV	192	99	0.01%	0.001%
7	3.102	546	548	550	rBV	135	44	0.00%	0.001%
8	3.224	576	586	603	rVB3	1645	3915	0.42%	0.051%
9	3.385	631	636	639	rBV2	622	602	0.06%	0.008%
10	3.610	701	706	708	rBV	265	188	0.02%	0.002%
11	3.684	726	729	732	rBV	96	82	0.01%	0.001%
12	3.848	778	780	783	rVB	169	51	0.01%	0.001%
13	3.922	801	803	804	rBV	109	48	0.01%	0.001%
14	3.945	808	810	811	rBV	138	40	0.00%	0.001%
15	3.973	816	819	823	rBV	118	87	0.01%	0.001%
16	4.015	829	832	834	rBV	165	102	0.01%	0.001%
17	4.141	870	871	875	rVB	126	38	0.00%	0.000%
18	4.182	882	884	886	rBV	109	64	0.01%	0.001%
19	4.256	904	907	908	rBV2	161	97	0.01%	0.001%
20	4.507	982	985	987	rBV	81	60	0.01%	0.001%
21	4.678	1023	1038	1074	rBV	93241	253593	27.05%	3.284%
22	4.996	1134	1137	1140	rBV2	144	137	0.01%	0.002%
23	5.108	1156	1172	1194	rBV	160393	355262	37.89%	4.600%
24	5.292	1226	1229	1235	rVB2	243	234	0.02%	0.003%
25	5.334	1235	1242	1249	rBV4	636	1062	0.11%	0.014%
26	5.420	1261	1269	1273	rBV3	460	646	0.07%	0.008%
27	5.456	1278	1280	1283	rVB2	180	101	0.01%	0.001%
28	5.549	1306	1309	1311	rBV	63	36	0.00%	0.000%
29	5.629	1332	1334	1338	rVB	63	38	0.00%	0.000%
30	5.652	1339	1341	1343	rBV	131	40	0.00%	0.001%
31	5.768	1355	1377	1404	rBV2	361058	937536	100.00%	12.139%
32	6.057	1464	1467	1470	rBV	276	171	0.02%	0.002%
33	6.076	1470	1473	1479	rVV	291	313	0.03%	0.004%
34	6.131	1488	1490	1493	rBV	161	69	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013020\
 Data File : VU036629.D
 Acq On : 30 Jan 2020 19:36
 Operator : JC/MD
 Sample : L1326-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBCS7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis

35	6.150	1493	1496	1497	rBV	285	163	0.02%	0.002%
36	6.289	1522	1539	1561	rBV	337256	626217	66.79%	8.108%
37	6.578	1618	1629	1644	rVB2	12739	23437	2.50%	0.303%
38	6.639	1644	1648	1652	rBV	219	223	0.02%	0.003%
39	6.729	1660	1676	1697	rBV	214963	415806	44.35%	5.384%
40	6.829	1705	1707	1709	rBV	216	116	0.01%	0.002%
41	6.874	1718	1721	1723	rBV	299	208	0.02%	0.003%
42	6.912	1730	1733	1736	rBV	234	191	0.02%	0.002%
43	6.970	1750	1751	1753	rVB	127	46	0.00%	0.001%
44	6.986	1753	1756	1758	rBV	69	34	0.00%	0.000%
45	7.047	1773	1775	1776	rVV	122	47	0.01%	0.001%
46	7.131	1796	1801	1804	rBV	112	107	0.01%	0.001%
47	7.144	1804	1805	1808	rVV	146	61	0.01%	0.001%
48	7.166	1808	1812	1816	rVV	86	84	0.01%	0.001%
49	7.218	1819	1828	1836	rVV3	1732	2701	0.29%	0.035%
50	7.250	1836	1838	1841	rVB	59	34	0.00%	0.000%
51	7.269	1841	1844	1847	rVB	92	53	0.01%	0.001%
52	7.472	1905	1907	1909	rVB	127	50	0.01%	0.001%
53	7.491	1909	1913	1917	rBV	50	55	0.01%	0.001%
54	7.600	1933	1947	1965	rBV	125480	218331	23.29%	2.827%
55	7.713	1975	1982	1995	rVB5	1419	2570	0.27%	0.033%
56	7.822	2013	2016	2018	rVB	178	93	0.01%	0.001%
57	7.858	2024	2027	2030	rBV	92	70	0.01%	0.001%
58	7.928	2035	2049	2068	rBV	463855	798573	85.18%	10.340%
59	8.211	2124	2137	2158	rBV	84448	143727	15.33%	1.861%
60	8.330	2172	2174	2178	rVB2	461	299	0.03%	0.004%
61	8.359	2178	2183	2185	rVB	188	176	0.02%	0.002%
62	8.375	2185	2188	2192	rBV	141	110	0.01%	0.001%
63	8.462	2211	2215	2219	rBB	83	59	0.01%	0.001%
64	8.501	2219	2227	2236	rBV2	932	1633	0.17%	0.021%
65	8.581	2241	2252	2265	rVV	68722	112389	11.99%	1.455%
66	8.668	2265	2279	2319	rVV	272684	541718	57.78%	7.014%
67	8.819	2320	2326	2341	rVB4	5496	8846	0.94%	0.115%
68	8.877	2341	2344	2346	rBV	97	55	0.01%	0.001%
69	8.993	2377	2380	2382	rBV	81	48	0.01%	0.001%
70	9.131	2417	2423	2429	rBV	100	149	0.02%	0.002%
71	9.218	2447	2450	2460	rVB	159	149	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013020\
 Data File : VU036629.D
 Acq On : 30 Jan 2020 19:36
 Operator : JC/MD
 Sample : L1326-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBCS7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
 Title : VOC Analysis

72	9.356	2489	2493	2496	rBV	79	70	0.01%	0.001%
73	9.443	2507	2520	2554	rVB	448940	756628	80.70%	9.797%
74	9.591	2564	2566	2567	rBV	305	143	0.02%	0.002%
75	9.626	2573	2577	2581	rVB	264	252	0.03%	0.003%
76	9.713	2600	2604	2608	rBV3	598	516	0.06%	0.007%
77	9.851	2642	2647	2648	rBV	124	113	0.01%	0.001%
78	9.941	2671	2675	2680	rBV	97	121	0.01%	0.002%
79	10.015	2696	2698	2700	rBV	76	42	0.00%	0.001%
80	10.099	2722	2724	2725	rBV	151	44	0.00%	0.001%
81	10.115	2726	2729	2733	rVV2	143	156	0.02%	0.002%
82	10.462	2835	2837	2840	rBV	158	109	0.01%	0.001%
83	10.719	2913	2917	2920	rBV	218	140	0.01%	0.002%
84	10.780	2923	2936	2954	rVB	316087	514952	54.93%	6.668%
85	10.925	2971	2981	2988	rBV	568	772	0.08%	0.010%
86	11.115	3037	3040	3042	rBV2	233	138	0.01%	0.002%
87	11.140	3046	3048	3050	rBV	136	58	0.01%	0.001%
88	11.494	3150	3158	3165	rBV3	555	824	0.09%	0.011%
89	11.652	3203	3207	3213	rBV2	532	694	0.07%	0.009%
90	11.764	3240	3242	3245	rVB	259	104	0.01%	0.001%
91	11.835	3251	3264	3282	rVB	435628	706424	75.35%	9.147%
92	11.915	3287	3289	3292	rBV	168	63	0.01%	0.001%
93	12.153	3361	3363	3367	rBV	195	137	0.01%	0.002%
94	12.214	3369	3382	3397	rVB	434529	706023	75.31%	9.142%
95	12.308	3409	3411	3413	rBV	173	76	0.01%	0.001%
96	12.414	3442	3444	3449	rVB	199	89	0.01%	0.001%
97	12.565	3487	3491	3495	rBV	239	262	0.03%	0.003%
98	12.761	3549	3552	3556	rBV2	198	154	0.02%	0.002%
99	12.912	3596	3599	3601	rBV	213	98	0.01%	0.001%
100	13.607	3813	3815	3818	rBV	246	152	0.02%	0.002%


Sum of corrected areas: 7723149

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU013020\
Data File : VU036629.D
Acq On : 30 Jan 2020 19:36
Operator : JC/MD
Sample : L1326-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBCS7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

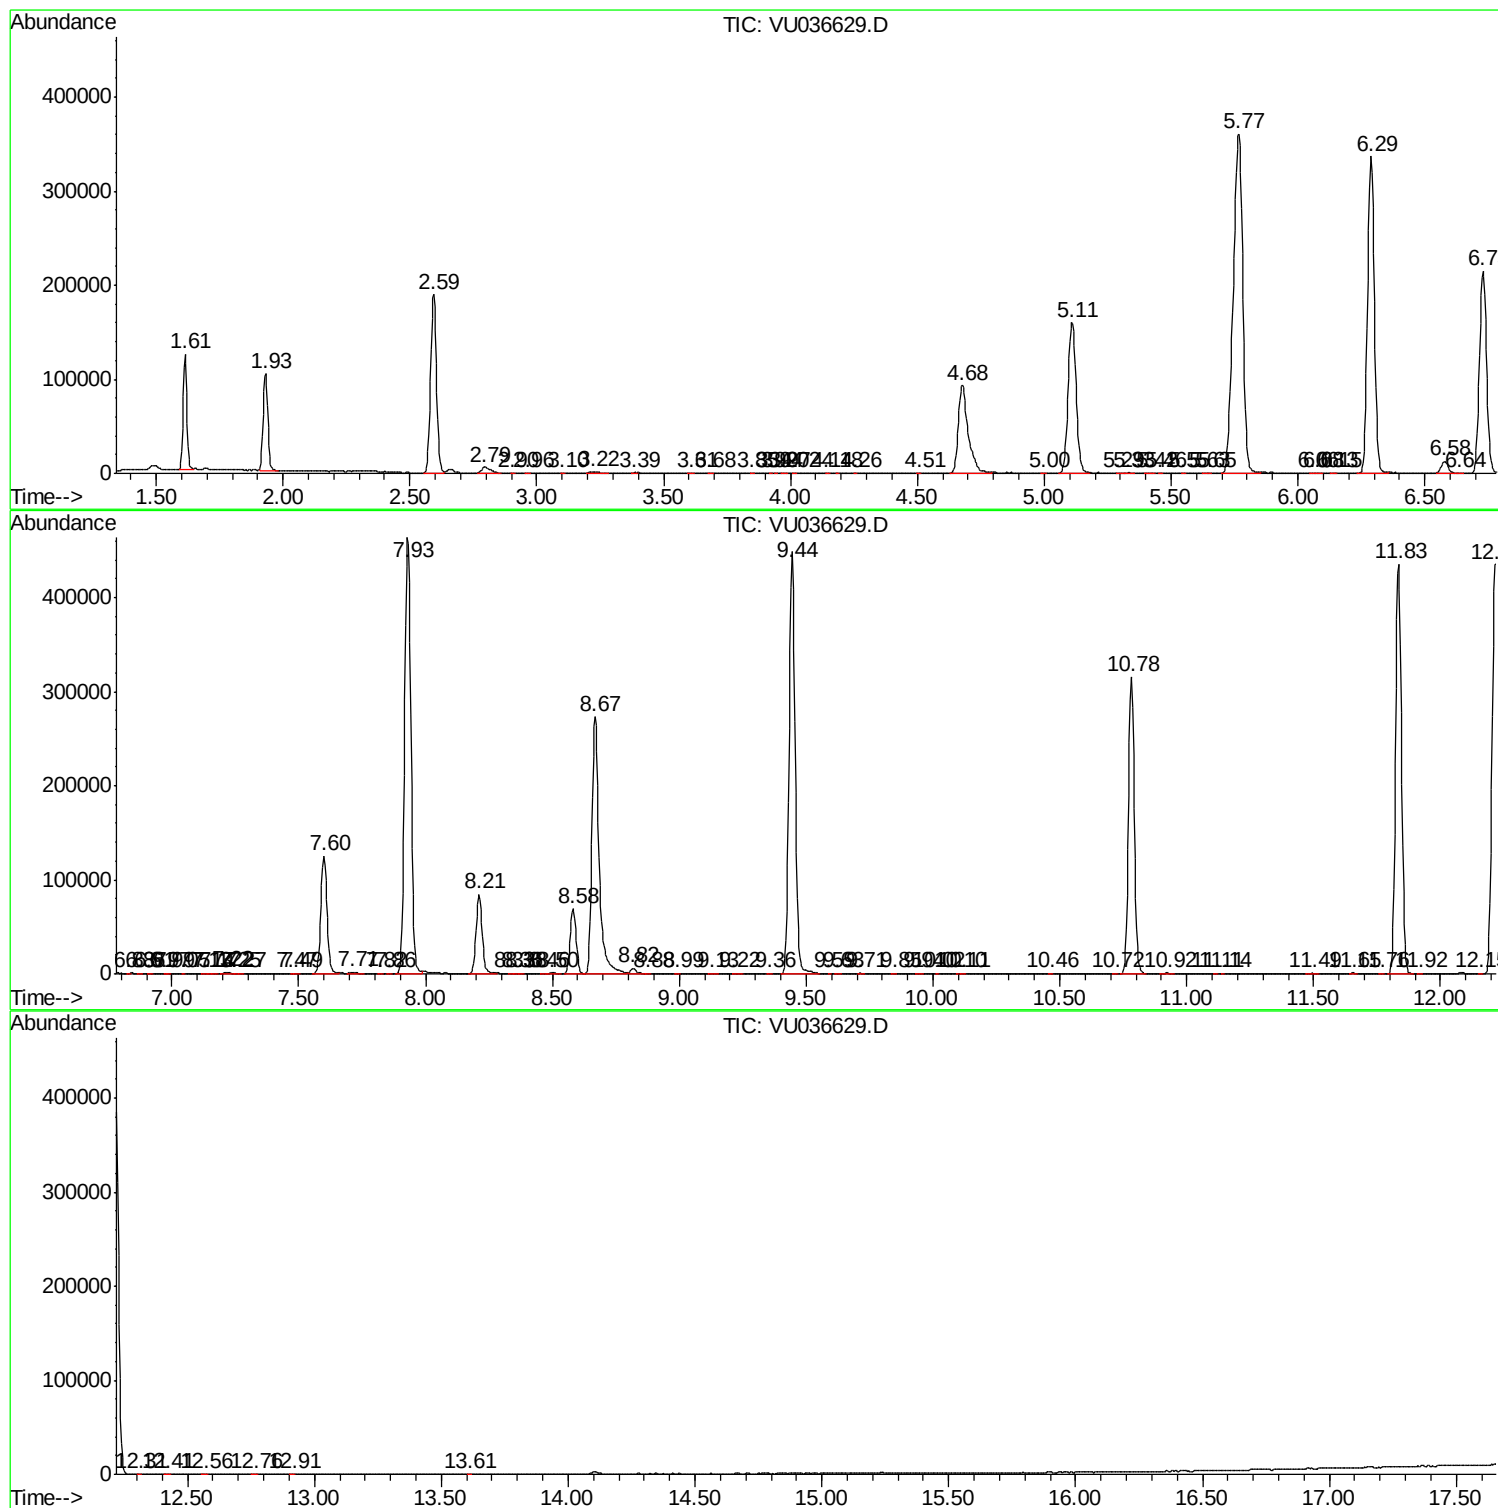

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU013020\
Data File : VU036629.D
Acq On : 30 Jan 2020 19:36
Operator : JC/MD
Sample : L1326-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBCS7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU013020\
Data File : VU036629.D
Acq On : 30 Jan 2020 19:36
Operator : JC/MD
Sample : L1326-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBCS7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc