


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU013020\
 Data File : VU036607.D
 Acq On : 30 Jan 2020 09:02
 Operator : JC/MD
 Sample : BFB45
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB45

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012820WMA.M
 Title : VOC Analysis
 Last Update : Mon Jan 27 00:51:24 2020

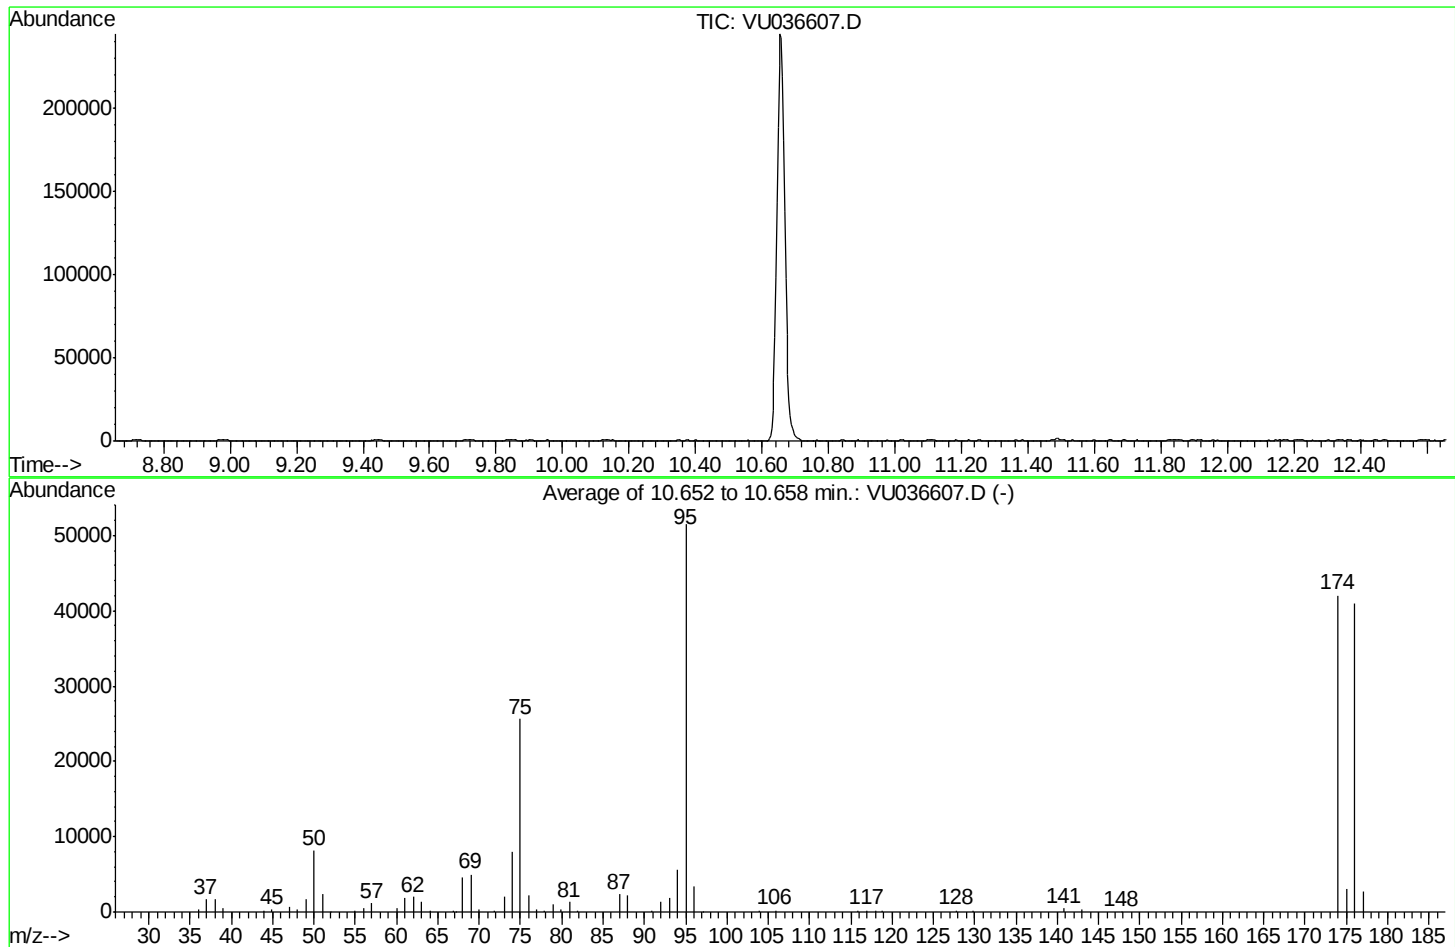

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	8114	PASS
75	95	30	80	49.8	25637	PASS
95	95	100	100	100.0	51480	PASS
96	95	5	9	6.6	3376	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.6	41989	PASS
175	174	5	9	7.4	3104	PASS
176	174	95	101	97.5	40928	PASS
177	176	5	9	6.6	2715	PASS

m/z	Abundance
36.00	325.0
36.90	1672.0
38.00	1575.0
39.00	545.0
44.00	416.0
44.90	341.0
47.00	689.0
47.90	303.0
49.00	1570.0
50.00	7753.0
51.00	2253.0
55.00	109.0
55.90	561.0
57.00	1129.0
60.00	447.0
61.00	1793.0
62.00	1877.0
63.00	1298.0
64.00	184.0
66.80	131.0
67.10	135.0
68.00	4429.0
69.00	4542.0
69.90	380.0
71.90	259.0
73.00	2051.0
74.00	7646.0
75.00	24760.0
76.00	2039.0
76.90	336.0
77.90	230.0
78.90	1092.0
79.90	343.0
80.90	1189.0
81.90	212.0
87.00	2273.0
88.00	2033.0
91.00	127.0
91.90	1197.0
93.00	1834.0
94.00	5272.0
95.00	48920.0
96.00	3318.0
97.10	107.0
104.00	171.0
105.90	191.0
115.80	123.0
117.00	236.0
118.00	156.0
118.80	188.0
127.80	182.0
129.80	134.0
140.90	424.0
142.90	326.0
174.00	39464.0
175.00	2909.0
176.00	38136.0
177.00	2658.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	316.0
37.00	1740.0
38.00	1689.0
39.00	591.0
43.90	445.0
44.90	362.0
47.00	647.0
47.90	298.0
49.00	1805.0
50.00	8300.0
51.00	2414.0
52.00	122.0
54.90	104.0
56.00	568.0
57.00	1206.0
60.00	498.0
61.00	1915.0
62.00	2095.0
63.00	1438.0
64.00	192.0
66.80	124.0
68.00	4868.0
69.00	5125.0
70.00	384.0
71.90	247.0
73.00	2105.0
74.00	8364.0
75.00	26520.0
76.00	2255.0
77.00	316.0
77.90	257.0
79.00	1152.0
80.00	403.0
81.00	1374.0
81.90	266.0
87.00	2409.0
87.90	2225.0
91.00	165.0
92.00	1406.0
93.00	1873.0
94.00	5730.0
95.00	53088.0
96.00	3473.0
97.00	103.0
104.00	187.0
105.90	190.0
115.80	117.0
117.00	261.0
118.00	154.0
118.80	201.0
127.80	212.0
129.80	122.0
140.90	448.0
142.90	336.0
174.00	43352.0
175.00	3186.0
176.00	42008.0
177.00	2768.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
35.90	270.0
37.00	1655.0
38.10	1642.0
39.00	631.0
43.90	429.0
44.90	313.0
47.00	516.0
47.90	271.0
49.00	1788.0
50.00	8289.0
51.00	2333.0
52.00	129.0
54.90	105.0
56.10	560.0
57.00	1215.0
60.00	471.0
61.00	1933.0
62.00	2118.0
63.00	1466.0
64.00	199.0
66.80	100.0
68.00	4732.0
69.00	5130.0
70.00	343.0
71.90	226.0
73.00	2059.0
74.00	8172.0
75.00	25632.0
76.00	2245.0
77.00	293.0
77.90	254.0
79.00	1076.0
80.00	425.0
81.00	1390.0
81.90	299.0
87.00	2410.0
87.90	2259.0
90.80	216.0
92.00	1466.0
93.00	1802.0
94.00	5751.0
95.00	52432.0
96.00	3339.0
103.90	166.0
105.90	173.0
115.80	119.0
116.90	261.0
118.00	152.0
118.80	190.0
127.80	201.0
129.80	121.0
140.80	424.0
142.90	310.0
147.80	116.0
174.00	43152.0
175.00	3218.0
176.00	42640.0
177.00	2720.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
44.00	244.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45