

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013023\
 Data File : VU052862.D
 Acq On : 30 Jan 2023 11:52
 Operator : JC/MD
 Sample : VU0130WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0130WBL01

Quant Time: Jan 31 07:41:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Jan 24 05:16:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.112	96	33860	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.632	95	8245	0.732	ug/l	0.00
Spiked Amount 1.000			Recovery	=	73.000%	
68) 1,2-Dichlorobenzene-d4	12.189	152	9952	0.859	ug/l	0.00
Spiked Amount 1.000			Recovery	=	86.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013023\
Data File : VU052862.D
Acq On : 30 Jan 2023 11:52
Operator : JC/MD
Sample : VU0130WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0130WBL01

Quant Time: Jan 31 07:41:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Jan 24 05:16:59 2023
Response via : Initial Calibration




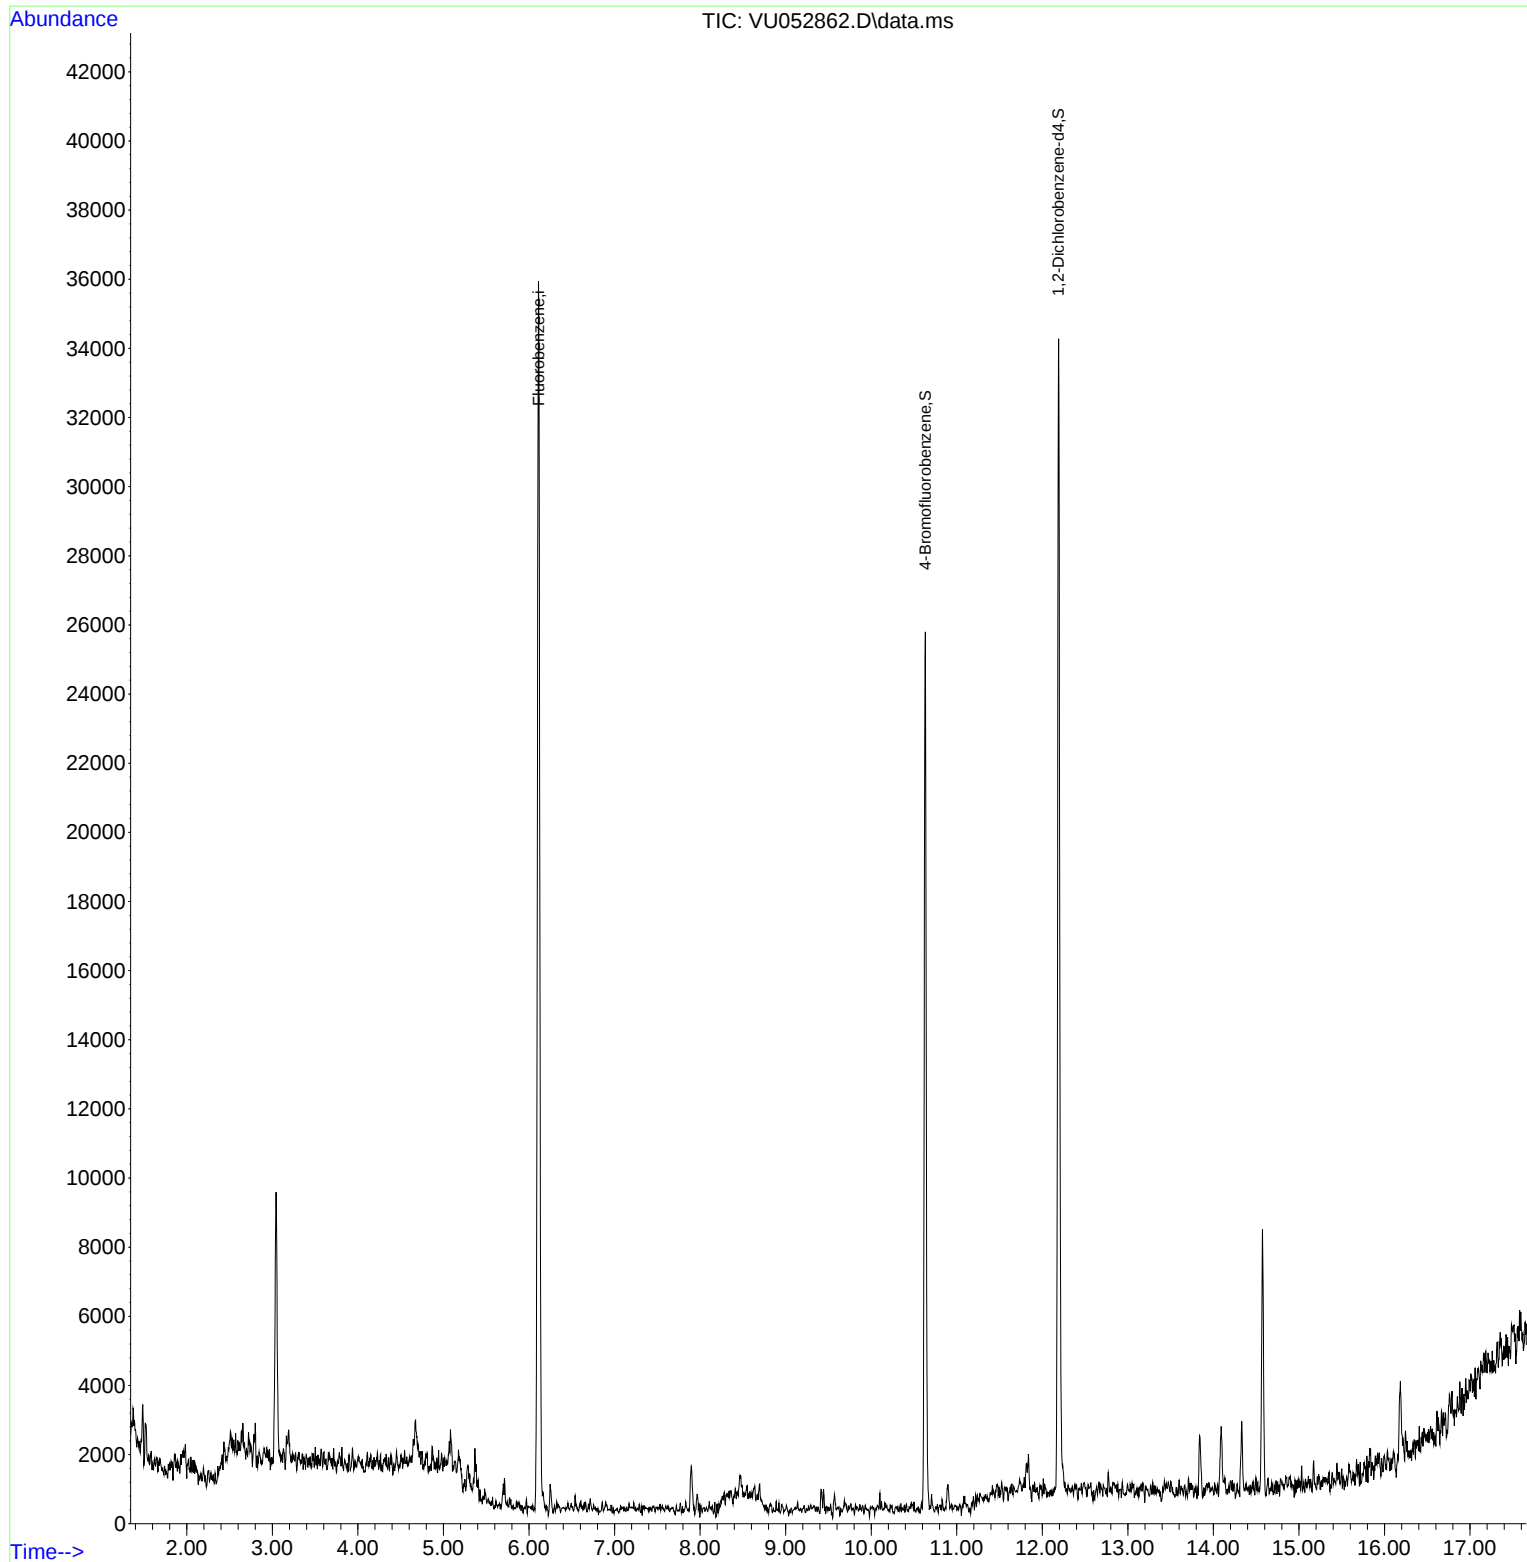


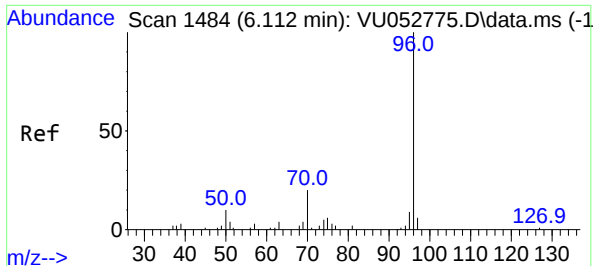

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.112 min Scan# 1484
Delta R.T. -0.000 min
Lab File: VU052862.D
Acq: 30 Jan 2023 11:52




Instrument :
MSVOA_U
ClientSampleId :
VU0130WBL01


Tgt Ion: 96	Resp:	33860
Ion Ratio	Lower	Upper
96	100	
70	17.9	16.2 24.4
95	9.3	7.4 11.0
97	6.0	0.0 0.0#

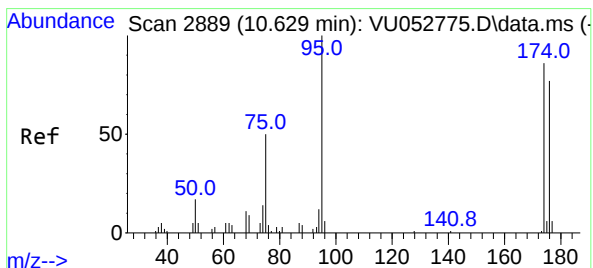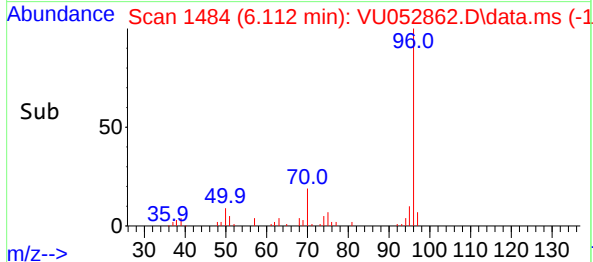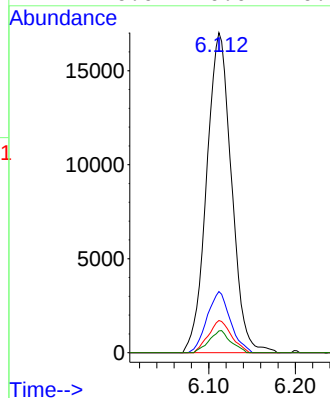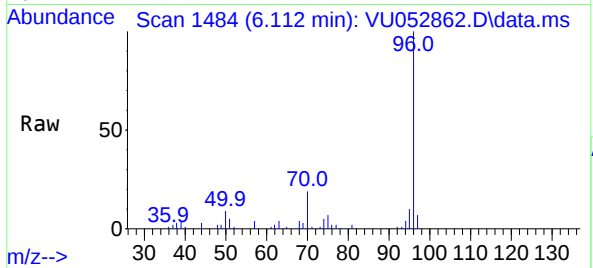

#57
4-Bromofluorobenzene
Concen: 0.732 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. 0.003 min
Lab File: VU052862.D
Acq: 30 Jan 2023 11:52


Tgt Ion: 95	Resp:	8245
Ion Ratio	Lower	Upper
95	100	
174	90.4	66.9 100.3
176	91.4	61.9 92.9

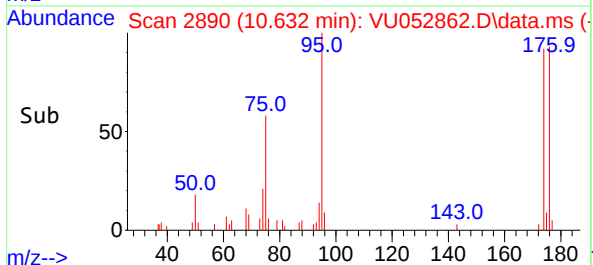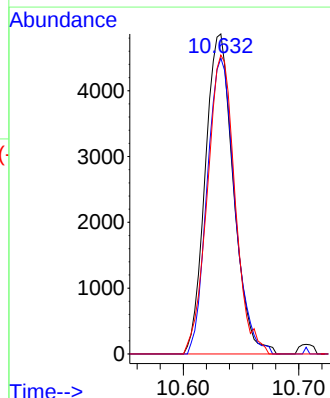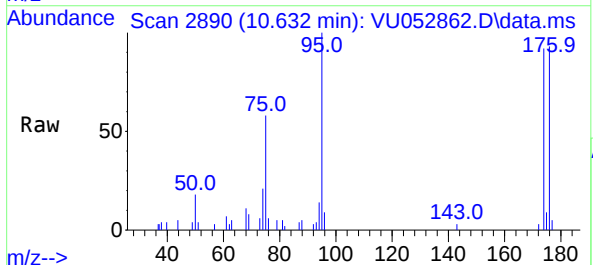

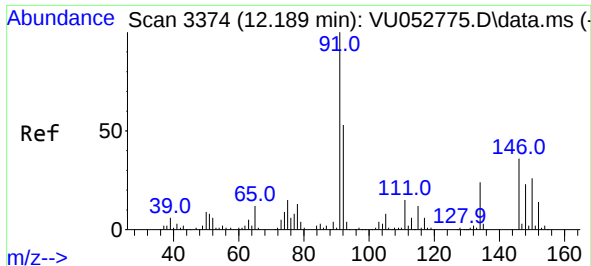

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.859 ug/l
 RT: 12.189 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VU052862.D
 Acq: 30 Jan 2023 11:52

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0130WBL01

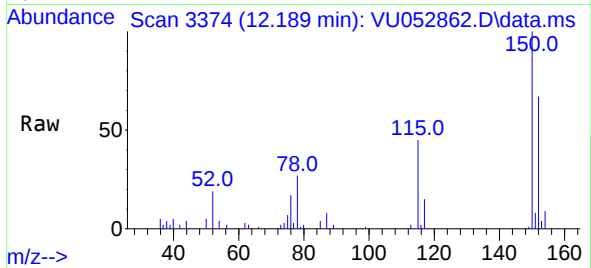

Tgt Ion:	152	Resp:	9952
Ion	Ratio	Lower	Upper
152	100		
115	62.3	0.0	262.6
150	148.4	0.0	638.0

