

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013023\
 Data File : VU052862.D
 Acq On : 30 Jan 2023 11:52
 Operator : JC/MD
 Sample : VU0130WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0130WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU052862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.861	155	162	166	rBV2	770	1164	1.70%	0.520%
2	2.784	444	449	451	rBV2	947	834	1.22%	0.372%
3	2.800	452	454	458	rVB2	1293	769	1.12%	0.343%
4	3.044	519	530	540	rBV3	7849	13794	20.13%	6.158%
5	3.163	563	567	569	rBV2	965	695	1.01%	0.310%
6	4.674	1033	1037	1044	rVB3	807	969	1.41%	0.433%
7	5.083	1162	1164	1171	rVB4	1207	1288	1.88%	0.575%
8	5.285	1221	1227	1231	rBV4	644	871	1.27%	0.389%
9	5.369	1249	1253	1256	rBV2	1017	819	1.20%	0.366%
10	6.112	1471	1484	1498	rBV	35533	68518	100.00%	30.590%
11	6.247	1519	1526	1537	rBV3	914	1368	2.00%	0.611%
12	7.896	2031	2039	2048	rBV3	1312	2173	3.17%	0.970%
13	7.964	2052	2060	2065	rBV3	582	827	1.21%	0.369%
14	9.414	2507	2511	2517	rBV3	701	851	1.24%	0.380%
15	9.571	2553	2560	2566	rBV4	694	1065	1.55%	0.475%
16	10.632	2879	2890	2905	rVB	25403	40016	58.40%	17.865%
17	11.812	3253	3257	3261	rBV4	712	849	1.24%	0.379%
18	11.838	3263	3265	3271	rVB4	1031	732	1.07%	0.327%
19	12.192	3364	3375	3389	rBV2	33233	56391	82.30%	25.176%
20	13.176	3678	3681	3688	rVB4	579	726	1.06%	0.324%
21	13.838	3882	3887	3898	rVB5	1799	2915	4.25%	1.301%
22	14.092	3956	3966	3974	rBV3	2039	3609	5.27%	1.611%
23	14.330	4033	4040	4049	rBV7	2182	3199	4.67%	1.428%
24	14.574	4106	4116	4126	rVB2	7669	11650	17.00%	5.201%
25	15.172	4296	4302	4305	rBV3	903	852	1.24%	0.380%
26	16.153	4602	4607	4610	rBV5	683	733	1.07%	0.327%
27	16.185	4610	4617	4623	rVV3	2273	3643	5.32%	1.626%
28	16.246	4633	4636	4640	rBV4	877	770	1.12%	0.344%
29	16.610	4746	4749	4754	rBV3	1016	1020	1.49%	0.455%
30	17.124	4907	4909	4914	rBV6	819	878	1.28%	0.392%




Sum of corrected areas: 223988

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013023\
Data File : VU052862.D
Acq On : 30 Jan 2023 11:52
Operator : JC/MD
Sample : VU0130WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0130WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

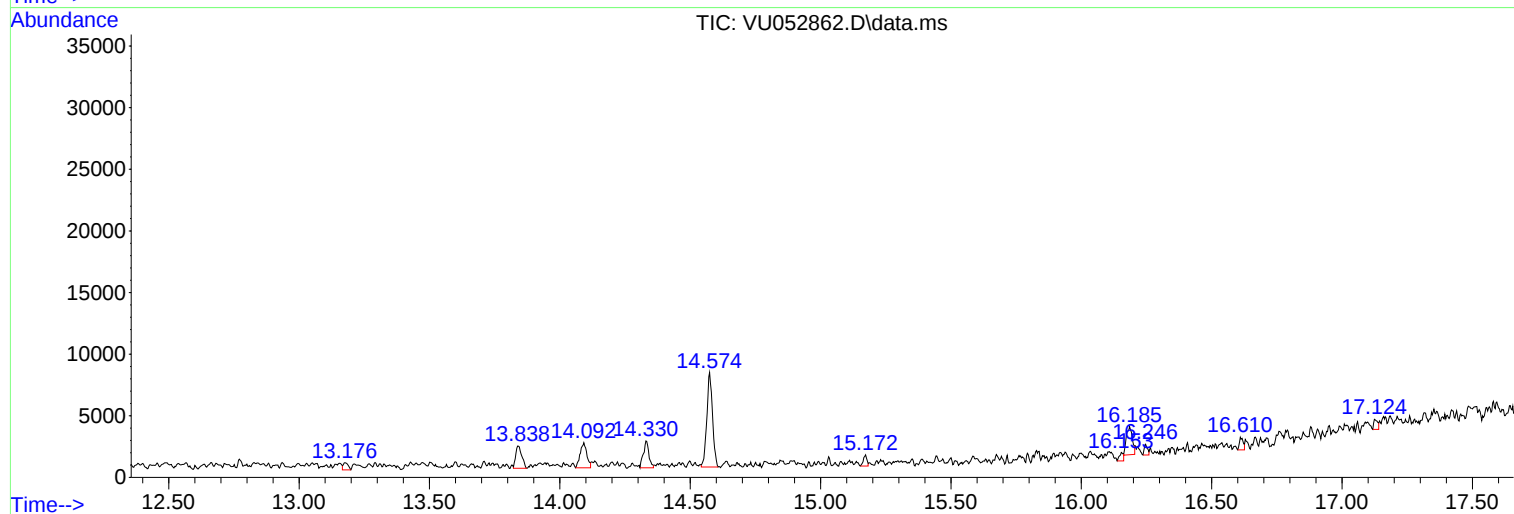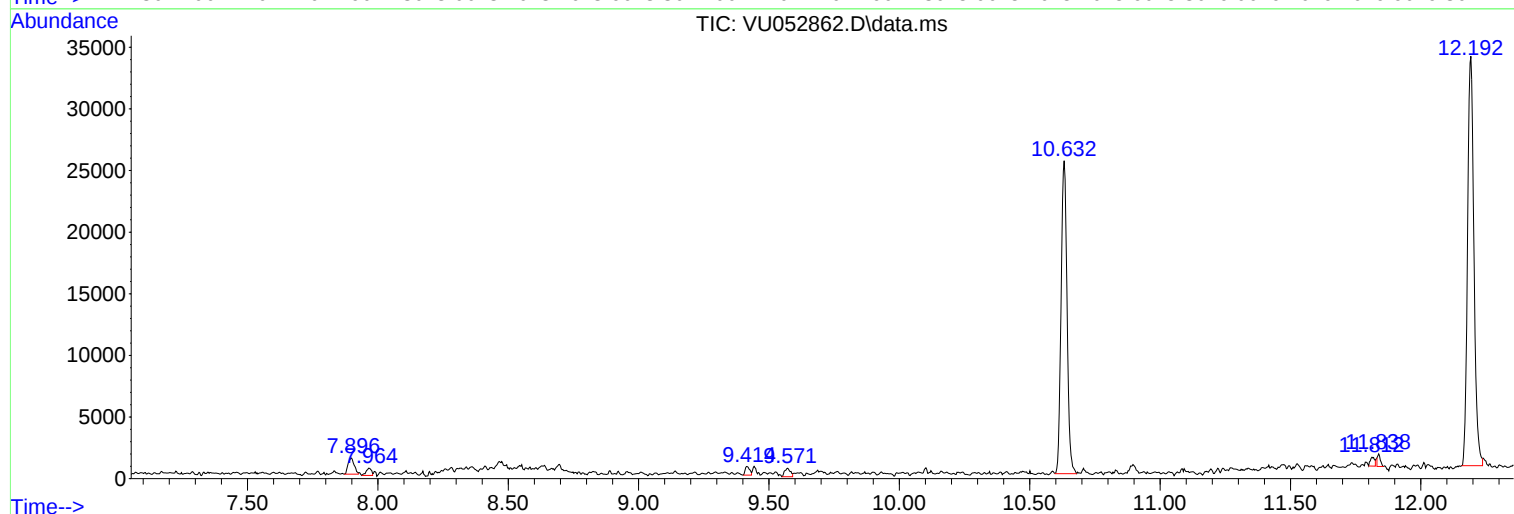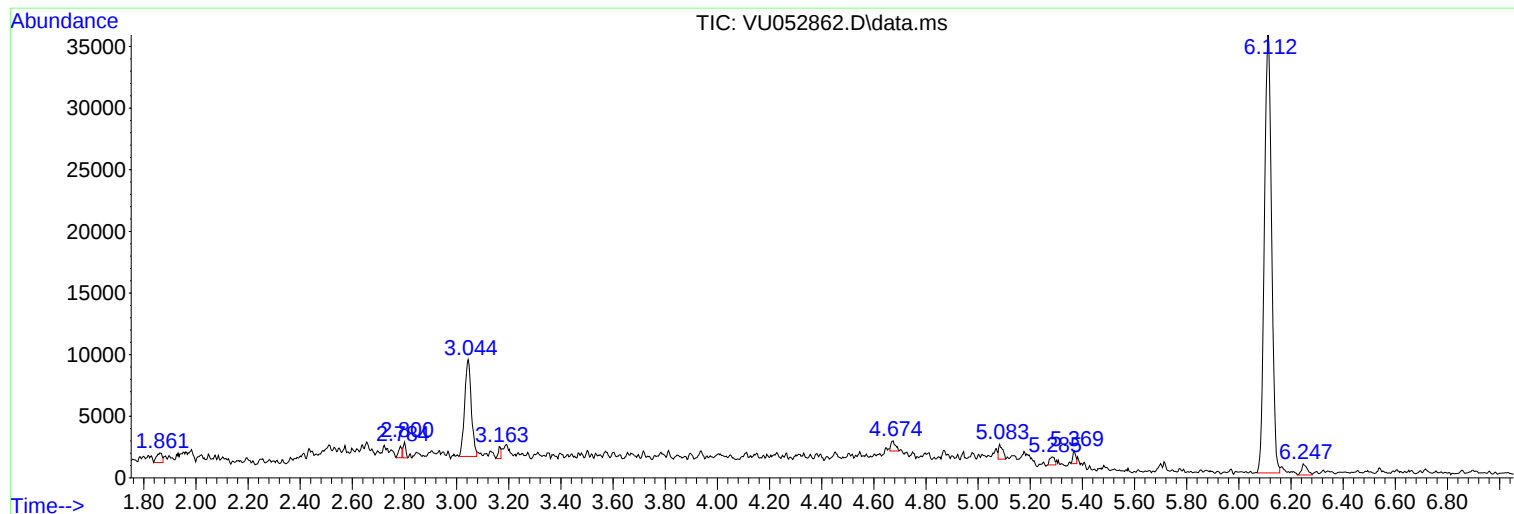

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013023\
Data File : VU052862.D
Acq On : 30 Jan 2023 11:52
Operator : JC/MD
Sample : VU0130WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0130WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013023\
Data File : VU052862.D
Acq On : 30 Jan 2023 11:52
Operator : JC/MD
Sample : VU0130WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0130WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------