


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013023\
Data File : VU052860.D
Acq On : 30 Jan 2023 10:17
Operator : JC/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Jan 24 05:16:59 2023

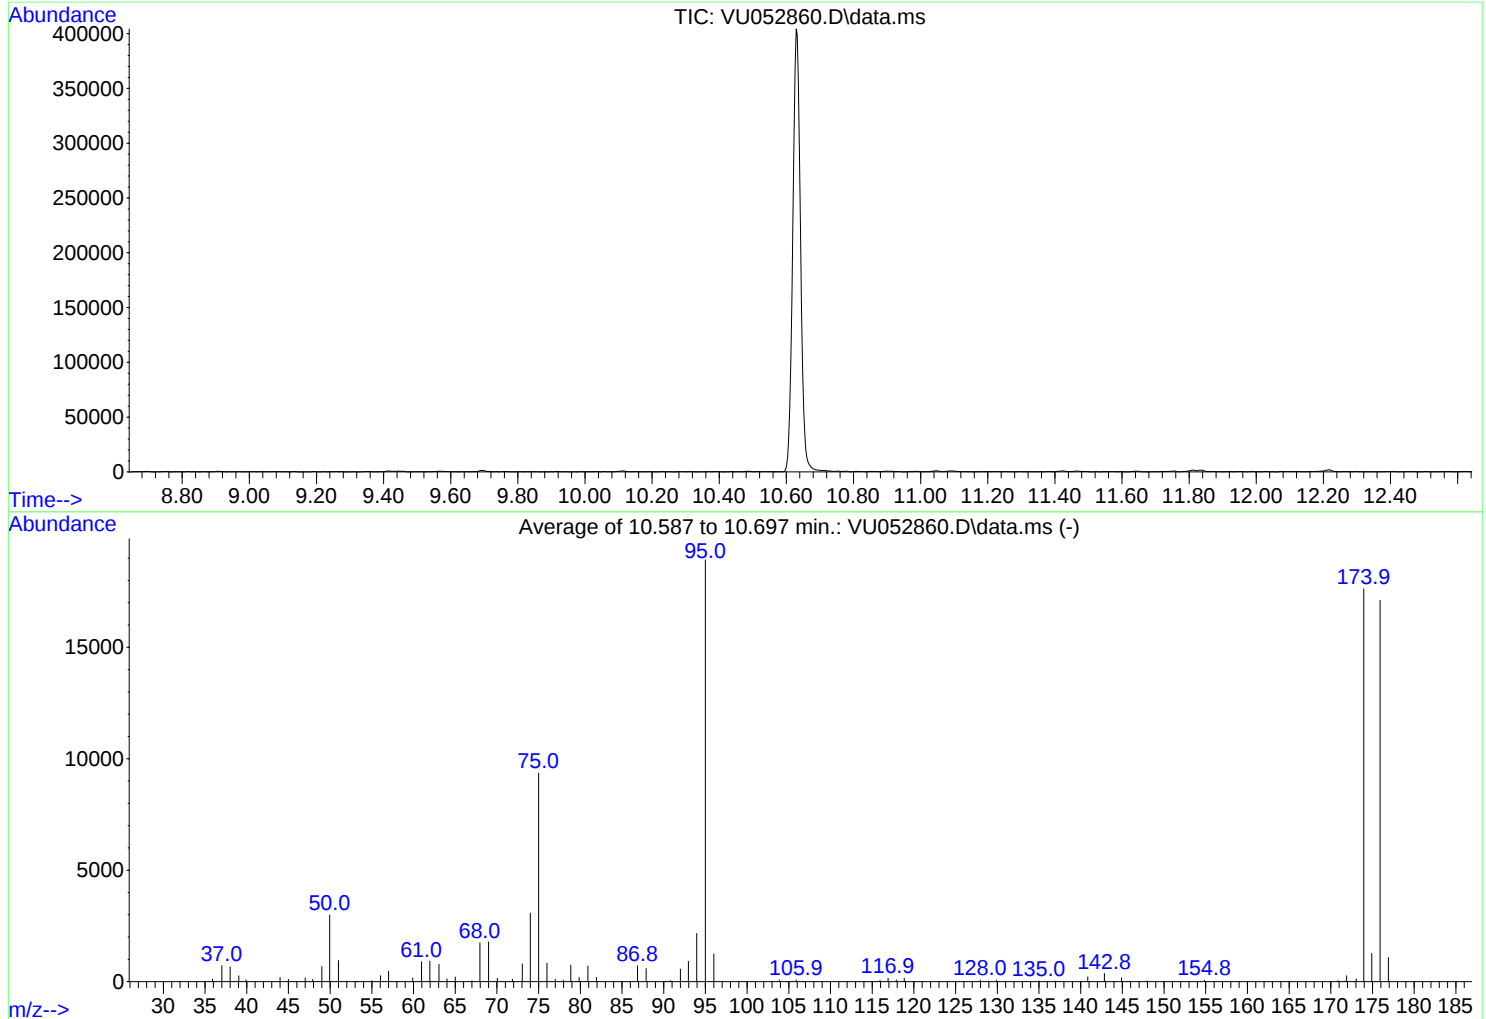

AutoFind: Averaged scan 2876 to 2910; Bkg corrected with scan 2875

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.8	2989	PASS
75	95	30	60	49.4	9354	PASS
95	95	100	100	100.0	18924	PASS
96	95	5	9	6.6	1242	PASS
173	174	0.00	2	0.7	125	PASS
174	95	50	100	93.1	17620	PASS
175	174	5	9	7.2	1261	PASS
176	174	95	101	97.1	17108	PASS
177	176	5	9	6.3	1086	PASS