

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013024\
 Data File : VU057744.D
 Acq On : 30 Jan 2024 15:23
 Operator : MD/SY
 Sample : P1239-14 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 30 22:37:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 30 22:31:02 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	64887	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	57856	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	26929	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	18738	5.241	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 104.800%		
7) Chloroethane-d5	1.911	69	15748	5.257	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 105.200%		
11) 1,1-Dichloroethene-d2	2.563	65	8486	5.048	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 101.000%		
20) 2-Butanone-d5	4.631	46	37553	55.681	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 111.360%		
24) Chloroform-d	5.055	84	36225	4.992	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 99.800%		
26) 1,2-Dichloroethane-d4	5.695	65	18524	5.617	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 112.400%		
32) Benzene-d6	5.721	84	74226	5.469	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 109.400%		
36) 1,2-Dichloropropane-d6	6.682	67	22035	5.383	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 107.600%		
41) Toluene-d8	7.891	98	67051	5.205	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 104.000%		
43) trans-1,3-Dichloroprop...	8.177	79	8093	4.961	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 99.200%		
46) 2-Hexanone-d5	8.631	63	28433	54.625	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 109.260%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84	14407	5.251	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 105.000%		
66) 1,2-Dichlorobenzene-d4	12.187	152	20980	5.552	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 111.000%		
Target Compounds						
5) Vinyl chloride	1.602	62	1793	0.306	ug/L #	79
19) 1,1-Dichloroethane	3.862	63	4387	0.478	ug/L	98
22) cis-1,2-Dichloroethene	4.657	96	69800	13.072	ug/L	99
29) 1,1,1-Trichloroethane	5.309	97	3186	0.375	ug/L	91
35) Methylcyclohexane	6.685	83	4675	0.529	ug/L #	18
37) 1,2-Dichloropropane	6.685	63	2370	0.477	ug/L #	89
61) 1,2,3-Trichloropropane	11.807	75	3566	1.319	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013024\
Data File : VU057744.D
Acq On : 30 Jan 2024 15:23
Operator : MD/SY
Sample : P1239-14 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jan 30 22:37:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 30 22:31:02 2024
Response via : Initial Calibration

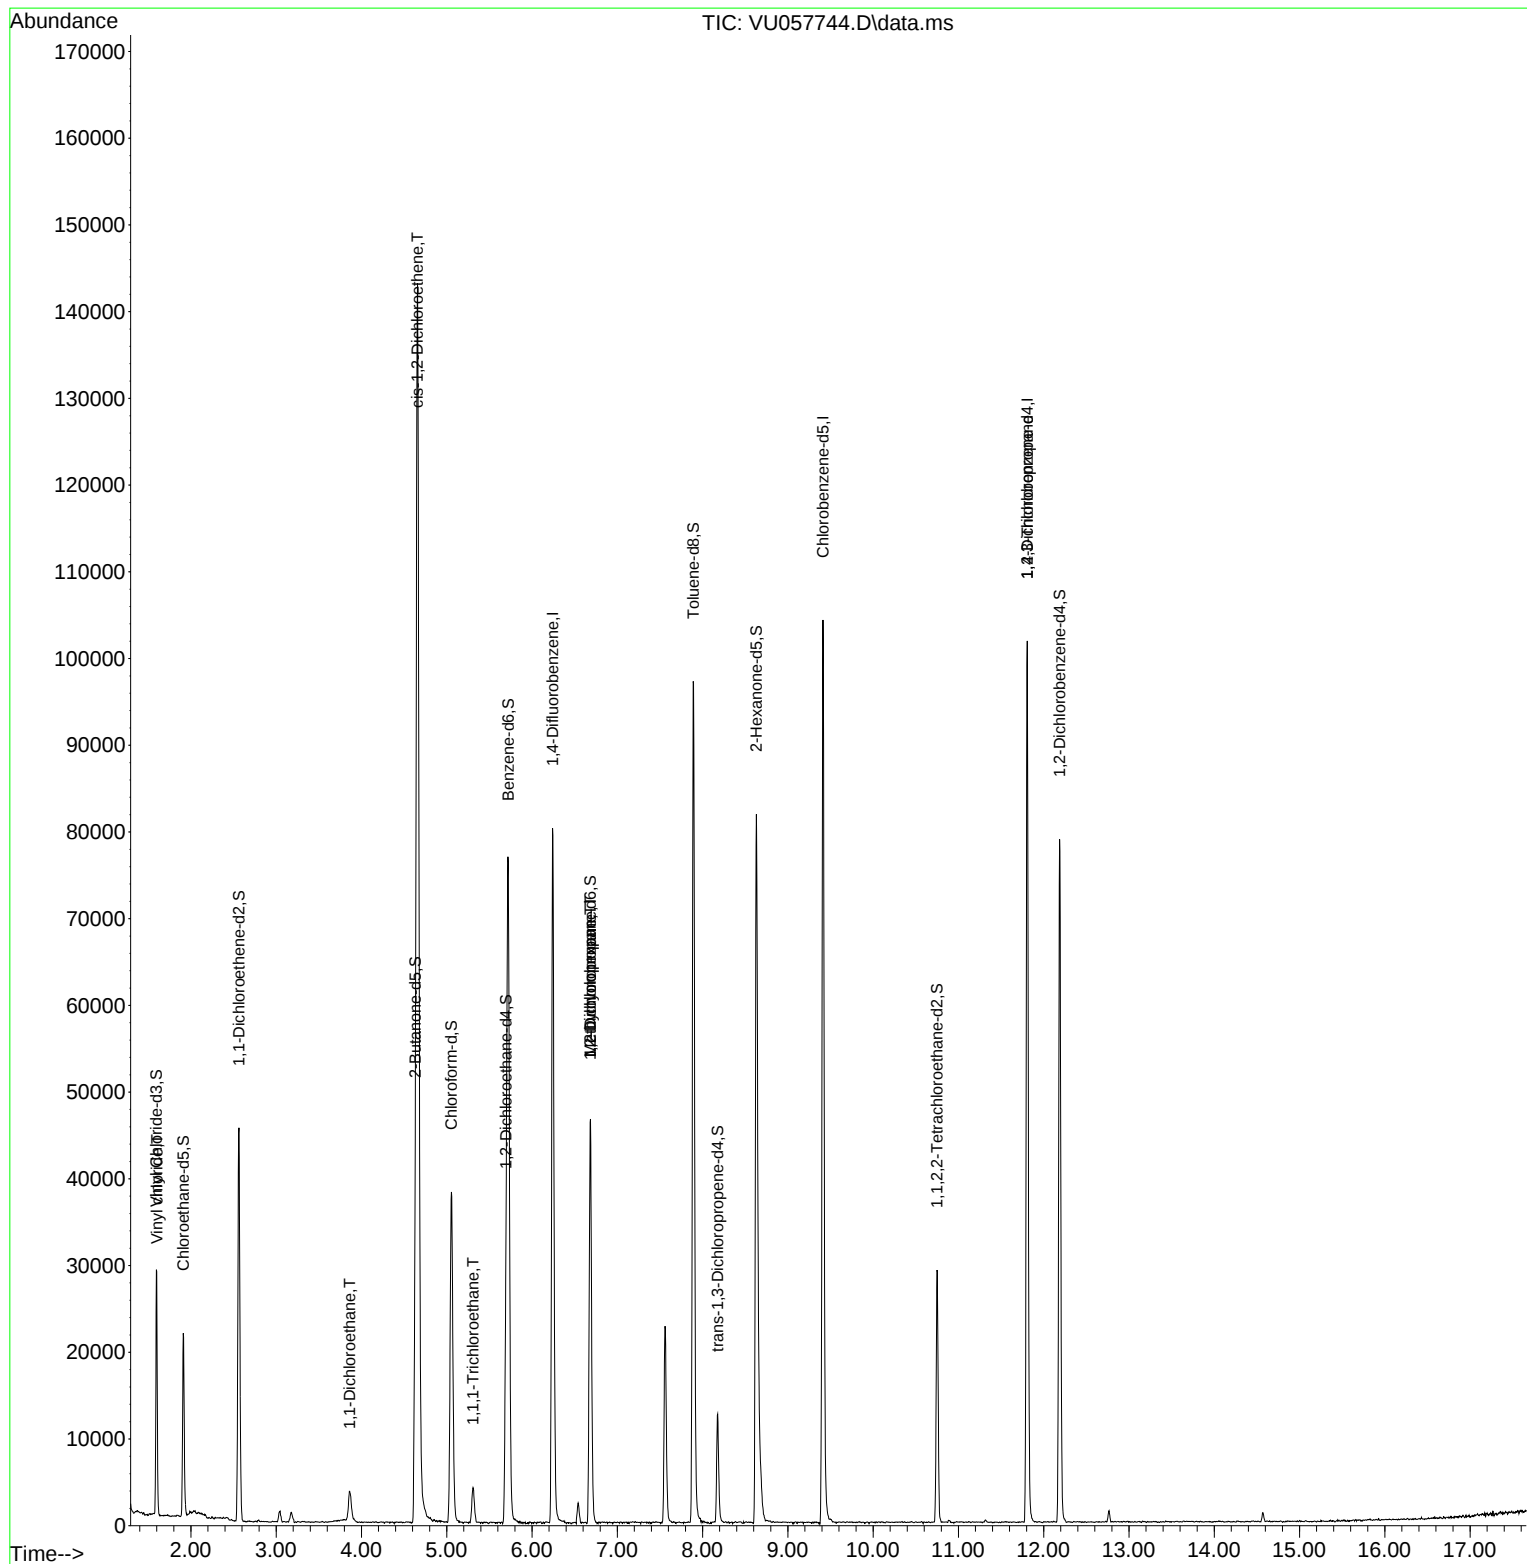

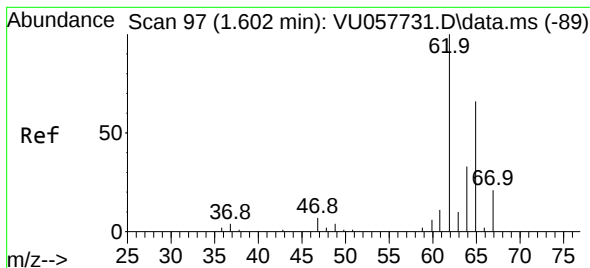

#5

Vinyl chloride

Concen: 0.306 ug/L

RT: 1.602 min Scan# 91

Delta R.T. -0.000 min

Lab File: VU057744.D

Acq: 30 Jan 2024 15:23

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 62 Resp: 1793

Ion Ratio Lower Upper

62 100

64 44.5 22.8 42.4#

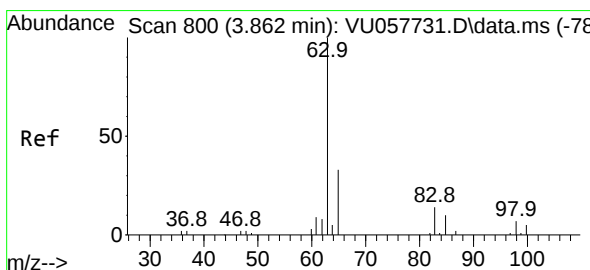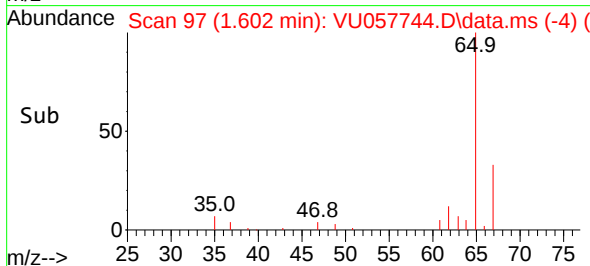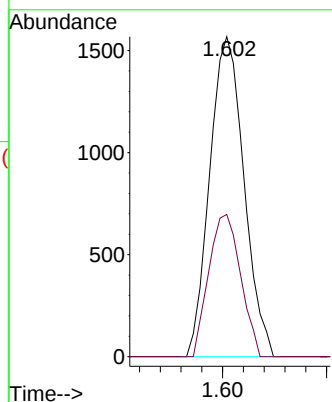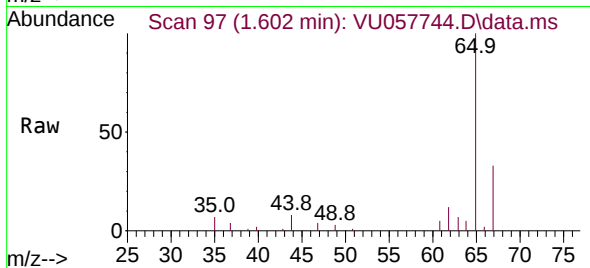

#19

1,1-Dichloroethane

Concen: 0.478 ug/L

RT: 3.862 min Scan# 800

Delta R.T. -0.000 min

Lab File: VU057744.D

Acq: 30 Jan 2024 15:23




Tgt Ion: 63 Resp: 4387


Ion Ratio Lower Upper

63 100

65 34.3 23.0 42.8

83 14.0 9.7 17.9

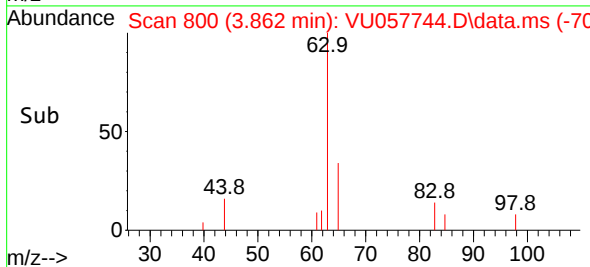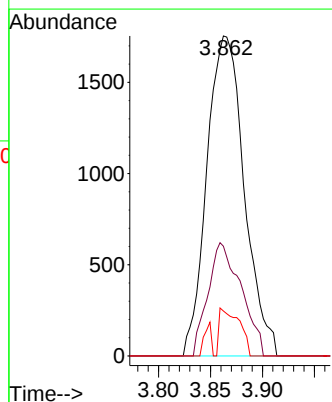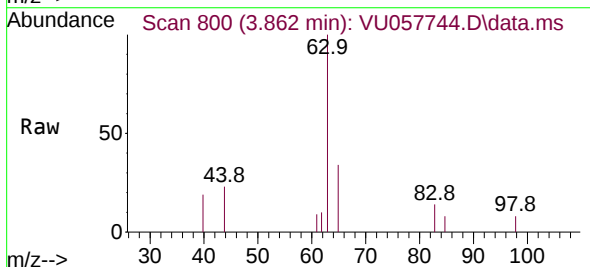

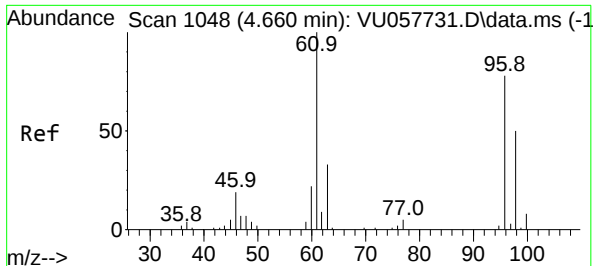

#22

cis-1,2-Dichloroethene

Concen: 13.072 ug/L

RT: 4.657 min Scan# 1047

Delta R.T. -0.003 min

Lab File: VU057744.D

Acq: 30 Jan 2024 15:23

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion: 96 Resp: 69800

Ion Ratio Lower Upper

96 100

61 131.9 92.7 172.1

98 65.3 44.9 83.5

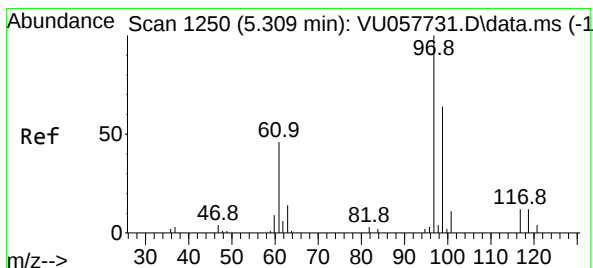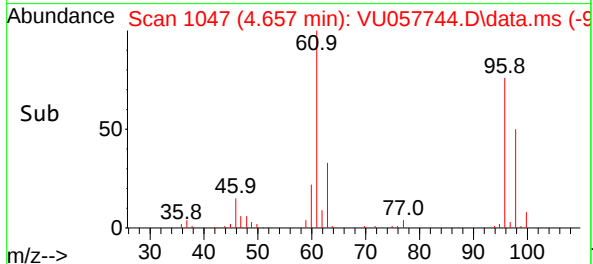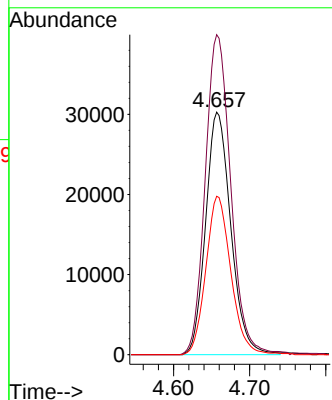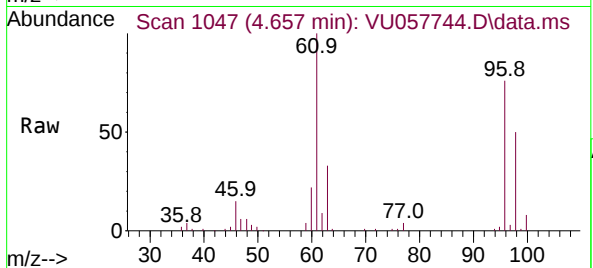

#29

1,1,1-Trichloroethane

Concen: 0.375 ug/L

RT: 5.309 min Scan# 1250

Delta R.T. -0.000 min

Lab File: VU057744.D

Acq: 30 Jan 2024 15:23




Tgt Ion: 97 Resp: 3186


Ion Ratio Lower Upper

97 100

99 53.6 52.0 78.0

61 44.2 35.3 52.9

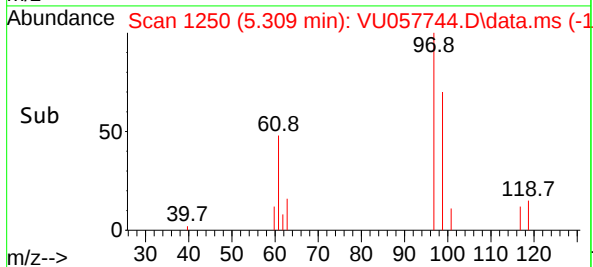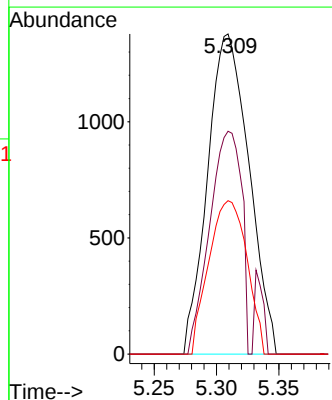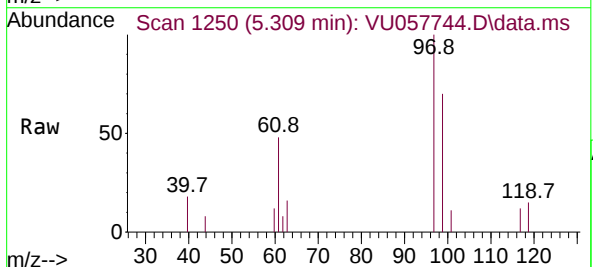

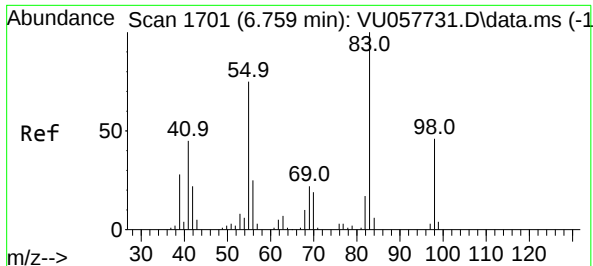

#35

Methylcyclohexane

Concen: 0.529 ug/L

RT: 6.685 min Scan# 1

Delta R.T. -0.074 min

Lab File: VU057744.D





Acq: 30 Jan 2024 15:23

Instrument :

MSVOA_U

ClientSampleId :

Tgt Ion: 83	Resp: 4675
Ion Ratio	Lower Upper
83	100
55	0.0 61.4 92.0#
98	0.0 38.2 57.4#

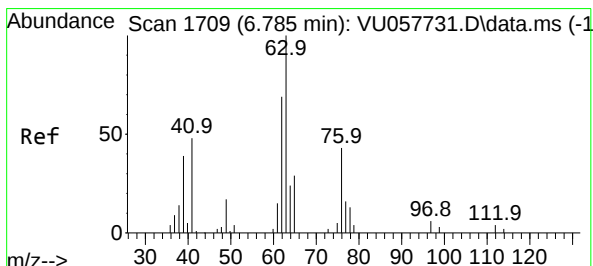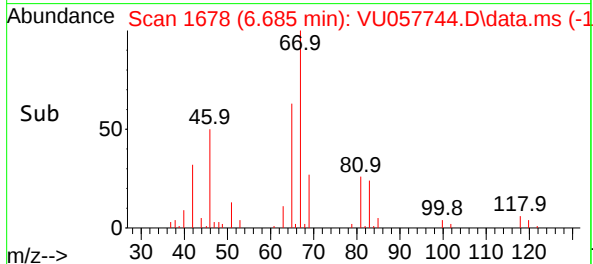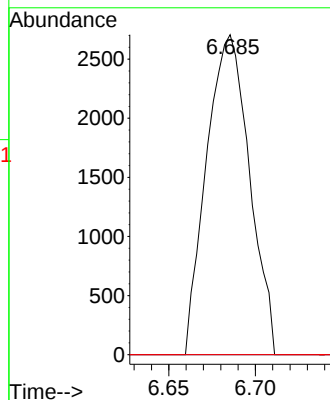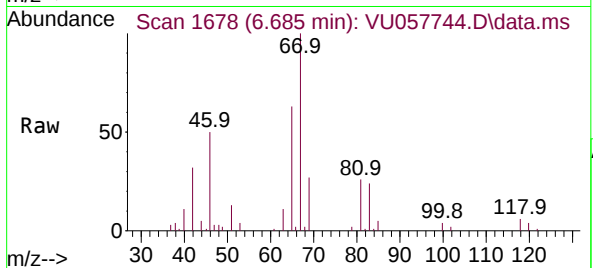

#37

1,2-Dichloropropane

Concen: 0.477 ug/L




RT: 6.685 min Scan# 1678


Delta R.T. -0.100 min

Lab File: VU057744.D

Acq: 30 Jan 2024 15:23


Tgt Ion: 63	Resp: 2370
Ion Ratio	Lower Upper
63	100
112	0.0 3.0 4.4#

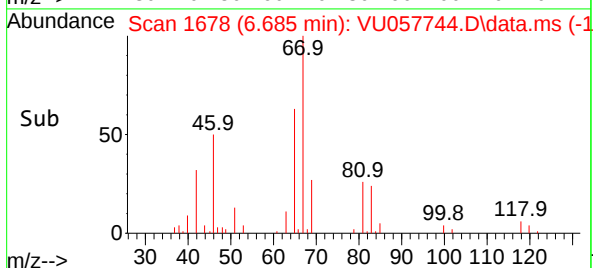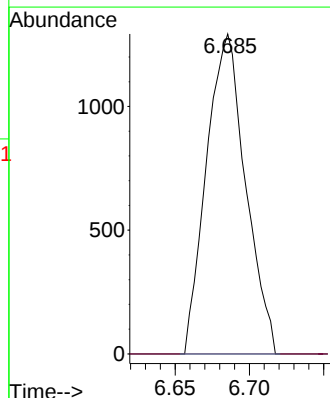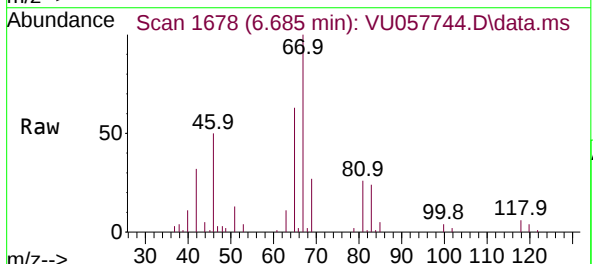

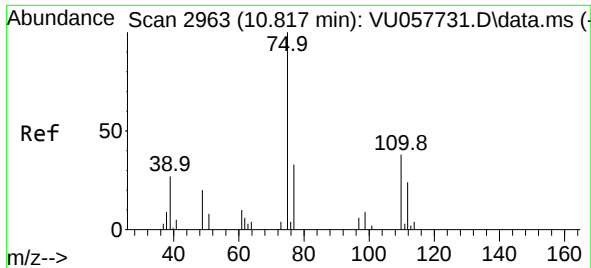

#61
1,2,3-Trichloropropane
Concen: 1.319 ug/L
RT: 11.807 min Scan# 31
Delta R.T. 0.990 min
Lab File: VU057744.D
Acq: 30 Jan 2024 15:23

Instrument :
MSVOA_U
ClientSampleId :

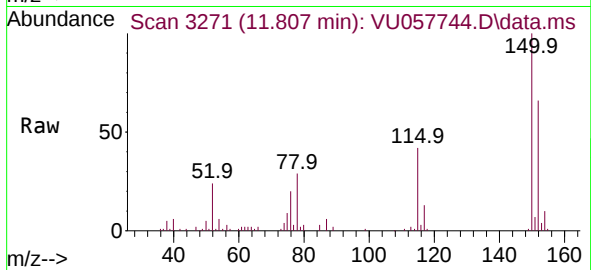

Tgt Ion: 75 Resp: 3566
Ion Ratio Lower Upper
75 100
110 0.0 30.1 45.1#
77 29.5 25.5 38.3

