

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013024\
 Data File : VU057733.D
 Acq On : 30 Jan 2024 10:56
 Operator : MD/SY
 Sample : P1239-14 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FC4

Quant Time: Jan 30 22:35:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 30 22:31:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	66057	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	58755	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	26201	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	18301	5.028	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	100.600%	
7) Chloroethane-d5	1.911	69	15486	5.078	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.600%	
11) 1,1-Dichloroethene-d2	2.563	65	8429	4.925	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	98.600%	
20) 2-Butanone-d5	4.634	46	33663	49.029	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	98.060%	
24) Chloroform-d	5.055	84	34984	4.735	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.800%	
26) 1,2-Dichloroethane-d4	5.698	65	17233	5.133	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.600%	
32) Benzene-d6	5.721	84	71895	5.217	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.400%	
36) 1,2-Dichloropropane-d6	6.685	67	20758	4.994	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.800%	
41) Toluene-d8	7.894	98	65536	5.009	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.200%	
43) trans-1,3-Dichloroprop...	8.177	79	7640	4.611	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	92.200%	
46) 2-Hexanone-d5	8.631	63	26656	50.428	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	100.860%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	13495	4.843	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.800%	
66) 1,2-Dichlorobenzene-d4	12.190	152	19202	5.222	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.400%	
Target Compounds						Qvalue
22) cis-1,2-Dichloroethene	4.660	96	17320	3.186	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013024\
Data File : VU057733.D
Acq On : 30 Jan 2024 10:56
Operator : MD/SY
Sample : P1239-14 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FC4

Quant Time: Jan 30 22:35:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 30 22:31:02 2024
Response via : Initial Calibration

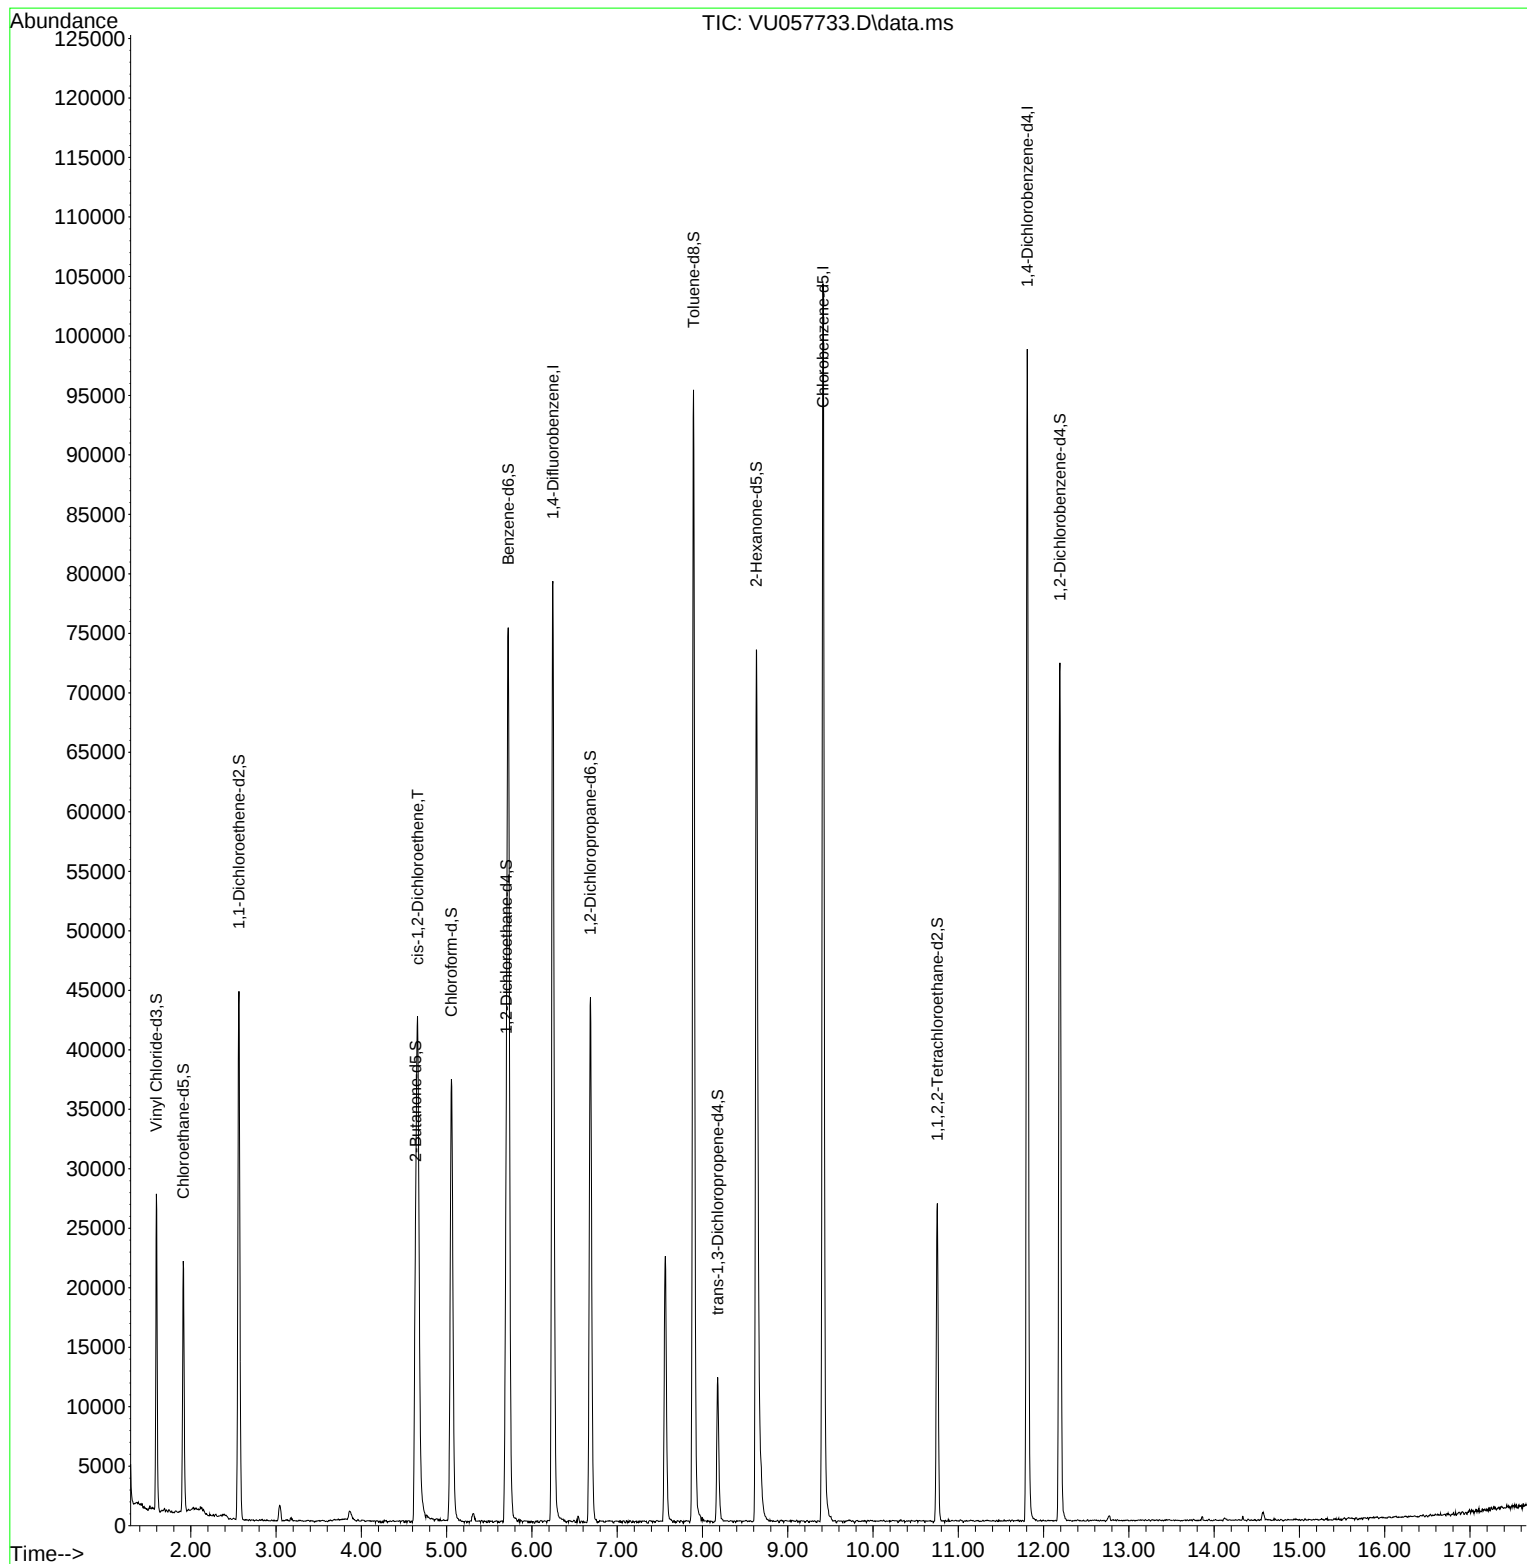

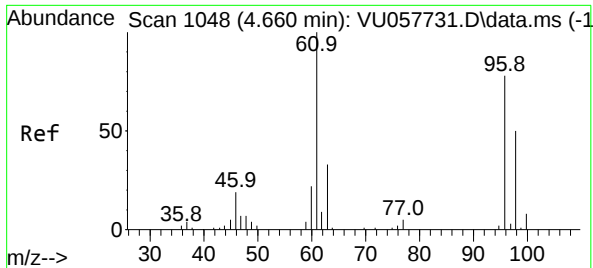

#22
 cis-1,2-Dichloroethene
 Concen: 3.186 ug/L
 RT: 4.660 min Scan# 1048
 Delta R.T. 0.000 min
 Lab File: VU057733.D
 Acq: 30 Jan 2024 10:56

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FC4

Tgt Ion: 96	Resp: 17320
Ion Ratio	Lower Upper
96	100
61	129.5 92.7 172.1
98	66.9 44.9 83.5

