

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013024\
 Data File : VU057747.D
 Acq On : 30 Jan 2024 16:36
 Operator : MD/SY
 Sample : P1239-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FC8

Quant Time: Jan 30 22:38:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 30 22:31:02 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	64861	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	59367	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	26765	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	17888	5.006	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 100.200%		
7) Chloroethane-d5	1.911	69	15539	5.189	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 103.800%		
11) 1,1-Dichloroethene-d2	2.560	65	8593	5.114	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 102.200%		
20) 2-Butanone-d5	4.634	46	37600	55.773	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 111.540%		
24) Chloroform-d	5.055	84	36130	4.981	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 99.600%		
26) 1,2-Dichloroethane-d4	5.695	65	17742	5.382	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 107.600%		
32) Benzene-d6	5.721	84	71945	5.166	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 103.400%		
36) 1,2-Dichloropropane-d6	6.685	67	22126	5.268	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 105.400%		
41) Toluene-d8	7.894	98	65885	4.984	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 99.600%		
43) trans-1,3-Dichloroprop...	8.177	79	7782	4.649	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 93.000%		
46) 2-Hexanone-d5	8.631	63	27959	52.347	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 104.700%		
56) 1,1,2,2-Tetrachloroeth...	10.750	84	14272	5.069	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 101.400%		
66) 1,2-Dichlorobenzene-d4	12.187	152	20834	5.547	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 111.000%		
Target Compounds						
13) Acetone	2.653	43	4043	6.311	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013024\
Data File : VU057747.D
Acq On : 30 Jan 2024 16:36
Operator : MD/SY
Sample : P1239-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FC8

Quant Time: Jan 30 22:38:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 30 22:31:02 2024
Response via : Initial Calibration

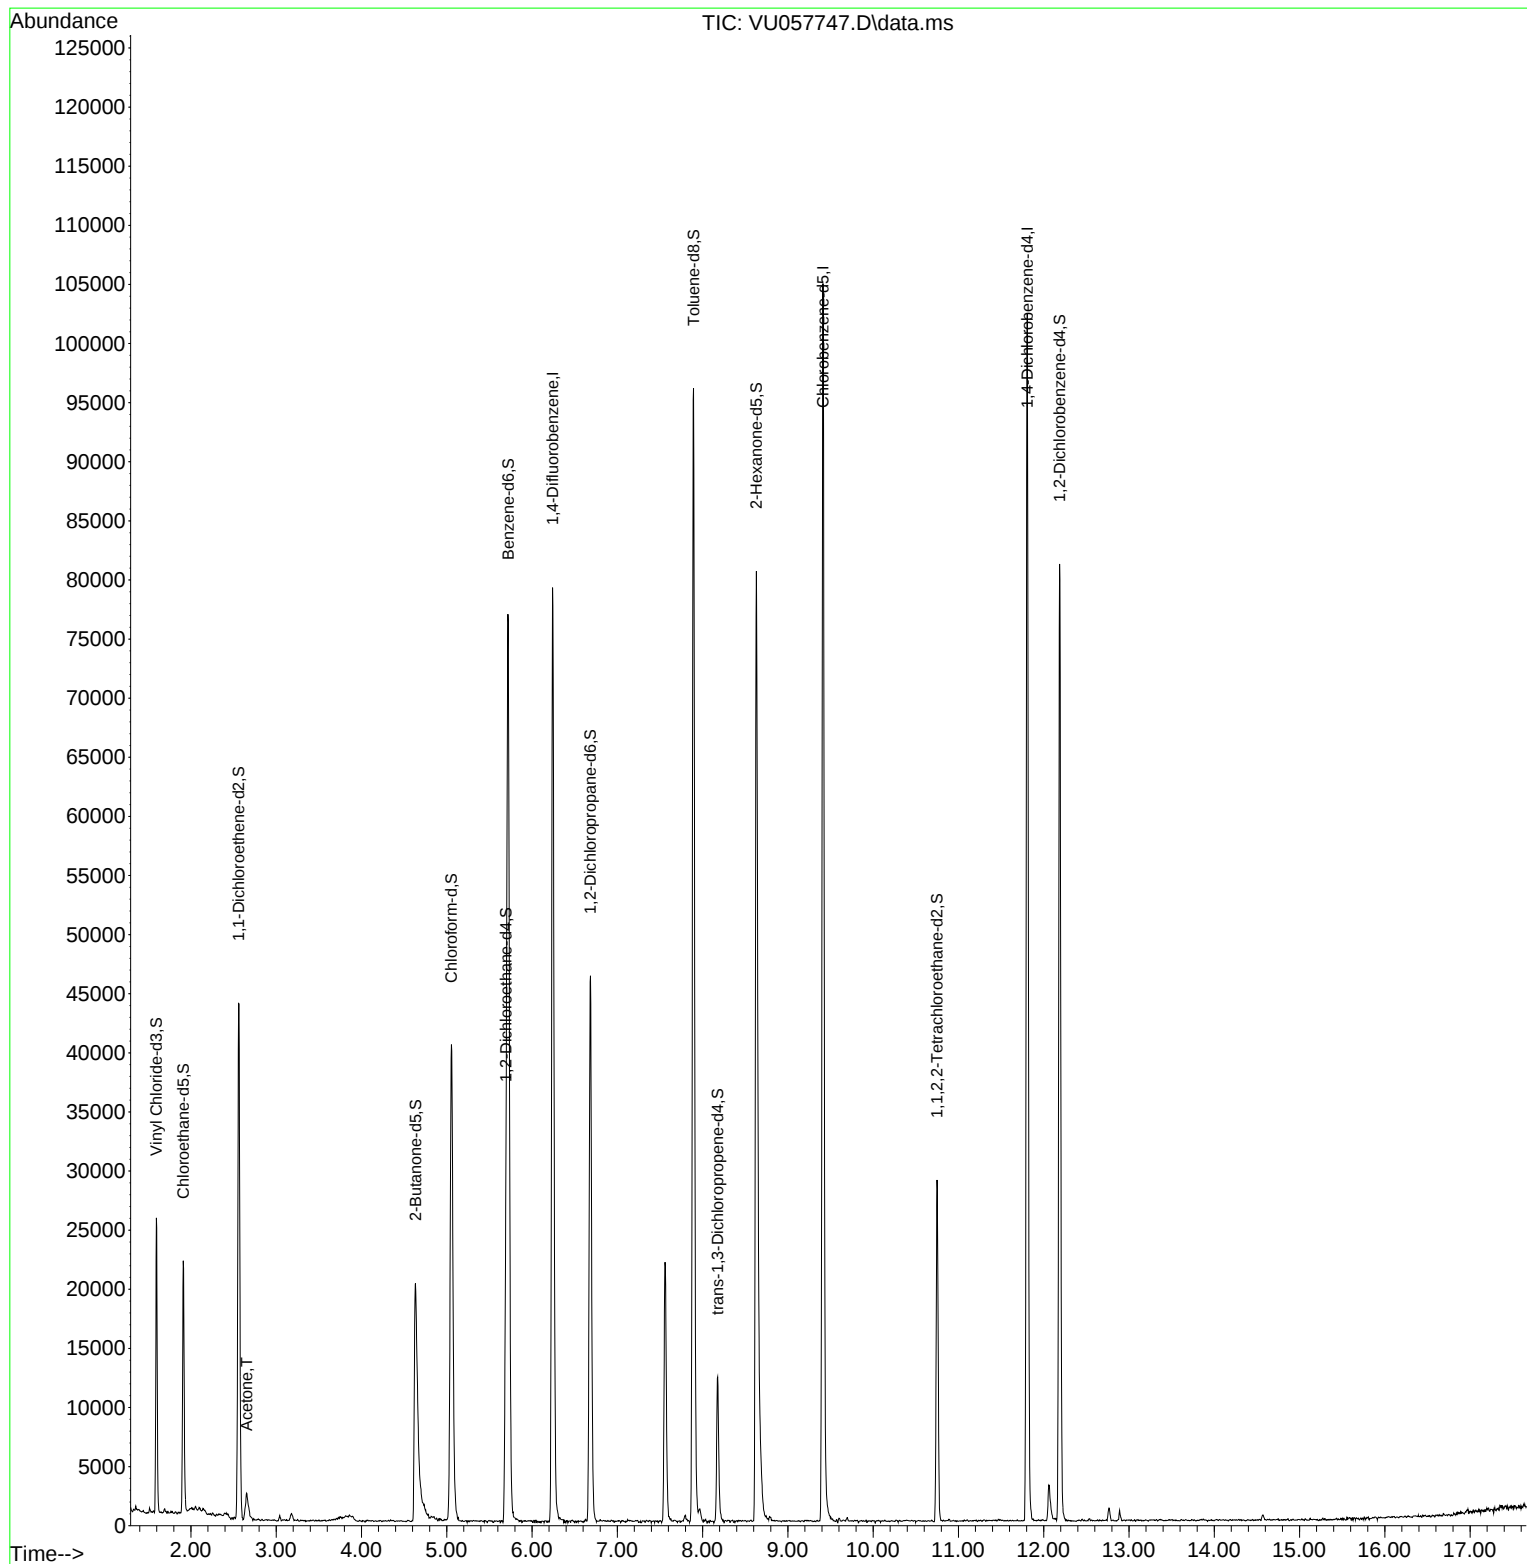

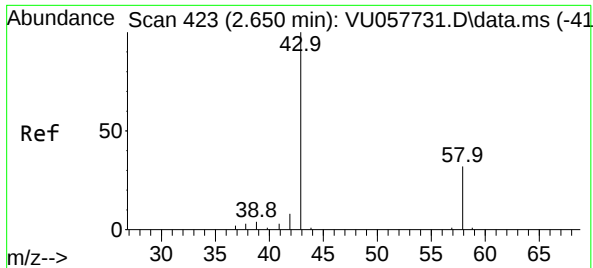

#13
 Acetone
 Concen: 6.311 ug/L
 RT: 2.653 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VU057747.D
 Acq: 30 Jan 2024 16:36

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FC8

Tgt Ion: 43 Resp: 4043
 Ion Ratio Lower Upper
 43 100
 58 28.1 0.0 61.4

