

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU013024\  
 Data File : VU057748.D  
 Acq On : 30 Jan 2024 16:58  
 Operator : MD/SY  
 Sample : P1230-10  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 VHBLK001

Quant Time: Jan 30 22:38:34 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR012324WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Tue Jan 30 22:31:02 2024  
 Response via : Initial Calibration


| Compound                      |        | R.T.   | QIon     | Response | Conc   | Units    | Dev(Min)  |
|-------------------------------|--------|--------|----------|----------|--------|----------|-----------|
| -----                         |        |        |          |          |        |          |           |
| Internal Standards            |        |        |          |          |        |          |           |
| 1) 1,4-Difluorobenzene        |        | 6.242  | 114      | 64813    | 5.000  | ug/L     | 0.00      |
| 28) Chlorobenzene-d5          |        | 9.412  | 117      | 58884    | 5.000  | ug/L     | 0.00      |
| 58) 1,4-Dichlorobenzene-d4    |        | 11.807 | 152      | 26839    | 5.000  | ug/L     | 0.00      |
| System Monitoring Compounds   |        |        |          |          |        |          |           |
| 4) Vinyl Chloride-d3          |        | 1.596  | 65       | 18576    | 5.202  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 40 - 130 | Recovery | =      | 104.000% |           |
| 7) Chloroethane-d5            |        | 1.911  | 69       | 16780    | 5.608  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 65 - 130 | Recovery | =      | 112.200% |           |
| 11) 1,1-Dichloroethene-d2     |        | 2.560  | 65       | 8561     | 5.098  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 60 - 125 | Recovery | =      | 102.000% |           |
| 20) 2-Butanone-d5             |        | 4.624  | 46       | 36048    | 53.510 | ug/L     | 0.00      |
| Spiked Amount                 | 50.000 | Range  | 40 - 130 | Recovery | =      | 107.020% |           |
| 24) Chloroform-d              |        | 5.055  | 84       | 35755    | 4.933  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 70 - 125 | Recovery | =      | 98.600%  |           |
| 26) 1,2-Dichloroethane-d4     |        | 5.695  | 65       | 18210    | 5.528  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 70 - 130 | Recovery | =      | 110.600% |           |
| 32) Benzene-d6                |        | 5.721  | 84       | 72187    | 5.226  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 70 - 125 | Recovery | =      | 104.600% |           |
| 36) 1,2-Dichloropropane-d6    |        | 6.682  | 67       | 22090    | 5.302  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 60 - 140 | Recovery | =      | 106.000% |           |
| 41) Toluene-d8                |        | 7.891  | 98       | 65965    | 5.031  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 70 - 130 | Recovery | =      | 100.600% |           |
| 43) trans-1,3-Dichloroprop... |        | 8.177  | 79       | 8001     | 4.819  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 55 - 130 | Recovery | =      | 96.400%  |           |
| 46) 2-Hexanone-d5             |        | 8.627  | 63       | 27862    | 52.594 | ug/L     | 0.00      |
| Spiked Amount                 | 50.000 | Range  | 45 - 130 | Recovery | =      | 105.180% |           |
| 56) 1,1,2,2-Tetrachloroeth... |        | 10.750 | 84       | 14128    | 5.059  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 65 - 120 | Recovery | =      | 101.200% |           |
| 66) 1,2-Dichlorobenzene-d4    |        | 12.187 | 152      | 20750    | 5.509  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 80 - 120 | Recovery | =      | 110.200% |           |
| Target Compounds              |        |        |          |          |        |          |           |
| 16) Methylene chloride        |        | 3.039  | 84       | 737      | 0.146  | ug/L     | Qvalue 87 |
| -----                         |        |        |          |          |        |          |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU013024\  
Data File : VU057748.D  
Acq On : 30 Jan 2024 16:58  
Operator : MD/SY  
Sample : P1230-10  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VHBLK001


Quant Time: Jan 30 22:38:34 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR012324WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Tue Jan 30 22:31:02 2024  
Response via : Initial Calibration

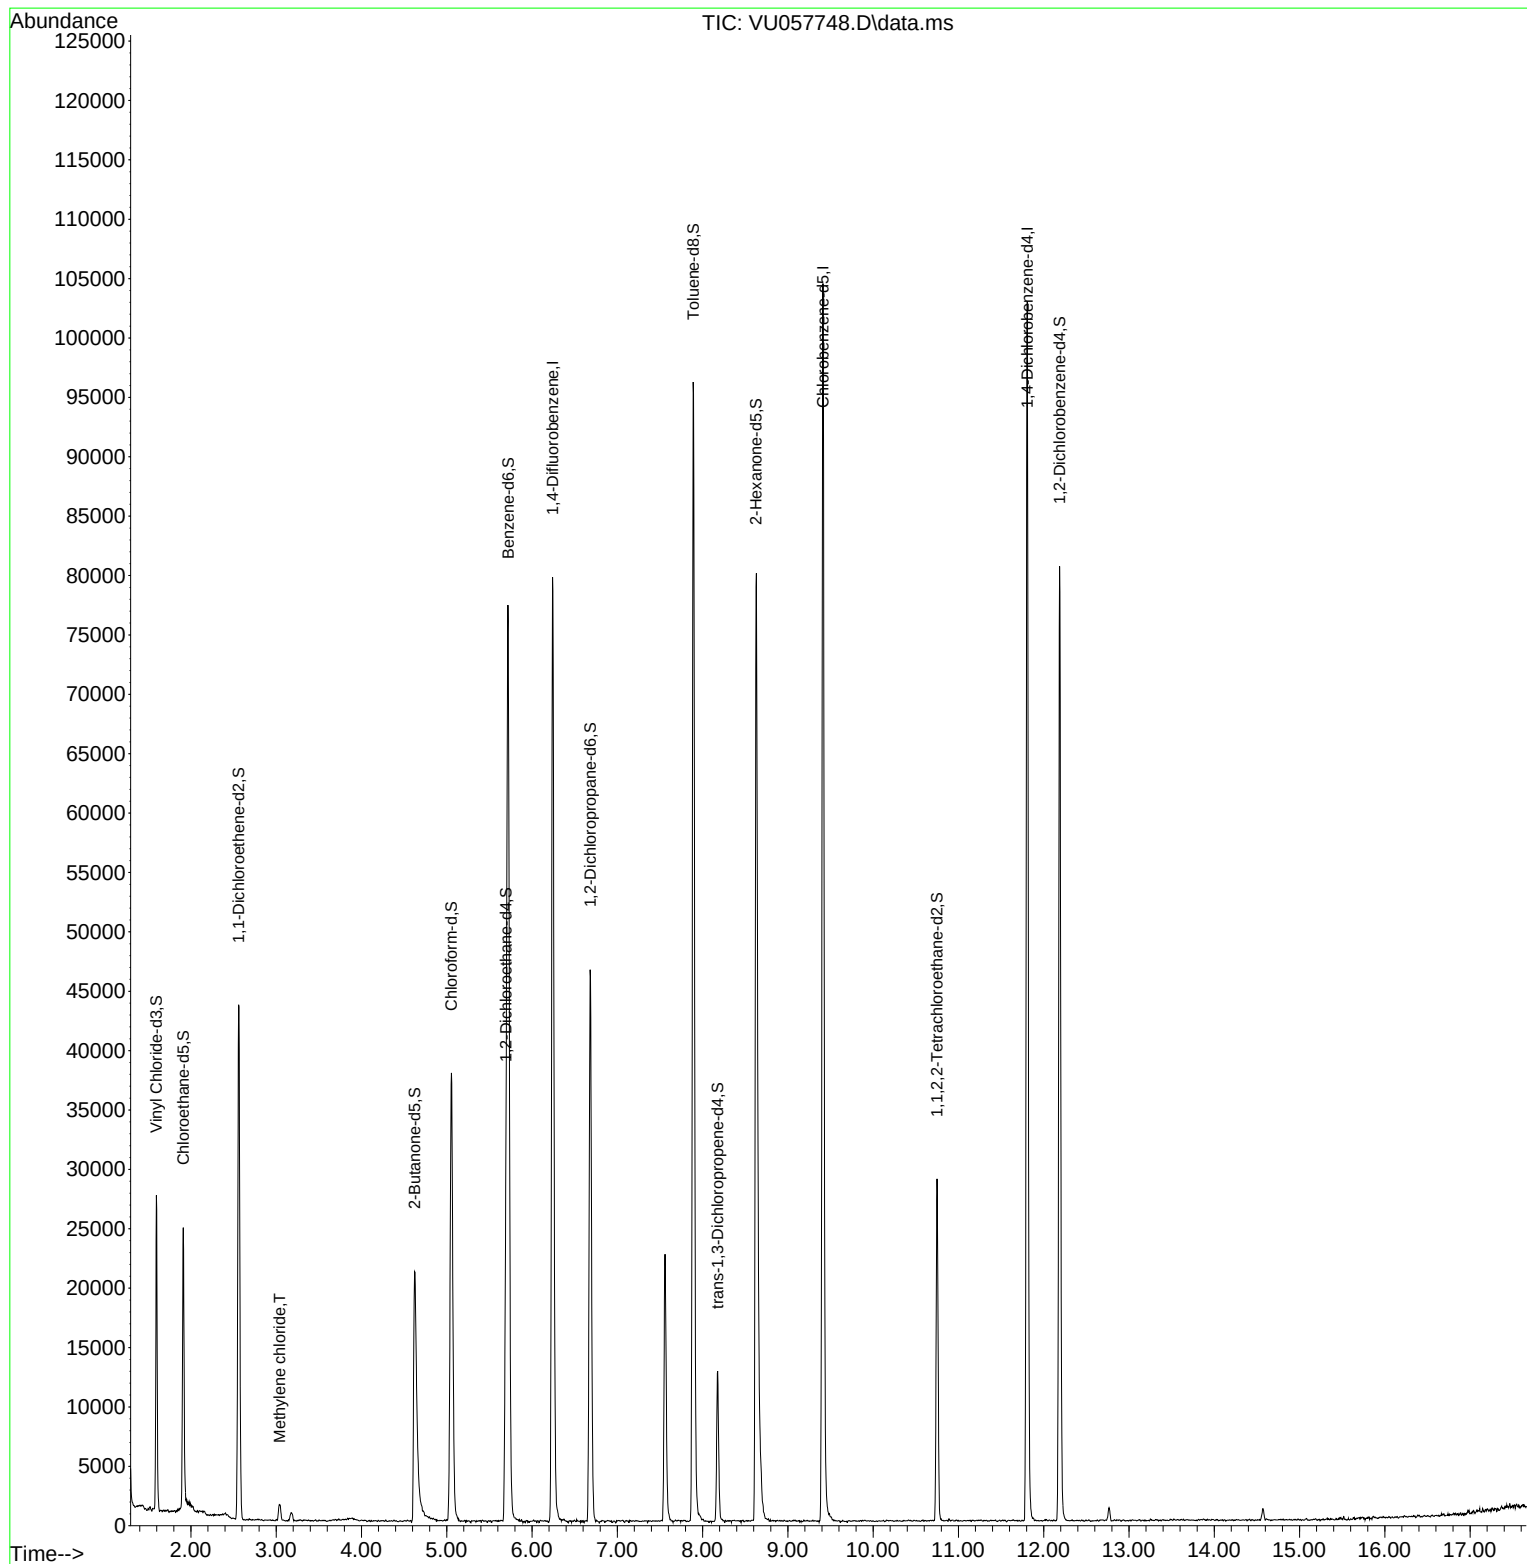

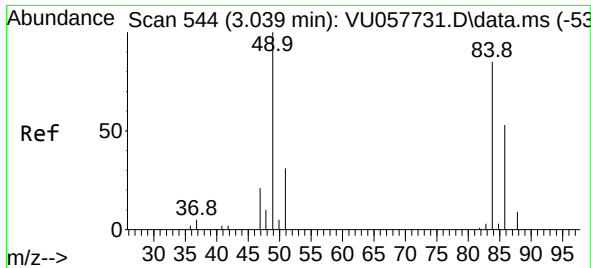

#16  
Methylene chloride  
Concen: 0.146 ug/L  
RT: 3.039 min Scan# 54  
Delta R.T. -0.000 min  
Lab File: VU057748.D  
Acq: 30 Jan 2024 16:58

Instrument :  
MSVOA\_U  
ClientSampleId :  
VHBLK001

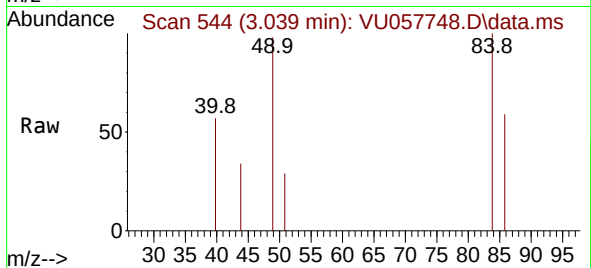

Tgt Ion: 84 Resp: 737

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 84  | 100   |       |       |
| 86  | 58.8  | 43.5  | 80.9  |
| 49  | 98.1  | 82.5  | 153.1 |

