


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013024\
Data File : VU057730.D
Acq On : 30 Jan 2024 08:51
Operator : MD/SY
Sample : BFB114
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB114

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jan 30 22:31:02 2024

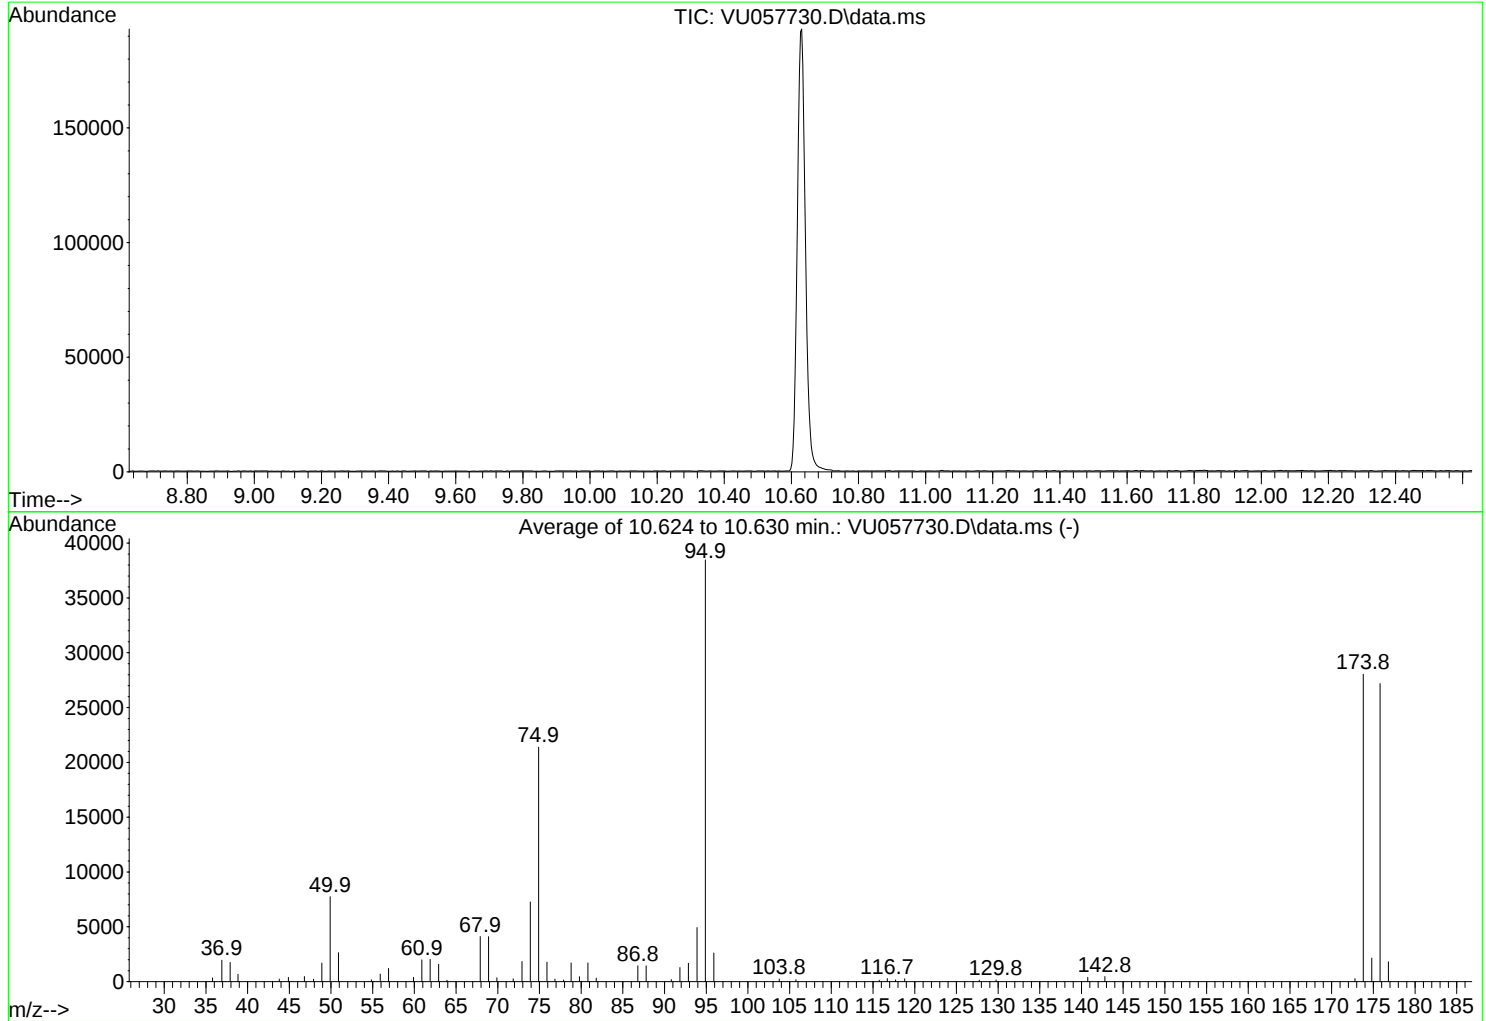

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	7752	PASS
75	95	30	80	55.6	21376	PASS
95	95	100	100	100.0	38475	PASS
96	95	5	9	6.8	2606	PASS
173	174	0.00	2	1.0	275	PASS
174	95	50	120	72.9	28043	PASS
175	174	5	9	7.6	2142	PASS
176	174	95	101	96.9	27187	PASS
177	176	5	9	6.6	1806	PASS

m/z	Abundance
39.80	318.0
43.80	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB114

m/z	Abundance
35.80	321.0
36.90	1865.0
37.90	1651.0
38.80	625.0
39.80	330.0
43.90	329.0
44.90	351.0
46.80	479.0
47.90	212.0
48.90	1634.0
49.90	7434.0
50.90	2496.0
54.90	164.0
55.90	639.0
56.90	1124.0
59.90	348.0
60.90	1903.0
61.90	1897.0
62.90	1536.0
63.90	127.0
67.90	3868.0
68.90	3853.0
69.90	329.0
71.90	250.0
72.90	1673.0
73.90	6905.0
74.90	20176.0
75.90	1719.0
76.80	243.0
77.90	139.0
78.80	1578.0
79.80	395.0
80.80	1606.0
81.80	313.0
86.80	1359.0
87.80	1387.0
90.80	164.0
91.80	1232.0
92.90	1542.0
93.90	4641.0
94.90	36304.0
95.90	2383.0
103.80	224.0
105.80	173.0
115.70	106.0
116.70	256.0
117.70	145.0
118.80	279.0
127.80	129.0
129.80	136.0
140.70	367.0
142.80	408.0
172.80	263.0
173.80	25600.0
174.80	1935.0
175.80	24712.0
176.80	1709.0

Instrument :
MSVOA_U
ClientSampleId :
BFB114

m/z	Abundance
35.80	355.0
36.90	2008.0
37.90	1802.0
38.90	679.0
39.80	301.0
43.80	357.0
44.90	403.0
46.80	493.0
47.90	227.0
48.90	1744.0
49.90	7962.0
50.90	2746.0
54.90	174.0
55.90	715.0
56.90	1228.0
59.90	408.0
60.90	2049.0
61.90	2087.0
62.90	1648.0
63.90	139.0
67.90	4238.0
68.90	4226.0
69.90	371.0
71.90	272.0
72.90	1881.0
73.90	7473.0
74.90	22056.0
75.90	1835.0
76.90	238.0
77.90	153.0
78.80	1755.0
79.80	462.0
80.80	1750.0
81.80	327.0
86.80	1496.0
87.80	1496.0
90.80	195.0
91.90	1322.0
92.80	1703.0
93.90	5107.0
94.90	39576.0
95.90	2683.0
103.80	230.0
105.80	176.0
115.80	128.0
116.70	293.0
117.70	171.0
118.80	279.0
127.80	130.0
129.70	162.0
140.80	403.0
142.80	478.0
172.80	288.0
173.80	28824.0
174.80	2219.0
175.80	28104.0
176.80	1873.0

Instrument :
MSVOA_U
ClientSampleId :
BFB114

m/z	Abundance
35.80	351.0
36.90	2004.0
37.90	1804.0
38.90	709.0
39.80	289.0
43.80	387.0
44.90	429.0
46.80	436.0
47.90	214.0
48.90	1709.0
49.90	7861.0
50.90	2677.0
54.80	151.0
55.90	716.0
56.90	1228.0
59.90	426.0
60.90	2019.0
61.90	2090.0
62.90	1596.0
63.90	144.0
67.90	4262.0
68.90	4234.0
69.90	376.0
71.80	257.0
72.90	1977.0
73.90	7416.0
74.90	21896.0
75.90	1782.0
76.80	218.0
77.90	153.0
78.80	1780.0
79.80	500.0
80.80	1787.0
81.80	317.0
86.80	1494.0
87.80	1458.0
90.80	208.0
91.90	1293.0
92.90	1784.0
93.90	5076.0
94.90	39544.0
95.90	2752.0
103.70	233.0
105.70	172.0
115.80	144.0
116.70	289.0
117.70	166.0
118.80	241.0
127.70	123.0
129.70	176.0
140.80	410.0
142.80	513.0
172.80	275.0
173.80	29704.0
174.80	2273.0
175.80	28744.0
176.80	1837.0

Instrument :
MSVOA_U
ClientSampleId :
BFB114