

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013025\
 Data File : VU063103.D
 Acq On : 30 Jan 2025 17:12
 Operator : MD/SY
 Sample : VU0130WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 31 07:53:41 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM013025WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 31 07:44:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.235	114	161256	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.406	117	135611	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.801	152	61685	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	57302	48.775	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	97.540%
7) Chloroethane-d5	1.895	69	33107	51.589	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.180%
11) 1,1-Dichloroethene-d2	2.554	63	74591	36.342	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.680%
21) 2-Butanone-d5	4.605	46	73972	97.555	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.550%
24) Chloroform-d	5.046	84	97236	44.964	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.920%
26) 1,2-Dichloroethane-d4	5.686	65	63020	51.233	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.460%
32) Benzene-d6	5.711	84	226440	56.066	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	112.140%
36) 1,2-Dichloropropane-d6	6.676	67	70850	53.610	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.220%
41) Toluene-d8	7.885	98	176681	48.318	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.640%
43) trans-1,3-Dichloroprop...	8.171	79	29724	48.888	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.780%
47) 2-Hexanone-d5	8.621	63	54374	95.992	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.990%
56) 1,1,2,2-Tetrachloroeth...	10.743	84	97187	50.140	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.280%
66) 1,2-Dichlorobenzene-d4	12.184	152	63366	53.338	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.680%
Target Compounds						
37) 1,2-Dichloropropane	6.676	63	6611	5.527	ug/L	Qvalue # 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013025\
Data File : VU063103.D
Acq On : 30 Jan 2025 17:12
Operator : MD/SY
Sample : VU0130WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jan 31 07:53:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM013025WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 07:44:25 2025
Response via : Initial Calibration

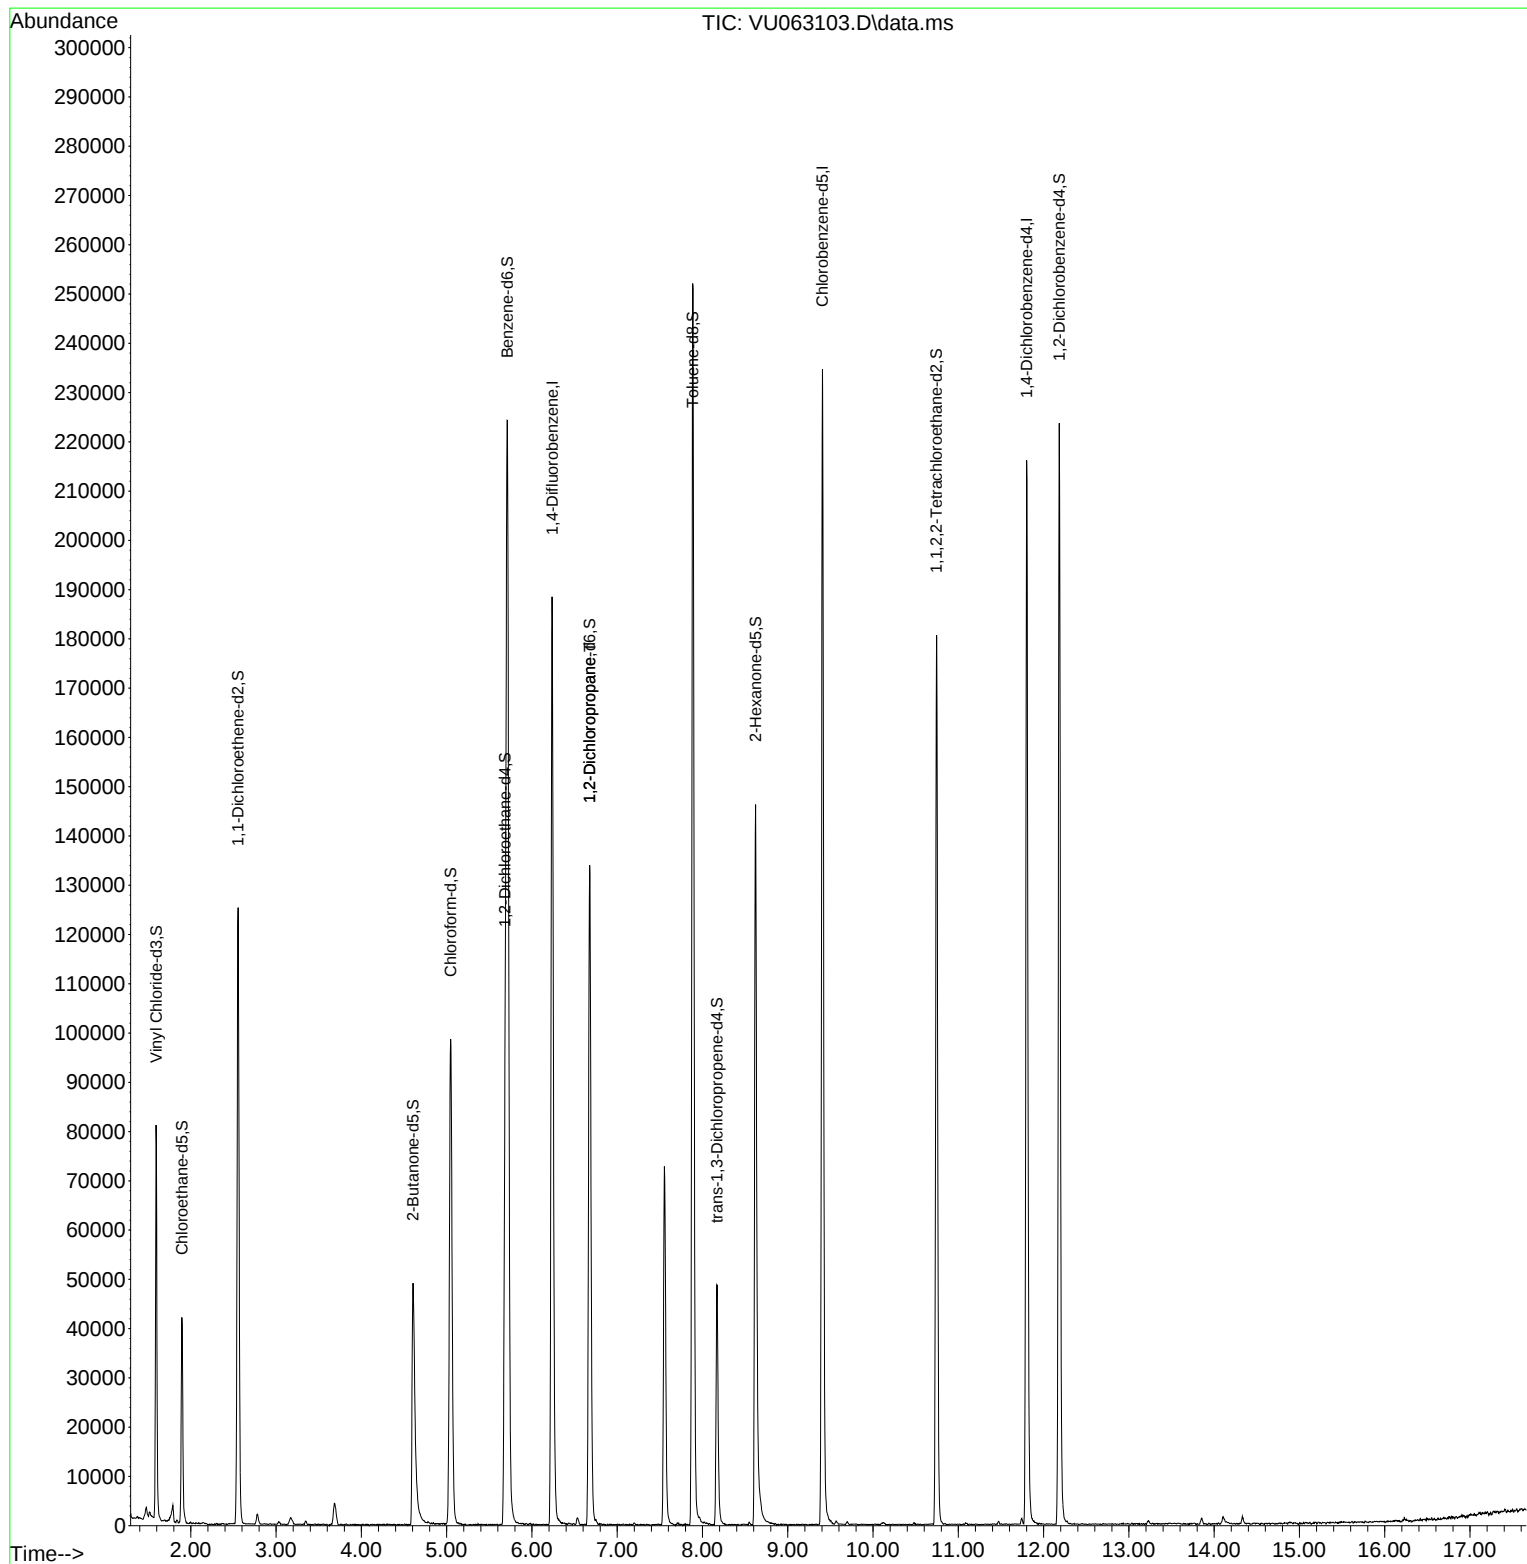

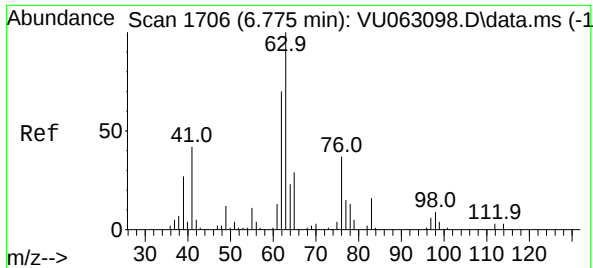

#37
1,2-Dichloropropane
Concen: 5.527 ug/L
RT: 6.676 min Scan# 1
Delta R.T. -0.100 min
Lab File: VU063103.D
Acq: 30 Jan 2025 17:12

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 63 Resp: 6611
Ion Ratio Lower Upper
63 100
112 0.0 2.6 4.0#

