

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013025\
 Data File : VU063106.D
 Acq On : 30 Jan 2025 18:24
 Operator : MD/SY
 Sample : Q1148-05
 Misc : 10.00g/10.0mL/100uL5.0mL/MSVOA_U/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 31 07:54:37 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM013025WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 31 07:44:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.235	114	141402	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	148221	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	75224	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	51045	49.550	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	99.100%
7) Chloroethane-d5	1.866	69	19888	35.342	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	70.680%
11) 1,1-Dichloroethene-d2	2.531	63	60273	33.490	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.980%
21) 2-Butanone-d5	4.618	46	71992	108.274	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.270%
24) Chloroform-d	5.046	84	95004	50.100	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.200%
26) 1,2-Dichloroethane-d4	5.686	65	52116	48.317	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.640%
32) Benzene-d6	5.708	84	180170	40.815	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.620%
36) 1,2-Dichloropropane-d6	6.676	67	57634	39.899	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	79.800%
41) Toluene-d8	7.885	98	165225	41.341	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.680%
43) trans-1,3-Dichloroprop...	8.171	79	28535	42.939	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.880%
47) 2-Hexanone-d5	8.631	63	69266	111.879	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	111.880%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	103248	48.735	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.460%
66) 1,2-Dichlorobenzene-d4	12.184	152	68836	47.514	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.020%
Target Compounds						
					Qvalue	
13) Acetone	2.625	43	151839	365.170	ug/L	98
15) Methyl Acetate	2.943	43	14304	14.362	ug/L	96
16) Methylene chloride	3.020	84	108576	97.828	ug/L	98
17) trans-1,2-Dichloroethene	3.329	96	48063	48.770	ug/L	99
18) Methyl tert-butyl Ether	3.351	73	626949	206.034	ug/L	100
20) cis-1,2-Dichloroethene	4.644	96	130104	116.273	ug/L	97
22) 2-Butanone	4.698	43	75688	111.446	ug/L	91
27) 1,2-Dichloroethane	5.776	62	101326	76.055	ug/L	97
31) Carbon tetrachloride	5.505	117	231712	150.256	ug/L	100
33) Benzene	5.753	78	709777	149.052	ug/L	100
34) Trichloroethene	6.528	95	190113	147.567	ug/L	97
37) 1,2-Dichloropropane	6.676	63	5754	4.401	ug/L #	90
38) Bromodichloromethane	7.094	83	244436	157.890	ug/L	98
39) cis-1,3-Dichloropropene	7.595	75	93858	48.060	ug/L	100
40) 4-Methyl-2-pentanone	7.785	43	334533	214.252	ug/L	99
42) Toluene	7.956	91	652327	129.897	ug/L	99
45) 1,1,2-Trichloroethane	8.390	97	172694	138.773	ug/L	97
46) Tetrachloroethene	8.541	164	68272	74.999	ug/L	99
48) 2-Hexanone	8.679	43	241376	202.911	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013025\
 Data File : VU063106.D
 Acq On : 30 Jan 2025 18:24
 Operator : MD/SY
 Sample : Q1148-05
 Misc : 10.00g/10.0mL/100uL5.0mL/MSVOA_U/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 31 07:54:37 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM013025WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 31 07:44:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


49) Dibromochloromethane	8.801	129	98592	78.186	ug/L	99
50) 1,2-Dibromoethane	8.911	107	233403	173.637	ug/L	97
52) Ethylbenzene	9.560	91	786012	144.616	ug/L	99
53) m,p-Xylene	9.682	106	197449	97.297	ug/L	99
54) o-Xylene	10.091	106	184992	90.462	ug/L	97
55) Styrene	10.107	104	602680	173.433	ug/L	98
57) 1,1,2,2-Tetrachloroethane	10.772	83	318699	145.050	ug/L	100
59) Bromoform	10.283	173	111534	110.707	ug/L	100
60) 1,2,3-Trichloropropane	10.814	75	138728	86.508	ug/L	98
64) 1,3-Dichlorobenzene	11.737	146	66979	27.237	ug/L	98
65) 1,4-Dichlorobenzene	11.827	146	273147	107.189	ug/L	99
67) 1,2-Dichlorobenzene	12.203	146	307210	126.634	ug/L	99
70) 1,2,4-trichlorobenzene	13.840	180	1488	1.045	ug/L	93
71) Naphthalene	14.078	128	202019	45.739	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013025\
Data File : VU063106.D
Acq On : 30 Jan 2025 18:24
Operator : MD/SY
Sample : Q1148-05
Misc : 10.00g/10.0mL/100uL5.0mL/MSVOA_U/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jan 31 07:54:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM013025WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 07:44:25 2025
Response via : Initial Calibration




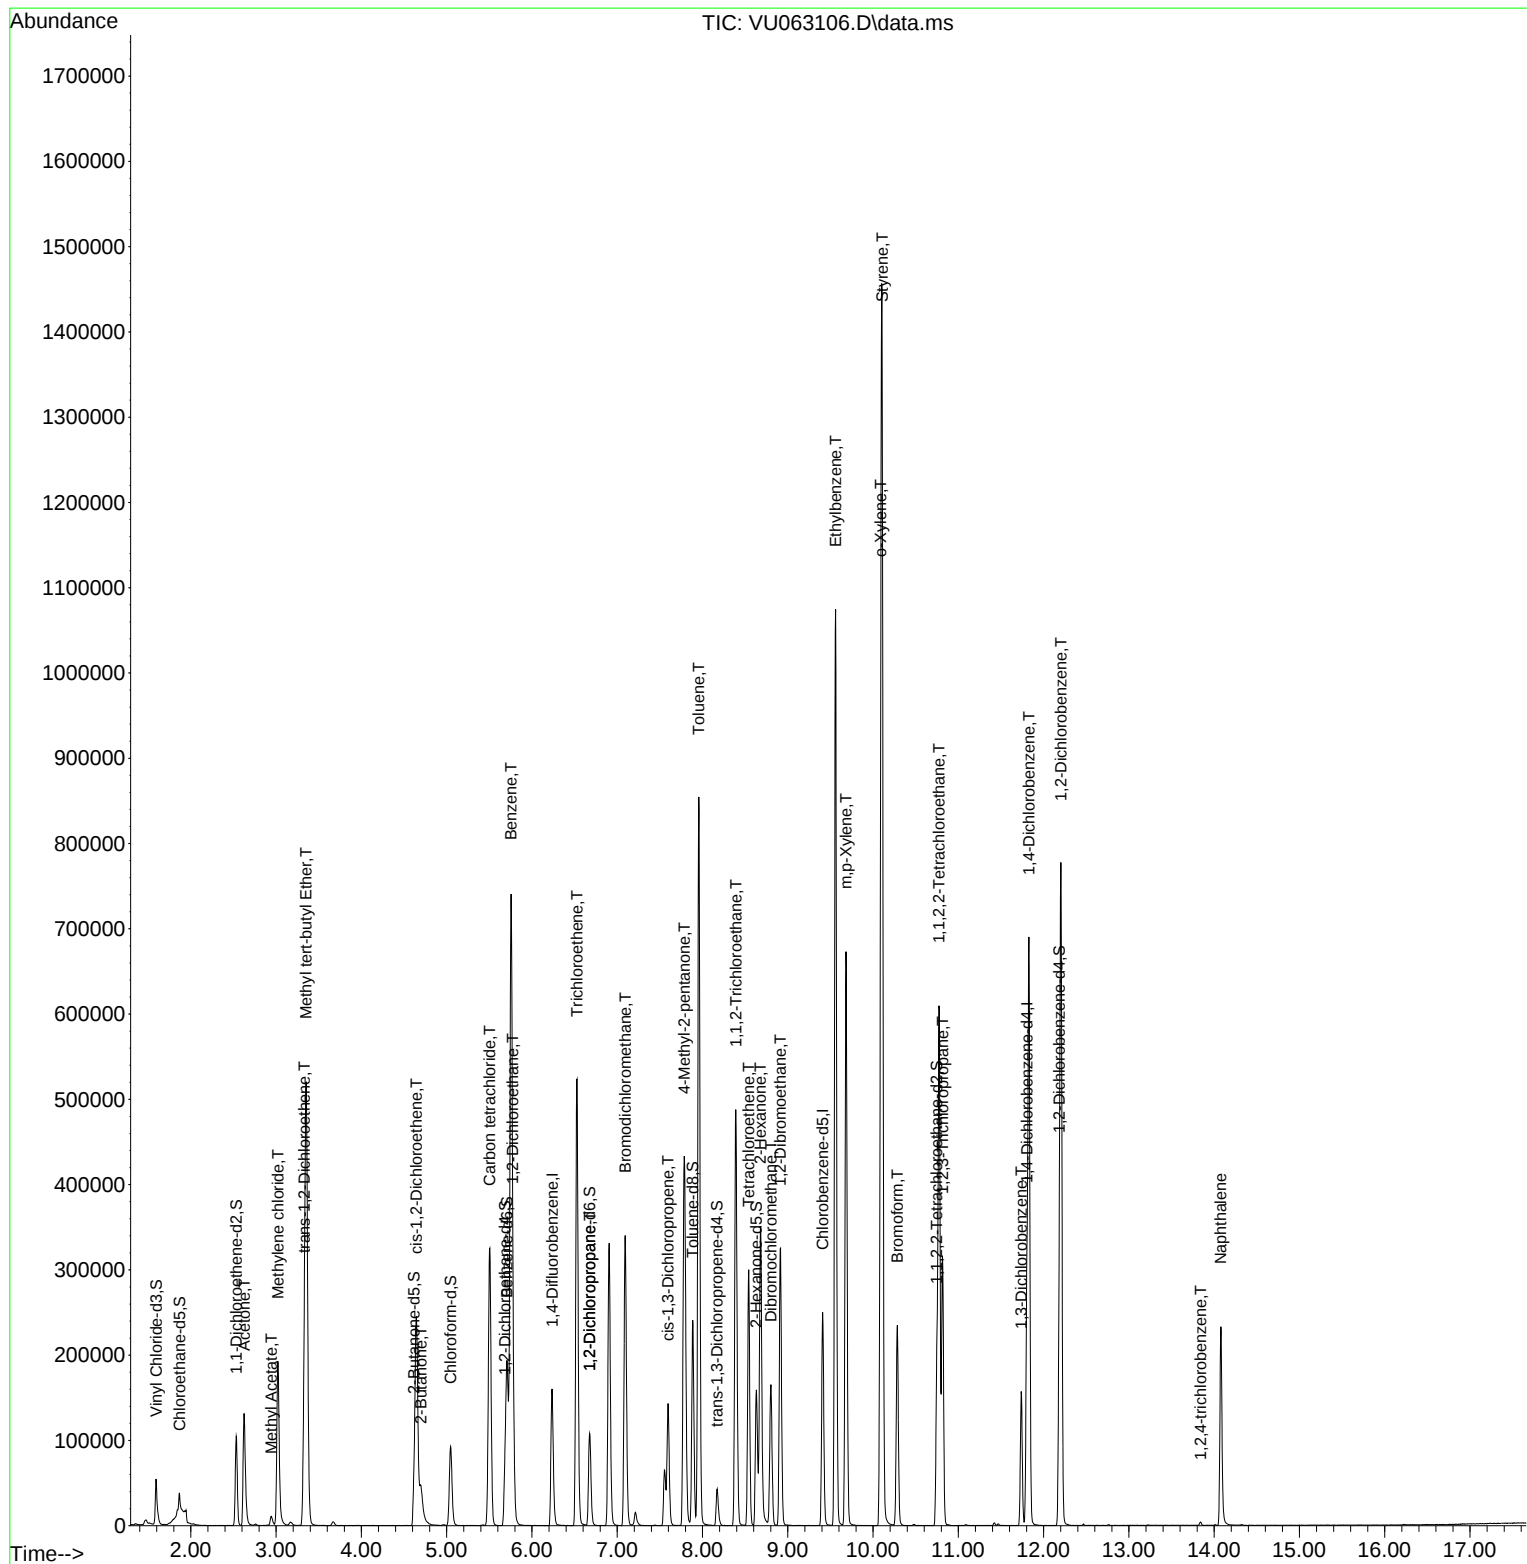


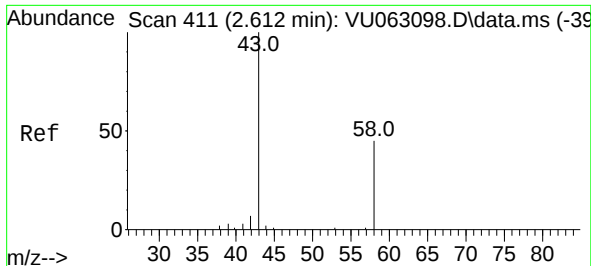

#13
Acetone
Concen: 365.170 ug/L
RT: 2.625 min Scan# 411
Delta R.T. 0.013 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 43 Resp: 151839
Ion Ratio Lower Upper
43 100
58 43.0 0.0 88.8

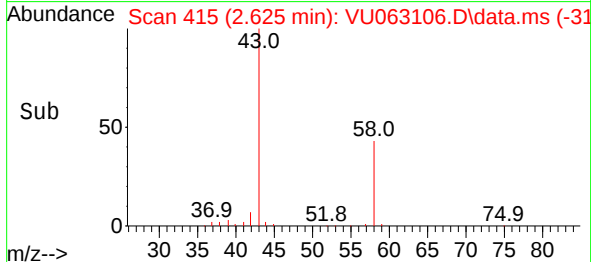

#15
Methyl Acetate
Concen: 14.362 ug/L
RT: 2.943 min Scan# 514
Delta R.T. 0.010 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24


Tgt Ion: 43 Resp: 14304
Ion Ratio Lower Upper
43 100
74 29.0 25.0 37.6

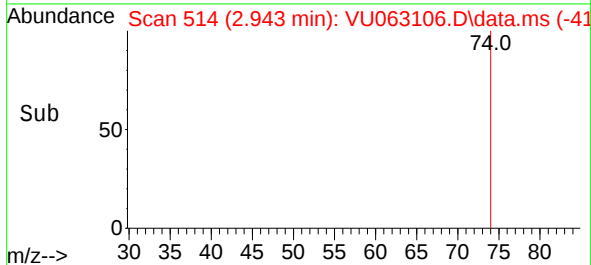



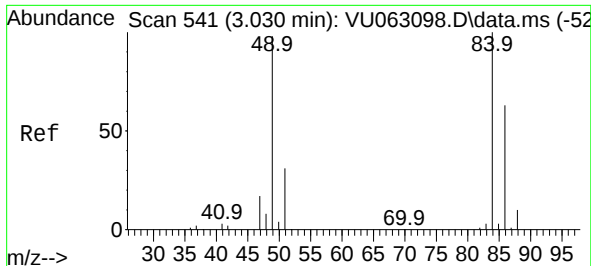


#16
Methylene chloride
Concen: 97.828 ug/L
RT: 3.020 min Scan# 541
Delta R.T. -0.010 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24


Instrument :
MSVOA_U
ClientSampleId :





Tgt Ion: 84 Resp: 108576
Ion Ratio Lower Upper
84 100
86 63.2 44.2 82.0
49 100.7 68.4 127.0

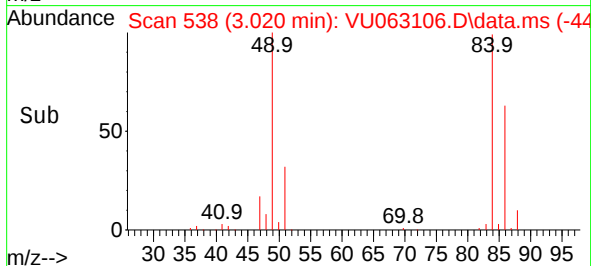


#17
trans-1,2-Dichloroethene
Concen: 48.770 ug/L
RT: 3.329 min Scan# 634
Delta R.T. -0.010 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24



Tgt Ion: 96 Resp: 48063
Ion Ratio Lower Upper
96 100
61 129.1 91.1 169.3
98 64.7 44.0 81.8

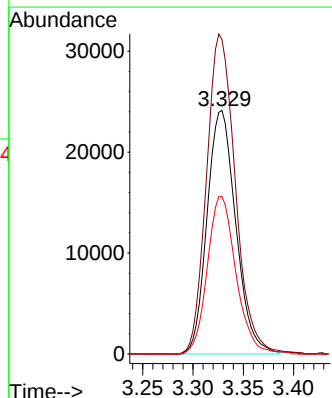

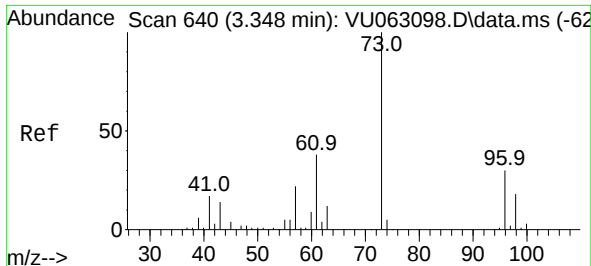

#18

Methyl tert-butyl Ether

Concen: 206.034 ug/L

RT: 3.351 min Scan# 640

Delta R.T. 0.003 min

Lab File: VU063106.D

Acq: 30 Jan 2025 18:24

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion: 73 Resp: 626949

Ion Ratio Lower Upper

73 100

43 14.3 11.4 17.2

57 21.6 17.2 25.8

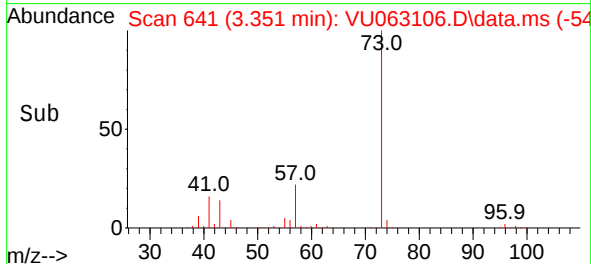

#20

cis-1,2-Dichloroethene

Concen: 116.273 ug/L

RT: 4.644 min Scan# 1043

Delta R.T. -0.006 min

Lab File: VU063106.D

Acq: 30 Jan 2025 18:24




Tgt Ion: 96 Resp: 130104


Ion Ratio Lower Upper

96 100

61 118.5 84.4 156.8

98 62.3 46.0 85.4







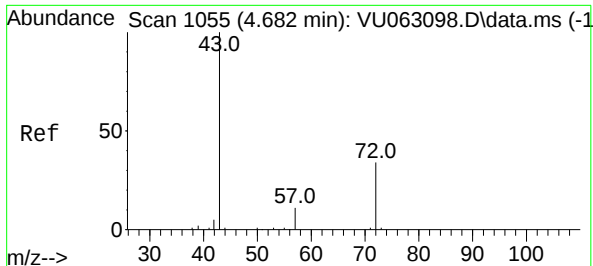

#22
2-Butanone
Concen: 111.446 ug/L
RT: 4.698 min Scan# 1060
Delta R.T. 0.016 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 43 Resp: 75688
Ion Ratio Lower Upper
43 100
72 30.1 17.5 52.6

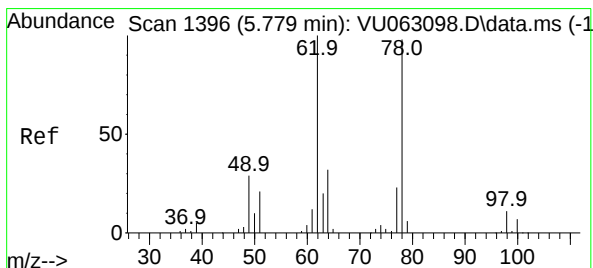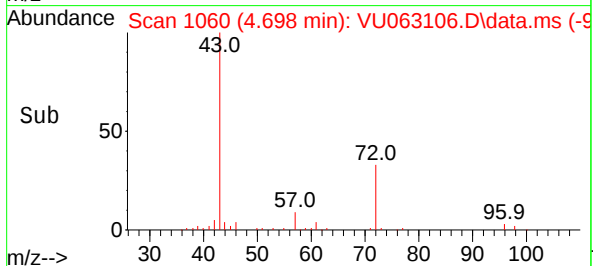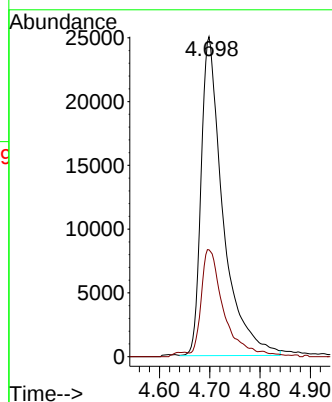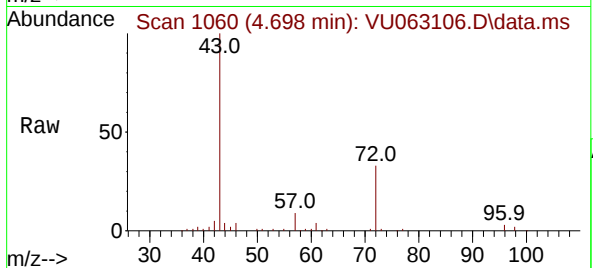

#27
1,2-Dichloroethane
Concen: 76.055 ug/L
RT: 5.776 min Scan# 1395
Delta R.T. -0.003 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24

Tgt Ion: 62 Resp: 101326
Ion Ratio Lower Upper
62 100
98 9.5 8.5 12.7


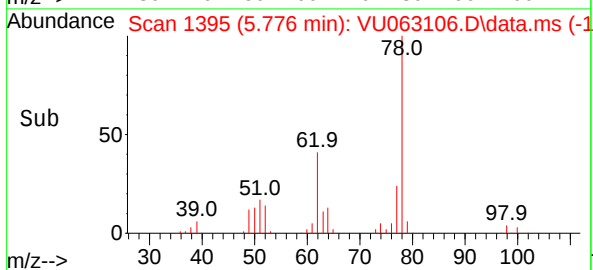
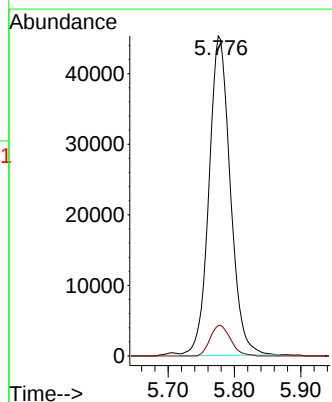
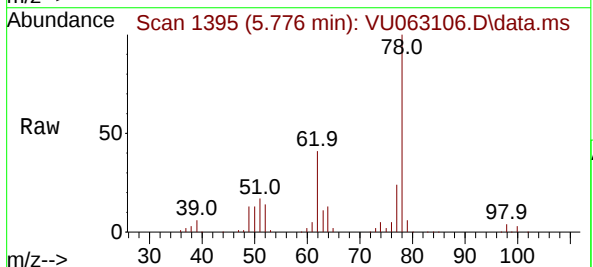


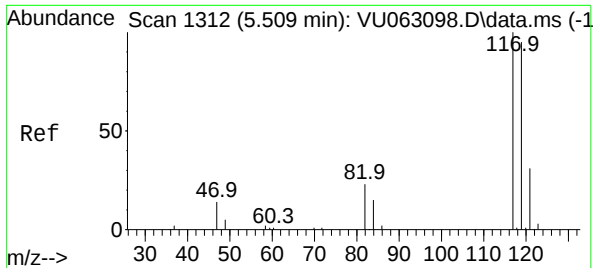

#31
Carbon tetrachloride
Concen: 150.256 ug/L
RT: 5.505 min Scan# 1312
Delta R.T. -0.003 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:117 Resp: 231712
Ion Ratio Lower Upper
117 100
119 97.0 77.7 116.5

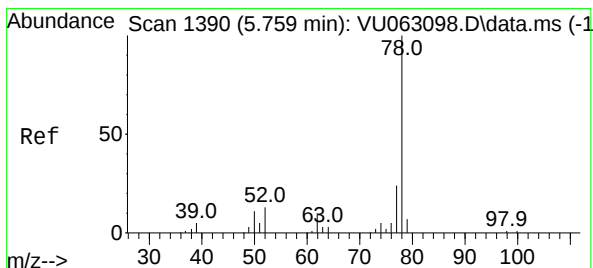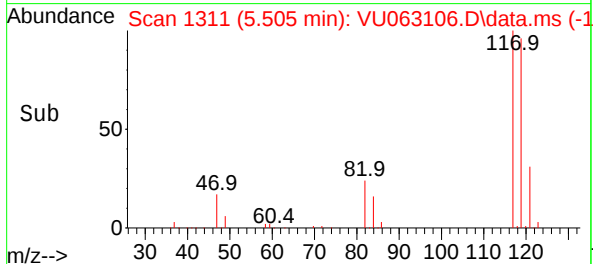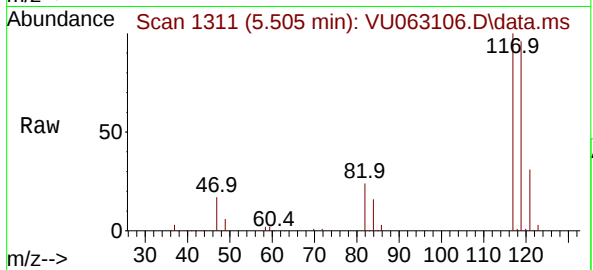

#33
Benzene
Concen: 149.052 ug/L
RT: 5.753 min Scan# 1388
Delta R.T. -0.006 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24

Tgt Ion: 78 Resp: 709777

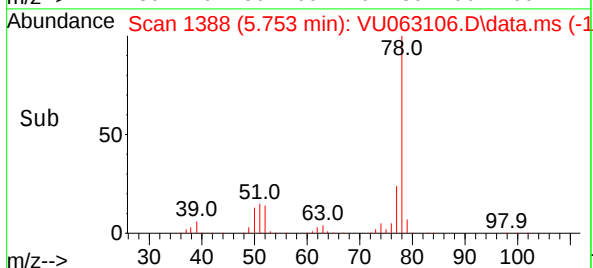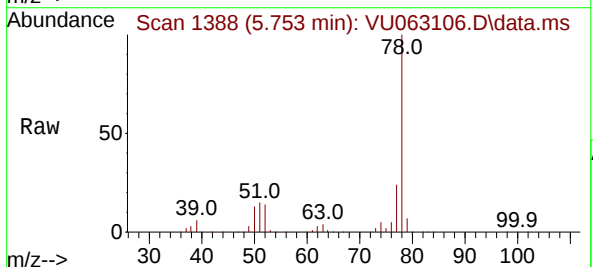

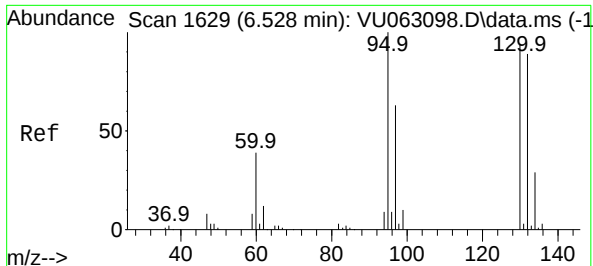

#34

Trichloroethene

Concen: 147.567 ug/L

RT: 6.528 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063106.D

Acq: 30 Jan 2025 18:24

Instrument :

MSVOA_U

ClientSampleId :

Tgt Ion: 95 Resp: 190113





Ion Ratio Lower Upper

95 100

97 64.1 44.3 82.3

132 92.7 62.4 116.0

130 97.6 65.9 122.3

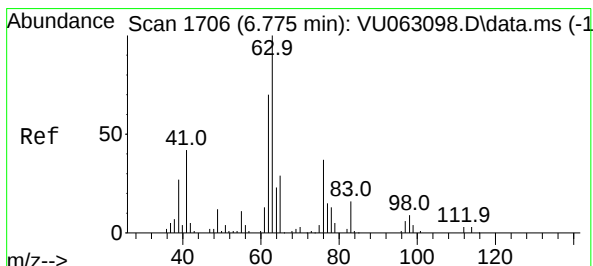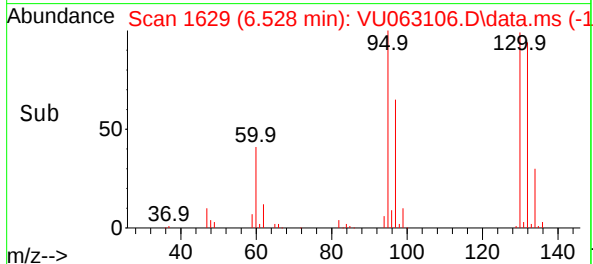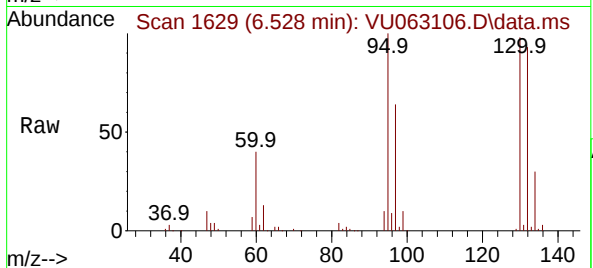

#37

1,2-Dichloropropane

Concen: 4.401 ug/L

RT: 6.676 min Scan# 1675

Delta R.T. -0.100 min

Lab File: VU063106.D




Acq: 30 Jan 2025 18:24


Tgt Ion: 63 Resp: 5754

Ion Ratio Lower Upper

63 100

112 0.0 2.6 4.0#


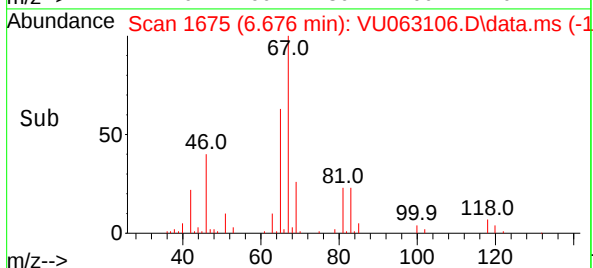
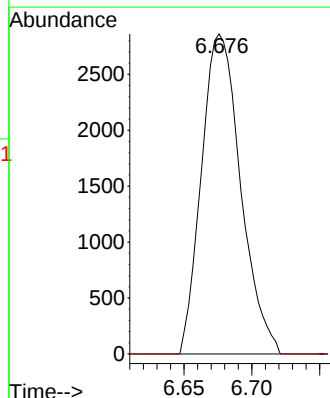
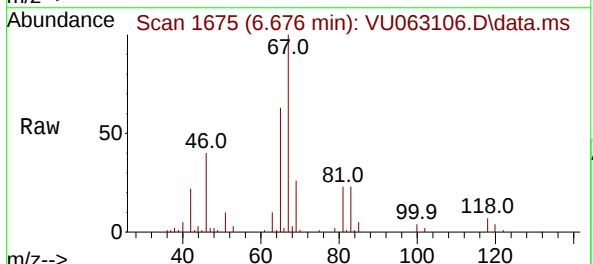


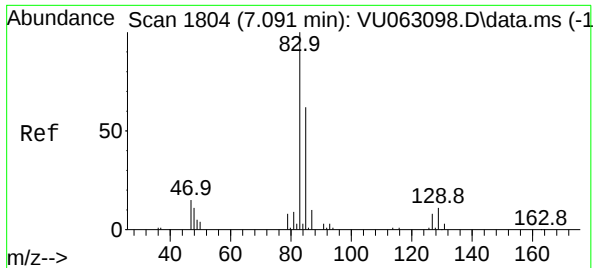

#38
Bromodichloromethane
Concen: 157.890 ug/L
RT: 7.094 min Scan# 1805
Delta R.T. 0.003 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 83 Resp: 244436
Ion Ratio Lower Upper
83 100
85 63.6 43.5 80.9
127 8.7 6.5 9.7

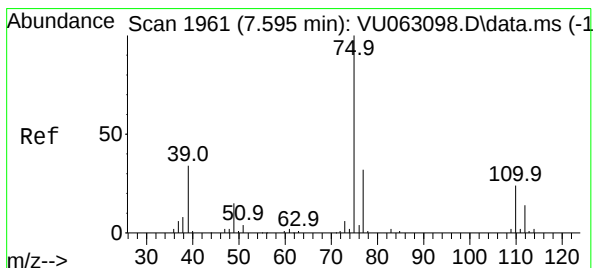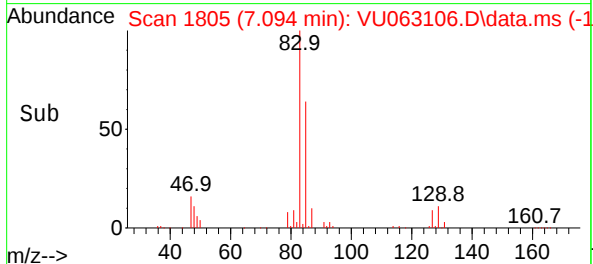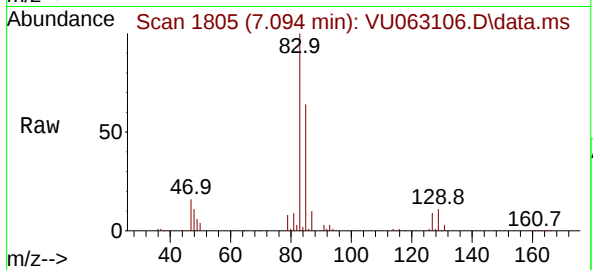

#39
cis-1,3-Dichloropropene
Concen: 48.060 ug/L
RT: 7.595 min Scan# 1961
Delta R.T. 0.000 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24

Tgt Ion: 75 Resp: 93858
Ion Ratio Lower Upper
75 100
77 32.0 22.5 41.9


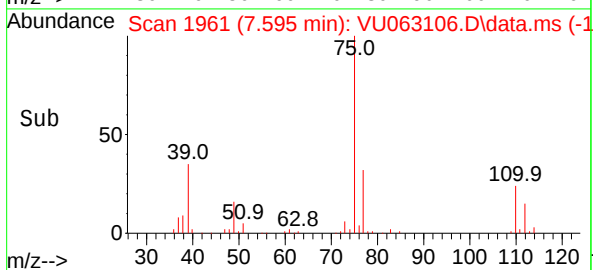

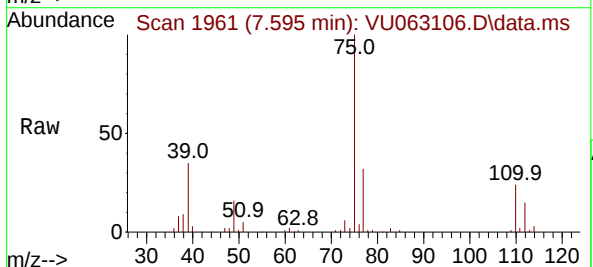


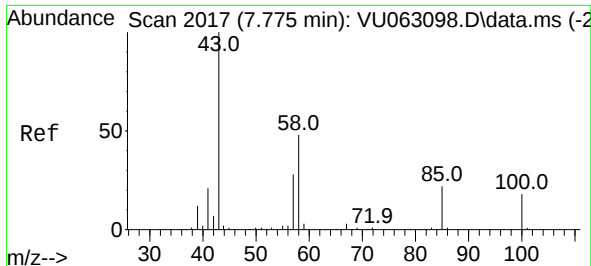

#40
4-Methyl-2-pentanone
Concen: 214.252 ug/L
RT: 7.785 min Scan# 2017
Delta R.T. 0.010 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 43 Resp: 334533
Ion Ratio Lower Upper
43 100
58 46.2 37.5 56.3
100 17.6 14.3 21.5

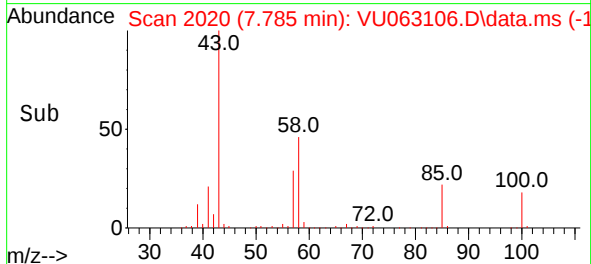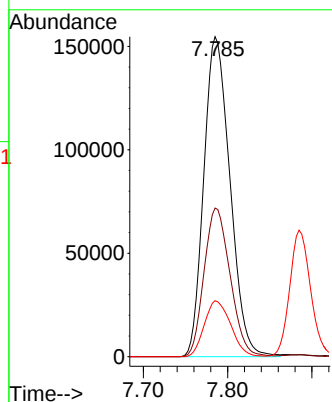

#42
Toluene
Concen: 129.897 ug/L
RT: 7.956 min Scan# 2073
Delta R.T. 0.000 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24

Tgt Ion: 91 Resp: 652327
Ion Ratio Lower Upper
91 100
92 57.2 39.3 73.1

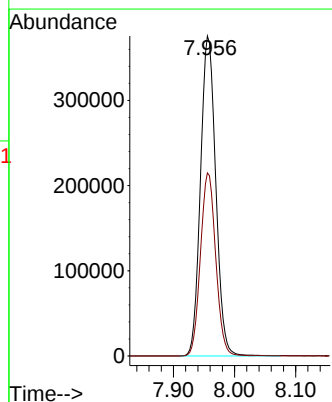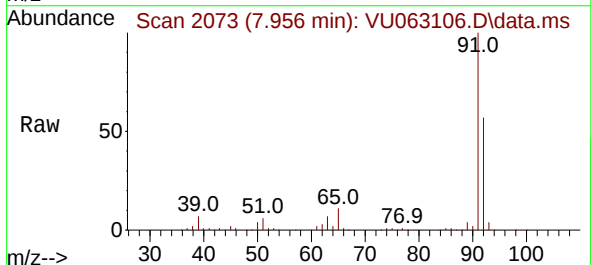



#45

1,1,2-Trichloroethane

Concen: 138.773 ug/L

RT: 8.390 min Scan# 2207

Delta R.T. 0.003 min

Lab File: VU063106.D

Acq: 30 Jan 2025 18:24

Instrument :

MSVOA_U

ClientSampleId :

Tgt Ion: 97 Resp: 172694





Ion Ratio Lower Upper

97 100

99 61.9 44.2 82.2

83 87.9 64.0 118.8

85 55.9 41.4 76.8

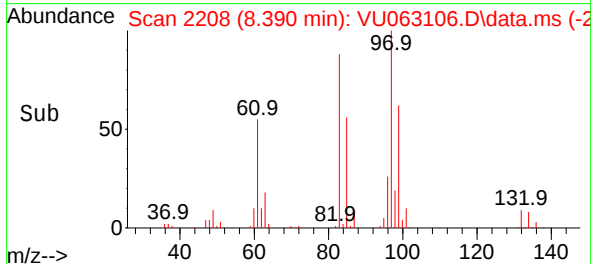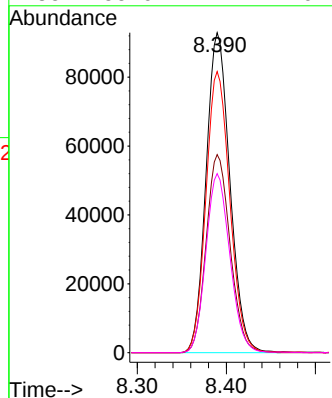

#46

Tetrachloroethene

Concen: 74.999 ug/L

RT: 8.541 min Scan# 2255

Delta R.T. 0.000 min

Lab File: VU063106.D

Acq: 30 Jan 2025 18:24

Tgt Ion:164 Resp: 68272




Ion Ratio Lower Upper


164 100

129 97.3 69.9 129.7

131 95.4 66.3 123.1

166 127.5 89.7 166.7

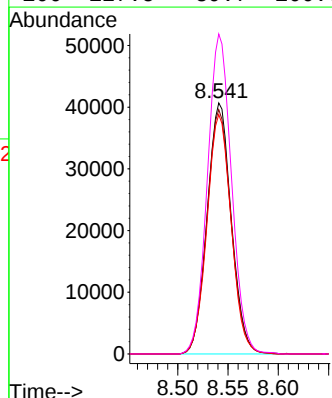




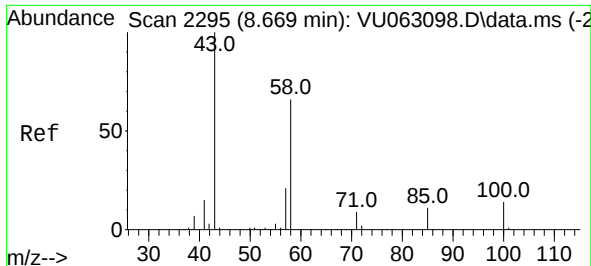


#48
2-Hexanone
Concen: 202.911 ug/L
RT: 8.679 min Scan# 2295
Delta R.T. 0.010 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 43 Resp: 241376




Ion	Ratio	Lower	Upper
43	100		
58	66.0	52.6	78.8
57	22.1	17.9	26.9
100	13.8	10.6	16.0

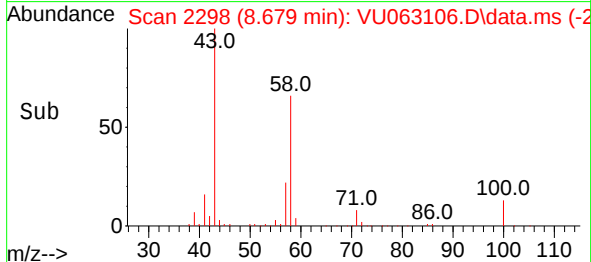


#49
Dibromochloromethane
Concen: 78.186 ug/L
RT: 8.801 min Scan# 2336
Delta R.T. 0.003 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24

Tgt Ion: 129 Resp: 98592

Ion	Ratio	Lower	Upper
129	100		
127	78.4	54.1	100.5




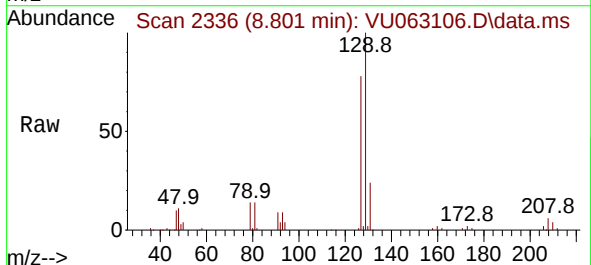


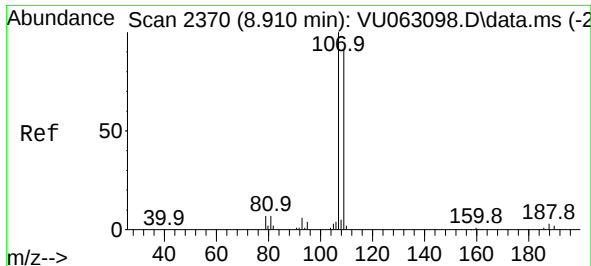

#50
1,2-Dibromoethane
Concen: 173.637 ug/L
RT: 8.911 min Scan# 2370
Delta R.T. 0.000 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:107 Resp: 233403
Ion Ratio Lower Upper
107 100
109 93.9 63.7 118.3
188 3.2 2.7 4.1

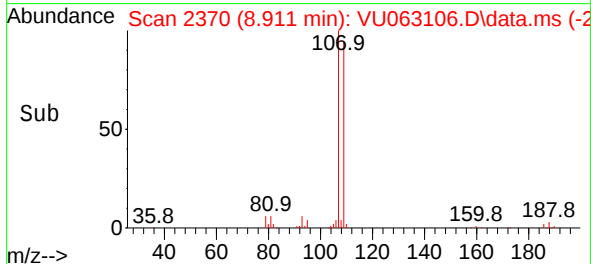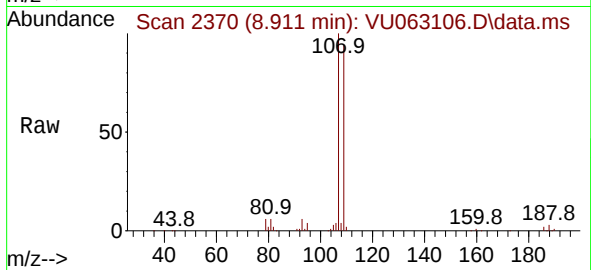

#52
Ethylbenzene
Concen: 144.616 ug/L
RT: 9.560 min Scan# 2572
Delta R.T. 0.000 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24

Tgt Ion: 91 Resp: 786012
Ion Ratio Lower Upper
91 100
106 30.6 22.0 40.8



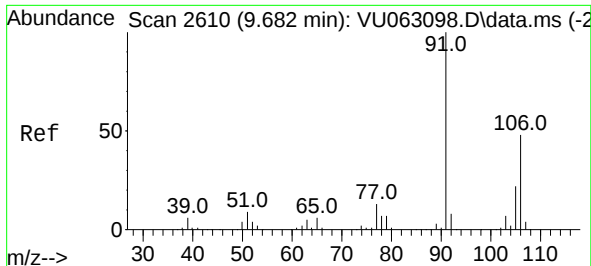

#53

m,p-Xylene

Concen: 97.297 ug/L

RT: 9.682 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063106.D

Acq: 30 Jan 2025 18:24

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion:106 Resp: 197449

Ion Ratio Lower Upper

106 100

91 206.8 145.5 270.1

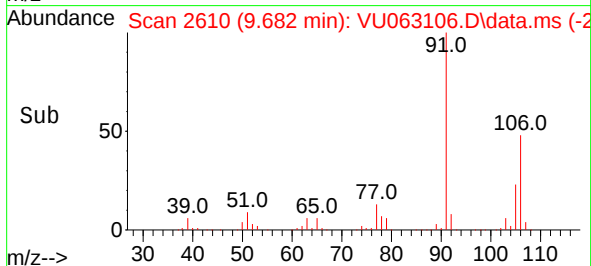

#54

o-Xylene

Concen: 90.462 ug/L

RT: 10.091 min Scan# 2737

Delta R.T. 0.003 min

Lab File: VU063106.D




Acq: 30 Jan 2025 18:24


Tgt Ion:106 Resp: 184992

Ion Ratio Lower Upper

106 100

91 213.1 152.8 283.8

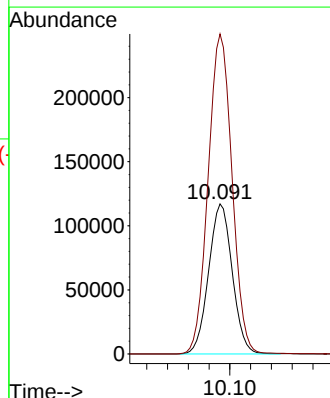

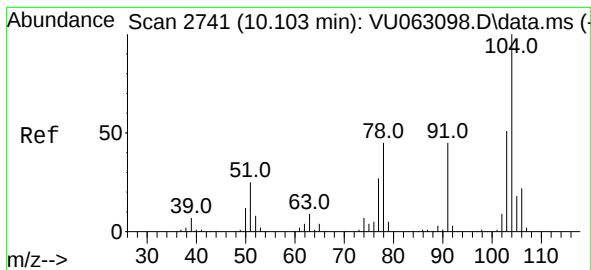

#55

Styrene

Concen: 173.433 ug/L

RT: 10.107 min Scan# 21

Delta R.T. 0.003 min

Lab File: VU063106.D

Acq: 30 Jan 2025 18:24

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion:104 Resp: 602680

Ion Ratio Lower Upper

104 100

78 43.4 31.4 58.2

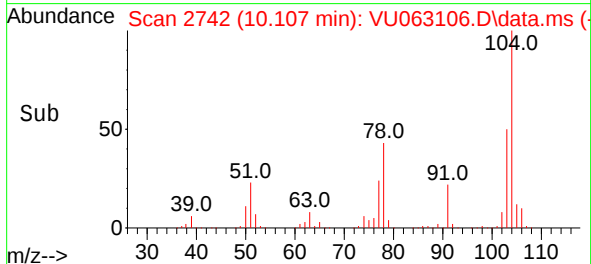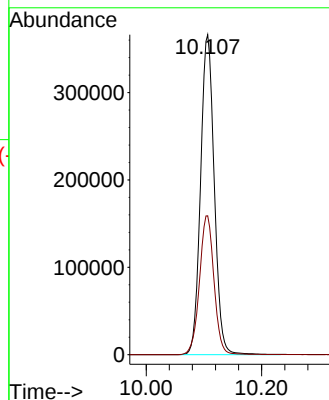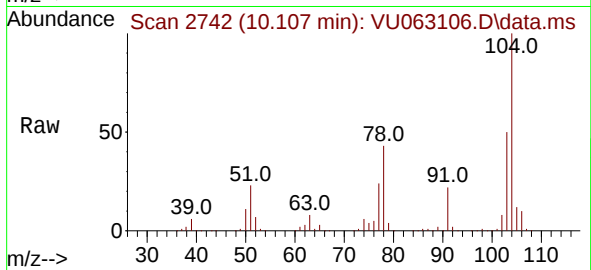

#57

1,1,2,2-Tetrachloroethane

Concen: 145.050 ug/L

RT: 10.772 min Scan# 2949

Delta R.T. 0.003 min

Lab File: VU063106.D

Acq: 30 Jan 2025 18:24




Tgt Ion: 83 Resp: 318699


Ion Ratio Lower Upper

83 100

85 64.1 44.9 83.3

131 9.1 7.1 10.7



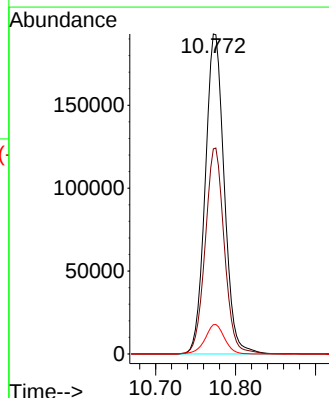





#59
Bromoform
Concen: 110.707 ug/L
RT: 10.283 min Scan# 21
Delta R.T. 0.003 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:173 Resp: 111534
Ion Ratio Lower Upper
173 100
175 48.4 38.6 57.8
254 9.5 7.6 11.4

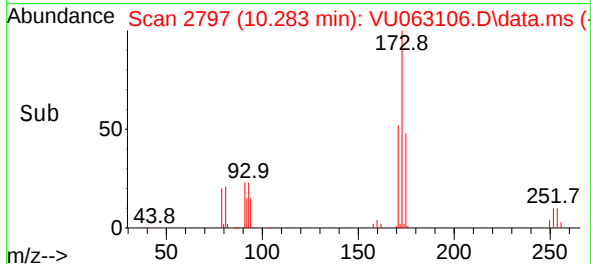

#60
1,2,3-Trichloropropane
Concen: 86.508 ug/L
RT: 10.814 min Scan# 2962
Delta R.T. 0.003 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24

Tgt Ion: 75 Resp: 138728
Ion Ratio Lower Upper
75 100
77 31.6 25.6 38.4
110 37.7 29.1 43.7

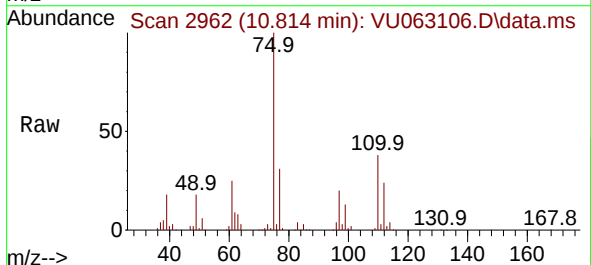



#64

1,3-Dichlorobenzene

Concen: 27.237 ug/L

RT: 11.737 min Scan# 3249

Delta R.T. 0.003 min


Lab File: VU063106.D

Acq: 30 Jan 2025 18:24

Instrument :

MSVOA_U

ClientSampleId :

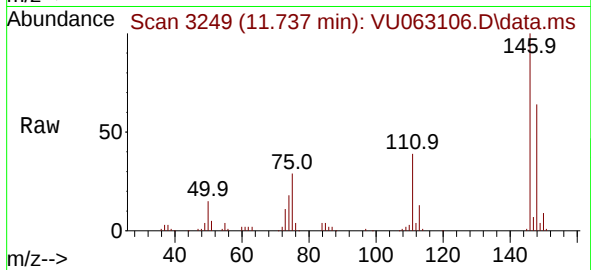




Tgt Ion:146 Resp: 66979

Ion Ratio Lower Upper

146 100

111 39.2 28.1 52.3

148 64.1 43.9 81.5

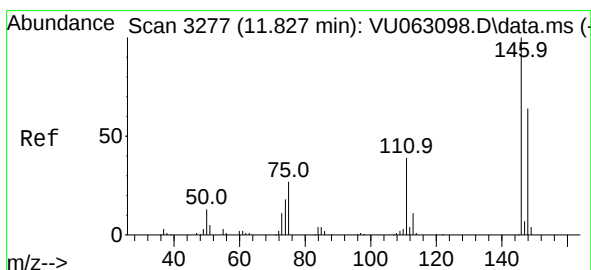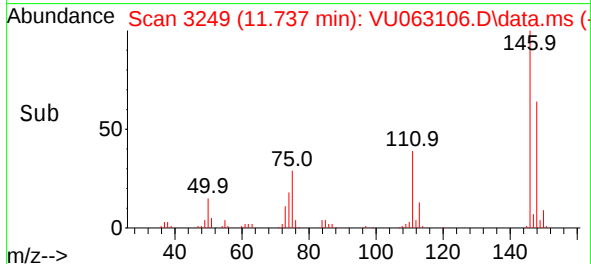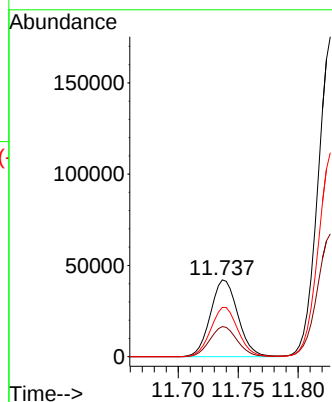

#65

1,4-Dichlorobenzene

Concen: 107.189 ug/L

RT: 11.827 min Scan# 3277

Delta R.T. 0.000 min

Lab File: VU063106.D

Acq: 30 Jan 2025 18:24




Tgt Ion:146 Resp: 273147


Ion Ratio Lower Upper

146 100

111 38.4 27.2 50.6

148 63.7 44.9 83.5



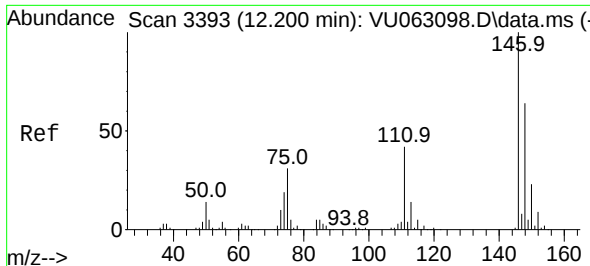

#67

1,2-Dichlorobenzene

Concen: 126.634 ug/L

RT: 12.203 min Scan# 3393

Delta R.T. 0.003 min

Lab File: VU063106.D

Acq: 30 Jan 2025 18:24

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion:146 Resp: 307210

Ion Ratio Lower Upper

146 100

111 42.1 33.6 50.4

148 64.9 51.2 76.8

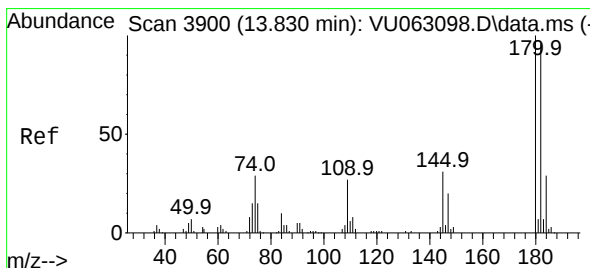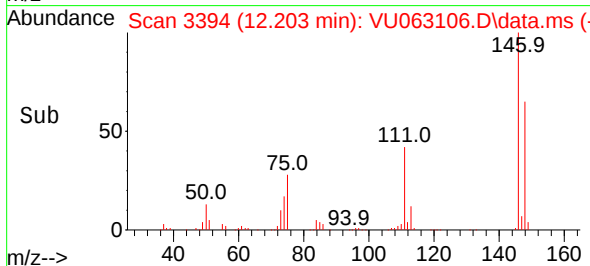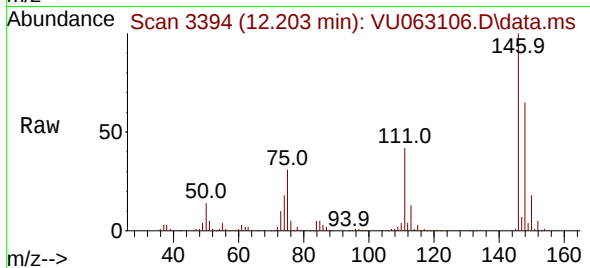

#70

1,2,4-trichlorobenzene

Concen: 1.045 ug/L

RT: 13.840 min Scan# 3903

Delta R.T. 0.010 min

Lab File: VU063106.D

Acq: 30 Jan 2025 18:24




Tgt Ion:180 Resp: 1488


Ion Ratio Lower Upper

180 100

182 102.7 75.5 113.3


145 28.6 24.6 36.8

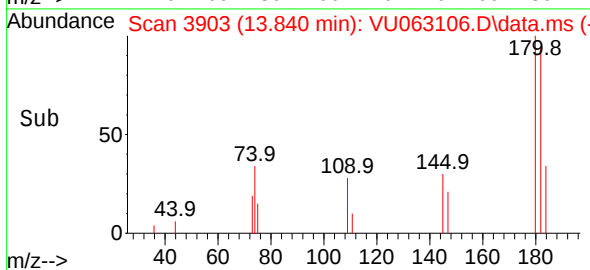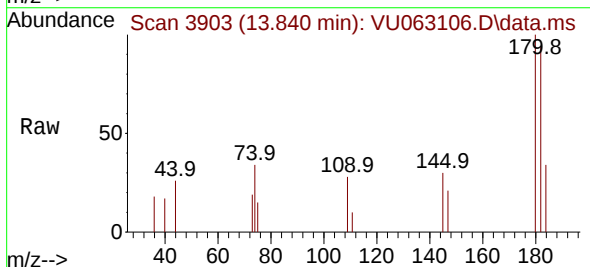

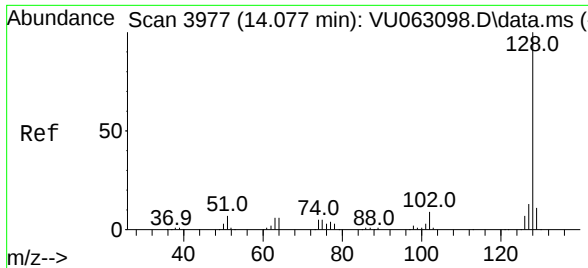

#71
Naphthalene
Concen: 45.739 ug/L
RT: 14.078 min Scan# 3977
Delta R.T. 0.000 min
Lab File: VU063106.D
Acq: 30 Jan 2025 18:24

Instrument :
MSVOA_U
ClientSampleId :

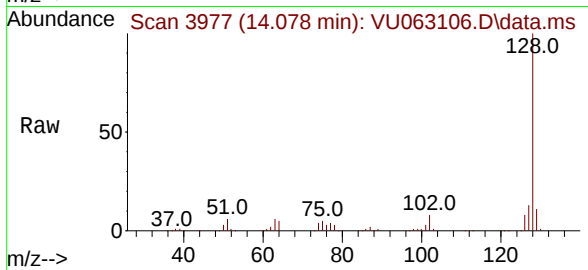

Tgt Ion:128 Resp: 202019
Ion Ratio Lower Upper
128 100
127 12.8 10.1 15.1
129 10.7 8.8 13.2

