

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013025\
 Data File : VU063102.D
 Acq On : 30 Jan 2025 16:48
 Operator : MD/SY
 Sample : VU0130MBL01
 Misc : 5.00g/5.0mL/100uL5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK113

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM013025WMA.M
 Title : VOC Analysis

Signal : TIC: VU063102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	113	rVB	79123	89947	15.13%	2.069%
2	1.846	167	173	181	rVB2	670	846	0.14%	0.019%
3	1.901	181	190	203	rBV	46205	61184	10.29%	1.407%
4	2.075	241	244	248	rBV	204	148	0.02%	0.003%
5	2.129	258	261	263	rVB	329	183	0.03%	0.004%
6	2.274	304	306	310	rBV2	213	142	0.02%	0.003%
7	2.554	381	393	415	rVB	132534	219143	36.87%	5.041%
8	2.782	455	464	478	rVB	2222	3825	0.64%	0.088%
9	3.026	536	540	547	rBV5	476	641	0.11%	0.015%
10	3.091	555	560	561	rBV	148	145	0.02%	0.003%
11	3.129	568	572	575	rBV	149	149	0.03%	0.003%
12	3.174	579	586	597	rVV4	623	1182	0.20%	0.027%
13	3.348	633	640	645	rBV5	1209	1748	0.29%	0.040%
14	3.393	652	654	660	rBV2	148	185	0.03%	0.004%
15	3.448	665	671	675	rVB2	191	239	0.04%	0.005%
16	3.509	685	690	695	rBV2	132	176	0.03%	0.004%
17	3.599	714	718	723	rBV2	245	297	0.05%	0.007%
18	3.692	736	747	759	rVV3	3292	7083	1.19%	0.163%
19	3.766	768	770	775	rVB2	176	167	0.03%	0.004%
20	3.805	779	782	786	rBV2	199	215	0.04%	0.005%
21	3.949	825	827	832	rVB	162	165	0.03%	0.004%
22	4.017	844	848	851	rBV2	131	147	0.02%	0.003%
23	4.216	905	910	915	rVB2	208	212	0.04%	0.005%
24	4.248	915	920	923	rBV2	169	211	0.04%	0.005%
25	4.293	931	934	939	rVB2	222	210	0.04%	0.005%
26	4.605	1021	1031	1063	rBV	50866	126923	21.35%	2.920%
27	5.046	1153	1168	1201	rVV	107732	242035	40.72%	5.568%
28	5.267	1234	1237	1240	rVB2	210	171	0.03%	0.004%
29	5.287	1240	1243	1247	rVB2	174	162	0.03%	0.004%
30	5.364	1264	1267	1269	rBV	250	143	0.02%	0.003%
31	5.390	1272	1275	1278	rVB	187	145	0.02%	0.003%
32	5.602	1338	1341	1344	rBV2	210	170	0.03%	0.004%
33	5.711	1355	1375	1404	rVV2	219997	594372	100.00%	13.673%
34	6.033	1472	1475	1477	rBV2	274	141	0.02%	0.003%
35	6.091	1491	1493	1499	rBV2	139	154	0.03%	0.004%
36	6.235	1526	1538	1559	rBV	170693	328015	55.19%	7.546%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013025\
 Data File : VU063102.D
 Acq On : 30 Jan 2025 16:48
 Operator : MD/SY
 Sample : VU0130MBL01
 Misc : 5.00g/5.0mL/100uL5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK113

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM013025WMA.M
 Title : VOC Analysis

37	6.480	1612	1614	1617	rBV	334	230	0.04%	0.005%
38	6.538	1625	1632	1642	rVV5	1419	2596	0.44%	0.060%
39	6.676	1660	1675	1695	rBV	128224	250980	42.23%	5.773%
40	6.862	1729	1733	1737	rVB2	221	178	0.03%	0.004%
41	7.129	1812	1816	1820	rBV2	181	210	0.04%	0.005%
42	7.200	1836	1838	1843	rBV2	340	259	0.04%	0.006%
43	7.312	1870	1873	1875	rBV2	243	169	0.03%	0.004%
44	7.370	1885	1891	1894	rBV	199	146	0.02%	0.003%
45	7.422	1901	1907	1910	rBV2	157	229	0.04%	0.005%
46	7.554	1937	1948	1970	rBV	76331	136188	22.91%	3.133%
47	7.650	1976	1978	1983	rVB2	339	330	0.06%	0.008%
48	7.689	1987	1990	1993	rBV2	322	246	0.04%	0.006%
49	7.766	2011	2014	2017	rBV	149	158	0.03%	0.004%
50	7.820	2027	2031	2033	rBV	179	157	0.03%	0.004%
51	7.888	2039	2052	2072	rBV	260015	450904	75.86%	10.372%
52	8.058	2103	2105	2108	rVB	391	188	0.03%	0.004%
53	8.078	2108	2111	2112	rBV2	225	143	0.02%	0.003%
54	8.168	2127	2139	2158	rBV	48161	83979	14.13%	1.932%
55	8.312	2182	2184	2192	rVB2	254	349	0.06%	0.008%
56	8.393	2202	2209	2211	rBV	305	297	0.05%	0.007%
57	8.541	2251	2255	2262	rVV5	774	884	0.15%	0.020%
58	8.621	2268	2280	2320	rBV	151534	278072	46.78%	6.397%
59	8.853	2350	2352	2355	rVV	216	141	0.02%	0.003%
60	8.917	2366	2372	2376	rBV4	503	581	0.10%	0.013%
61	9.033	2404	2408	2411	rVB2	210	177	0.03%	0.004%
62	9.058	2411	2416	2419	rBV2	197	140	0.02%	0.003%
63	9.081	2419	2423	2425	rBV2	164	160	0.03%	0.004%
64	9.193	2453	2458	2461	rVB2	221	225	0.04%	0.005%
65	9.361	2507	2510	2513	rBV2	185	170	0.03%	0.004%
66	9.406	2513	2524	2551	rVV	237268	402307	67.69%	9.254%
67	9.560	2570	2572	2574	rBV2	499	293	0.05%	0.007%
68	9.666	2601	2605	2608	rVB2	182	159	0.03%	0.004%
69	9.689	2608	2612	2615	rBV2	580	632	0.11%	0.015%
70	9.843	2656	2660	2664	rBV2	173	197	0.03%	0.005%
71	9.981	2700	2703	2705	rBV	216	142	0.02%	0.003%
72	10.045	2717	2723	2727	rBV2	263	362	0.06%	0.008%
73	10.097	2734	2739	2743	rBV2	686	812	0.14%	0.019%
74	10.123	2743	2747	2751	rVV3	577	611	0.10%	0.014%
75	10.177	2761	2764	2769	rVB2	217	180	0.03%	0.004%
76	10.316	2804	2807	2812	rVB2	178	189	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013025\
 Data File : VU063102.D
 Acq On : 30 Jan 2025 16:48
 Operator : MD/SY
 Sample : VU0130MBL01
 Misc : 5.00g/5.0mL/100uL5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK113

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM013025WMA.M
 Title : VOC Analysis

77	10.344	2812	2816	2819	rBV	193	189	0.03%	0.004%
78	10.479	2852	2858	2866	rBV	568	739	0.12%	0.017%
79	10.582	2886	2890	2895	rVB2	178	229	0.04%	0.005%
80	10.611	2895	2899	2904	rBV	215	266	0.04%	0.006%
81	10.640	2904	2908	2913	rBV2	205	247	0.04%	0.006%
82	10.743	2928	2940	2964	rBV	193484	318320	53.56%	7.322%
83	11.084	3043	3046	3053	rVB2	453	472	0.08%	0.011%
84	11.229	3087	3091	3099	rBV2	209	318	0.05%	0.007%
85	11.348	3123	3128	3132	rBV2	171	257	0.04%	0.006%
86	11.470	3159	3166	3172	rVB2	584	844	0.14%	0.019%
87	11.743	3243	3251	3258	rBV3	1705	2560	0.43%	0.059%
88	11.801	3258	3269	3291	rVV	215254	359199	60.43%	8.263%
89	12.184	3375	3388	3414	rBV	210268	354510	59.64%	8.155%
90	13.225	3706	3712	3721	rVB6	874	1220	0.21%	0.028%
91	13.351	3747	3751	3753	rBV2	252	222	0.04%	0.005%
92	13.589	3821	3825	3829	rBV2	183	192	0.03%	0.004%
93	13.846	3900	3905	3914	rVB4	2065	2533	0.43%	0.058%
94	14.016	3955	3958	3965	rVB2	180	229	0.04%	0.005%
95	14.052	3965	3969	3973	rBV	221	280	0.05%	0.006%
96	14.097	3975	3983	3997	rVV	2420	4940	0.83%	0.114%
97	14.232	4022	4025	4031	rVB3	266	302	0.05%	0.007%
98	14.331	4049	4056	4066	rVB3	2274	3256	0.55%	0.075%
99	14.695	4165	4169	4172	rBV2	286	292	0.05%	0.007%
100	15.351	4370	4373	4375	rBV	239	149	0.03%	0.003%

Sum of corrected areas: 4347156




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013025\
Data File : VU063102.D
Acq On : 30 Jan 2025 16:48
Operator : MD/SY
Sample : VU0130MBL01
Misc : 5.00g/5.0mL/100uL5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM013025WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

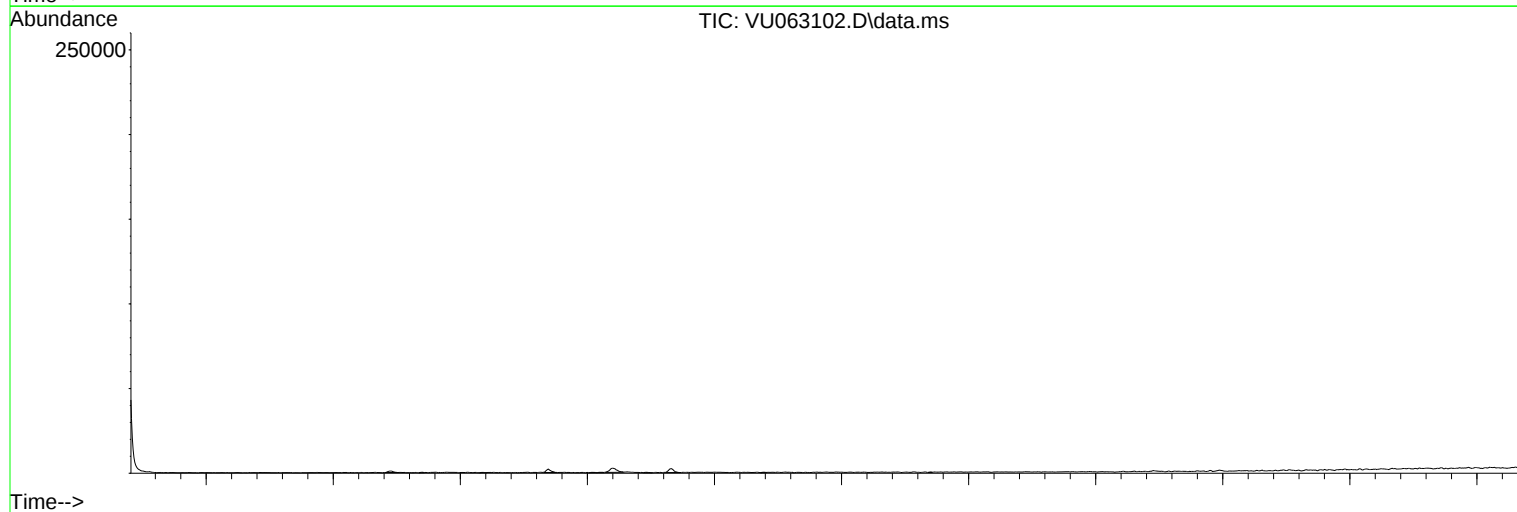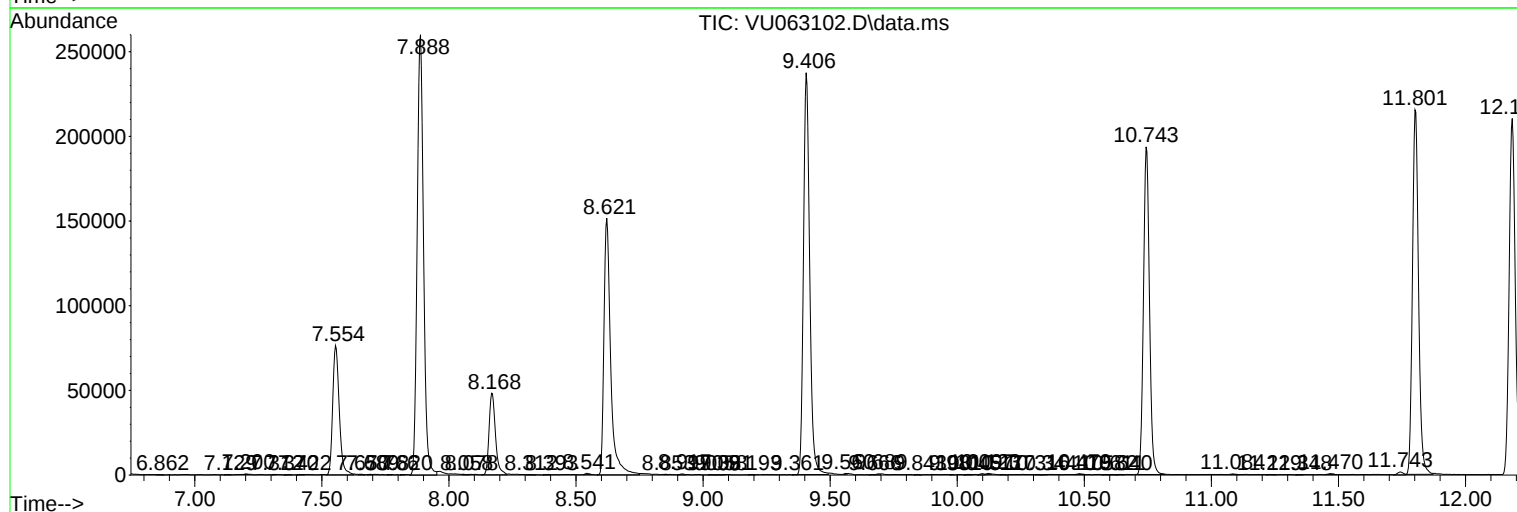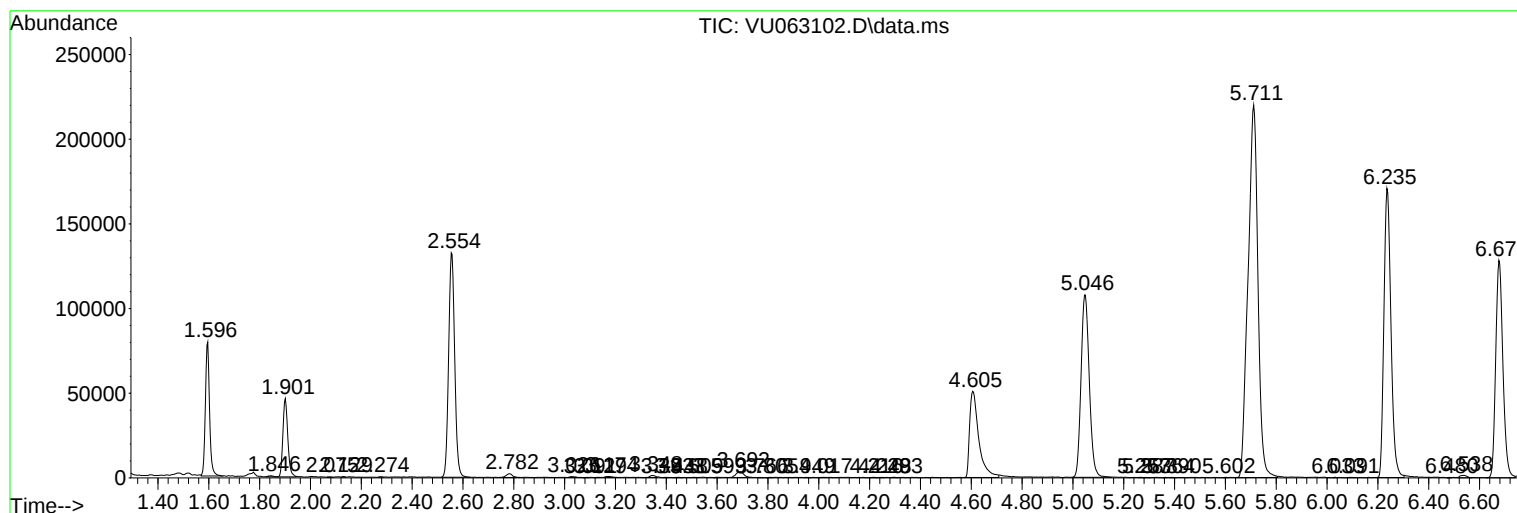

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013025\
Data File : VU063102.D
Acq On : 30 Jan 2025 16:48
Operator : MD/SY
Sample : VU0130MBL01
Misc : 5.00g/5.0mL/100uL5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM013025WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013025\
Data File : VU063102.D
Acq On : 30 Jan 2025 16:48
Operator : MD/SY
Sample : VU0130MBL01
Misc : 5.00g/5.0mL/100uL5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM013025WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc