
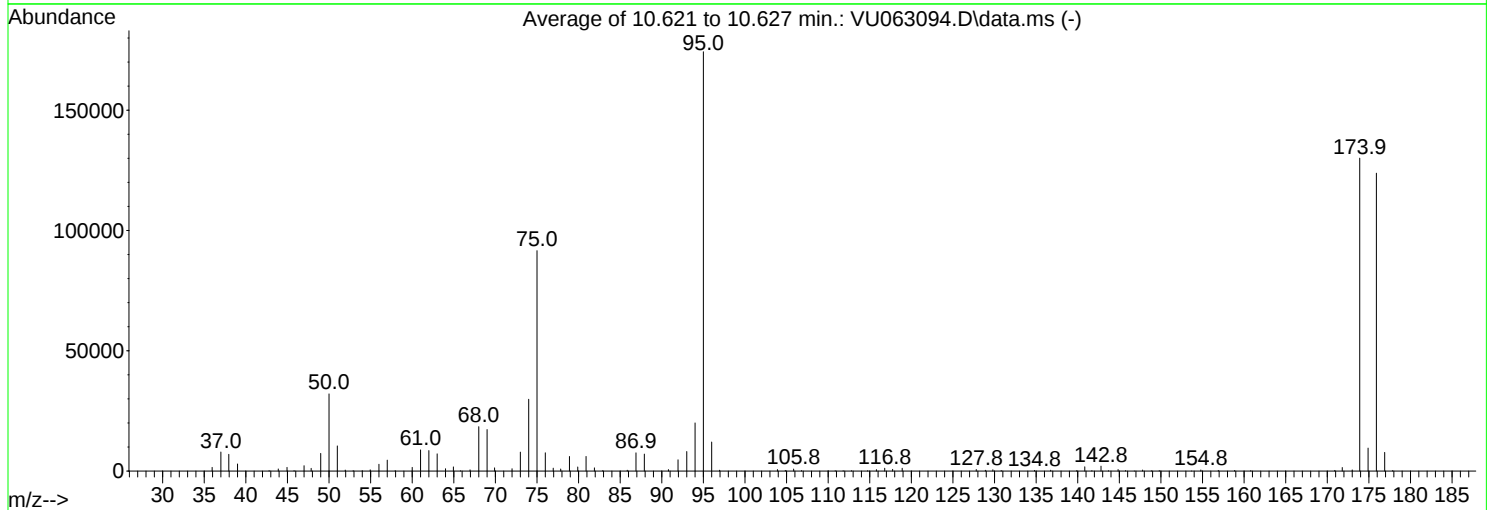


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013025\
Data File : VU063094.D
Acq On : 30 Jan 2025 10:46
Operator : MD/SY
Sample : BFB083
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB083

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM013025WMA.M
Title : VOC Analysis
Last Update : Fri Jan 31 07:44:25 2025

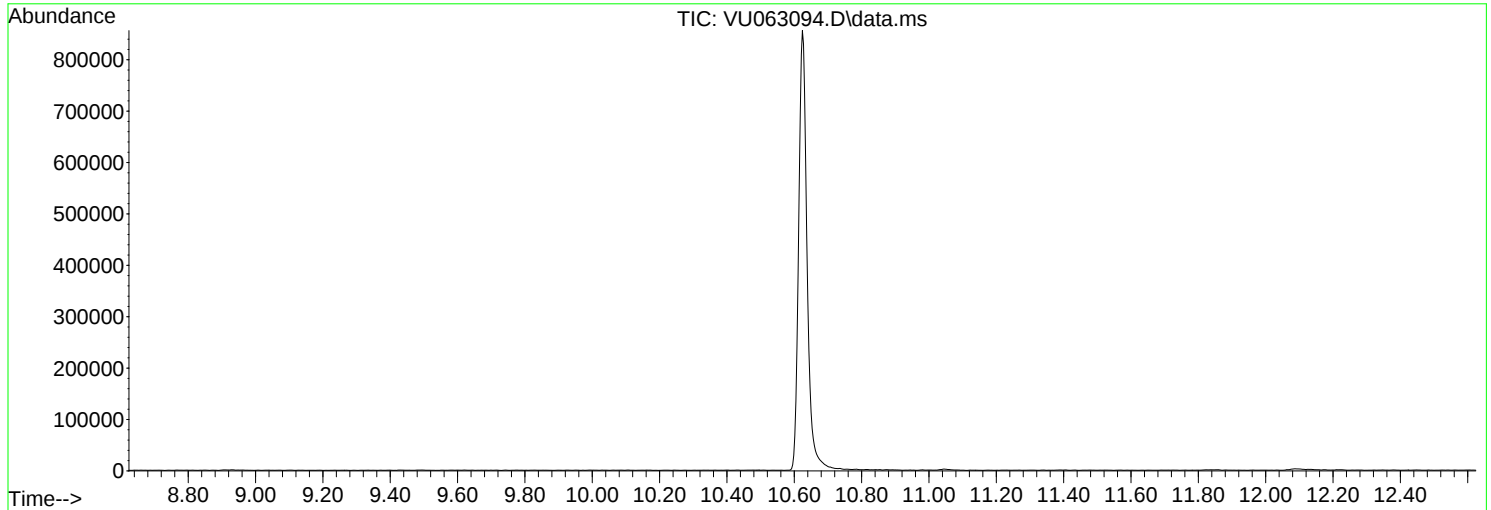

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	32080	PASS
75	95	30	80	52.6	91621	PASS
95	95	100	100	100.0	174293	PASS
96	95	5	9	6.9	12080	PASS
173	174	0.00	2	0.4	488	PASS
174	95	50	120	74.6	130056	PASS
175	174	5	9	7.4	9563	PASS
176	174	95	101	95.2	123829	PASS
177	176	5	9	6.3	7766	PASS

m/z	Abundance
39.90	776.0
43.90	635.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
36.00	1610.0
37.00	7681.0
37.90	6702.0
39.00	3067.0
39.90	762.0
42.80	184.0
43.90	1603.0
45.00	1539.0
45.80	171.0
47.00	2388.0
47.90	1070.0
49.00	6982.0
50.00	31904.0
51.00	10293.0
52.00	430.0
52.90	125.0
54.00	101.0
55.00	550.0
56.00	2661.0
57.00	4304.0
57.90	172.0
60.00	1465.0
61.00	8920.0
62.00	8448.0
63.00	7112.0
64.00	1006.0
64.90	1607.0
65.80	114.0
66.90	590.0
68.00	18600.0
69.00	16664.0
69.90	1241.0
72.00	913.0
73.00	7749.0
74.00	29408.0
75.00	90752.0
76.00	7818.0
77.00	1190.0
77.80	807.0
78.90	6143.0
79.90	1837.0
80.90	6104.0
81.90	1309.0
82.90	167.0
85.90	431.0
86.90	7428.0
87.90	7189.0
90.80	621.0
91.90	4498.0
93.00	8374.0
94.00	19232.0
95.00	170816.0
96.00	11864.0
97.00	341.0
103.90	605.0
104.90	242.0
105.80	794.0
106.90	220.0
110.90	130.0
111.80	112.0
112.80	194.0
114.70	116.0
115.80	569.0
116.80	1241.0
117.70	647.0
118.90	1137.0
127.80	710.0
128.90	344.0
129.80	506.0
130.90	292.0
134.70	328.0
136.70	369.0
139.80	147.0
140.90	1906.0
141.70	185.0
142.80	1889.0
143.60	155.0
144.80	679.0
145.80	197.0
146.80	102.0
147.80	414.0
148.90	116.0
149.80	209.0
153.70	138.0
154.80	434.0
156.90	257.0
158.80	247.0
160.80	192.0
170.90	244.0
171.80	1412.0
173.90	122968.0
174.90	9170.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

175.90

176.90

178.00

117728.0

7315.0

185.0

Instrument :

MSVOA_U

ClientSampleId :

BFB083

m/z	Abundance
36.00	1629.0
37.00	8217.0
38.00	7146.0
39.00	2985.0
39.90	731.0
42.80	218.0
43.90	1533.0
45.00	1538.0
45.80	179.0
47.00	2247.0
47.80	1145.0
49.00	7601.0
50.00	32976.0
51.00	10818.0
51.90	412.0
52.90	167.0
54.00	129.0
55.00	552.0
56.00	3007.0
57.00	4674.0
57.90	140.0
60.00	1571.0
61.00	9050.0
62.00	8778.0
63.00	7423.0
64.00	986.0
64.90	1831.0
65.80	143.0
66.90	544.0
68.00	19112.0
69.00	17736.0
69.90	1379.0
72.00	987.0
73.00	8107.0
74.00	30744.0
75.00	94496.0
76.00	7787.0
76.90	1224.0
77.90	911.0
78.90	6231.0
79.90	1722.0
80.90	6252.0
81.90	1374.0
82.90	176.0
85.80	391.0
86.90	7783.0
87.90	7255.0
90.80	615.0
91.90	4854.0
93.00	8369.0
94.00	20552.0
95.00	179520.0
96.00	12521.0
96.90	358.0
103.90	636.0
104.80	273.0
105.80	885.0
106.80	217.0
110.00	137.0
110.80	143.0
111.80	140.0
112.80	164.0
114.80	177.0
115.80	604.0
116.80	1191.0
117.80	724.0
118.90	1191.0
127.80	695.0
128.90	382.0
129.80	587.0
130.80	231.0
134.80	258.0
136.80	377.0
139.90	133.0
140.80	1833.0
141.70	187.0
142.80	2109.0
143.70	139.0
144.90	669.0
145.70	225.0
147.80	477.0
148.80	134.0
149.80	215.0
154.80	477.0
156.90	298.0
158.90	270.0
160.80	195.0
170.90	301.0
171.80	1486.0
173.90	133824.0
174.90	10054.0
175.90	127480.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

176.90	8048.0
177.80	207.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
35.90	1409.0
37.00	7845.0
38.00	7039.0
39.00	2834.0
39.90	706.0
42.80	188.0
44.00	1401.0
44.90	1513.0
45.80	204.0
47.00	2081.0
47.80	1210.0
49.00	7451.0
50.00	31360.0
51.00	10232.0
51.90	436.0
52.90	183.0
54.00	105.0
54.90	470.0
56.00	2836.0
57.00	4654.0
58.00	115.0
60.00	1598.0
61.00	8469.0
62.00	8324.0
63.00	6969.0
64.00	955.0
65.00	1769.0
65.80	148.0
67.00	455.0
68.00	17656.0
69.00	17392.0
69.90	1422.0
72.00	1043.0
73.00	7820.0
74.00	29400.0
75.00	89616.0
76.00	7200.0
76.90	1238.0
77.90	892.0
78.90	5806.0
79.90	1530.0
80.90	5916.0
81.90	1318.0
82.90	231.0
85.80	286.0
86.90	7537.0
87.90	6773.0
90.80	621.0
92.00	4714.0
93.00	7640.0
94.00	20272.0
95.00	172544.0
96.00	11855.0
96.90	375.0
103.90	609.0
104.80	311.0
105.90	860.0
106.70	179.0
110.00	183.0
110.80	170.0
111.80	172.0
112.80	146.0
114.80	222.0
115.80	642.0
116.80	1092.0
117.80	796.0
118.90	1186.0
127.80	602.0
128.90	325.0
129.80	627.0
130.70	193.0
134.90	231.0
136.80	364.0
139.90	143.0
140.90	1611.0
141.70	198.0
142.80	2186.0
143.80	128.0
144.90	607.0
145.70	197.0
147.80	466.0
148.80	145.0
149.80	172.0
154.80	494.0
156.90	299.0
158.90	188.0
160.80	165.0
170.90	318.0
171.80	1528.0
173.00	1463.0
173.90	133376.0
174.90	9466.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

175.90	126280.0
176.90	7934.0
177.80	208.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083