


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU013120\
 Data File : VU036647.D
 Acq On : 31 Jan 2020 17:01
 Operator : JC/MD
 Sample : BFB46
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB46

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Title : VOC Analysis
 Last Update : Mon Jan 27 00:51:24 2020

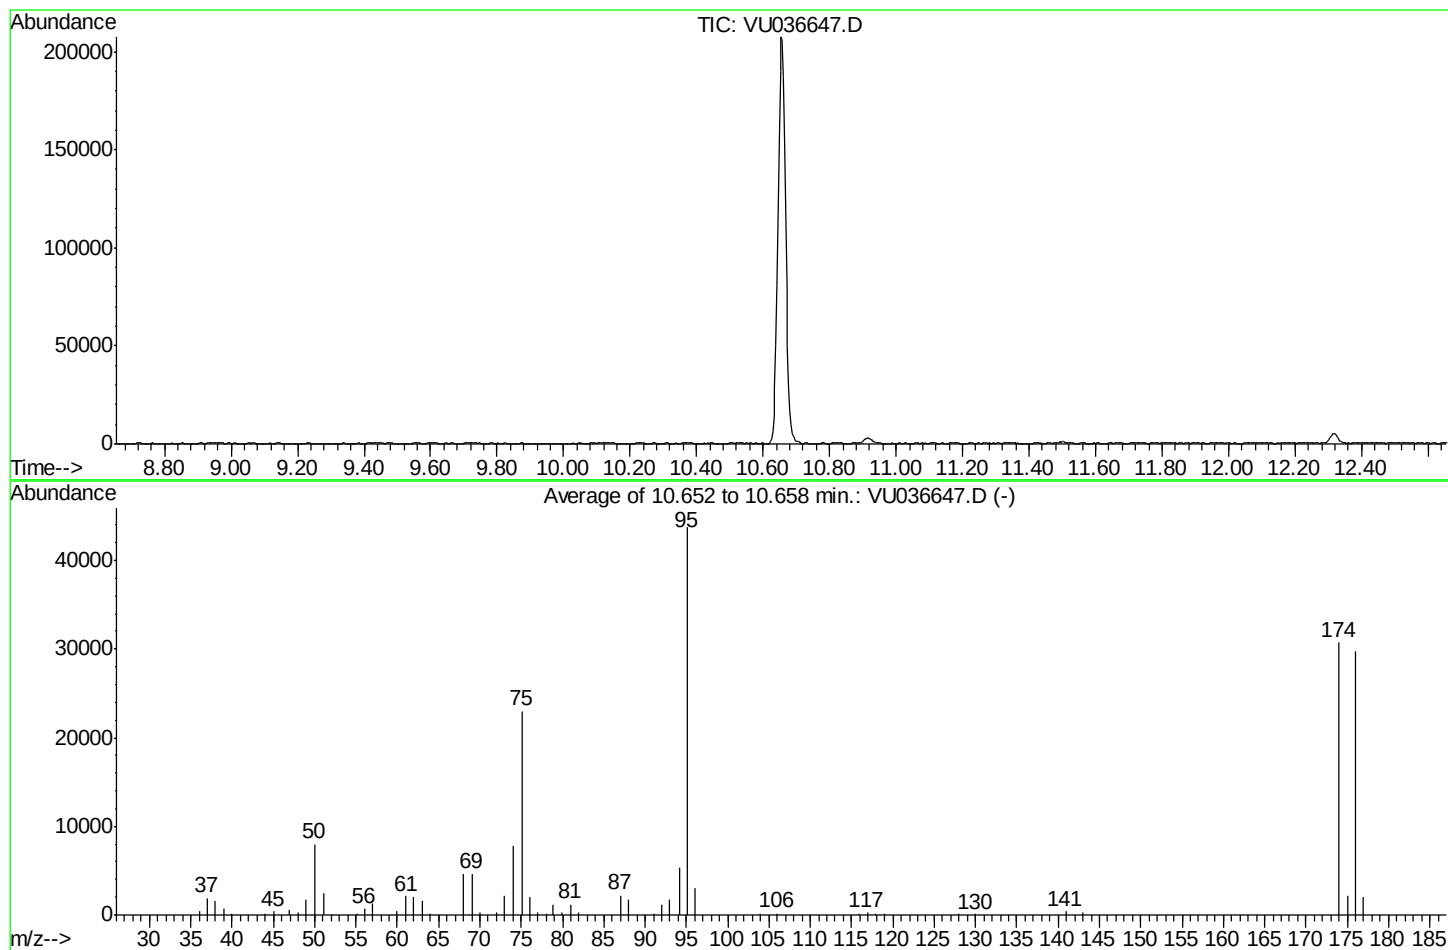

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	7976	PASS
75	95	30	80	52.6	23026	PASS
95	95	100	100	100.0	43744	PASS
96	95	5	9	7.0	3045	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.2	30720	PASS
175	174	5	9	7.0	2137	PASS
176	174	95	101	96.8	29746	PASS
177	176	5	9	6.8	2028	PASS

m/z	Abundance
36.00	376.0
37.00	1831.0
37.90	1523.0
39.00	694.0
40.00	139.0
44.00	436.0
45.00	385.0
47.00	549.0
48.00	268.0
49.00	1784.0
50.00	7532.0
51.10	2232.0
55.10	125.0
56.00	624.0
57.00	1199.0
60.00	357.0
61.00	1990.0
62.00	1898.0
63.00	1581.0
63.90	138.0
68.00	4337.0
69.00	4310.0
70.00	323.0
72.00	233.0
73.00	2072.0
74.00	7392.0
75.10	21976.0
76.10	1866.0
77.00	263.0
78.00	208.0
78.90	1064.0
79.90	336.0
81.00	1137.0
82.00	297.0
87.00	2108.0
88.00	1538.0
91.00	199.0
92.00	992.0
93.00	1682.0
94.10	5059.0
95.10	41736.0
96.00	3095.0
103.90	130.0
106.00	196.0
115.90	130.0
116.90	229.0
117.90	145.0
118.90	164.0
127.90	128.0
130.00	109.0
140.90	388.0
143.00	325.0
174.00	28480.0
175.10	1997.0
176.00	27520.0
177.00	1938.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	379.0
37.00	1995.0
37.90	1569.0
39.00	679.0
40.00	118.0
44.00	450.0
45.00	420.0
46.90	522.0
48.00	326.0
49.00	1867.0
50.00	8149.0
51.10	2563.0
52.00	100.0
55.10	133.0
56.00	681.0
57.00	1302.0
60.00	436.0
61.10	2207.0
62.00	1992.0
63.00	1621.0
63.90	175.0
68.00	4791.0
69.00	4797.0
70.00	367.0
72.00	242.0
73.00	2248.0
74.00	8116.0
75.00	23712.0
76.00	2060.0
77.00	296.0
78.00	213.0
78.90	1231.0
79.90	359.0
81.00	1211.0
81.90	279.0
87.00	2325.0
88.00	1725.0
91.00	200.0
92.00	1194.0
93.00	1768.0
94.10	5632.0
95.10	45096.0
96.00	3129.0
103.90	156.0
106.00	202.0
115.90	133.0
117.00	273.0
117.90	130.0
118.90	169.0
127.90	119.0
130.00	137.0
140.90	403.0
143.00	388.0
174.00	31584.0
175.10	2185.0
176.00	30824.0
177.00	2101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	363.0
37.00	2014.0
38.00	1522.0
39.00	609.0
44.00	485.0
45.00	392.0
47.00	509.0
48.00	348.0
49.00	1778.0
50.00	8247.0
51.10	2685.0
55.10	152.0
56.00	678.0
57.00	1276.0
60.00	481.0
61.10	2243.0
62.00	1990.0
63.00	1503.0
64.00	183.0
68.00	4781.0
69.00	4808.0
70.00	364.0
71.90	264.0
73.00	2144.0
74.10	8071.0
75.00	23392.0
76.00	2046.0
77.00	290.0
78.00	194.0
78.90	1282.0
79.90	370.0
80.90	1308.0
81.90	223.0
87.00	2240.0
88.00	1889.0
91.00	176.0
92.00	1233.0
93.00	1804.0
94.10	5530.0
95.10	44400.0
96.10	2911.0
103.90	154.0
106.00	192.0
115.90	112.0
117.00	296.0
117.90	135.0
118.90	155.0
128.00	122.0
130.00	142.0
140.90	361.0
142.90	359.0
174.00	32096.0
175.10	2231.0
176.00	30896.0
177.00	2047.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
43.90	250.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46