




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052881.D
Acq On : 31 Jan 2023 15:42
Operator : JC/MD
Sample : 01314-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 02/01/2023
Supervised By :Mahesh Dadoda 02/01/2023

Quant Time: Feb 01 00:56:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 01 00:53:48 2023
Response via : Initial Calibration

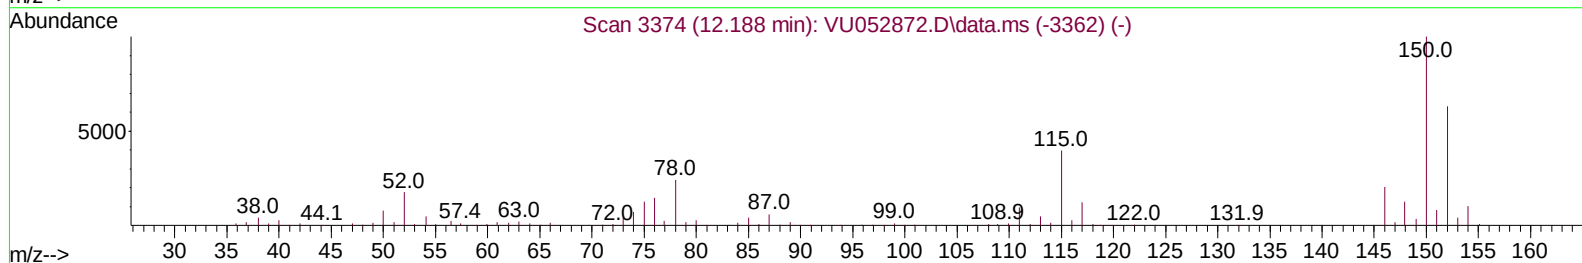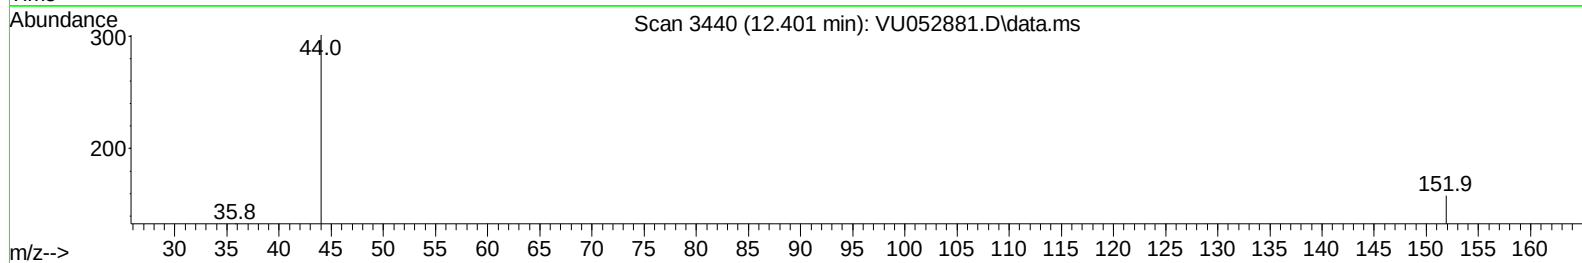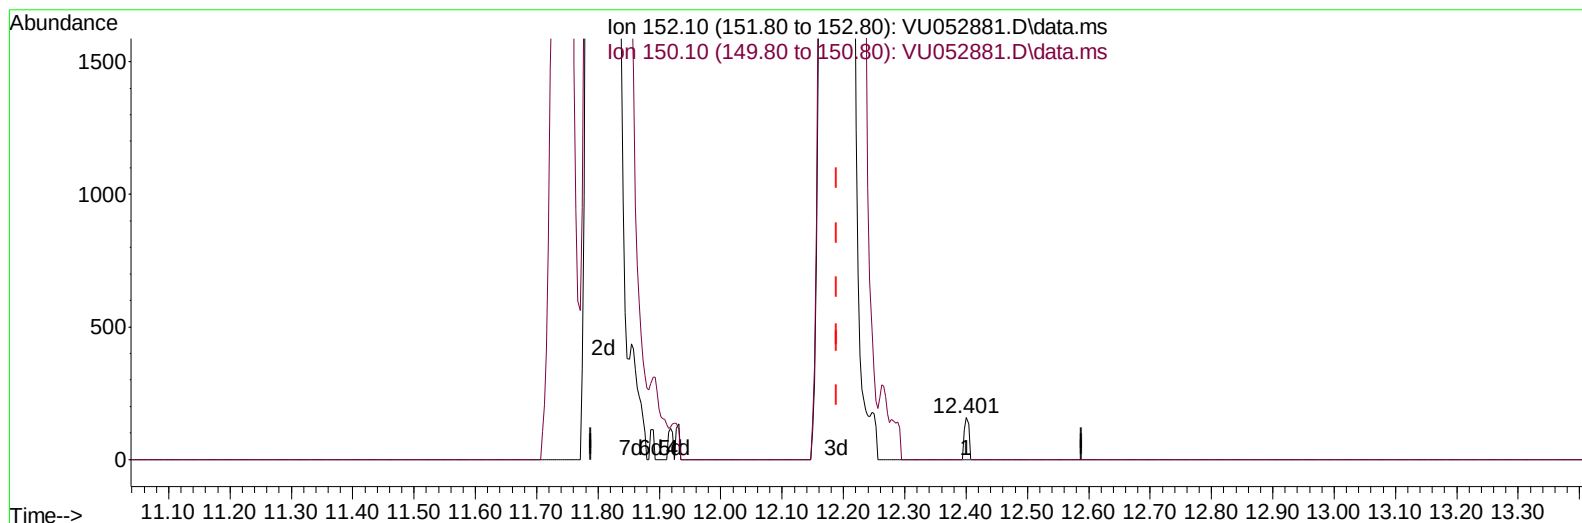

TIC: VU052881.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

12.401min (+ 0.212) 0.03 ug/L

response 78

Ion	Exp%	Act%
152.10	100.00	100.00
150.10	173.00	141.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052881.D
 Acq On : 31 Jan 2023 15:42
 Operator : JC/MD
 Sample : 01314-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M0

Manual IntegrationsAPPROVED

Quant Time: Feb 01 00:56:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 01 00:53:48 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/01/2023
 Supervised By :Mahesh Dadoda 02/01/2023

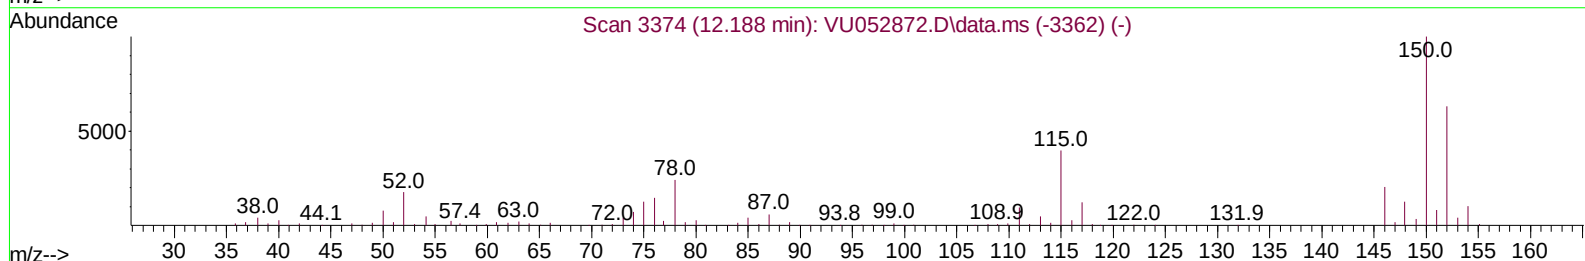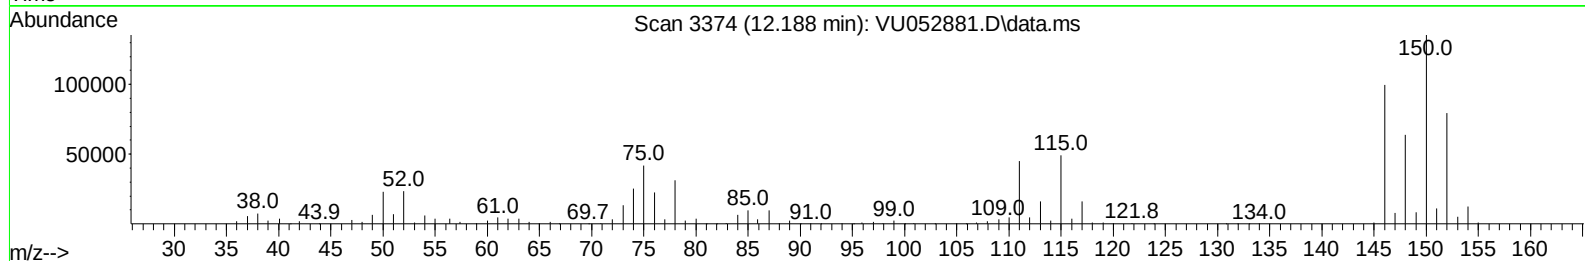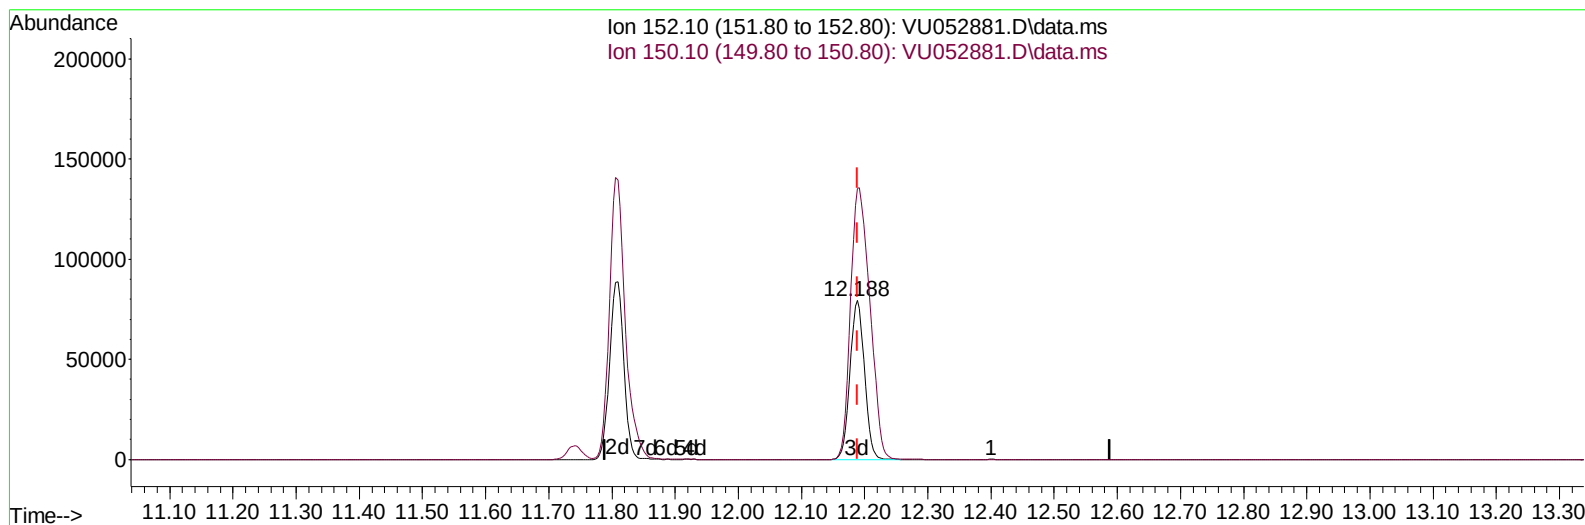

TIC: VU052881.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

12.188min (-0.000) 46.86 ug/L m

response 125614

Ion	Exp%	Act%
152.10	100.00	100.00
150.10	173.00	0.09#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052881.D
 Acq On : 31 Jan 2023 15:42
 Operator : JC/MD
 Sample : 01314-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M0

Manual IntegrationsAPPROVED

Quant Time: Feb 01 00:56:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 01 00:53:48 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/01/2023
 Supervised By :Mahesh Dadoda 02/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	238737	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	244885	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	138044	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	62415	36.323	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	72.640%	
7) Chloroethane-d5	1.909	69	62978	44.480	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	88.960%	
11) 1,1-Dichloroethene-d2	2.565	63	102422	29.968	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	59.940%#	
21) 2-Butanone-d5	4.620	46	104922	98.843	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	98.840%	
24) Chloroform-d	5.057	84	168404	45.922	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.840%	
26) 1,2-Dichloroethane-d4	5.697	65	111997	47.830	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.660%	
32) Benzene-d6	5.722	84	306170	40.923	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	81.840%	
36) 1,2-Dichloropropane-d6	6.687	67	97683	44.518	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	89.040%	
41) Toluene-d8	7.893	98	261179	38.337	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	76.680%#	
43) trans-1,3-Dichloroprop...	8.176	79	45056	40.968	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	81.940%	
47) 2-Hexanone-d5	8.629	63	69037	89.543	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	89.540%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84	148127	45.691	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	91.380%	
66) 1,2-Dichlorobenzene-d4	12.188	152	125614m	46.863	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	93.720%	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.604	62	5948	2.916	ug/L #	82
20) cis-1,2-Dichloroethene	4.661	96	21399	10.501	ug/L	98
33) Benzene	5.771	78	57609	6.911	ug/L	100
34) Trichloroethene	6.539	95	57470	27.124	ug/L	99
51) Chlorobenzene	9.443	112	706641	120.223	ug/L	99
52) Ethylbenzene	9.565	91	142847	15.646	ug/L	100
63) 1,2,4-Trimethylbenzene	11.465	105	8291	1.154	ug/L	98
64) 1,3-Dichlorobenzene	11.742	146	109238	24.285	ug/L	100
65) 1,4-Dichlorobenzene	11.832	146	263865	56.664	ug/L	99
67) 1,2-Dichlorobenzene	12.208	146	864657	190.045	ug/L	99
70) 1,2,4-trichlorobenzene	13.848	180	13526761	4845.013	ug/L	98
72) 1,2,3-Trichlorobenzene	14.327	180	2969600	1006.462	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052881.D
Acq On : 31 Jan 2023 15:42
Operator : JC/MD
Sample : 01314-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 02/01/2023
Supervised By :Mahesh Dadoda 02/01/2023

Quant Time: Feb 01 00:56:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 01 00:53:48 2023
Response via : Initial Calibration

