




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052887.D
 Acq On : 31 Jan 2023 18:27
 Operator : JC/MD
 Sample : 01381-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M6

Manual IntegrationsAPPROVED

Quant Time: Feb 01 00:58:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 01 00:53:48 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/01/2023
 Supervised By :Mahesh Dadoda 02/01/2023

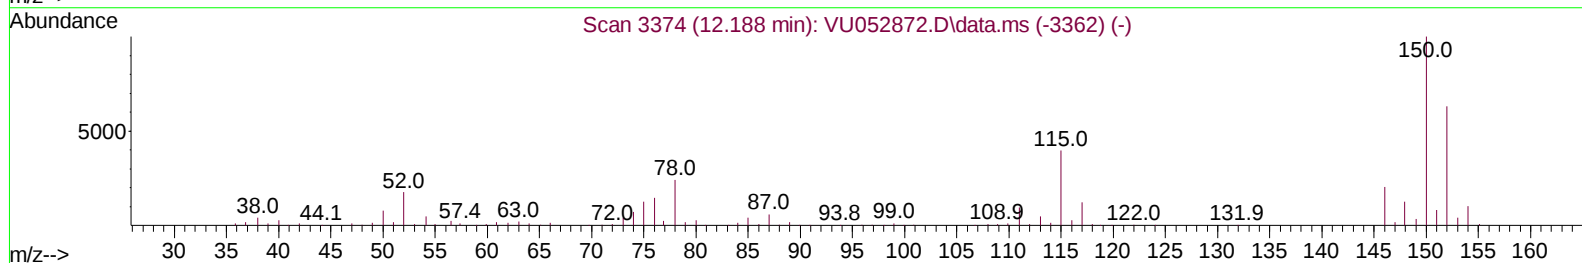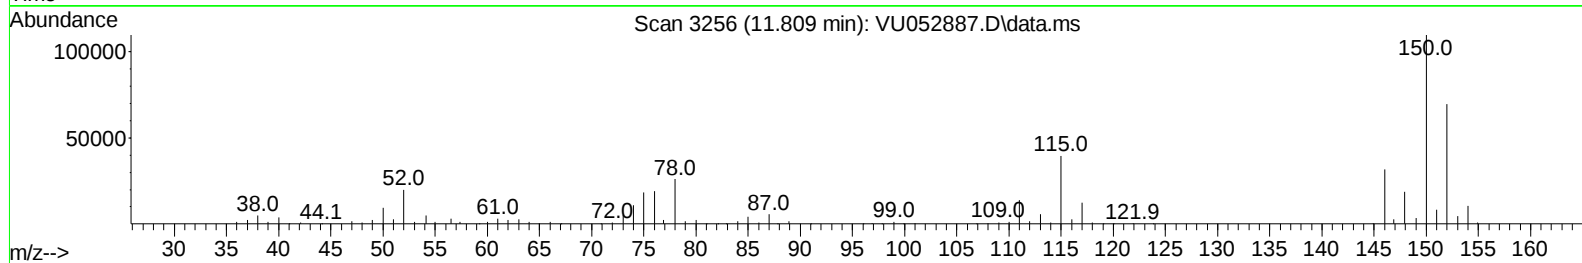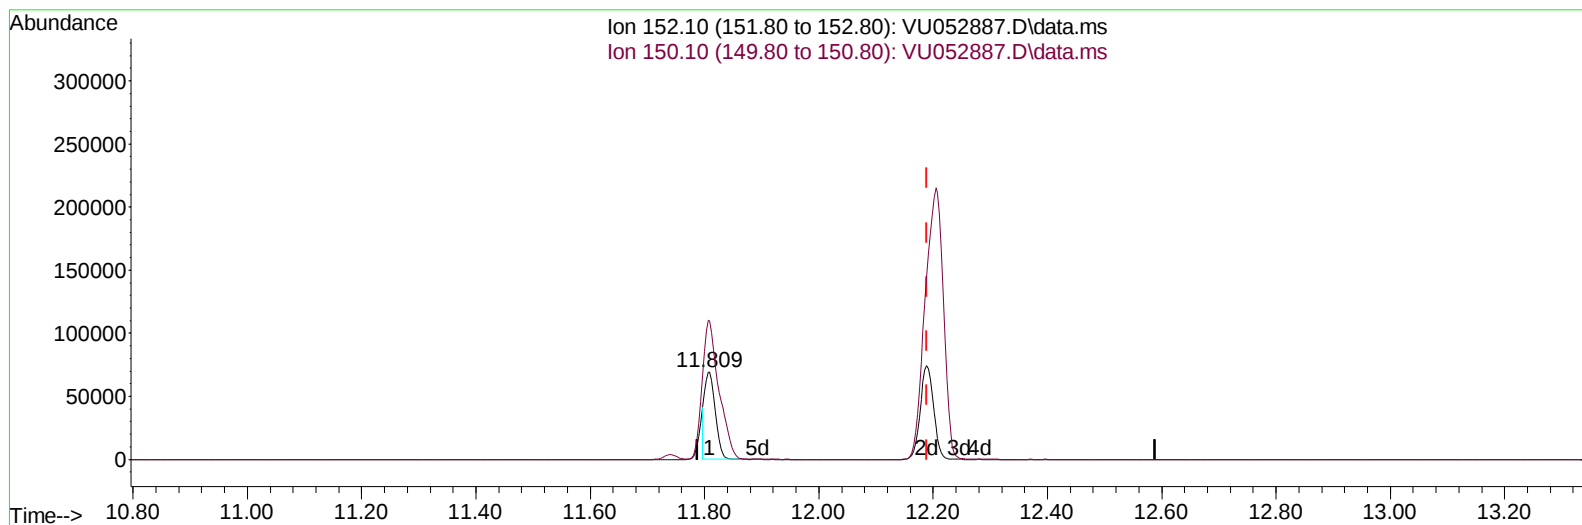

TIC: VU052887.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

11.809min (-0.379) 41.67 ug/L

response 89619

Ion	Exp%	Act%
152.10	100.00	100.00
150.10	173.00	213.69
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052887.D
 Acq On : 31 Jan 2023 18:27
 Operator : JC/MD
 Sample : 01381-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M6

Manual IntegrationsAPPROVED

Quant Time: Feb 01 00:58:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 01 00:53:48 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/01/2023
 Supervised By :Mahesh Dadoda 02/01/2023

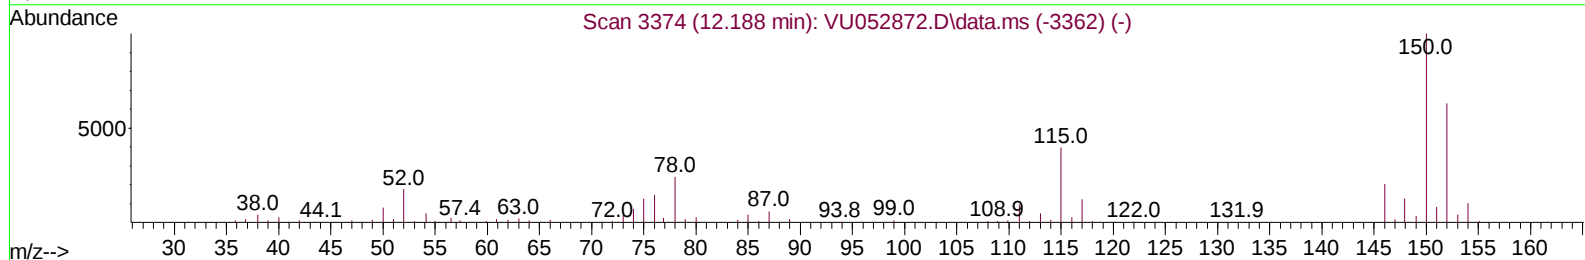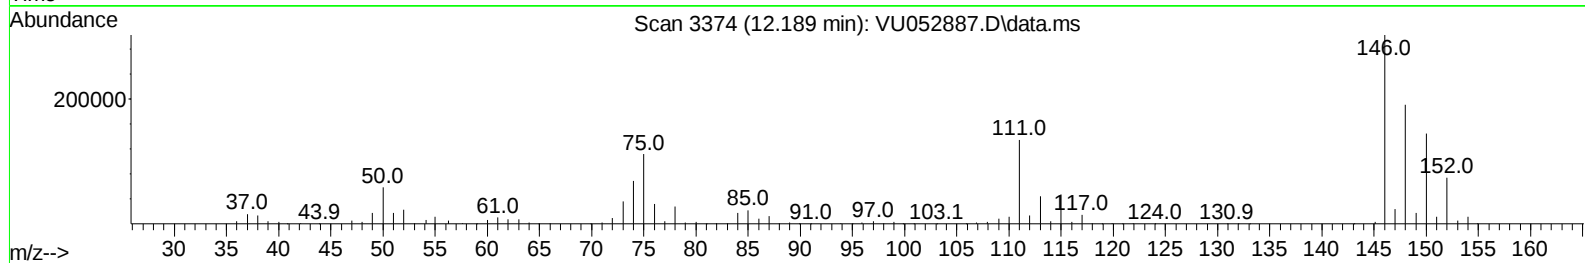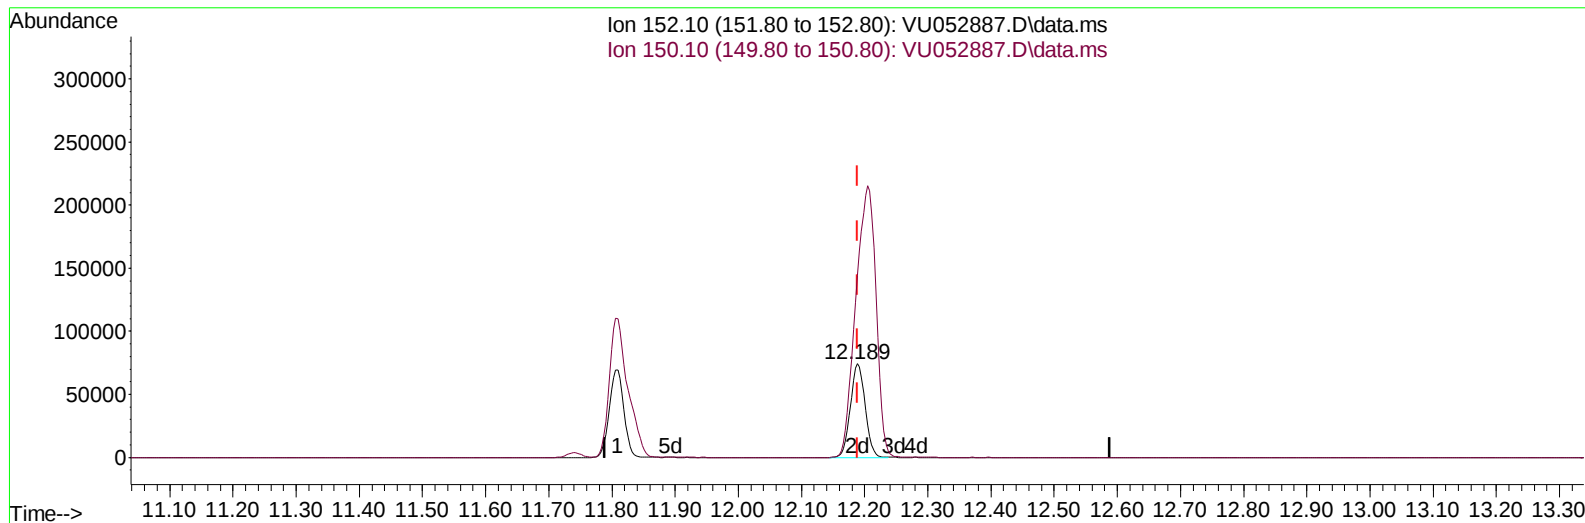

TIC: VU052887.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

12.189min (+ 0.000) 55.93 ug/L m

response 120267

Ion	Exp%	Act%
152.10	100.00	100.00
150.10	173.00	159.23
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052887.D
 Acq On : 31 Jan 2023 18:27
 Operator : JC/MD
 Sample : 01381-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M6

Manual IntegrationsAPPROVED

Quant Time: Feb 01 00:58:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 01 00:53:48 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/01/2023
 Supervised By :Mahesh Dadoda 02/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	211172	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	212147	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	110750	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	58606	38.559	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery =	77.120%		
7) Chloroethane-d5	1.909	69	59700	47.669	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery =	95.340%		
11) 1,1-Dichloroethene-d2	2.565	63	97766	32.340	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery =	64.680%		
21) 2-Butanone-d5	4.620	46	108227	115.266	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery =	115.270%		
24) Chloroform-d	5.057	84	163506	50.406	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	100.820%		
26) 1,2-Dichloroethane-d4	5.697	65	109157	52.702	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	105.400%		
32) Benzene-d6	5.723	84	290972	44.893	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	89.780%		
36) 1,2-Dichloropropane-d6	6.684	67	94808	49.875	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery =	99.740%		
41) Toluene-d8	7.896	98	248150	42.046	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	84.100%		
43) trans-1,3-Dichloroprop...	8.176	79	43798	45.970	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery =	91.940%		
47) 2-Hexanone-d5	8.629	63	70615	105.723	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery =	105.720%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	142765	50.832	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery =	101.660%		
66) 1,2-Dichlorobenzene-d4	12.189	152	120267m	55.926	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	111.860%		
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.604	62	4588	2.543	ug/L #	73
12) 1,1-Dichloroethene	2.578	96	3291	2.107	ug/L #	1
17) trans-1,2-Dichloroethene	3.350	96	4025	2.384	ug/L	90
20) cis-1,2-Dichloroethene	4.662	96	570734	316.643	ug/L	97
33) Benzene	5.771	78	78772	10.908	ug/L	100
34) Trichloroethene	6.536	95	366513	199.680	ug/L	97
51) Chlorobenzene	9.443	112	3221388	632.642	ug/L	100
64) 1,3-Dichlorobenzene	11.742	146	58017	16.077	ug/L	99
65) 1,4-Dichlorobenzene	11.832	146	511486	136.909	ug/L	98
67) 1,2-Dichlorobenzene	12.208	146	2874095	787.387	ug/L	99
70) 1,2,4-trichlorobenzene	13.835	180	490330	218.909	ug/L	99
72) 1,2,3-Trichlorobenzene	14.324	180	110913	46.855	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052887.D
Acq On : 31 Jan 2023 18:27
Operator : JC/MD
Sample : 01381-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M6

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 02/01/2023
Supervised By :Mahesh Dadoda 02/01/2023

Quant Time: Feb 01 00:58:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 01 00:53:48 2023
Response via : Initial Calibration

