

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052878.D
 Acq On : 31 Jan 2023 14:32
 Operator : JC/MD
 Sample : 01314-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L3

Quant Time: Feb 01 00:56:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 01 00:53:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.246	114	189053	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	207342	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	93788	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	45193	33.213	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	66.420%	
7) Chloroethane-d5	1.909	69	51251	45.711	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	91.420%	
11) 1,1-Dichloroethene-d2	2.565	63	89944	33.233	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	66.460%	
21) 2-Butanone-d5	4.616	46	75224	89.490	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	89.490%	
24) Chloroform-d	5.057	84	134897	46.452	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.900%	
26) 1,2-Dichloroethane-d4	5.697	65	88282	47.610	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.220%	
32) Benzene-d6	5.722	84	239856	37.864	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	75.720%	
36) 1,2-Dichloropropane-d6	6.684	67	71691	38.588	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	77.180%	
41) Toluene-d8	7.893	98	206888	35.867	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	71.740%#	
43) trans-1,3-Dichloroprop...	8.176	79	34969	37.554	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	75.100%	
47) 2-Hexanone-d5	8.629	63	50610	77.528	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	77.530%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84	137582	50.122	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	100.240%	
66) 1,2-Dichlorobenzene-d4	12.188	152	98951	54.336	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	108.680%	
Target Compounds						
					Qvalue	
13) Acetone	2.632	43	2648	2.579	ug/L	89
20) cis-1,2-Dichloroethene	4.658	96	9151	5.671	ug/L	88
34) Trichloroethene	6.545	95	1419	0.791	ug/L	88
51) Chlorobenzene	9.442	112	42762	8.593	ug/L	97
65) 1,4-Dichlorobenzene	11.831	146	6687	2.114	ug/L	98
67) 1,2-Dichlorobenzene	12.208	146	21040	6.807	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052878.D
Acq On : 31 Jan 2023 14:32
Operator : JC/MD
Sample : 01314-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L3

Quant Time: Feb 01 00:56:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 01 00:53:48 2023
Response via : Initial Calibration




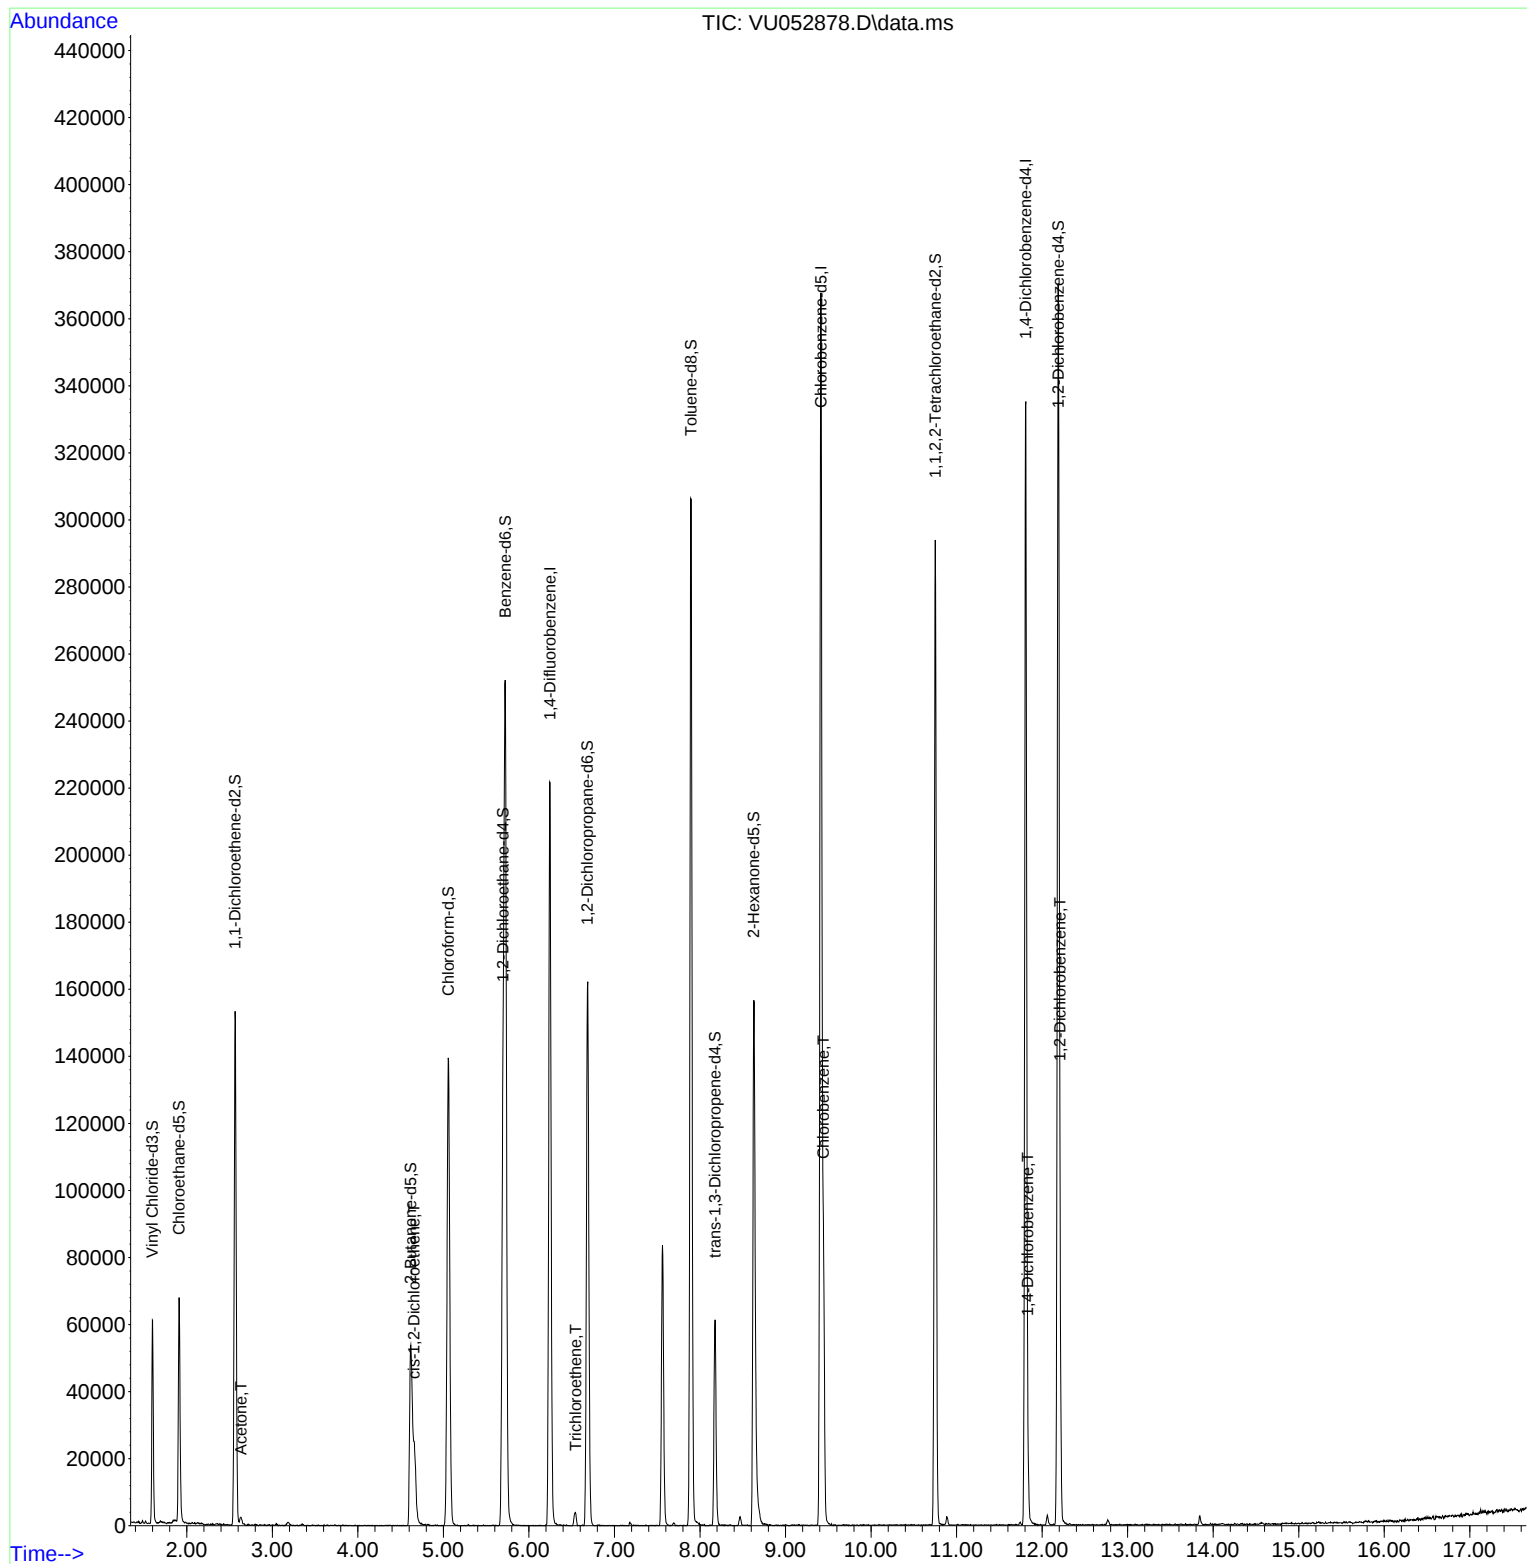


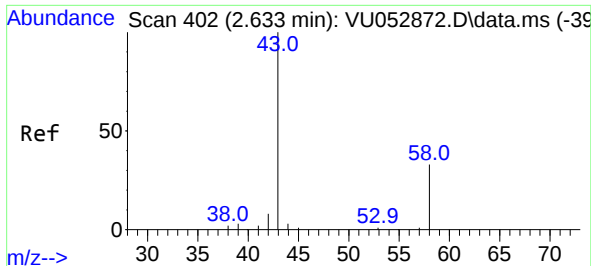

#13
Acetone
Concen: 2.579 ug/L
RT: 2.632 min Scan# 402
Delta R.T. -0.000 min
Lab File: VU052878.D
Acq: 31 Jan 2023 14:32




Instrument :
MSVOA_U
ClientSampleId :
A44L3


Tgt Ion: 43 Resp: 2648
Ion Ratio Lower Upper
43 100
58 41.7 0.0 70.2

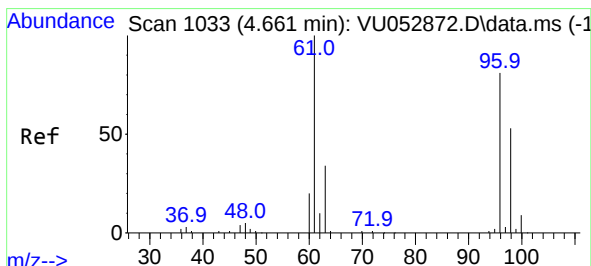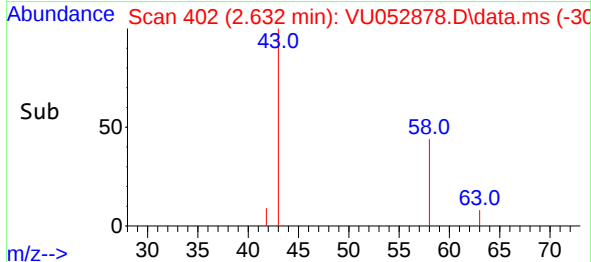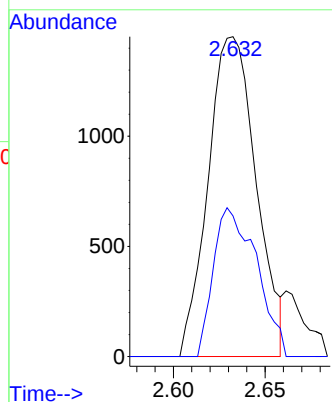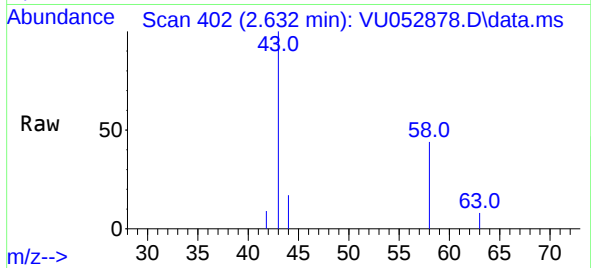

#20
cis-1,2-Dichloroethene
Concen: 5.671 ug/L
RT: 4.658 min Scan# 1032
Delta R.T. -0.003 min
Lab File: VU052878.D
Acq: 31 Jan 2023 14:32

Tgt Ion: 96 Resp: 9151
Ion Ratio Lower Upper
96 100
61 106.8 84.1 156.1
68 0.0 0.0 0.0

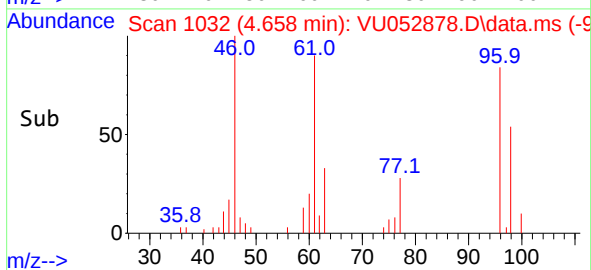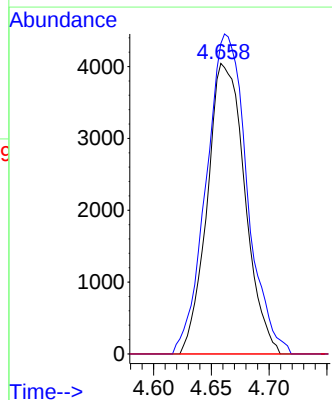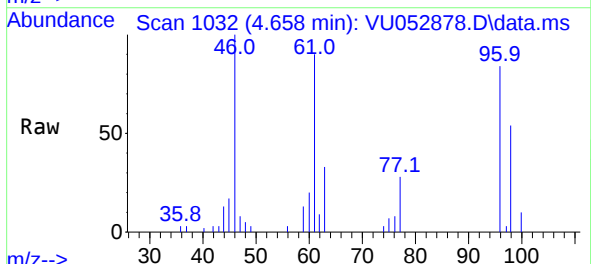




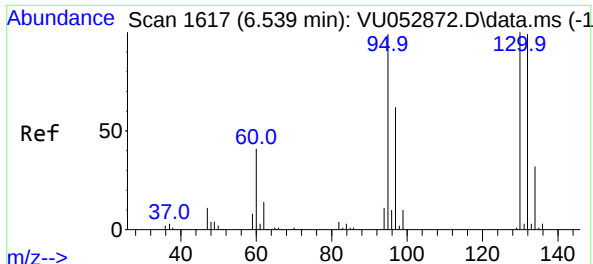


#34
Trichloroethene
Concen: 0.791 ug/L
RT: 6.545 min Scan# 1
Delta R.T. 0.006 min
Lab File: VU052878.D
Acq: 31 Jan 2023 14:32

Instrument :
MSVOA_U
ClientSampleId :
A44L3

Tgt Ion: 95 Resp: 1419




Ion	Ratio	Lower	Upper
95	100		
97	46.1	44.5	82.7
132	95.3	66.8	124.0
130	86.4	71.9	133.5

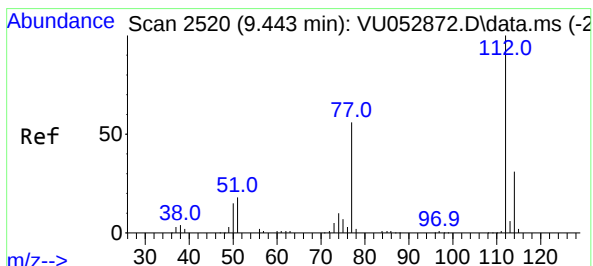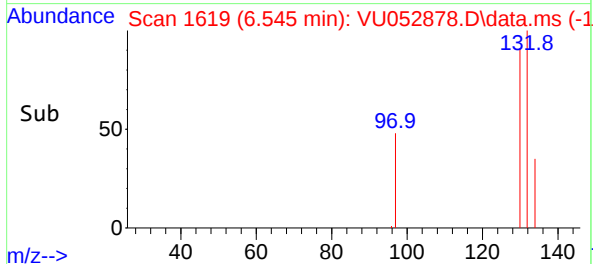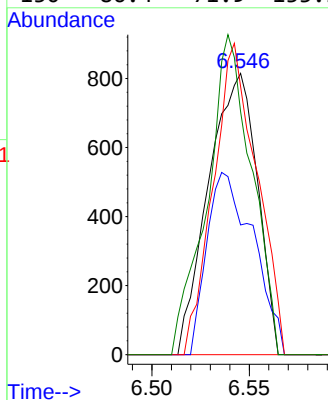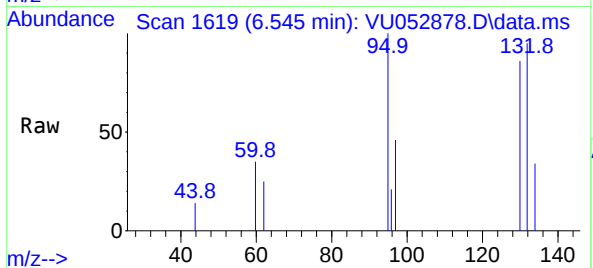


#51
Chlorobenzene
Concen: 8.593 ug/L
RT: 9.442 min Scan# 2520
Delta R.T. -0.000 min
Lab File: VU052878.D
Acq: 31 Jan 2023 14:32

Tgt Ion: 112 Resp: 42762

Ion	Ratio	Lower	Upper
112	100		
114	32.6	22.8	42.4
77	60.4	45.9	68.9


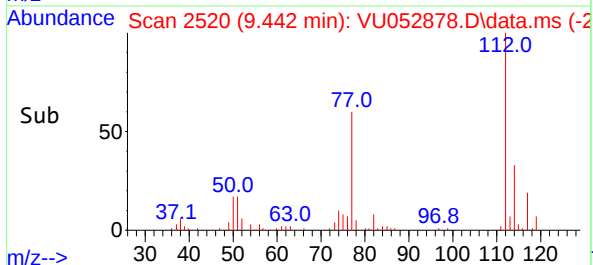
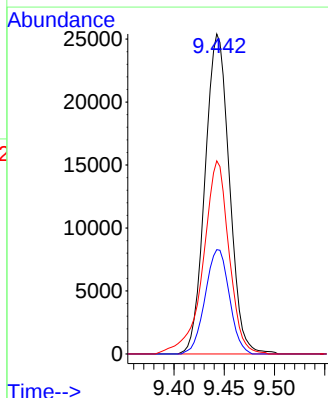
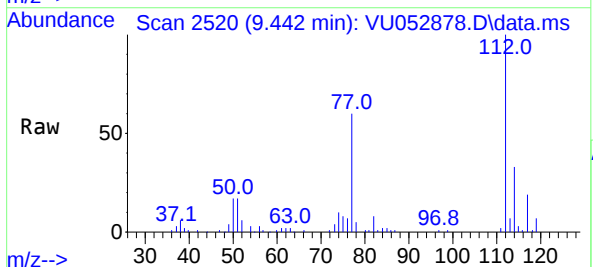


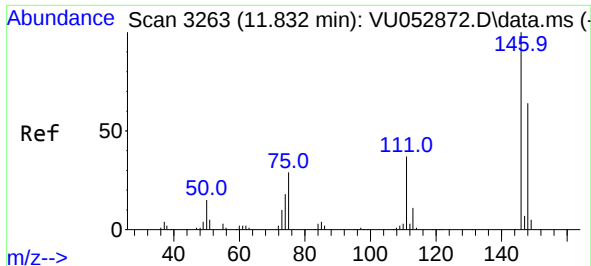

#65
1,4-Dichlorobenzene
Concen: 2.114 ug/L
RT: 11.831 min Scan# 31
Delta R.T. -0.000 min
Lab File: VU052878.D
Acq: 31 Jan 2023 14:32

Instrument :
MSVOA_U
ClientSampleId :
A44L3

Tgt Ion:	146	Resp:	6687
Ion	Ratio	Lower	Upper
146	100		
111	38.8	26.7	49.7
148	62.8	45.6	84.6

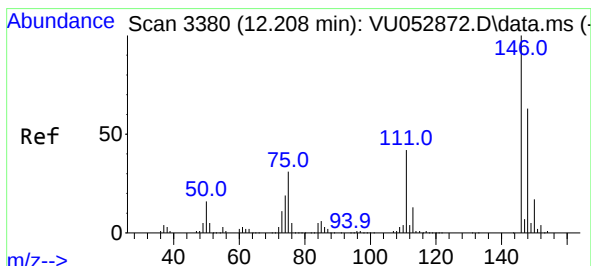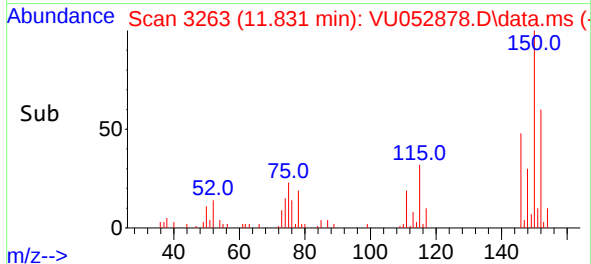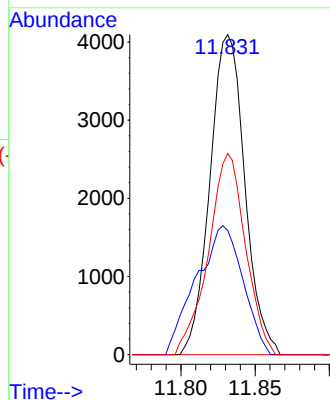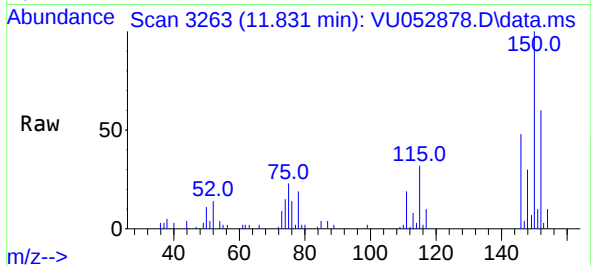

#67
1,2-Dichlorobenzene
Concen: 6.807 ug/L
RT: 12.208 min Scan# 3380
Delta R.T. -0.000 min
Lab File: VU052878.D
Acq: 31 Jan 2023 14:32

Tgt Ion:	146	Resp:	21040
Ion	Ratio	Lower	Upper
146	100		
111	40.2	33.2	49.8
148	64.0	50.2	75.4

