

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052880.D
 Acq On : 31 Jan 2023 15:19
 Operator : JC/MD
 Sample : 01314-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L8

Quant Time: Feb 01 00:56:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 01 00:53:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	237651	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	238351	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	103095	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	61796	36.127	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	72.260%
7) Chloroethane-d5	1.909	69	63432	45.006	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.020%
11) 1,1-Dichloroethene-d2	2.565	63	100683	29.594	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.180%#
21) 2-Butanone-d5	4.620	46	104581	98.972	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.970%
24) Chloroform-d	5.057	84	165076	45.220	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.440%
26) 1,2-Dichloroethane-d4	5.697	65	112014	48.056	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.120%
32) Benzene-d6	5.723	84	302510	41.542	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.080%
36) 1,2-Dichloropropane-d6	6.684	67	97890	45.835	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.660%
41) Toluene-d8	7.893	98	253131	38.174	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.340%#
43) trans-1,3-Dichloroprop...	8.176	79	44774	41.828	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.660%
47) 2-Hexanone-d5	8.629	63	67671	90.177	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.180%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	143466	45.466	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.940%
66) 1,2-Dichlorobenzene-d4	12.188	152	101515	50.711	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.420%
Target Compounds						
					Qvalue	
20) cis-1,2-Dichloroethene	4.661	96	28993	14.293	ug/L	99
34) Trichloroethene	6.539	95	23883	11.581	ug/L	97
67) 1,2-Dichlorobenzene	12.208	146	8693	2.558	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052880.D
Acq On : 31 Jan 2023 15:19
Operator : JC/MD
Sample : 01314-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L8

Quant Time: Feb 01 00:56:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 01 00:53:48 2023
Response via : Initial Calibration




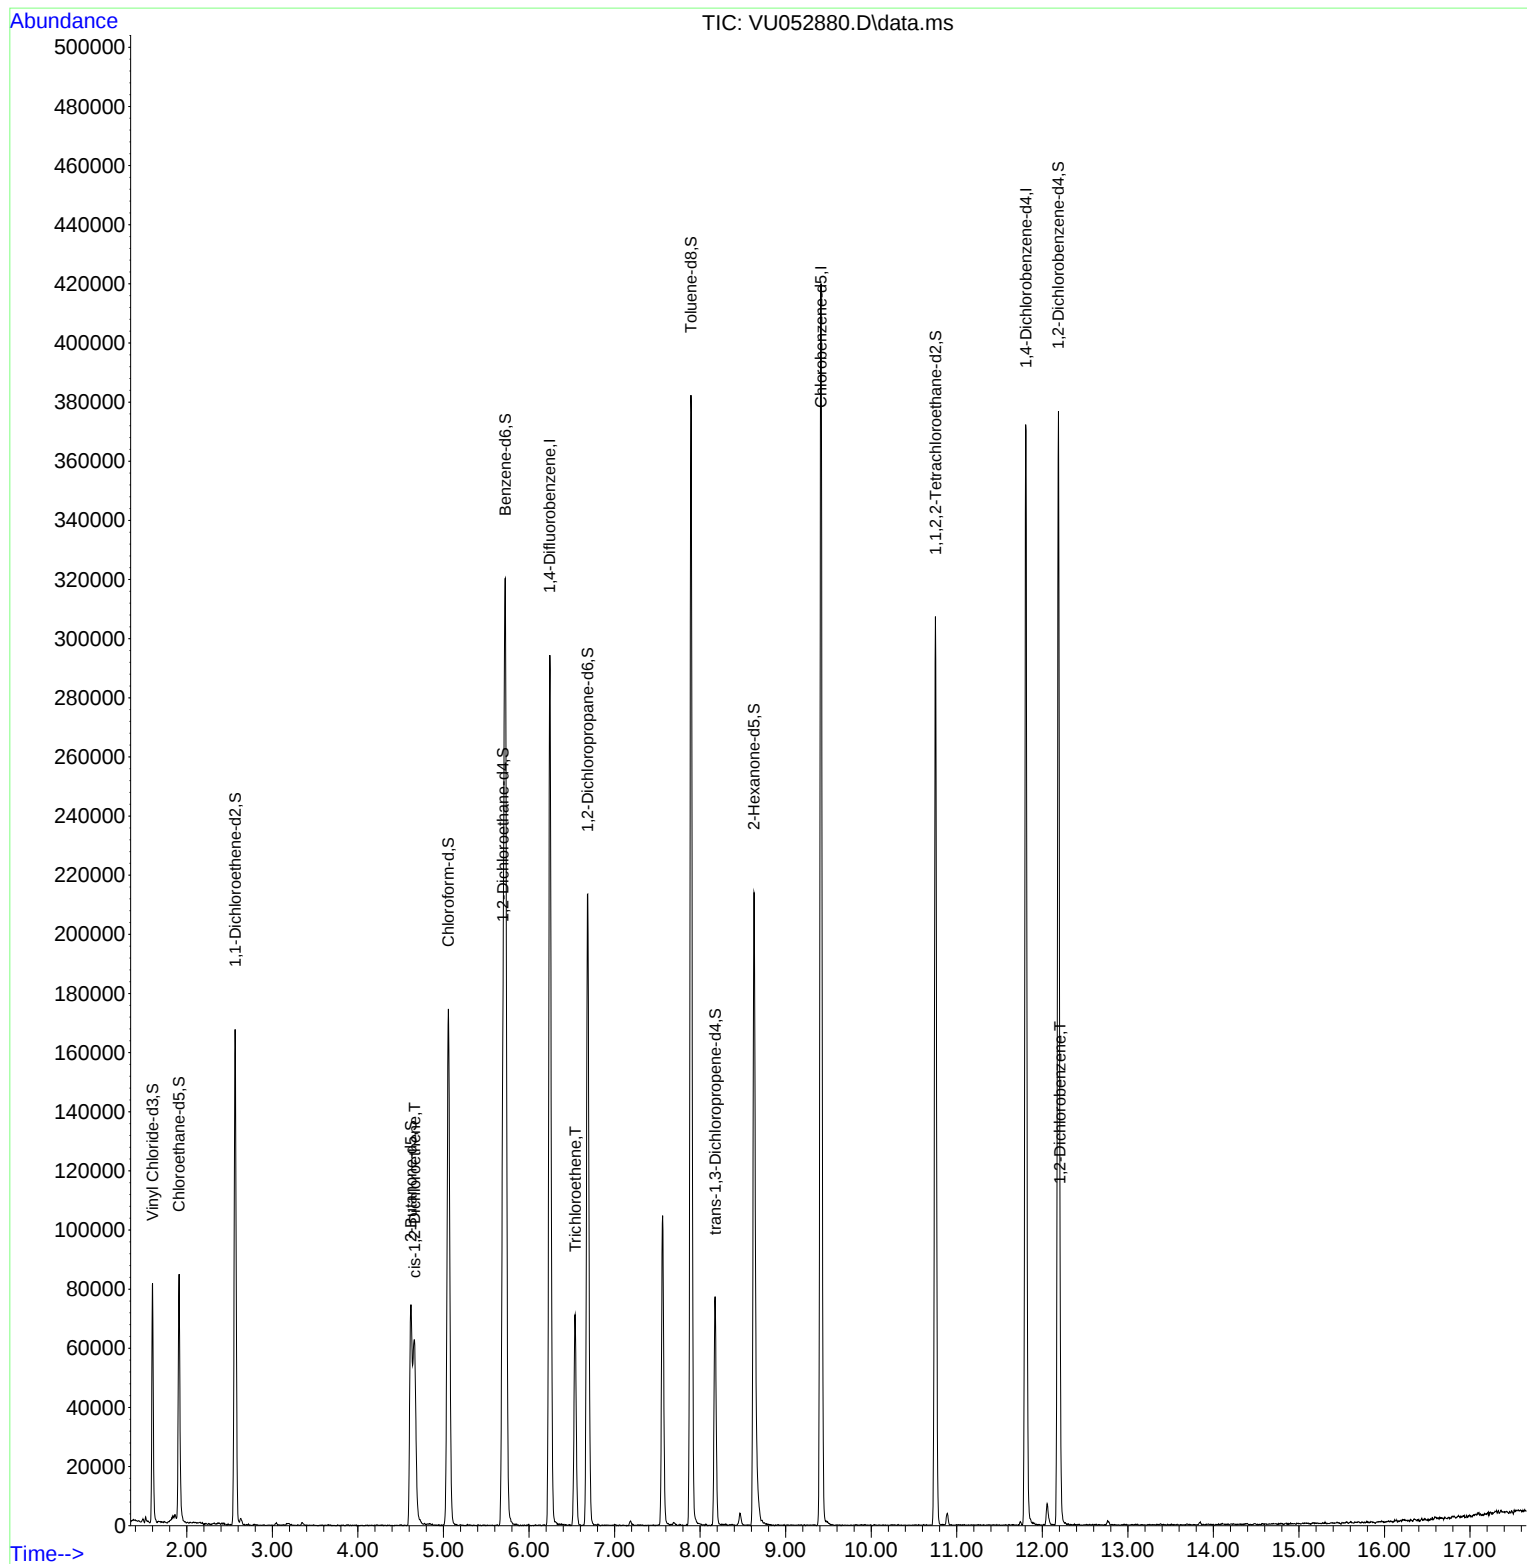


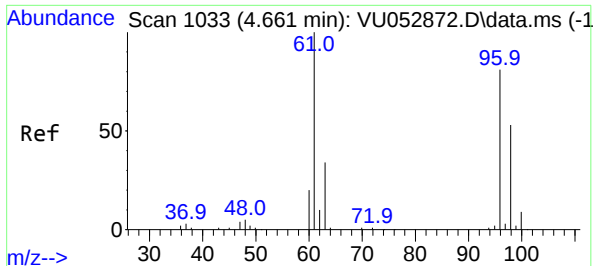

#20
cis-1,2-Dichloroethene
Concen: 14.293 ug/L
RT: 4.661 min Scan# 1033
Delta R.T. 0.000 min
Lab File: VU052880.D
Acq: 31 Jan 2023 15:19




Instrument :
MSVOA_U
ClientSampleId :
A44L8


Tgt Ion: 96 Resp: 28993
Ion Ratio Lower Upper
96 100
61 118.8 84.1 156.1
68 0.0 0.0 0.0

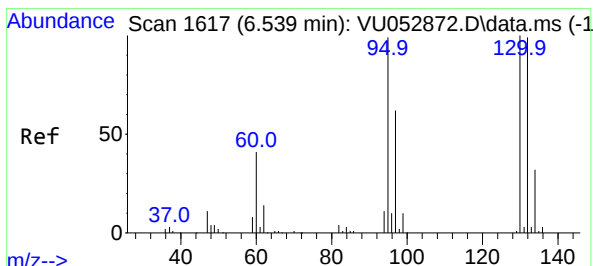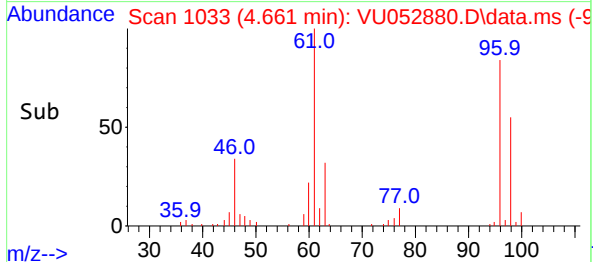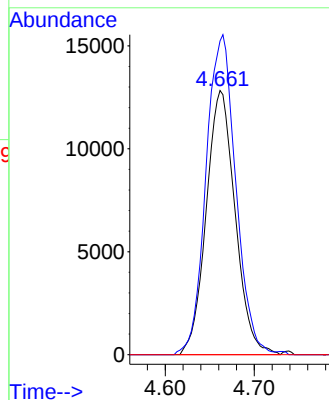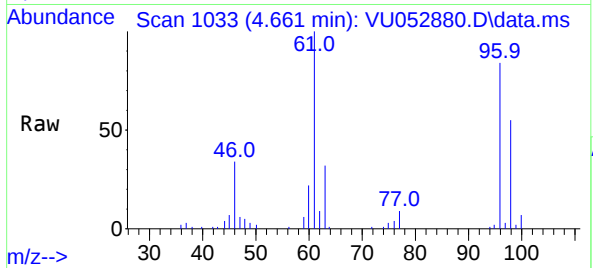

#34
Trichloroethene
Concen: 11.581 ug/L
RT: 6.539 min Scan# 1617
Delta R.T. 0.000 min
Lab File: VU052880.D
Acq: 31 Jan 2023 15:19


Tgt Ion: 95 Resp: 23883
Ion Ratio Lower Upper
95 100
97 62.6 44.5 82.7
132 101.7 66.8 124.0
130 103.5 71.9 133.5

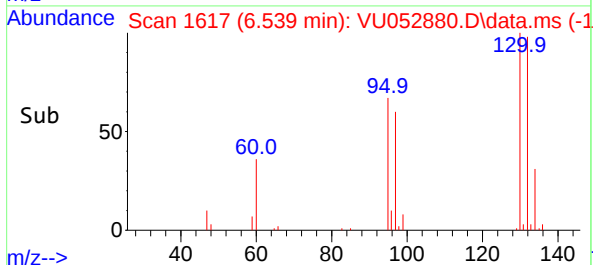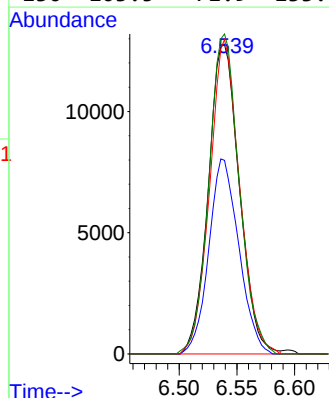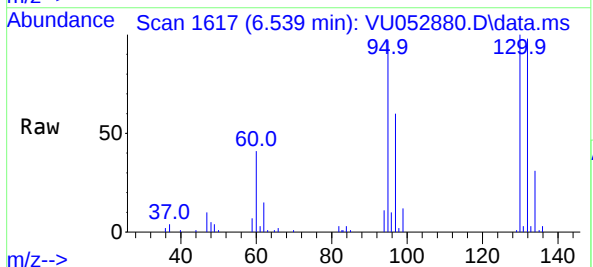

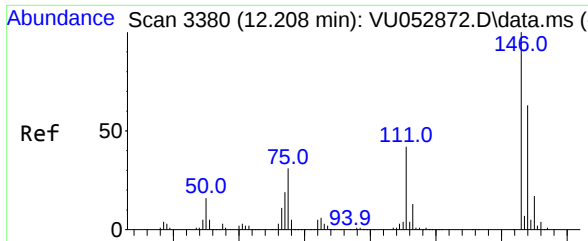

#67
 1,2-Dichlorobenzene
 Concen: 2.558 ug/L
 RT: 12.208 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VU052880.D
 Acq: 31 Jan 2023 15:19

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L8

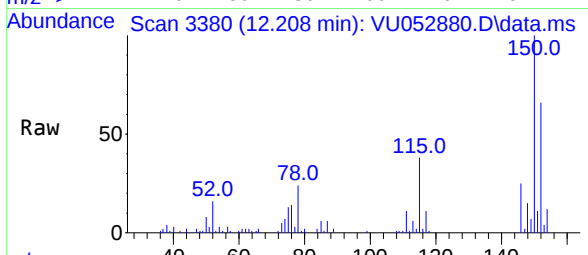

Tgt Ion:146 Resp: 8693

Ion	Ratio	Lower	Upper
146	100		
111	41.7	33.2	49.8
148	58.7	50.2	75.4

