

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052890.D
 Acq On : 31 Jan 2023 19:37
 Operator : JC/MD
 Sample : 01381-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N1

Quant Time: Feb 01 00:59:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 01 00:53:48 2023
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	232379	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	225349	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	102036	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	84141	50.307	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery	= 100.620%		
7) Chloroethane-d5	1.906	69	74208	53.846	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery	= 107.700%		
11) 1,1-Dichloroethene-d2	2.562	63	123988	37.271	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery	= 74.540%		
21) 2-Butanone-d5	4.620	46	96553	93.448	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery	= 93.450%		
24) Chloroform-d	5.057	84	173700	48.662	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	= 97.320%		
26) 1,2-Dichloroethane-d4	5.697	65	116968	51.320	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	= 102.640%		
32) Benzene-d6	5.722	84	336184	48.830	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	= 97.660%		
36) 1,2-Dichloropropane-d6	6.684	67	102101	50.565	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery	= 101.120%		
41) Toluene-d8	7.893	98	289600	46.194	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery	= 92.380%		
43) trans-1,3-Dichloroprop...	8.176	79	47000	46.440	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery	= 92.880%		
47) 2-Hexanone-d5	8.635	63	64781	91.307	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery	= 91.310%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	139955	46.912	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery	= 93.820%		
66) 1,2-Dichlorobenzene-d4	12.188	152	108663	54.845	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery	= 109.700%		
Target Compounds						
						Qvalue
20) cis-1,2-Dichloroethene	4.661	96	19857	10.011	ug/L	99
34) Trichloroethene	6.539	95	56626	29.043	ug/L	96
51) Chlorobenzene	9.443	112	55977	10.349	ug/L	97
64) 1,3-Dichlorobenzene	11.745	146	3034	0.913	ug/L	97
65) 1,4-Dichlorobenzene	11.831	146	20228	5.877	ug/L	96
67) 1,2-Dichlorobenzene	12.208	146	97719	29.057	ug/L	96
70) 1,2,4-trichlorobenzene	13.838	180	12102	5.864	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052890.D
Acq On : 31 Jan 2023 19:37
Operator : JC/MD
Sample : 01381-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N1

Quant Time: Feb 01 00:59:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 01 00:53:48 2023
Response via : Initial Calibration




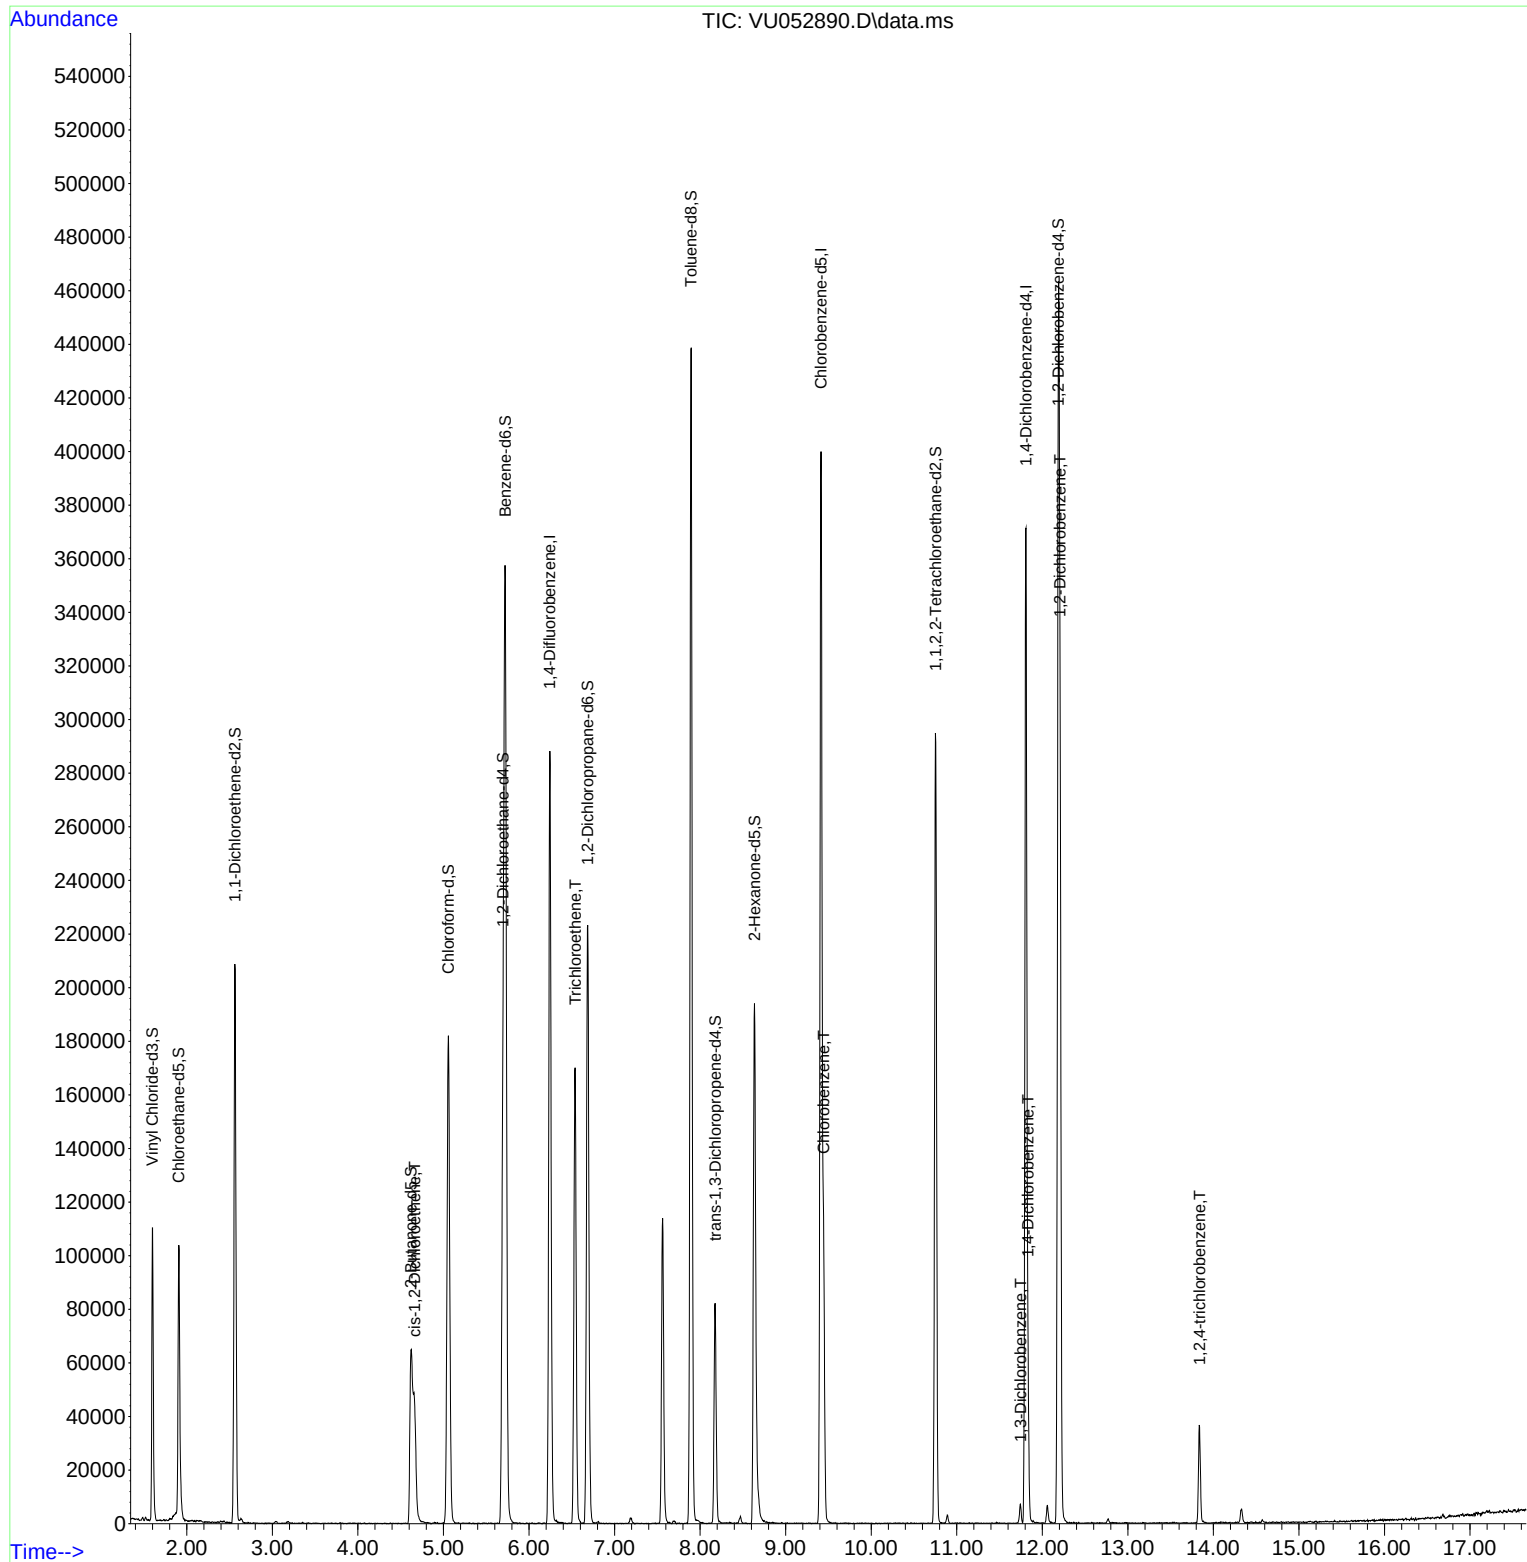


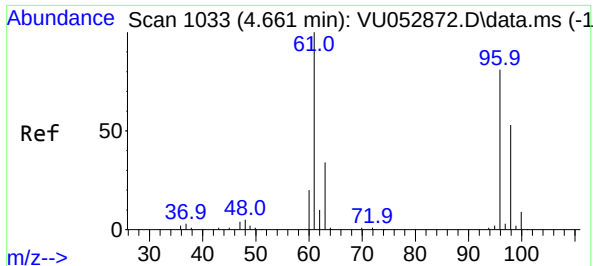

#20
cis-1,2-Dichloroethene
Concen: 10.011 ug/L
RT: 4.661 min Scan# 1033
Delta R.T. -0.000 min
Lab File: VU052890.D
Acq: 31 Jan 2023 19:37




Instrument :
MSVOA_U
ClientSampleId :
A44N1


Tgt Ion: 96 Resp: 19857
Ion Ratio Lower Upper
96 100
61 121.0 84.1 156.1
68 0.0 0.0 0.0

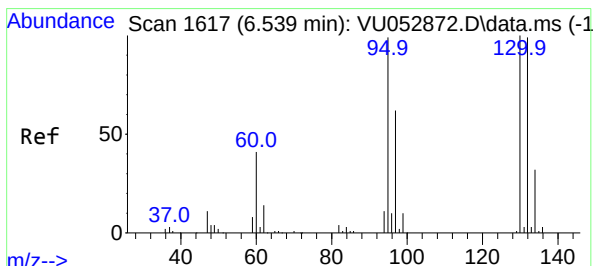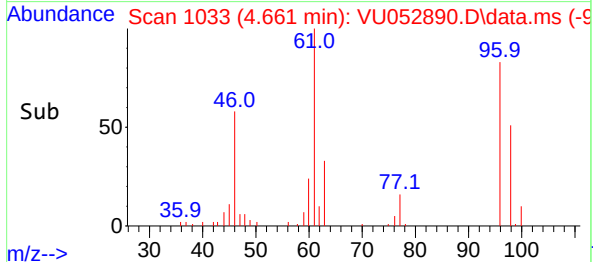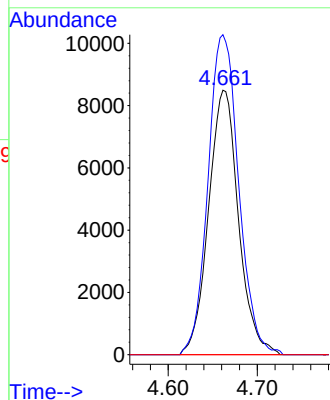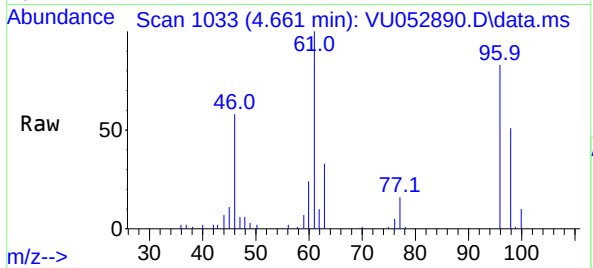

#34
Trichloroethene
Concen: 29.043 ug/L
RT: 6.539 min Scan# 1617
Delta R.T. -0.000 min
Lab File: VU052890.D
Acq: 31 Jan 2023 19:37

Tgt Ion: 95 Resp: 56626
Ion Ratio Lower Upper
95 100
97 65.5 44.5 82.7
132 104.3 66.8 124.0
130 104.0 71.9 133.5

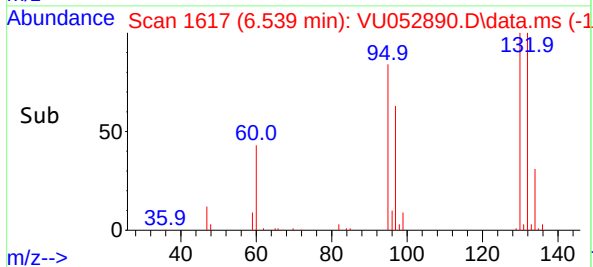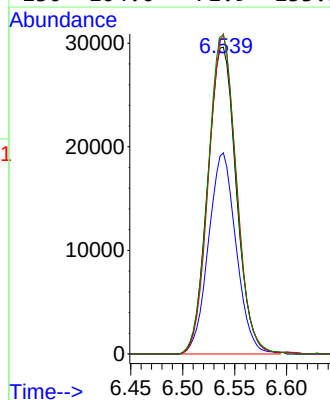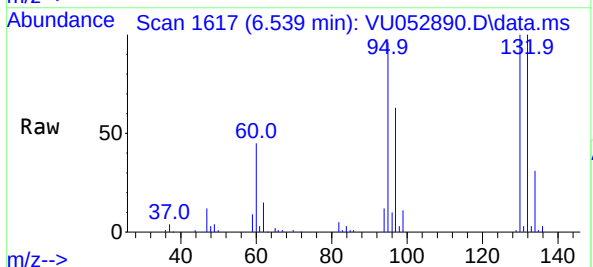

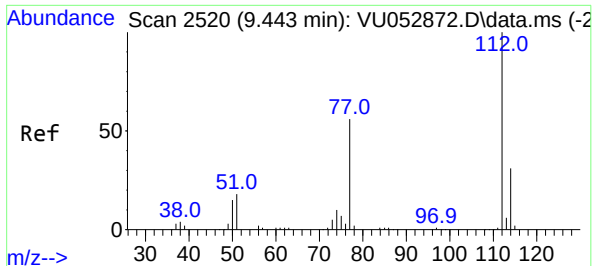

#51

Chlorobenzene

Concen: 10.349 ug/L

RT: 9.443 min Scan# 21

Delta R.T. -0.000 min

Lab File: VU052890.D

Acq: 31 Jan 2023 19:37

Instrument :

MSVOA_U

ClientSampleId :

A44N1





Tgt Ion:112 Resp: 55977

Ion Ratio Lower Upper

112 100

114 34.5 22.8 42.4

77 60.0 45.9 68.9

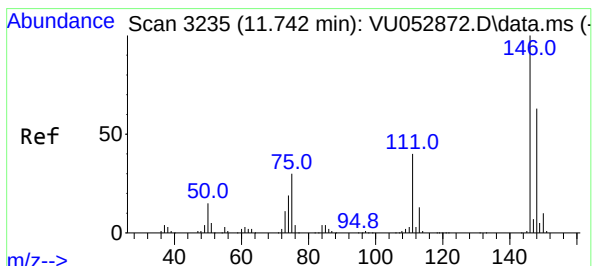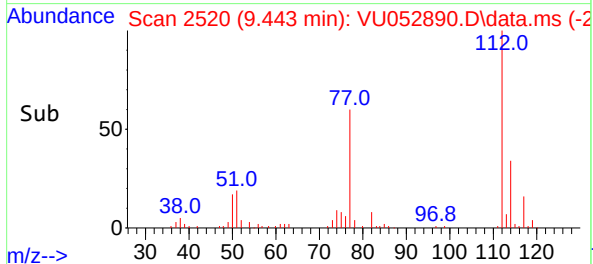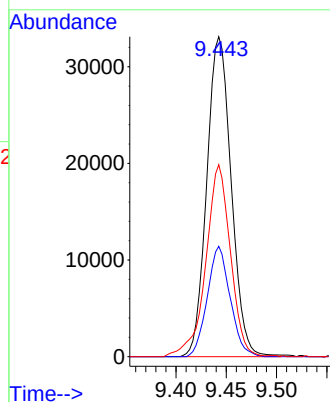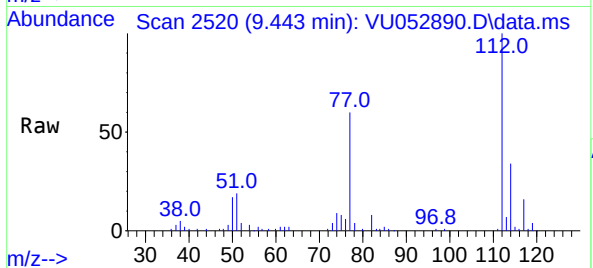

#64

1,3-Dichlorobenzene

Concen: 0.913 ug/L

RT: 11.745 min Scan# 3236

Delta R.T. 0.003 min

Lab File: VU052890.D

Acq: 31 Jan 2023 19:37




Tgt Ion:146 Resp: 3034


Ion Ratio Lower Upper

146 100

111 41.7 27.8 51.6

148 66.7 45.5 84.5


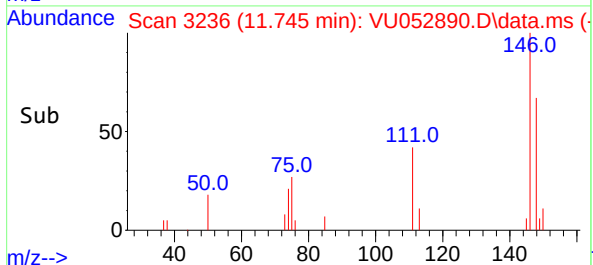
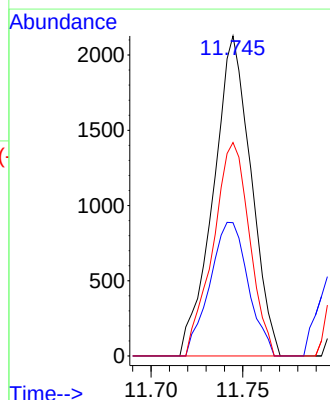
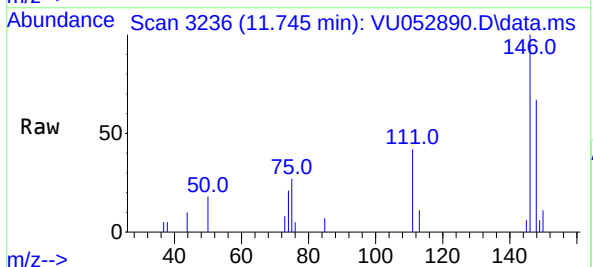


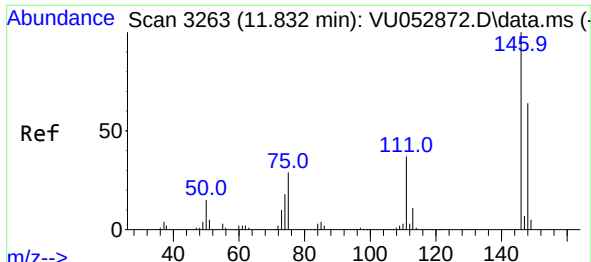

#65
1,4-Dichlorobenzene
Concen: 5.877 ug/L
RT: 11.831 min Scan# 31
Delta R.T. -0.000 min
Lab File: VU052890.D
Acq: 31 Jan 2023 19:37




Instrument :
MSVOA_U
ClientSampleId :
A44N1


Tgt Ion:146 Resp: 20228
Ion Ratio Lower Upper
146 100
111 36.3 26.7 49.7
148 61.0 45.6 84.6

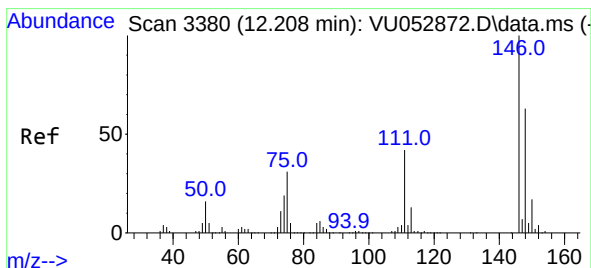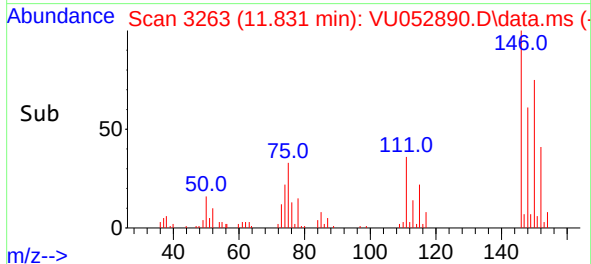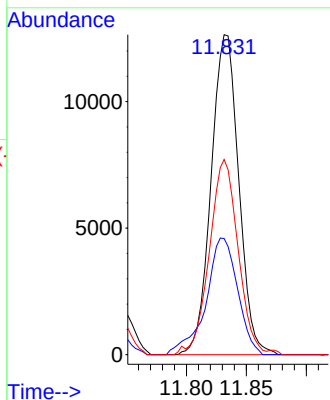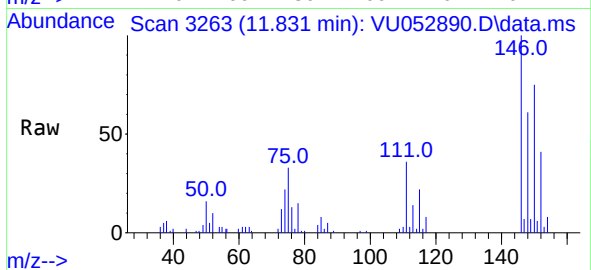

#67
1,2-Dichlorobenzene
Concen: 29.057 ug/L
RT: 12.208 min Scan# 3380
Delta R.T. -0.000 min
Lab File: VU052890.D
Acq: 31 Jan 2023 19:37


Tgt Ion:146 Resp: 97719
Ion Ratio Lower Upper
146 100
111 43.7 33.2 49.8
148 66.1 50.2 75.4

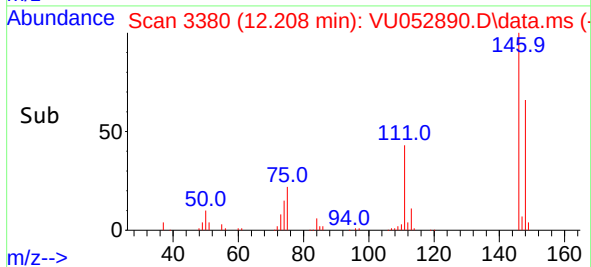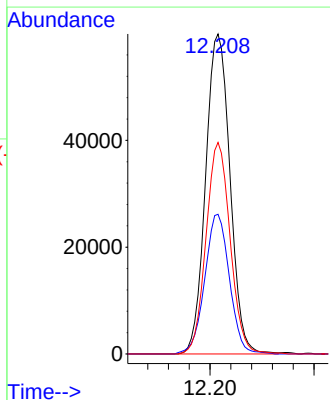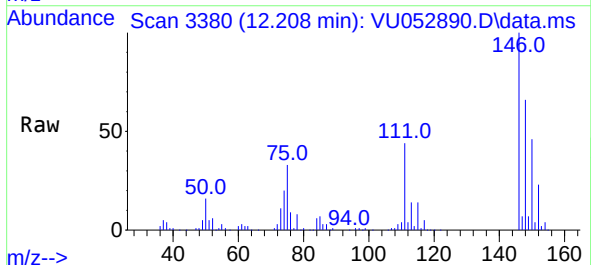

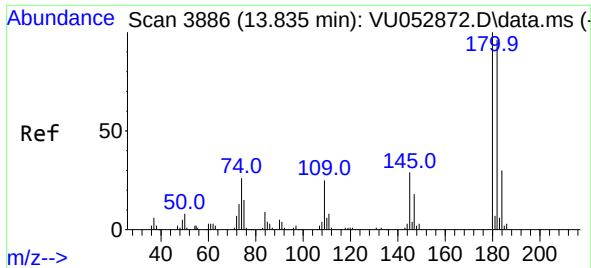

#70
 1,2,4-trichlorobenzene
 Concen: 5.864 ug/L
 RT: 13.838 min Scan# 3887
 Delta R.T. 0.003 min
 Lab File: VU052890.D
 Acq: 31 Jan 2023 19:37

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N1

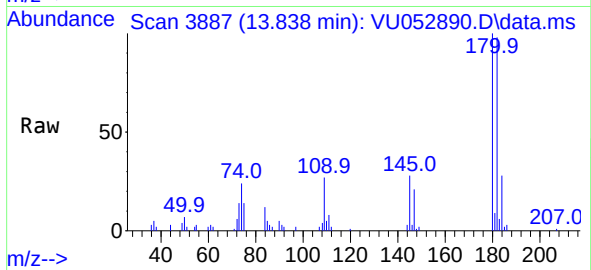

Tgt Ion:	180	Resp:	12102
Ion	Ratio	Lower	Upper
180	100		
182	99.0	78.2	117.2
145	28.2	23.4	35.2

