

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052892.D
 Acq On : 31 Jan 2023 20:24
 Operator : JC/MD
 Sample : 01381-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M7

Quant Time: Feb 01 01:00:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 01 00:53:48 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	246179	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	247939	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	144985	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	83197	46.954	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	93.900%		
7) Chloroethane-d5	1.909	69	74468	51.006	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	102.020%		
11) 1,1-Dichloroethene-d2	2.565	63	127429	36.158	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	72.320%		
21) 2-Butanone-d5	4.620	46	101586	92.808	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	92.810%		
24) Chloroform-d	5.060	84	172187	45.534	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.060%		
26) 1,2-Dichloroethane-d4	5.697	65	116185	48.118	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.240%		
32) Benzene-d6	5.723	84	340306	44.925	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.860%		
36) 1,2-Dichloropropane-d6	6.684	67	101065	45.492	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	90.980%		
41) Toluene-d8	7.893	98	298537	43.281	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.560%		
43) trans-1,3-Dichloroprop...	8.173	79	48950	43.960	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.920%		
47) 2-Hexanone-d5	8.629	63	67462	86.422	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.420%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	139373	42.461	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	84.920%		
66) 1,2-Dichlorobenzene-d4	12.195	152	139748	49.640	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.280%		
Target Compounds						Qvalue
5) Vinyl chloride	1.604	62	11621	5.525	ug/L	83
12) 1,1-Dichloroethene	2.581	96	10614	5.828	ug/L #	1
17) trans-1,2-Dichloroethene	3.353	96	19331	9.822	ug/L	98
18) Methyl tert-butyl Ether	3.359	73	10172	1.758	ug/L #	89
20) cis-1,2-Dichloroethene	4.661	96	2427816	1155.412	ug/L	98
33) Benzene	5.771	78	279316	33.095	ug/L	100
34) Trichloroethene	6.536	95	160515	74.826	ug/L	96
35) Methylcyclohexane	6.761	83	3406	1.003	ug/L	87
51) Chlorobenzene	9.449	112	13393570	2250.628	ug/L	98
52) Ethylbenzene	9.568	91	213132	23.057	ug/L	99
54) o-xylene	10.099	106	5181	1.450	ug/L	97
64) 1,3-Dichlorobenzene	11.742	146	242373	51.303	ug/L	99
65) 1,4-Dichlorobenzene	11.832	146	2204122	450.666	ug/L	99
67) 1,2-Dichlorobenzene	12.217	146	11797705	2468.911	ug/L	98
70) 1,2,4-trichlorobenzene	13.838	180	3029913	1033.298	ug/L	98
72) 1,2,3-Trichlorobenzene	14.323	180	649834	209.699	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_U
ClientSampleId :
A44M7

Quant Time: Feb 01 01:00:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 01 00:53:48 2023
Response via : Initial Calibration







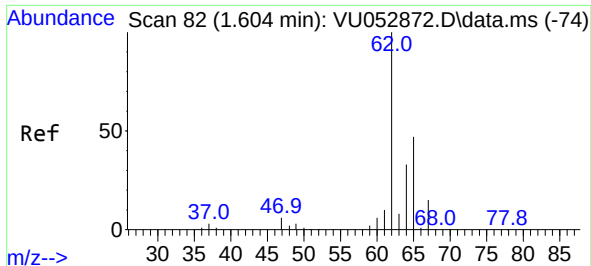

#5
 Vinyl chloride
 Concen: 5.525 ug/L
 RT: 1.604 min Scan# 81
 Delta R.T. 0.000 min
 Lab File: VU052892.D
 Acq: 31 Jan 2023 20:24




Instrument :
 MSVOA_U
 ClientSampleId :
 A44M7


Tgt Ion: 62 Resp: 11621
 Ion Ratio Lower Upper
 62 100
 64 41.5 22.4 41.6

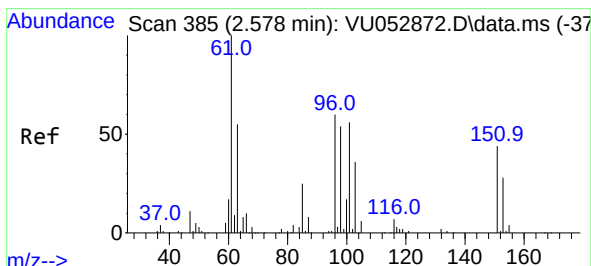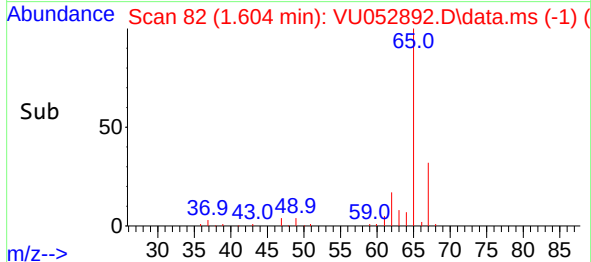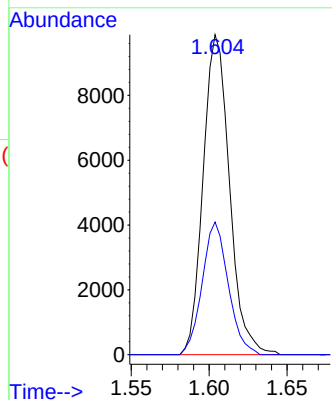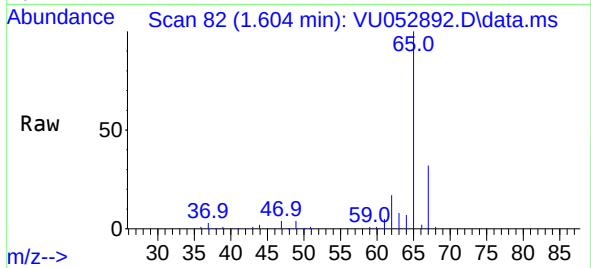

#12
 1,1-Dichloroethene
 Concen: 5.828 ug/L
 RT: 2.581 min Scan# 386
 Delta R.T. 0.003 min
 Lab File: VU052892.D
 Acq: 31 Jan 2023 20:24

Tgt Ion: 96 Resp: 10614
 Ion Ratio Lower Upper
 96 100
 61 198.5 114.3 212.3
 63 465.3 80.6 149.6#


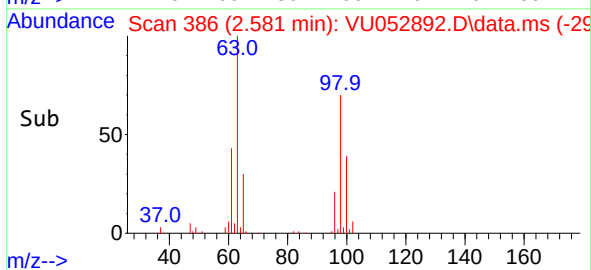
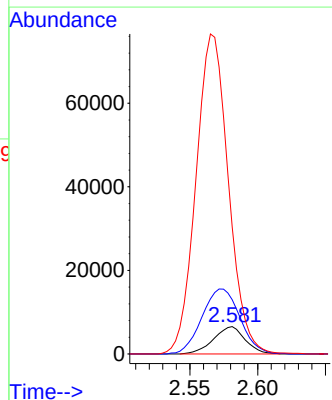
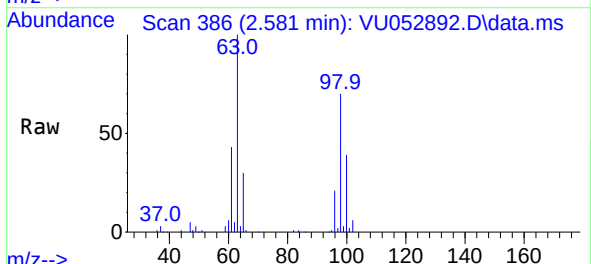


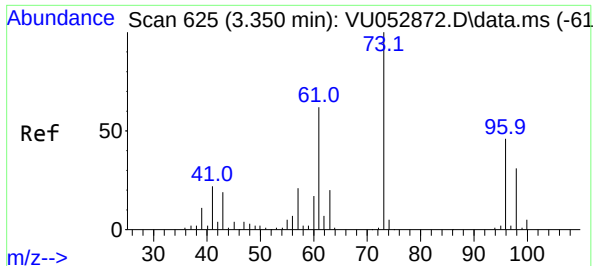

#17
trans-1,2-Dichloroethene
Concen: 9.822 ug/L
RT: 3.353 min Scan# 61
Delta R.T. 0.003 min
Lab File: VU052892.D
Acq: 31 Jan 2023 20:24




Instrument :
MSVOA_U
ClientSampleId :
A44M7


Tgt Ion: 96 Resp: 19331
Ion Ratio Lower Upper
96 100
61 130.5 92.7 172.3
98 62.9 44.7 82.9

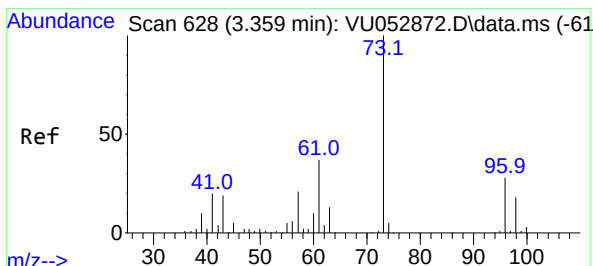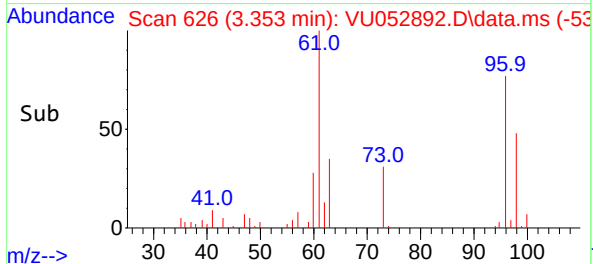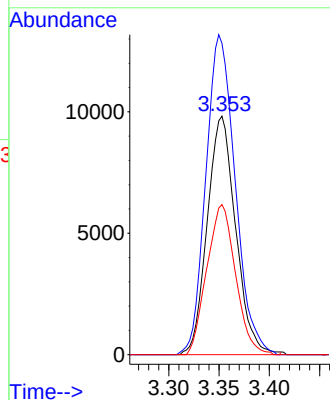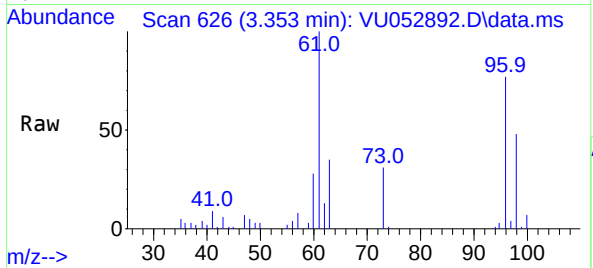

#18
Methyl tert-butyl Ether
Concen: 1.758 ug/L
RT: 3.359 min Scan# 628
Delta R.T. 0.000 min
Lab File: VU052892.D
Acq: 31 Jan 2023 20:24

Tgt Ion: 73 Resp: 10172
Ion Ratio Lower Upper
73 100
43 22.0 14.2 21.2#
57 25.6 16.3 24.5#


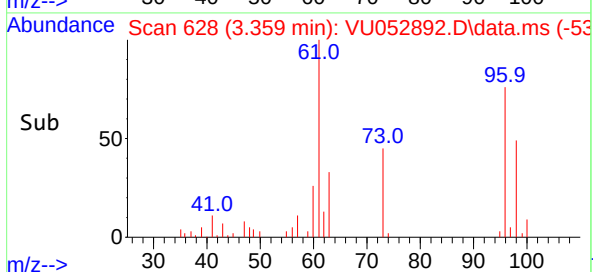
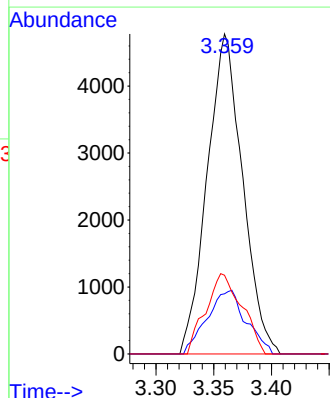
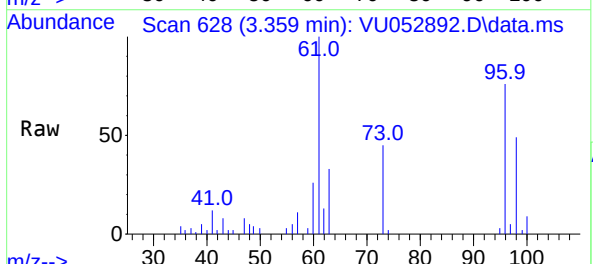


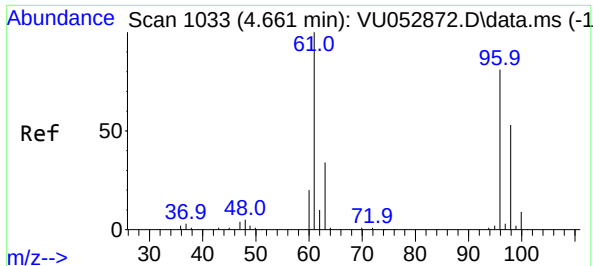

#20
cis-1,2-Dichloroethene
Concen: 1155.412 ug/L
RT: 4.661 min Scan# 1033
Delta R.T. 0.000 min
Lab File: VU052892.D
Acq: 31 Jan 2023 20:24




Instrument :
MSVOA_U
ClientSampleId :
A44M7


Tgt Ion: 96 Resp: 2427816
Ion Ratio Lower Upper
96 100
61 122.7 84.1 156.1
68 0.0 0.0 0.0

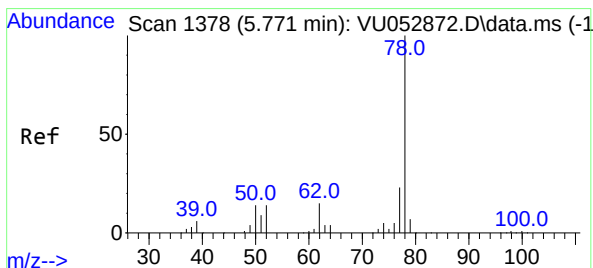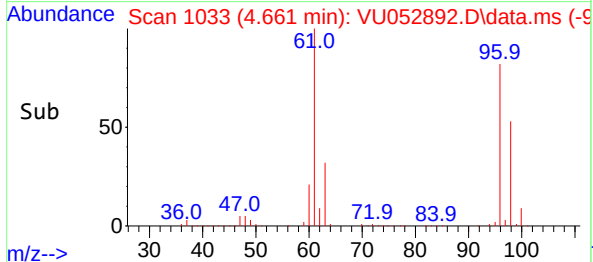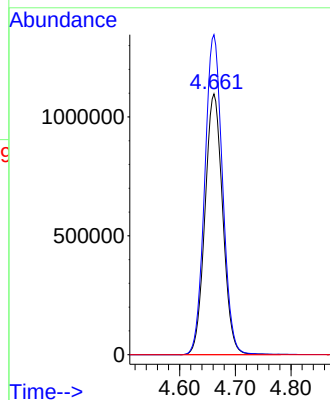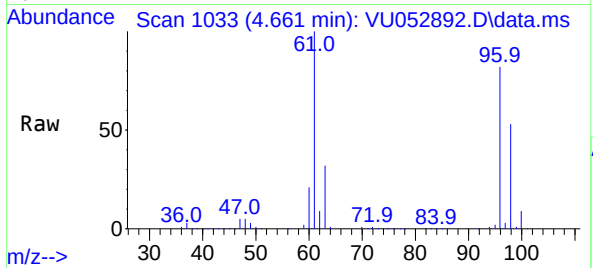

#33
Benzene
Concen: 33.095 ug/L
RT: 5.771 min Scan# 1378
Delta R.T. 0.000 min
Lab File: VU052892.D
Acq: 31 Jan 2023 20:24

Tgt Ion: 78 Resp: 279316

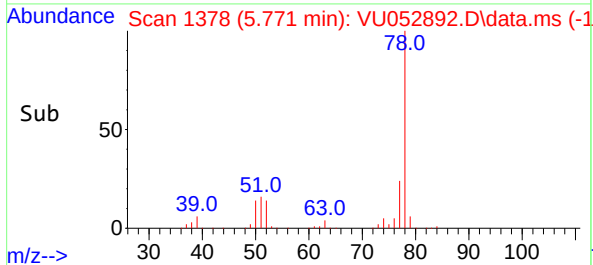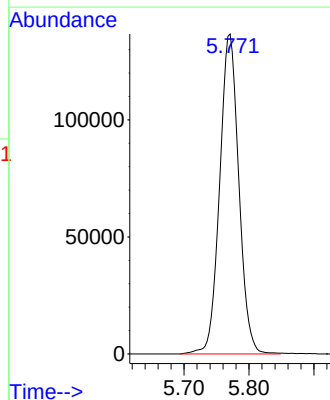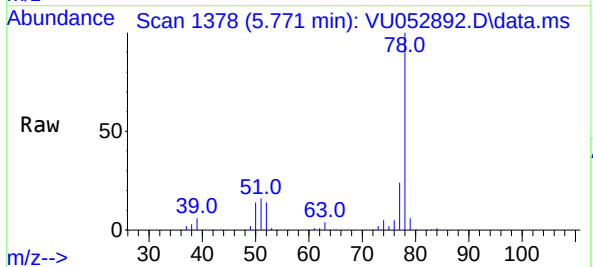

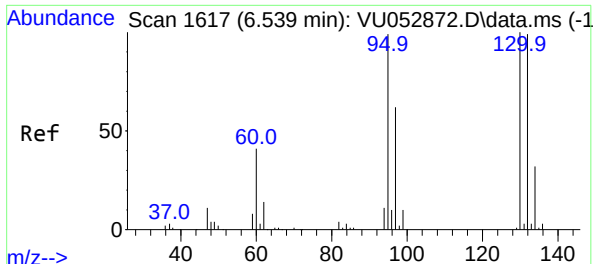

#34

Trichloroethene

Concen: 74.826 ug/L

RT: 6.536 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU052892.D

Acq: 31 Jan 2023 20:24

Instrument :

MSVOA_U

ClientSampleId :

A44M7

Tgt Ion: 95 Resp: 160515





Ion Ratio Lower Upper

95 100

97 65.3 44.5 82.7

132 102.9 66.8 124.0

130 103.3 71.9 133.5

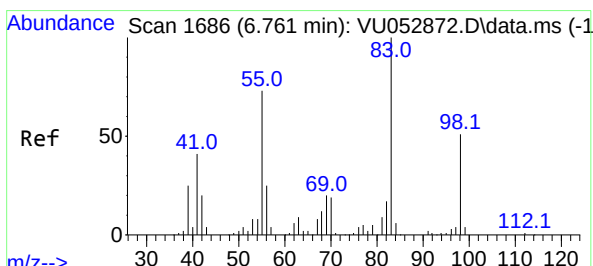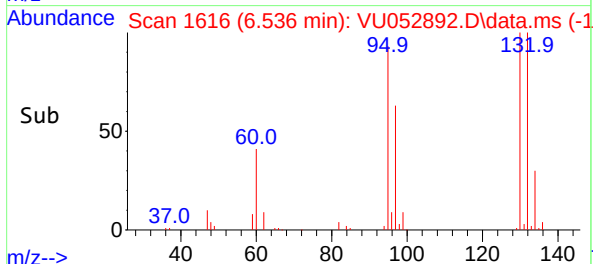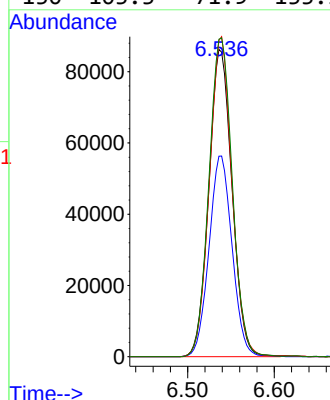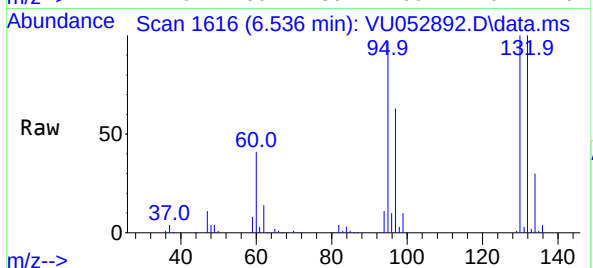

#35

Methylcyclohexane

Concen: 1.003 ug/L

RT: 6.761 min Scan# 1686

Delta R.T. 0.000 min

Lab File: VU052892.D

Acq: 31 Jan 2023 20:24




Tgt Ion: 83 Resp: 3406


Ion Ratio Lower Upper

83 100

55 82.6 57.1 85.7

98 40.9 38.9 58.3


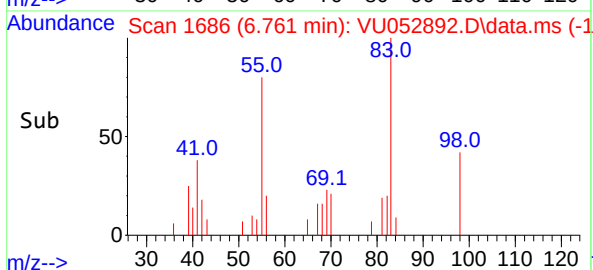
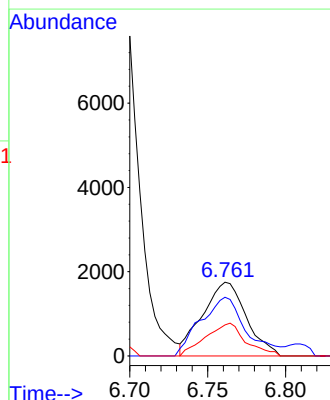
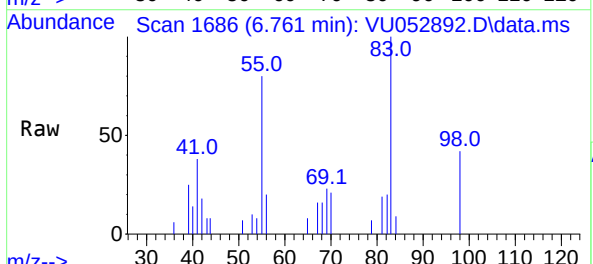


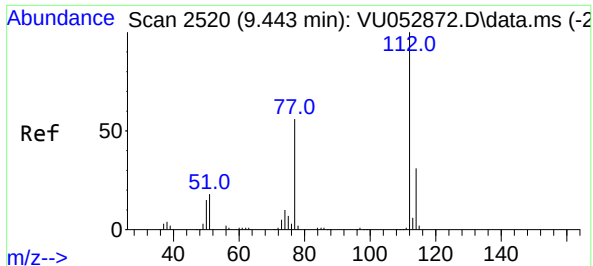

#51
Chlorobenzene
Concen: 2250.628 ug/L
RT: 9.449 min Scan# 21
Delta R.T. 0.007 min
Lab File: VU052892.D
Acq: 31 Jan 2023 20:24




Instrument :
MSVOA_U
ClientSampleId :
A44M7


Tgt Ion:112 Resp:13393570
Ion Ratio Lower Upper
112 100
114 33.0 22.8 42.4
77 59.2 45.9 68.9

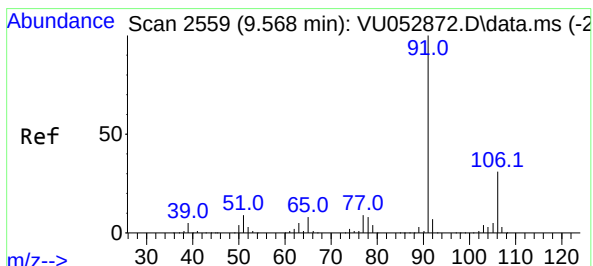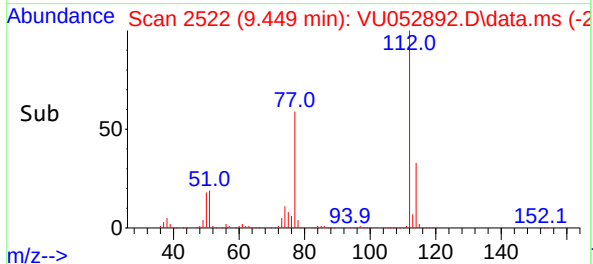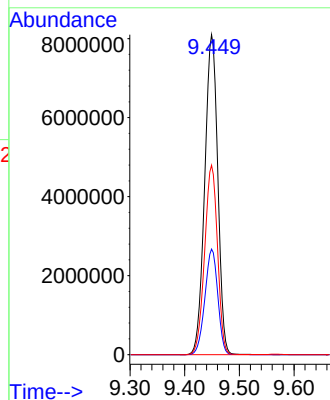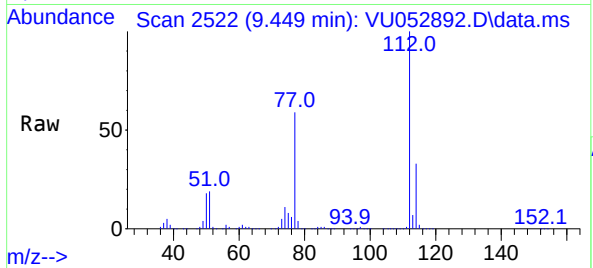

#52
Ethylbenzene
Concen: 23.057 ug/L
RT: 9.568 min Scan# 2559
Delta R.T. 0.000 min
Lab File: VU052892.D
Acq: 31 Jan 2023 20:24

Tgt Ion: 91 Resp: 213132
Ion Ratio Lower Upper
91 100
106 31.7 22.0 40.8


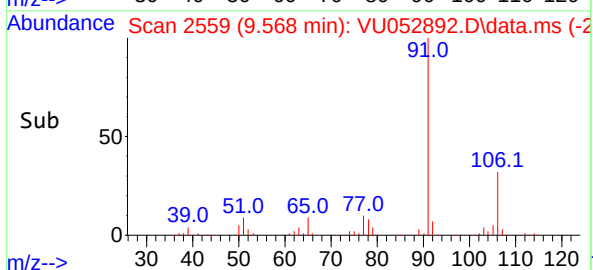
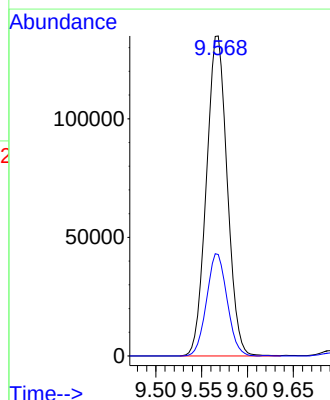
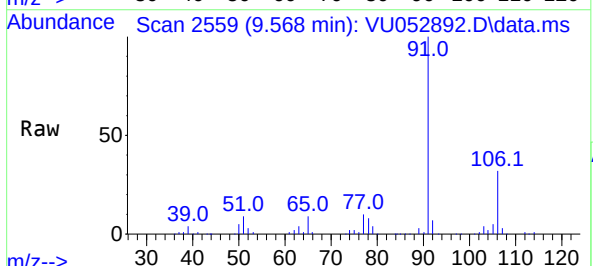


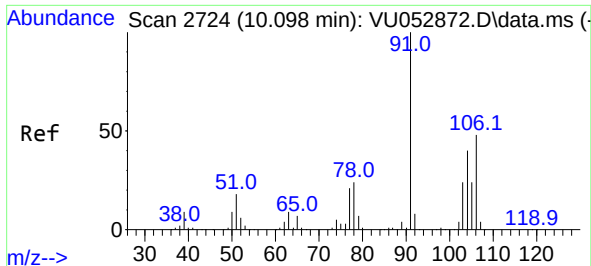

#54
o-xylene
Concen: 1.450 ug/L
RT: 10.099 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU052892.D
Acq: 31 Jan 2023 20:24




Instrument :
MSVOA_U
ClientSampleId :
A44M7


Tgt Ion:106 Resp: 5181
Ion Ratio Lower Upper
106 100
91 200.9 143.4 266.2

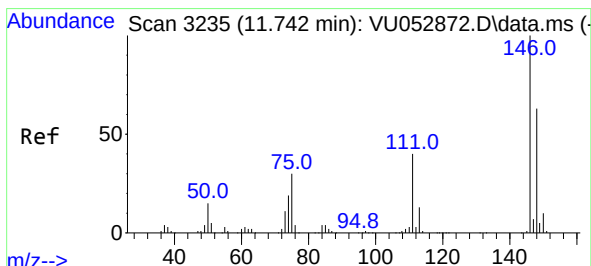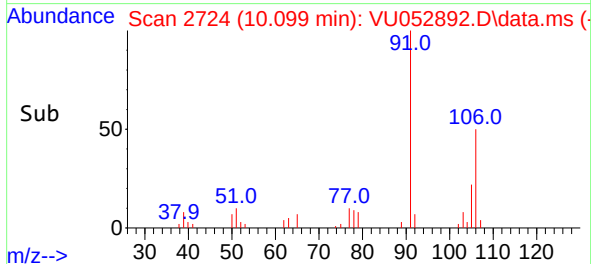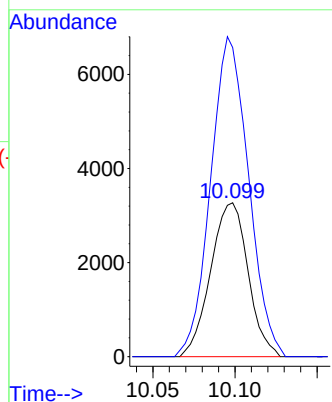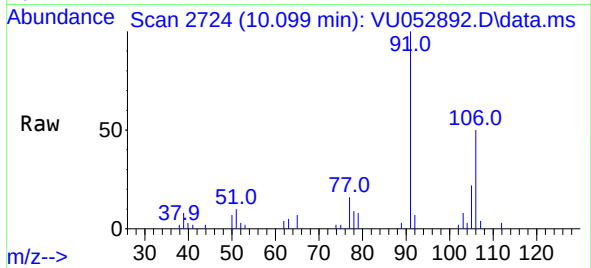

#64
1,3-Dichlorobenzene
Concen: 51.303 ug/L
RT: 11.742 min Scan# 3235
Delta R.T. 0.000 min
Lab File: VU052892.D
Acq: 31 Jan 2023 20:24


Tgt Ion:146 Resp: 242373
Ion Ratio Lower Upper
146 100
111 39.0 27.8 51.6
148 64.4 45.5 84.5

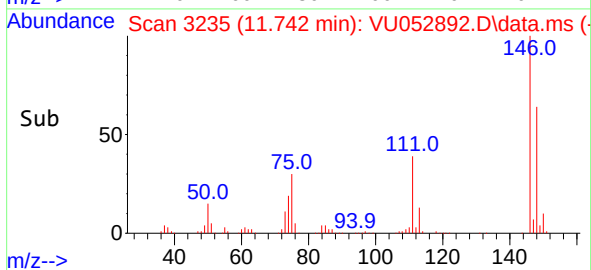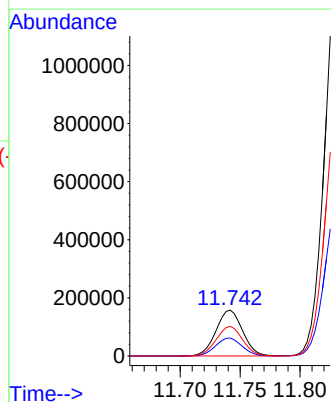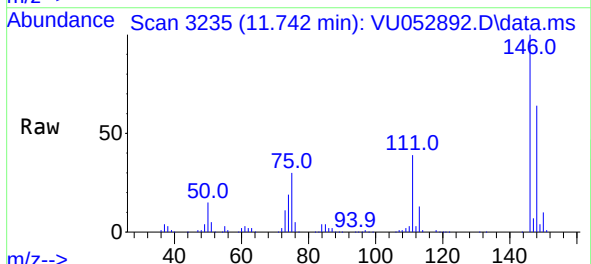

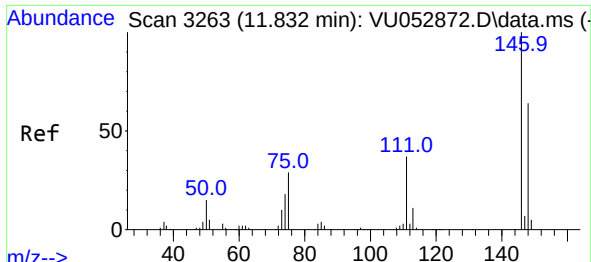




#65
1,4-Dichlorobenzene
Concen: 450.666 ug/L
RT: 11.832 min Scan# 31
Delta R.T. 0.000 min
Lab File: VU052892.D
Acq: 31 Jan 2023 20:24

Instrument :
MSVOA_U
ClientSampleId :
A44M7

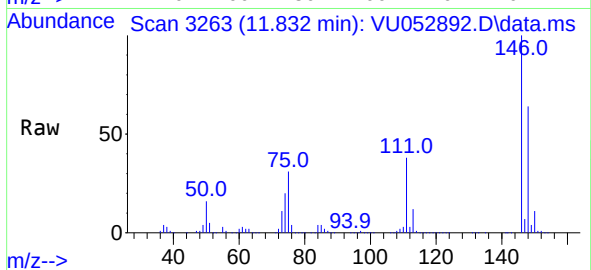


Tgt Ion:146 Resp: 2204122

Ion	Ratio	Lower	Upper
146	100		
111	38.5	26.7	49.7
148	64.1	45.6	84.6

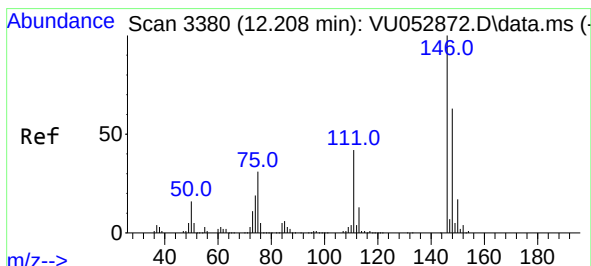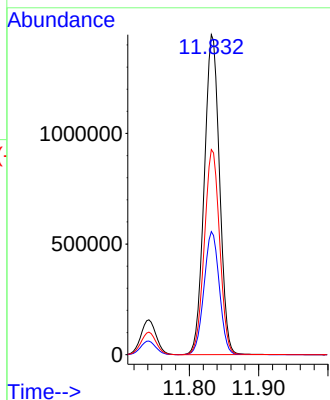
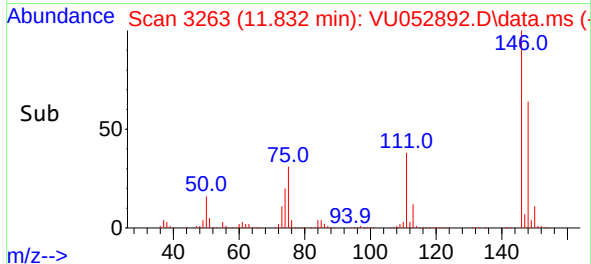



#67
1,2-Dichlorobenzene
Concen: 2468.911 ug/L
RT: 12.217 min Scan# 3383
Delta R.T. 0.010 min
Lab File: VU052892.D
Acq: 31 Jan 2023 20:24

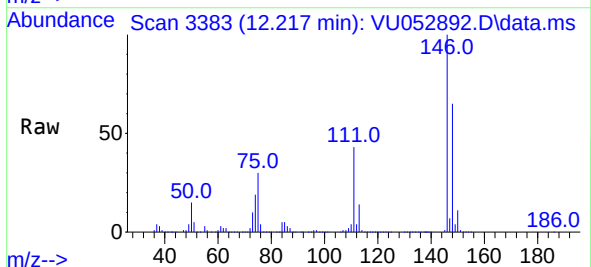

Tgt Ion:146 Resp:11797705

Ion	Ratio	Lower	Upper
146	100		
111	42.6	33.2	49.8
148	64.7	50.2	75.4



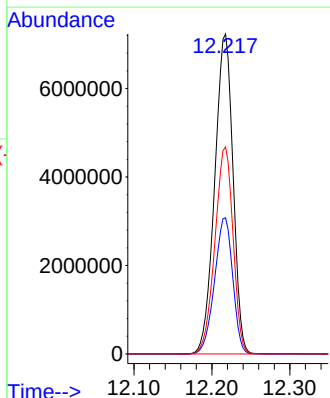
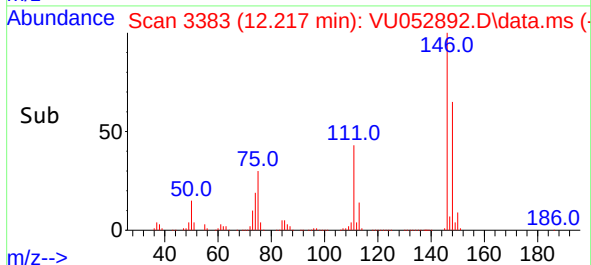


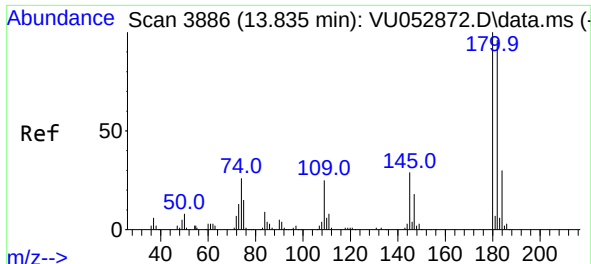

#70
1,2,4-trichlorobenzene
Concen: 1033.298 ug/L
RT: 13.838 min Scan# 3887
Delta R.T. 0.003 min
Lab File: VU052892.D
Acq: 31 Jan 2023 20:24

Instrument :
MSVOA_U
ClientSampleId :
A44M7

Tgt Ion:180 Resp: 3029913
Ion Ratio Lower Upper
180 100
182 95.9 78.2 117.2
145 30.1 23.4 35.2

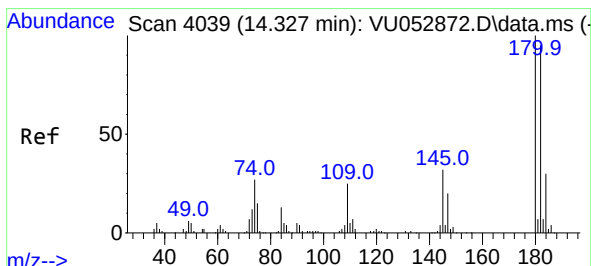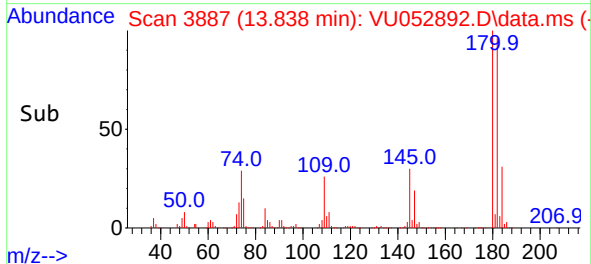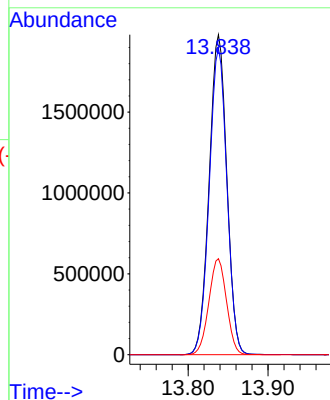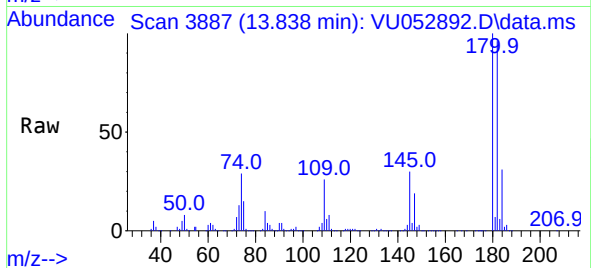

#72
1,2,3-Trichlorobenzene
Concen: 209.699 ug/L
RT: 14.323 min Scan# 4038
Delta R.T. -0.003 min
Lab File: VU052892.D
Acq: 31 Jan 2023 20:24

Tgt Ion:180 Resp: 649834
Ion Ratio Lower Upper
180 100
182 95.1 77.5 116.3
145 31.7 24.2 36.4

