

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052876.D
 Acq On : 31 Jan 2023 13:45
 Operator : JC/MD
 Sample : 01314-03DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M

Title : VOC Analysis

Signal : TIC: VU052876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	70511	85467	10.85%	1.311%
2	1.909	169	177	196	rVB	73885	103664	13.16%	1.590%
3	2.472	349	352	356	rVB	306	178	0.02%	0.003%
4	2.565	369	381	397	rBV	154297	247808	31.46%	3.802%
5	2.813	455	458	461	rVB	202	130	0.02%	0.002%
6	3.048	523	531	539	rVB4	1352	2148	0.27%	0.033%
7	3.118	550	553	557	rBV	290	285	0.04%	0.004%
8	3.183	562	573	584	rVV3	3665	7958	1.01%	0.122%
9	3.404	639	642	645	rBB	158	129	0.02%	0.002%
10	3.568	688	693	695	rBB	176	168	0.02%	0.003%
11	3.588	695	699	702	rBV	232	243	0.03%	0.004%
12	3.697	729	733	735	rBV	183	165	0.02%	0.003%
13	3.742	745	747	750	rBB	281	134	0.02%	0.002%
14	3.819	768	771	773	rBV	336	185	0.02%	0.003%
15	3.906	795	798	800	rBB	308	149	0.02%	0.002%
16	4.105	857	860	862	rVB	269	149	0.02%	0.002%
17	4.141	866	871	872	rBV	248	208	0.03%	0.003%
18	4.260	905	908	911	rBV	177	171	0.02%	0.003%
19	4.388	945	948	950	rBV2	234	174	0.02%	0.003%
20	4.475	972	975	977	rBB2	233	128	0.02%	0.002%
21	4.620	1007	1020	1049	rVV	64236	182953	23.23%	2.807%
22	4.861	1092	1095	1099	rBV2	201	177	0.02%	0.003%
23	4.880	1099	1101	1103	rVB	391	158	0.02%	0.002%
24	4.900	1104	1107	1110	rBV	229	177	0.02%	0.003%
25	4.938	1116	1119	1122	rBV	285	216	0.03%	0.003%
26	5.006	1136	1140	1141	rBV	383	259	0.03%	0.004%
27	5.057	1141	1156	1183	rVB	156780	343627	43.62%	5.272%
28	5.202	1198	1201	1203	rBV	162	126	0.02%	0.002%
29	5.256	1215	1218	1219	rBV	279	141	0.02%	0.002%
30	5.285	1224	1227	1229	rBV	429	278	0.04%	0.004%
31	5.359	1245	1250	1251	rBV	194	186	0.02%	0.003%
32	5.404	1261	1264	1268	rBB	153	148	0.02%	0.002%
33	5.620	1326	1331	1334	rBV	224	260	0.03%	0.004%
34	5.719	1341	1362	1388	rBV2	284514	787727	100.00%	12.085%
35	5.903	1415	1419	1422	rBB	152	146	0.02%	0.002%
36	6.063	1466	1469	1474	rBV2	369	286	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052876.D
 Acq On : 31 Jan 2023 13:45
 Operator : JC/MD
 Sample : 01314-03DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.173	1500	1503	1505	rBV	167	143	0.02%	0.002%
38	6.244	1512	1525	1551	rBV	279213	524973	66.64%	8.054%
39	6.536	1603	1616	1635	rBV	256687	480653	61.02%	7.374%
40	6.687	1647	1663	1686	rBV	187613	364664	46.29%	5.595%
41	6.903	1726	1730	1733	rBV	220	221	0.03%	0.003%
42	6.961	1744	1748	1753	rBB	218	207	0.03%	0.003%
43	6.989	1754	1757	1759	rBV	253	171	0.02%	0.003%
44	7.057	1775	1778	1783	rBV	233	282	0.04%	0.004%
45	7.186	1810	1818	1820	rBV2	1243	1589	0.20%	0.024%
46	7.231	1830	1832	1835	rBV	188	145	0.02%	0.002%
47	7.288	1846	1850	1851	rBV	239	139	0.02%	0.002%
48	7.324	1859	1861	1866	rBV	216	219	0.03%	0.003%
49	7.398	1879	1884	1887	rBV	206	217	0.03%	0.003%
50	7.504	1913	1917	1918	rBV	196	159	0.02%	0.002%
51	7.562	1923	1935	1954	rVV	95360	165092	20.96%	2.533%
52	7.652	1961	1963	1967	rVB2	280	210	0.03%	0.003%
53	7.694	1968	1976	1986	rBV3	924	1914	0.24%	0.029%
54	7.784	2002	2004	2007	rBV	187	149	0.02%	0.002%
55	7.816	2011	2014	2018	rVB	305	252	0.03%	0.004%
56	7.893	2024	2038	2058	rBV	343175	584180	74.16%	8.962%
57	8.025	2076	2079	2084	rBV2	377	427	0.05%	0.007%
58	8.051	2084	2087	2092	rBV3	355	379	0.05%	0.006%
59	8.092	2098	2100	2103	rBB2	305	186	0.02%	0.003%
60	8.121	2107	2109	2113	rBB	259	150	0.02%	0.002%
61	8.176	2114	2126	2140	rBV	67270	113716	14.44%	1.745%
62	8.327	2169	2173	2175	rBV	266	166	0.02%	0.003%
63	8.465	2208	2216	2226	rBV3	1612	2550	0.32%	0.039%
64	8.555	2240	2244	2247	rBV	215	225	0.03%	0.003%
65	8.632	2256	2268	2295	rBV3	174492	341529	43.36%	5.240%
66	8.841	2330	2333	2336	rBV2	244	153	0.02%	0.002%
67	8.893	2346	2349	2351	rVB2	276	179	0.02%	0.003%
68	8.915	2351	2356	2357	rBV	144	146	0.02%	0.002%
69	8.944	2363	2365	2368	rBV	176	134	0.02%	0.002%
70	8.967	2368	2372	2373	rBV	230	163	0.02%	0.003%
71	9.044	2393	2396	2402	rVB2	320	354	0.04%	0.005%
72	9.083	2403	2408	2410	rBV2	313	297	0.04%	0.005%
73	9.208	2443	2447	2449	rBV	219	213	0.03%	0.003%
74	9.292	2469	2473	2475	rBV	221	214	0.03%	0.003%
75	9.414	2498	2511	2532	rBV	388000	644769	81.85%	9.892%
76	9.629	2574	2578	2579	rBV	219	141	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052876.D
 Acq On : 31 Jan 2023 13:45
 Operator : JC/MD
 Sample : 01314-03DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	9.694	2596	2598	2601	rVB	321	192	0.02%	0.003%
78	9.854	2645	2648	2651	rBV	214	183	0.02%	0.003%
79	10.044	2703	2707	2711	rVB2	210	188	0.02%	0.003%
80	10.179	2745	2749	2750	rBV2	273	156	0.02%	0.002%
81	10.295	2783	2785	2788	rVB2	358	221	0.03%	0.003%
82	10.333	2795	2797	2802	rVB	378	283	0.04%	0.004%
83	10.359	2802	2805	2806	rBV	211	137	0.02%	0.002%
84	10.391	2813	2815	2817	rBV	206	146	0.02%	0.002%
85	10.546	2860	2863	2867	rVB	243	126	0.02%	0.002%
86	10.565	2867	2869	2873	rVB	364	277	0.04%	0.004%
87	10.597	2874	2879	2880	rBV	282	199	0.03%	0.003%
88	10.623	2884	2887	2892	rVB	226	145	0.02%	0.002%
89	10.751	2914	2927	2943	rBV	265987	425971	54.08%	6.535%
90	10.980	2995	2998	3001	rBV	198	126	0.02%	0.002%
91	11.320	3102	3104	3105	rBV	261	127	0.02%	0.002%
92	11.809	3243	3256	3273	rBV	343067	552097	70.09%	8.470%
93	11.912	3286	3288	3292	rVB2	400	239	0.03%	0.004%
94	12.073	3335	3338	3341	rVB2	433	246	0.03%	0.004%
95	12.189	3361	3374	3390	rBV	332096	537751	68.27%	8.250%
96	12.407	3437	3442	3444	rBV	191	194	0.02%	0.003%
97	12.475	3458	3463	3466	rBV	274	280	0.04%	0.004%
98	12.944	3607	3609	3614	rVB2	390	278	0.04%	0.004%
99	13.996	3933	3936	3937	rBV	348	210	0.03%	0.003%
100	14.140	3979	3981	3983	rBV	278	135	0.02%	0.002%




Sum of corrected areas: 6518083

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052876.D
Acq On : 31 Jan 2023 13:45
Operator : JC/MD
Sample : 01314-03DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

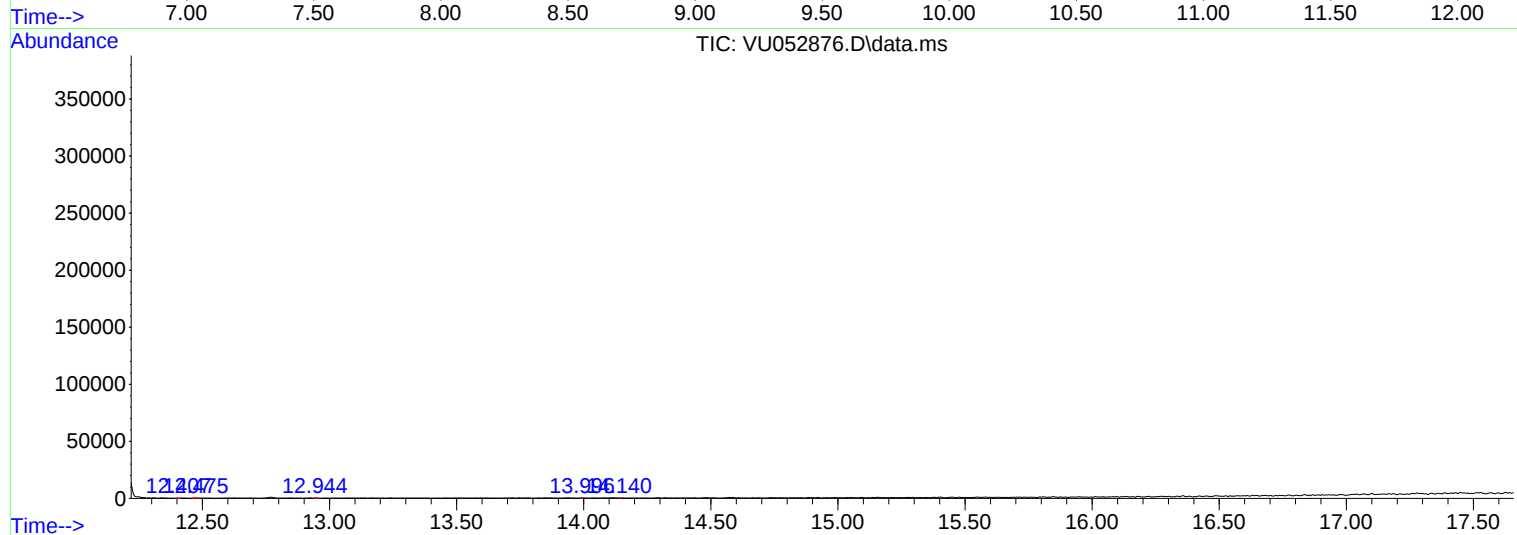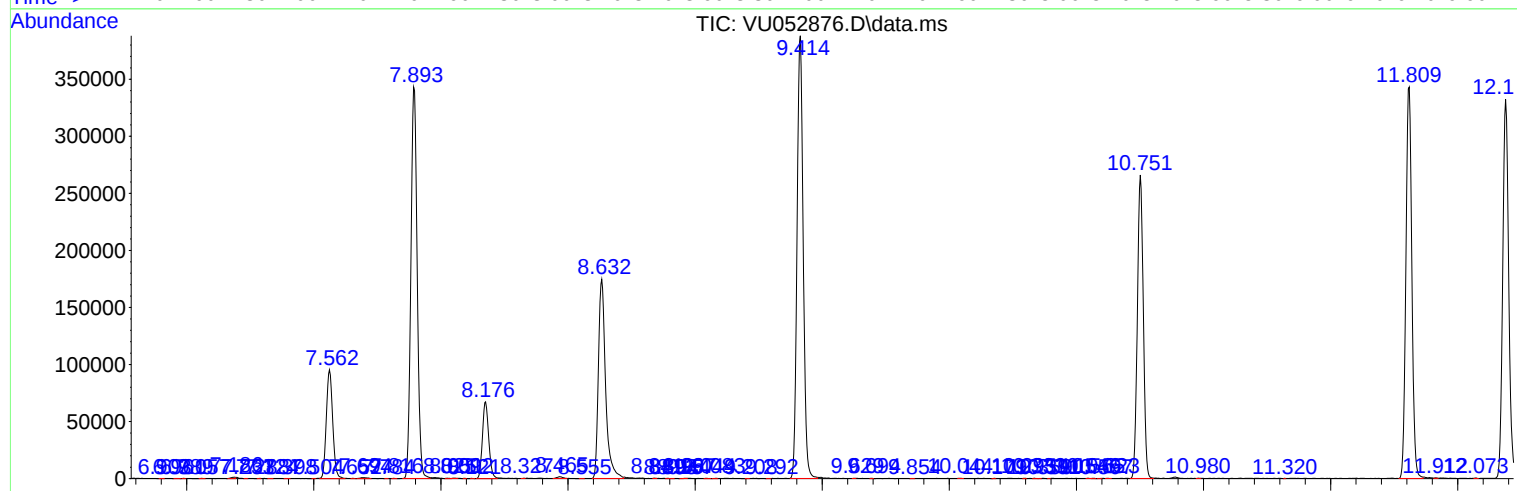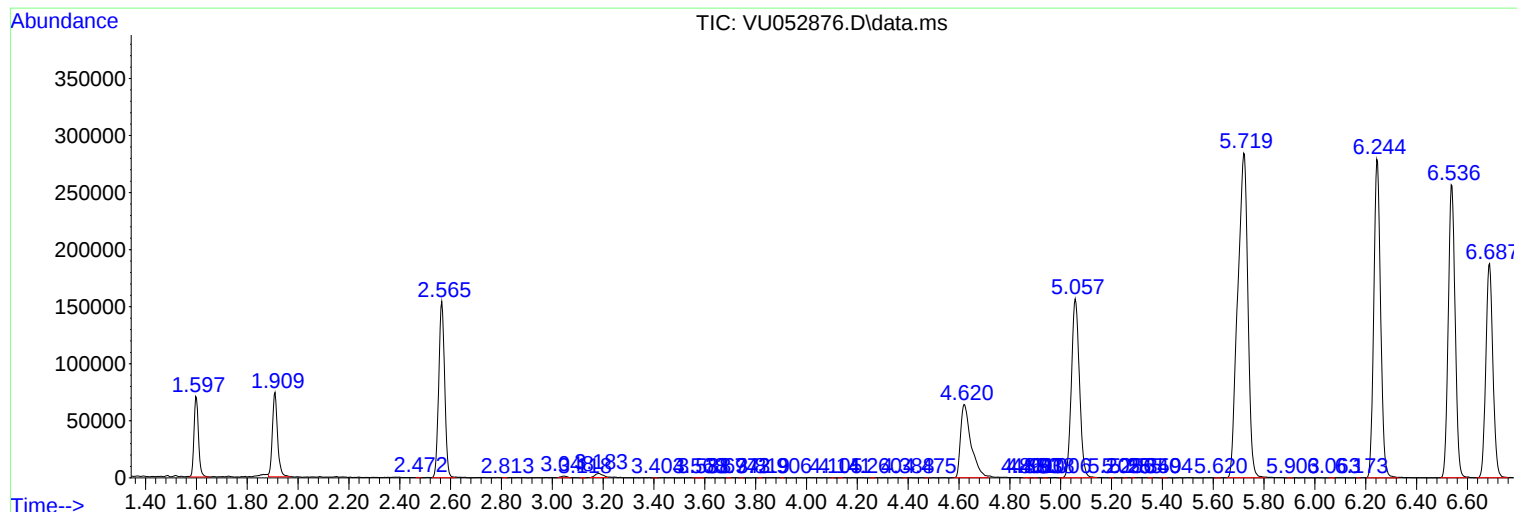

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052876.D
Acq On : 31 Jan 2023 13:45
Operator : JC/MD
Sample : 01314-03DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052876.D
Acq On : 31 Jan 2023 13:45
Operator : JC/MD
Sample : 01314-03DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------