

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052877.D
 Acq On : 31 Jan 2023 14:08
 Operator : JC/MD
 Sample : 01314-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	95	rBV	66520	80911	12.03%	1.479%
2	1.909	169	177	204	rVB	71763	98385	14.62%	1.799%
3	2.256	282	285	288	rVB2	570	336	0.05%	0.006%
4	2.359	314	317	321	rVV2	289	267	0.04%	0.005%
5	2.565	369	381	399	rBV	149383	239864	35.65%	4.385%
6	2.691	416	420	423	rBV	351	259	0.04%	0.005%
7	2.716	424	428	430	rBV2	151	133	0.02%	0.002%
8	2.793	448	452	456	rBV	333	369	0.05%	0.007%
9	2.822	458	461	463	rVV2	223	145	0.02%	0.003%
10	2.896	482	484	487	rVB	271	160	0.02%	0.003%
11	2.919	488	491	493	rBV	193	154	0.02%	0.003%
12	3.038	524	528	530	rBV3	713	489	0.07%	0.009%
13	3.125	550	555	558	rBV	162	195	0.03%	0.004%
14	3.182	570	573	576	rVB	228	150	0.02%	0.003%
15	3.234	586	589	592	rBB	183	157	0.02%	0.003%
16	3.289	601	606	609	rBB	225	190	0.03%	0.003%
17	3.321	610	616	617	rBV	237	219	0.03%	0.004%
18	3.343	621	623	625	rBV2	390	237	0.04%	0.004%
19	3.430	646	650	652	rBB	144	125	0.02%	0.002%
20	3.498	668	671	674	rVB2	256	173	0.03%	0.003%
21	3.555	686	689	691	rBB	183	124	0.02%	0.002%
22	3.674	723	726	730	rBV	265	252	0.04%	0.005%
23	3.752	748	750	754	rBV	177	171	0.03%	0.003%
24	3.845	775	779	782	rBV	177	163	0.02%	0.003%
25	3.906	796	798	801	rBB	220	123	0.02%	0.002%
26	4.157	871	876	879	rBB	205	206	0.03%	0.004%
27	4.337	928	932	936	rBB	378	187	0.03%	0.003%
28	4.620	1004	1020	1048	rBV3	59423	191525	28.47%	3.501%
29	4.771	1065	1067	1074	rVB2	412	371	0.06%	0.007%
30	4.809	1074	1079	1080	rBV	412	290	0.04%	0.005%
31	4.916	1109	1112	1115	rBV	270	212	0.03%	0.004%
32	4.948	1119	1122	1125	rBB2	273	212	0.03%	0.004%
33	5.057	1140	1156	1182	rBV	148669	329229	48.94%	6.019%
34	5.208	1199	1203	1205	rBB	150	120	0.02%	0.002%
35	5.346	1242	1246	1248	rBV	158	152	0.02%	0.003%
36	5.372	1252	1254	1256	rBB	248	112	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052877.D
 Acq On : 31 Jan 2023 14:08
 Operator : JC/MD
 Sample : 01314-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	5.719	1341	1362	1387	rVV3	241616	672760	100.00%	12.299%
38	5.825	1393	1395	1396	rBV	249	121	0.02%	0.002%
39	5.858	1402	1405	1409	rBB2	298	209	0.03%	0.004%
40	6.144	1491	1494	1497	rBB	171	136	0.02%	0.002%
41	6.243	1512	1525	1543	rBV	206360	390195	58.00%	7.133%
42	6.353	1556	1559	1560	rBV	279	119	0.02%	0.002%
43	6.372	1563	1565	1571	rVB2	178	125	0.02%	0.002%
44	6.539	1606	1617	1627	rBV7	4325	8186	1.22%	0.150%
45	6.687	1649	1663	1682	rBV	157807	304308	45.23%	5.563%
46	7.124	1796	1799	1802	rBV	129	134	0.02%	0.002%
47	7.192	1811	1820	1826	rBV3	749	1331	0.20%	0.024%
48	7.562	1923	1935	1951	rBV	80958	139654	20.76%	2.553%
49	7.665	1965	1967	1969	rBV	241	151	0.02%	0.003%
50	7.687	1969	1974	1980	rVV4	749	737	0.11%	0.013%
51	7.748	1991	1993	1996	rBV	139	116	0.02%	0.002%
52	7.784	2001	2004	2007	rBB	149	127	0.02%	0.002%
53	7.809	2008	2012	2014	rBV	149	120	0.02%	0.002%
54	7.893	2026	2038	2056	rBV	296438	508717	75.62%	9.300%
55	8.176	2115	2126	2143	rBV	57353	97341	14.47%	1.779%
56	8.240	2143	2146	2150	rVB	312	295	0.04%	0.005%
57	8.266	2151	2154	2157	rBB	311	209	0.03%	0.004%
58	8.314	2166	2169	2172	rVB2	292	202	0.03%	0.004%
59	8.343	2173	2178	2182	rBV3	386	442	0.07%	0.008%
60	8.407	2195	2198	2203	rBB2	285	231	0.03%	0.004%
61	8.632	2254	2268	2298	rBV3	176944	346989	51.58%	6.343%
62	8.867	2338	2341	2344	rBV2	342	268	0.04%	0.005%
63	8.909	2352	2354	2357	rBV	312	212	0.03%	0.004%
64	8.967	2368	2372	2374	rBV	177	169	0.03%	0.003%
65	9.134	2421	2424	2427	rBV	201	198	0.03%	0.004%
66	9.414	2498	2511	2536	rBV2	333717	650887	96.75%	11.899%
67	9.575	2558	2561	2564	rBV2	174	123	0.02%	0.002%
68	9.648	2581	2584	2586	rBV	181	141	0.02%	0.003%
69	9.700	2597	2600	2603	rBV	118	129	0.02%	0.002%
70	9.861	2647	2650	2653	rBV	155	149	0.02%	0.003%
71	10.144	2731	2738	2742	rBV	281	389	0.06%	0.007%
72	10.214	2758	2760	2763	rBV	160	132	0.02%	0.002%
73	10.266	2771	2776	2779	rBV	246	256	0.04%	0.005%
74	10.330	2794	2796	2800	rBV	153	156	0.02%	0.003%
75	10.414	2819	2822	2824	rBV	166	141	0.02%	0.003%
76	10.504	2846	2850	2853	rBV	146	173	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052877.D
 Acq On : 31 Jan 2023 14:08
 Operator : JC/MD
 Sample : 01314-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.584	2871	2875	2882	rBV	206	330	0.05%	0.006%
78	10.632	2886	2890	2892	rBV	190	147	0.02%	0.003%
79	10.751	2914	2927	2944	rBV	239926	379534	56.41%	6.938%
80	10.915	2975	2978	2983	rBB	205	204	0.03%	0.004%
81	10.954	2986	2990	2991	rBV	244	192	0.03%	0.004%
82	11.060	3020	3023	3026	rBV	151	153	0.02%	0.003%
83	11.205	3066	3068	3074	rBB	200	202	0.03%	0.004%
84	11.359	3113	3116	3119	rBV	215	179	0.03%	0.003%
85	11.465	3145	3149	3152	rBV2	382	339	0.05%	0.006%
86	11.671	3210	3213	3214	rBV	204	137	0.02%	0.003%
87	11.738	3229	3234	3238	rBV3	654	762	0.11%	0.014%
88	11.809	3243	3256	3283	rVV	279238	458678	68.18%	8.385%
89	12.025	3317	3323	3327	rBV	267	394	0.06%	0.007%
90	12.189	3361	3374	3394	rBV2	318782	551659	82.00%	10.085%
91	12.610	3502	3505	3508	rBV	237	135	0.02%	0.002%
92	12.761	3548	3552	3556	rBV2	283	334	0.05%	0.006%
93	12.909	3595	3598	3599	rBV	166	112	0.02%	0.002%
94	13.012	3629	3630	3634	rBV	247	198	0.03%	0.004%
95	13.465	3767	3771	3775	rBV	145	145	0.02%	0.003%
96	13.838	3882	3887	3898	rVB5	1466	2448	0.36%	0.045%
97	14.327	4036	4039	4045	rBV2	504	469	0.07%	0.009%
98	14.780	4178	4180	4183	rBV2	324	169	0.03%	0.003%
99	15.021	4252	4255	4257	rBV	267	180	0.03%	0.003%
100	15.221	4314	4317	4320	rBV2	368	215	0.03%	0.004%




Sum of corrected areas: 5470160

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052877.D
Acq On : 31 Jan 2023 14:08
Operator : JC/MD
Sample : 01314-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

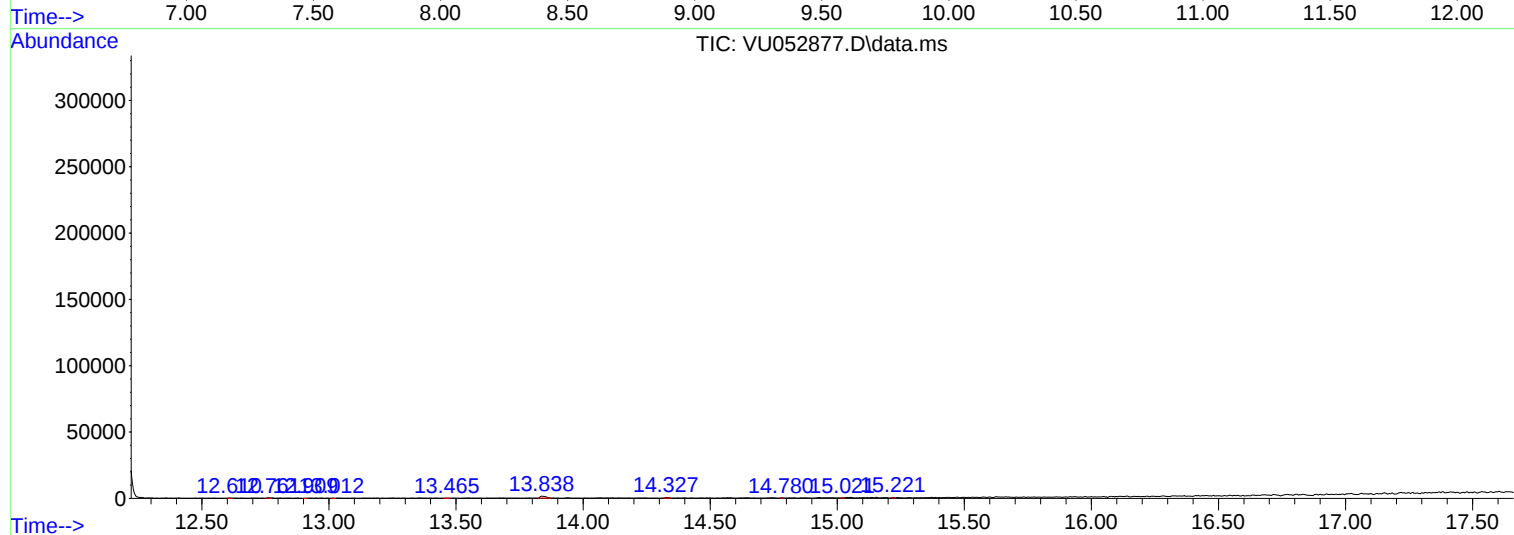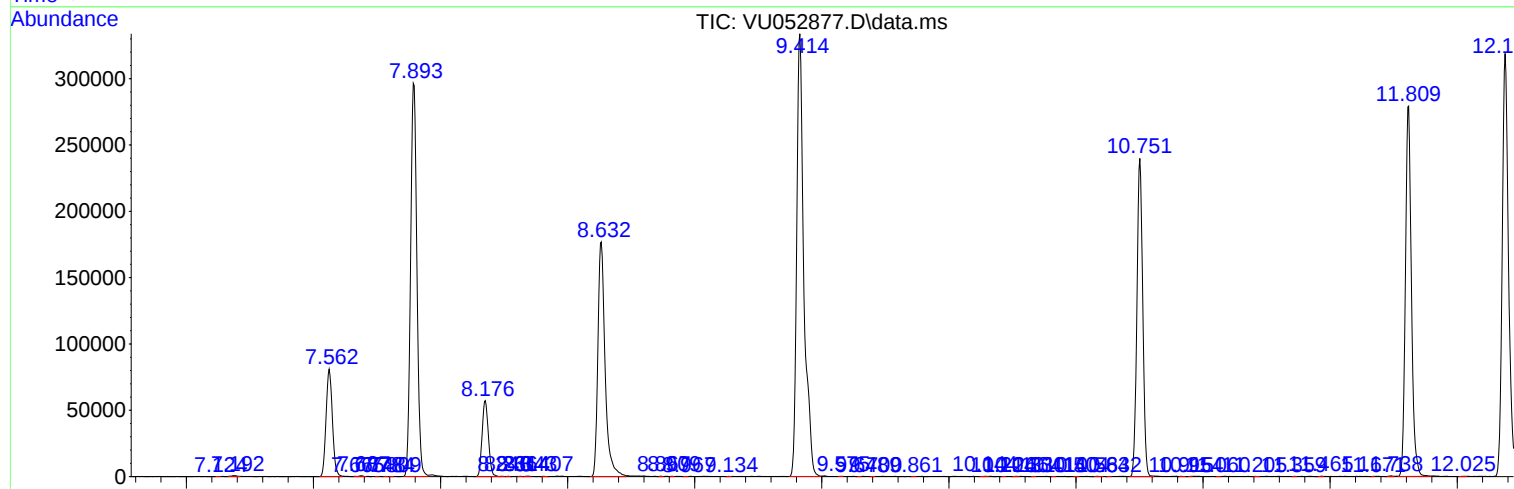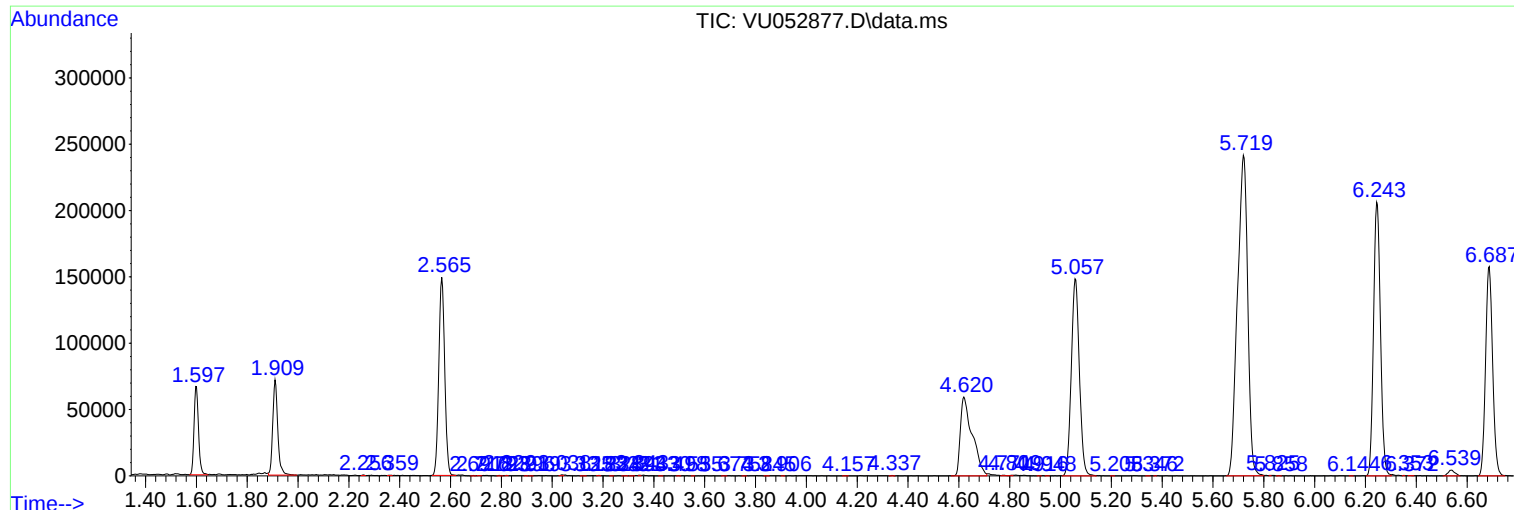

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052877.D
Acq On : 31 Jan 2023 14:08
Operator : JC/MD
Sample : 01314-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052877.D
Acq On : 31 Jan 2023 14:08
Operator : JC/MD
Sample : 01314-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc