

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052880.D
 Acq On : 31 Jan 2023 15:19
 Operator : JC/MD
 Sample : 01314-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rVB	80873	98411	10.97%	1.434%
2	1.909	169	177	199	rVB	83876	113953	12.70%	1.660%
3	2.482	353	355	363	rVB2	392	280	0.03%	0.004%
4	2.565	368	381	396	rBV	167521	274787	30.62%	4.004%
5	2.697	419	422	426	rVB2	261	190	0.02%	0.003%
6	2.719	426	429	432	rBV2	405	213	0.02%	0.003%
7	3.047	525	531	536	rVB3	925	1121	0.12%	0.016%
8	3.073	536	539	544	rVB2	201	197	0.02%	0.003%
9	3.166	562	568	570	rBV3	654	551	0.06%	0.008%
10	3.295	606	608	615	rVB2	201	210	0.02%	0.003%
11	3.346	617	624	636	rVV5	989	1581	0.18%	0.023%
12	3.404	639	642	646	rBV	298	275	0.03%	0.004%
13	3.481	663	666	668	rBV	168	112	0.01%	0.002%
14	3.617	704	708	711	rBV	216	230	0.03%	0.003%
15	3.761	750	753	754	rBV	271	142	0.02%	0.002%
16	3.809	766	768	771	rBV	192	151	0.02%	0.002%
17	3.829	771	774	778	rVB	252	203	0.02%	0.003%
18	3.871	782	787	789	rBV2	300	310	0.03%	0.005%
19	3.912	797	800	803	rBB2	288	183	0.02%	0.003%
20	3.935	803	807	809	rBV	196	174	0.02%	0.003%
21	4.141	866	871	874	rBV	183	196	0.02%	0.003%
22	4.195	886	888	891	rBV	225	169	0.02%	0.002%
23	4.350	932	936	938	rBV	240	138	0.02%	0.002%
24	4.433	960	962	964	rBV	178	114	0.01%	0.002%
25	4.507	981	985	988	rVB	359	313	0.03%	0.005%
26	4.530	989	992	994	rBB	169	113	0.01%	0.002%
27	4.546	994	997	1001	rBV	209	204	0.02%	0.003%
28	4.620	1004	1020	1026	rBV	74794	155631	17.34%	2.268%
29	4.948	1120	1122	1125	rVB	376	235	0.03%	0.003%
30	4.973	1126	1130	1132	rBB	326	143	0.02%	0.002%
31	4.996	1133	1137	1139	rBV2	359	272	0.03%	0.004%
32	5.057	1140	1156	1180	rVV	174553	382284	42.59%	5.570%
33	5.224	1206	1208	1213	rVB2	253	209	0.02%	0.003%
34	5.279	1220	1225	1227	rBV	445	346	0.04%	0.005%
35	5.343	1243	1245	1247	rBV	174	118	0.01%	0.002%
36	5.398	1259	1262	1264	rBV	293	193	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052880.D
 Acq On : 31 Jan 2023 15:19
 Operator : JC/MD
 Sample : 01314-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	5.465	1280	1283	1287	rVV2	248	208	0.02%	0.003%
38	5.485	1287	1289	1292	rVB	258	163	0.02%	0.002%
39	5.504	1293	1295	1297	rBV	171	114	0.01%	0.002%
40	5.604	1323	1326	1329	rBV	188	174	0.02%	0.003%
41	5.629	1330	1334	1338	rVB2	323	330	0.04%	0.005%
42	5.723	1339	1363	1392	rBV2	320495	897495	100.00%	13.077%
43	5.848	1398	1402	1404	rBV3	334	272	0.03%	0.004%
44	5.903	1416	1419	1423	rBB	261	163	0.02%	0.002%
45	5.948	1429	1433	1436	rBV2	281	249	0.03%	0.004%
46	5.973	1439	1441	1443	rBV	259	138	0.02%	0.002%
47	5.999	1443	1449	1452	rVB2	428	385	0.04%	0.006%
48	6.076	1470	1473	1475	rBV	201	129	0.01%	0.002%
49	6.160	1496	1499	1501	rBV	199	160	0.02%	0.002%
50	6.176	1501	1504	1506	rVV	242	155	0.02%	0.002%
51	6.243	1512	1525	1543	rBV	294123	553168	61.63%	8.060%
52	6.539	1602	1617	1632	rBV	71423	130354	14.52%	1.899%
53	6.636	1641	1647	1649	rBV	243	287	0.03%	0.004%
54	6.687	1649	1663	1684	rVV	213519	415504	46.30%	6.054%
55	6.806	1696	1700	1707	rBB4	463	524	0.06%	0.008%
56	6.854	1709	1715	1717	rBV2	262	272	0.03%	0.004%
57	7.057	1775	1778	1784	rBB2	280	316	0.04%	0.005%
58	7.308	1853	1856	1859	rVB	191	157	0.02%	0.002%
59	7.330	1860	1863	1867	rVB	281	225	0.03%	0.003%
60	7.359	1868	1872	1875	rBB	174	141	0.02%	0.002%
61	7.378	1876	1878	1880	rBV	184	127	0.01%	0.002%
62	7.485	1908	1911	1914	rBV	197	175	0.02%	0.003%
63	7.510	1916	1919	1921	rVV	193	121	0.01%	0.002%
64	7.562	1923	1935	1954	rVV	104590	183670	20.46%	2.676%
65	7.655	1960	1964	1966	rBV3	255	172	0.02%	0.003%
66	7.764	1996	1998	2002	rBV	378	183	0.02%	0.003%
67	7.845	2021	2023	2025	rBV2	318	145	0.02%	0.002%
68	7.893	2025	2038	2065	rVV	382205	656510	73.15%	9.565%
69	8.066	2089	2092	2099	rVB3	584	606	0.07%	0.009%
70	8.108	2100	2105	2109	rBB	181	217	0.02%	0.003%
71	8.176	2115	2126	2146	rVV2	77202	130076	14.49%	1.895%
72	8.346	2175	2179	2182	rBV	240	220	0.02%	0.003%
73	8.465	2206	2216	2228	rBV3	4017	6745	0.75%	0.098%
74	8.629	2255	2267	2293	rBV2	214205	409341	45.61%	5.964%
75	8.825	2327	2328	2331	rVB	300	138	0.02%	0.002%
76	8.857	2334	2338	2341	rVB2	274	248	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052880.D
 Acq On : 31 Jan 2023 15:19
 Operator : JC/MD
 Sample : 01314-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	9.218	2446	2450	2454	rVB2	375	359	0.04%	0.005%
78	9.414	2494	2511	2527	rBV	420143	690422	76.93%	10.060%
79	9.661	2585	2588	2591	rBV	336	280	0.03%	0.004%
80	9.819	2634	2637	2640	rBV	251	196	0.02%	0.003%
81	9.928	2667	2671	2674	rVB2	267	224	0.02%	0.003%
82	10.034	2698	2704	2706	rBV	402	417	0.05%	0.006%
83	10.314	2788	2791	2795	rBV	323	231	0.03%	0.003%
84	10.555	2864	2866	2875	rBV	204	156	0.02%	0.002%
85	10.751	2914	2927	2946	rBV	307200	485108	54.05%	7.068%
86	10.848	2954	2957	2960	rBV2	207	171	0.02%	0.002%
87	10.890	2963	2970	2978	rVB3	3937	6051	0.67%	0.088%
88	11.742	3230	3235	3243	rBV2	1276	1499	0.17%	0.022%
89	11.806	3243	3255	3271	rBV	372190	602468	67.13%	8.778%
90	12.018	3318	3321	3324	rBV	284	191	0.02%	0.003%
91	12.057	3325	3333	3346	rBV4	7215	12368	1.38%	0.180%
92	12.189	3361	3374	3397	rBV	376663	636143	70.88%	9.269%
93	12.587	3495	3498	3502	rBV	311	203	0.02%	0.003%
94	12.764	3547	3553	3555	rBV2	1527	1475	0.16%	0.021%
95	13.465	3768	3771	3774	rBV	307	193	0.02%	0.003%
96	13.510	3782	3785	3788	rBV	350	256	0.03%	0.004%
97	14.359	4047	4049	4052	rBV	314	218	0.02%	0.003%
98	14.561	4110	4112	4114	rBV2	292	150	0.02%	0.002%
99	14.761	4172	4174	4176	rBV	416	209	0.02%	0.003%
100	15.503	4402	4405	4410	rBV3	603	620	0.07%	0.009%




Sum of corrected areas: 6863337

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052880.D
Acq On : 31 Jan 2023 15:19
Operator : JC/MD
Sample : 01314-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

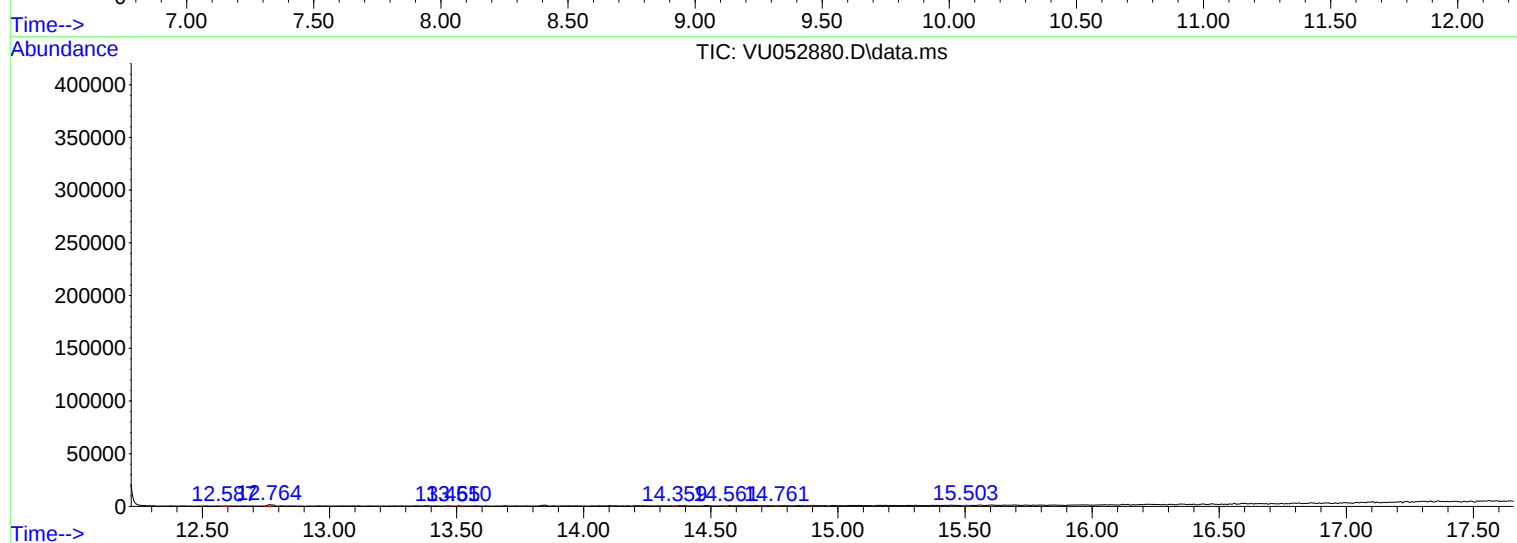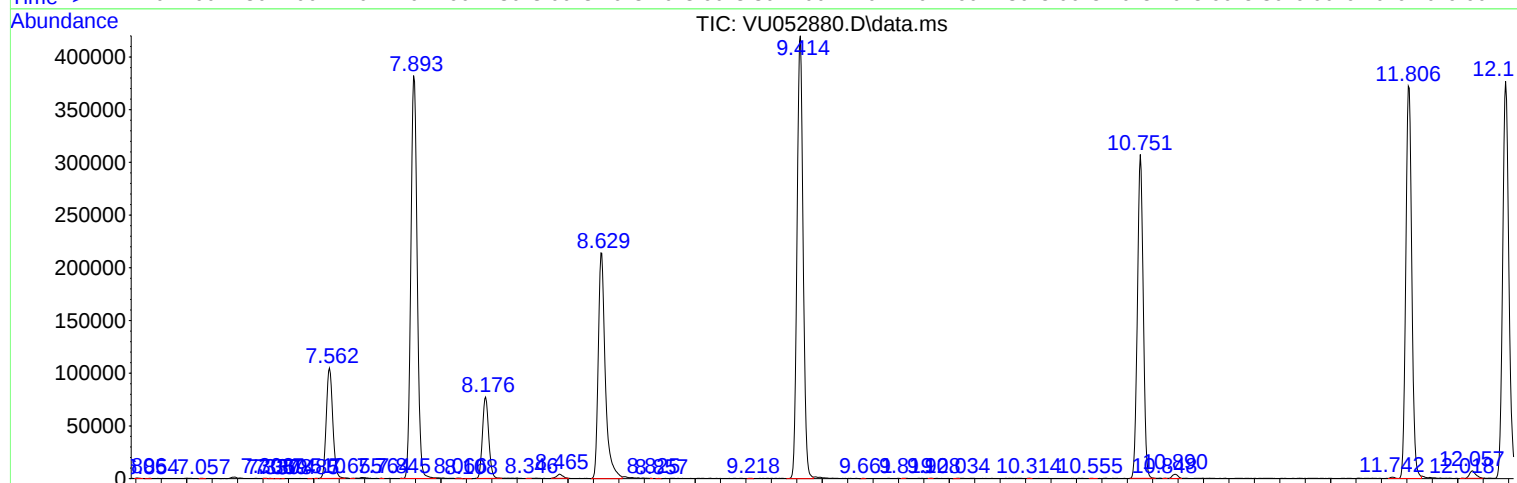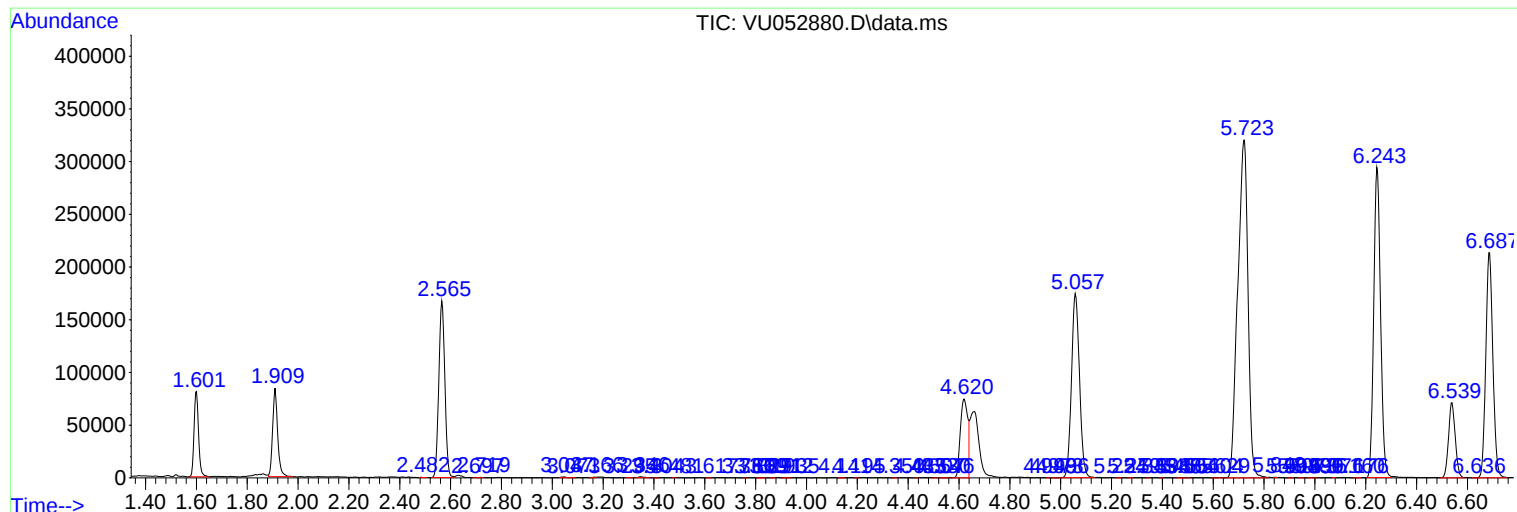

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052880.D
Acq On : 31 Jan 2023 15:19
Operator : JC/MD
Sample : 01314-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052880.D
Acq On : 31 Jan 2023 15:19
Operator : JC/MD
Sample : 01314-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------