

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052883.D
 Acq On : 31 Jan 2023 16:54
 Operator : JC/MD
 Sample : VIBLK107
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK107

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052883.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rVB	122103	142861	13.93%	1.928%
2	1.912	170	178	193	rVB	105401	144563	14.09%	1.951%
3	2.565	369	381	396	rBV	221467	359511	35.05%	4.851%
4	2.813	454	458	460	rBV2	276	168	0.02%	0.002%
5	2.912	485	489	491	rBV	261	157	0.02%	0.002%
6	3.044	522	530	542	rVB4	2435	4372	0.43%	0.059%
7	3.096	543	546	548	rBV	212	128	0.01%	0.002%
8	3.459	656	659	660	rBV	194	134	0.01%	0.002%
9	3.652	716	719	721	rBV	196	153	0.01%	0.002%
10	3.668	721	724	726	rVB2	232	153	0.01%	0.002%
11	3.851	776	781	782	rBV	214	187	0.02%	0.003%
12	3.903	794	797	800	rVB2	321	228	0.02%	0.003%
13	3.922	800	803	805	rBV	179	146	0.01%	0.002%
14	3.935	805	807	809	rVV	267	161	0.02%	0.002%
15	4.044	836	841	843	rBV	153	174	0.02%	0.002%
16	4.137	866	870	872	rBB	233	168	0.02%	0.002%
17	4.154	872	875	878	rBB	314	239	0.02%	0.003%
18	4.189	883	886	891	rBB	216	211	0.02%	0.003%
19	4.215	891	894	898	rBV	332	276	0.03%	0.004%
20	4.231	898	899	905	rVB2	296	239	0.02%	0.003%
21	4.366	938	941	942	rBV	226	129	0.01%	0.002%
22	4.475	973	975	980	rBB2	295	263	0.03%	0.004%
23	4.572	1003	1005	1009	rBV	263	196	0.02%	0.003%
24	4.620	1009	1020	1049	rBV	76176	194141	18.93%	2.620%
25	4.871	1096	1098	1101	rBV	308	224	0.02%	0.003%
26	4.912	1109	1111	1116	rVB2	428	249	0.02%	0.003%
27	5.057	1139	1156	1184	rBV	192969	424349	41.37%	5.726%
28	5.195	1197	1199	1203	rVB2	313	195	0.02%	0.003%
29	5.285	1225	1227	1233	rVB2	412	350	0.03%	0.005%
30	5.334	1239	1242	1244	rBV	205	154	0.02%	0.002%
31	5.372	1251	1254	1256	rBV	379	236	0.02%	0.003%
32	5.408	1263	1265	1270	rBV	150	172	0.02%	0.002%
33	5.430	1270	1272	1277	rVV	289	239	0.02%	0.003%
34	5.456	1277	1280	1283	rVB2	282	195	0.02%	0.003%
35	5.501	1291	1294	1297	rBB	295	177	0.02%	0.002%
36	5.536	1302	1305	1306	rBV	257	138	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052883.D
 Acq On : 31 Jan 2023 16:54
 Operator : JC/MD
 Sample : VIBLK107
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK107

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	5.607	1325	1327	1331	rBV	155	153	0.01%	0.002%
38	5.723	1340	1363	1392	rVV2	375920	1025799	100.00%	13.841%
39	5.874	1408	1410	1414	rBV	323	215	0.02%	0.003%
40	5.925	1421	1426	1431	rBV2	215	299	0.03%	0.004%
41	5.970	1438	1440	1446	rBV2	430	364	0.04%	0.005%
42	6.022	1452	1456	1460	rBV2	265	277	0.03%	0.004%
43	6.047	1462	1464	1468	rBV	299	233	0.02%	0.003%
44	6.086	1473	1476	1478	rBB	268	163	0.02%	0.002%
45	6.105	1479	1482	1485	rBV	197	203	0.02%	0.003%
46	6.192	1507	1509	1512	rBV	261	181	0.02%	0.002%
47	6.247	1512	1526	1545	rBV	291701	553423	53.95%	7.467%
48	6.459	1589	1592	1594	rBV	159	130	0.01%	0.002%
49	6.475	1594	1597	1600	rVB2	442	216	0.02%	0.003%
50	6.536	1606	1616	1626	rBV7	2857	4998	0.49%	0.067%
51	6.636	1644	1647	1649	rBV	233	149	0.01%	0.002%
52	6.687	1649	1663	1683	rBV	237173	458613	44.71%	6.188%
53	6.806	1696	1700	1702	rBV3	308	295	0.03%	0.004%
54	6.887	1722	1725	1727	rVV	273	214	0.02%	0.003%
55	6.896	1727	1728	1731	rVV	300	151	0.01%	0.002%
56	6.919	1733	1735	1740	rVB2	313	278	0.03%	0.004%
57	7.083	1781	1786	1793	rBV2	412	521	0.05%	0.007%
58	7.182	1811	1817	1823	rBV4	1666	2255	0.22%	0.030%
59	7.456	1894	1902	1904	rBV	347	454	0.04%	0.006%
60	7.562	1923	1935	1955	rBV	120401	208671	20.34%	2.816%
61	7.629	1955	1956	1958	rVV	343	134	0.01%	0.002%
62	7.642	1958	1960	1967	rVB2	363	207	0.02%	0.003%
63	7.687	1972	1974	1978	rBV2	870	692	0.07%	0.009%
64	7.751	1989	1994	1998	rBV2	368	415	0.04%	0.006%
65	7.893	2025	2038	2058	rBV	463881	789865	77.00%	10.658%
66	8.108	2102	2105	2108	rBV	295	226	0.02%	0.003%
67	8.176	2114	2126	2147	rVV	87096	147663	14.39%	1.992%
68	8.575	2246	2250	2253	rBB	208	188	0.02%	0.003%
69	8.632	2254	2268	2297	rBV3	223511	437880	42.69%	5.908%
70	8.858	2335	2338	2342	rVB	323	220	0.02%	0.003%
71	8.880	2342	2345	2346	rBV	309	164	0.02%	0.002%
72	8.925	2356	2359	2368	rBB	365	444	0.04%	0.006%
73	8.967	2368	2372	2373	rBV	243	187	0.02%	0.003%
74	8.976	2373	2375	2379	rVB	247	168	0.02%	0.002%
75	9.259	2460	2463	2468	rVB2	246	251	0.02%	0.003%
76	9.353	2489	2492	2495	rBV2	223	149	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052883.D
 Acq On : 31 Jan 2023 16:54
 Operator : JC/MD
 Sample : VIBLK107
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK107

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	9.414	2496	2511	2531	rBV	418231	676383	65.94%	9.126%
78	9.562	2554	2557	2560	rVB	372	240	0.02%	0.003%
79	9.861	2647	2650	2652	rBV	260	197	0.02%	0.003%
80	10.459	2833	2836	2840	rBB	200	179	0.02%	0.002%
81	10.565	2862	2869	2873	rBV2	222	285	0.03%	0.004%
82	10.751	2915	2927	2950	rBV	323407	504136	49.15%	6.802%
83	10.893	2965	2971	2978	rBV	425	645	0.06%	0.009%
84	11.748	3234	3237	3240	rBV2	285	188	0.02%	0.003%
85	11.806	3243	3255	3279	rVV	374834	591057	57.62%	7.975%
86	12.009	3314	3318	3320	rVB	206	144	0.01%	0.002%
87	12.189	3361	3374	3395	rBV	407172	661504	64.49%	8.926%
88	12.333	3418	3419	3423	rBV	379	151	0.01%	0.002%
89	12.539	3481	3483	3485	rBV	335	191	0.02%	0.003%
90	12.812	3564	3568	3570	rVB	268	143	0.01%	0.002%
91	13.211	3690	3692	3695	rBB	355	150	0.01%	0.002%
92	13.465	3769	3771	3775	rVB2	316	165	0.02%	0.002%
93	13.568	3801	3803	3808	rBV	295	167	0.02%	0.002%
94	13.594	3808	3811	3813	rBV	259	161	0.02%	0.002%
95	13.838	3876	3887	3904	rBV2	30613	49512	4.83%	0.668%
96	14.082	3960	3963	3965	rBV2	534	345	0.03%	0.005%
97	14.192	3993	3997	4001	rBV	368	352	0.03%	0.005%
98	14.240	4009	4012	4014	rBV	306	225	0.02%	0.003%
99	14.327	4031	4039	4051	rBV3	7281	11727	1.14%	0.158%
100	14.687	4148	4151	4155	rBV2	341	255	0.02%	0.003%




Sum of corrected areas: 7411246

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052883.D
Acq On : 31 Jan 2023 16:54
Operator : JC/MD
Sample : VIBLK107
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK107

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

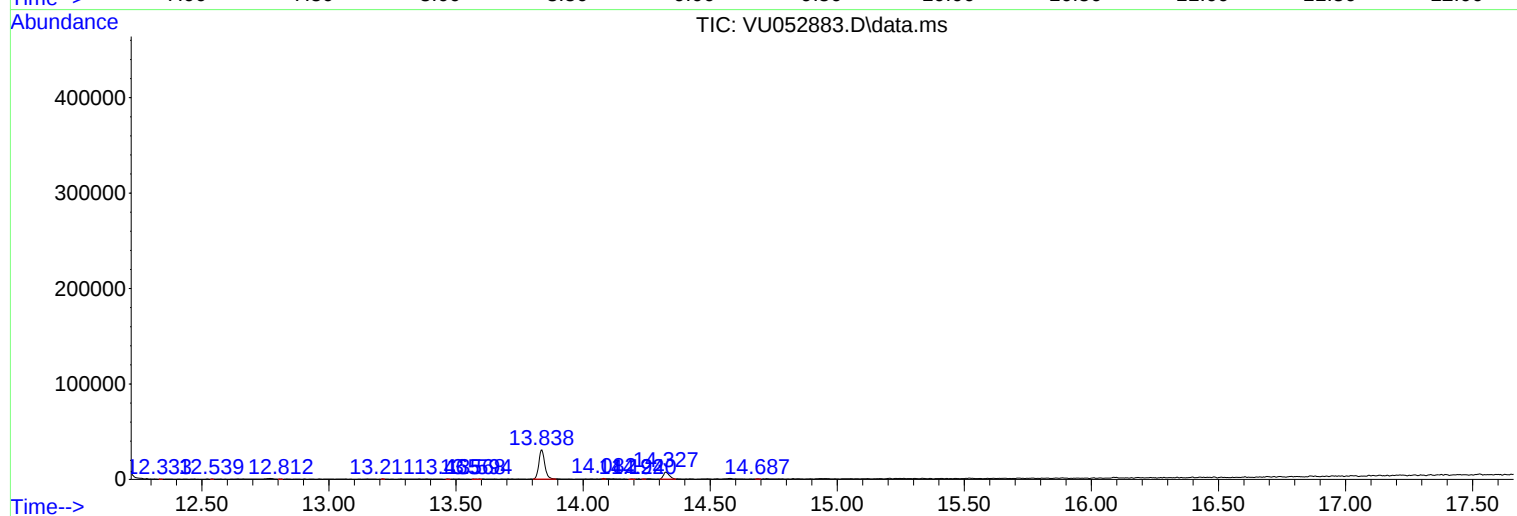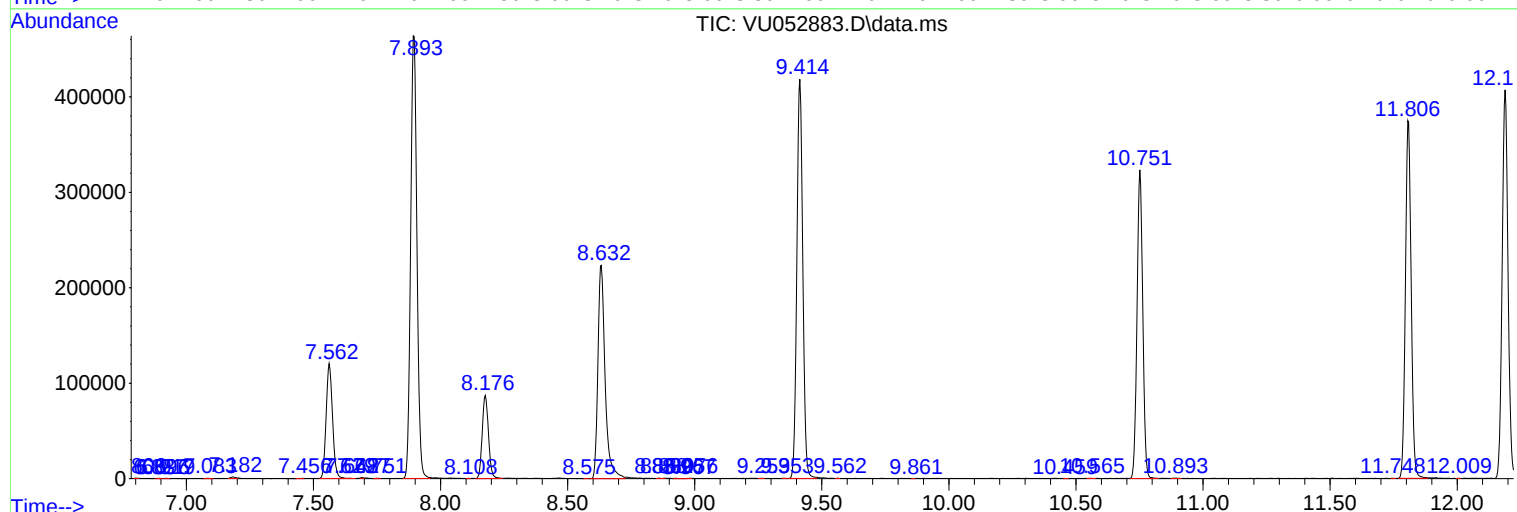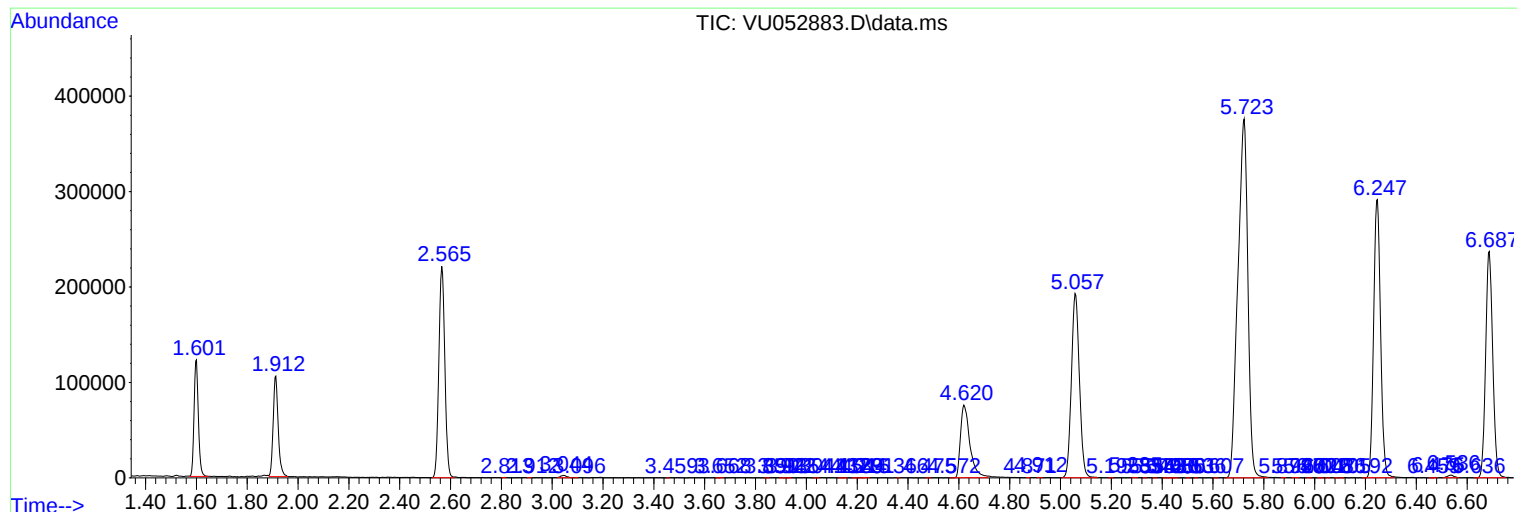

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052883.D
Acq On : 31 Jan 2023 16:54
Operator : JC/MD
Sample : VIBLK107
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK107

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052883.D
Acq On : 31 Jan 2023 16:54
Operator : JC/MD
Sample : VIBLK107
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK107

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------