

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052884.D
 Acq On : 31 Jan 2023 17:17
 Operator : JC/MD
 Sample : 01314-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	72192	85585	3.38%	0.947%
2	1.909	170	177	194	rVB	72513	100512	3.96%	1.113%
3	2.504	360	362	366	rBV2	268	156	0.01%	0.002%
4	2.565	369	381	395	rBV	148429	243246	9.59%	2.693%
5	2.697	420	422	426	rBV	184	124	0.00%	0.001%
6	2.761	436	442	443	rBV	301	200	0.01%	0.002%
7	3.044	522	530	540	rVB3	3009	5065	0.20%	0.056%
8	3.115	549	552	558	rVB2	276	253	0.01%	0.003%
9	3.179	566	572	575	rBV4	480	615	0.02%	0.007%
10	3.263	595	598	599	rBV	329	191	0.01%	0.002%
11	3.340	619	622	623	rBV	312	143	0.01%	0.002%
12	3.411	640	644	646	rBV	290	182	0.01%	0.002%
13	3.446	653	655	657	rBV	183	122	0.00%	0.001%
14	3.546	683	686	688	rBB	293	161	0.01%	0.002%
15	3.575	691	695	696	rBV	155	124	0.00%	0.001%
16	3.719	738	740	742	rVB	268	128	0.01%	0.001%
17	3.758	749	752	754	rBV	263	212	0.01%	0.002%
18	3.819	766	771	776	rBV	227	312	0.01%	0.003%
19	3.941	807	809	813	rVB2	290	181	0.01%	0.002%
20	4.028	832	836	839	rBV2	379	310	0.01%	0.003%
21	4.327	927	929	933	rVB2	241	183	0.01%	0.002%
22	4.362	937	940	942	rBV	254	168	0.01%	0.002%
23	4.424	955	959	960	rBV	171	147	0.01%	0.002%
24	4.440	961	964	967	rVB	394	246	0.01%	0.003%
25	4.481	974	977	981	rBB	203	151	0.01%	0.002%
26	4.501	982	983	987	rBB	225	132	0.01%	0.001%
27	4.542	992	996	1001	rBB	177	198	0.01%	0.002%
28	4.620	1008	1020	1029	rBV	78545	190601	7.52%	2.110%
29	4.893	1104	1105	1109	rVB2	339	186	0.01%	0.002%
30	4.925	1110	1115	1118	rBV	292	304	0.01%	0.003%
31	4.944	1118	1121	1124	rVV	198	156	0.01%	0.002%
32	5.057	1140	1156	1175	rBV2	161141	355498	14.02%	3.935%
33	5.195	1196	1199	1202	rBB	322	222	0.01%	0.002%
34	5.224	1202	1208	1210	rBV2	273	288	0.01%	0.003%
35	5.276	1221	1224	1227	rBV2	322	276	0.01%	0.003%
36	5.317	1227	1237	1245	rVV3	1294	2205	0.09%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052884.D
 Acq On : 31 Jan 2023 17:17
 Operator : JC/MD
 Sample : 01314-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	5.462	1275	1282	1286	rBB	195	290	0.01%	0.003%
38	5.510	1295	1297	1300	rBV	174	137	0.01%	0.002%
39	5.533	1300	1304	1308	rVB	267	254	0.01%	0.003%
40	5.645	1334	1339	1341	rBB	227	182	0.01%	0.002%
41	5.719	1341	1362	1382	rBV2	297273	825806	32.57%	9.142%
42	5.890	1412	1415	1418	rBV3	356	249	0.01%	0.003%
43	5.980	1440	1443	1448	rBB2	264	228	0.01%	0.003%
44	6.009	1449	1452	1455	rBV	216	192	0.01%	0.002%
45	6.044	1461	1463	1469	rBV	331	324	0.01%	0.004%
46	6.243	1511	1525	1544	rBV	269236	511734	20.19%	5.665%
47	6.436	1583	1585	1588	rVB	353	189	0.01%	0.002%
48	6.472	1593	1596	1601	rVB2	375	316	0.01%	0.003%
49	6.536	1601	1616	1643	rBV	1357384	2535167	100.00%	28.064%
50	6.687	1649	1663	1684	rVB	201981	394347	15.56%	4.365%
51	6.993	1755	1758	1766	rBB2	314	266	0.01%	0.003%
52	7.028	1767	1769	1771	rVB	283	135	0.01%	0.001%
53	7.105	1791	1793	1797	rVB	265	193	0.01%	0.002%
54	7.134	1798	1802	1803	rBV	304	208	0.01%	0.002%
55	7.182	1811	1817	1830	rBV3	1984	3232	0.13%	0.036%
56	7.320	1856	1860	1862	rBV	202	175	0.01%	0.002%
57	7.349	1866	1869	1870	rBV	194	126	0.00%	0.001%
58	7.398	1881	1884	1885	rBV	237	118	0.00%	0.001%
59	7.423	1890	1892	1894	rBV	181	123	0.00%	0.001%
60	7.504	1912	1917	1920	rBV	313	363	0.01%	0.004%
61	7.562	1923	1935	1953	rVV	101756	181563	7.16%	2.010%
62	7.639	1958	1959	1963	rBV2	266	134	0.01%	0.001%
63	7.893	2025	2038	2057	rBV	347867	598979	23.63%	6.631%
64	8.063	2088	2091	2093	rVB2	291	141	0.01%	0.002%
65	8.083	2093	2097	2099	rBV2	175	156	0.01%	0.002%
66	8.176	2114	2126	2147	rBV	73086	123484	4.87%	1.367%
67	8.346	2177	2179	2182	rBV	170	141	0.01%	0.002%
68	8.462	2211	2215	2226	rVB3	1404	2052	0.08%	0.023%
69	8.629	2256	2267	2295	rBV2	220431	425883	16.80%	4.715%
70	9.041	2391	2395	2398	rBV2	196	171	0.01%	0.002%
71	9.156	2427	2431	2434	rBV2	292	211	0.01%	0.002%
72	9.288	2467	2472	2473	rVB2	346	250	0.01%	0.003%
73	9.414	2498	2511	2535	rBV	388203	666031	26.27%	7.373%
74	9.581	2561	2563	2566	rBV	198	132	0.01%	0.001%
75	9.674	2588	2592	2594	rBV	382	314	0.01%	0.003%
76	9.719	2603	2606	2611	rBV	221	285	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052884.D
 Acq On : 31 Jan 2023 17:17
 Operator : JC/MD
 Sample : 01314-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.189	2749	2752	2756	rBV	290	248	0.01%	0.003%
78	10.388	2810	2814	2817	rBV	214	151	0.01%	0.002%
79	10.436	2823	2829	2833	rBV	413	565	0.02%	0.006%
80	10.751	2915	2927	2948	rBV	304084	482210	19.02%	5.338%
81	10.889	2960	2970	2978	rVB3	1436	2089	0.08%	0.023%
82	11.462	3146	3148	3152	rVB	183	132	0.01%	0.001%
83	11.488	3154	3156	3163	rVB2	287	307	0.01%	0.003%
84	11.542	3170	3173	3174	rBV	211	119	0.00%	0.001%
85	11.742	3229	3235	3242	rBV4	1069	1457	0.06%	0.016%
86	11.806	3242	3255	3281	rBV	351773	568418	22.42%	6.292%
87	11.992	3310	3313	3320	rVB	364	305	0.01%	0.003%
88	12.021	3320	3322	3324	rBV	247	132	0.01%	0.001%
89	12.063	3328	3335	3345	rVV7	2540	3588	0.14%	0.040%
90	12.188	3361	3374	3401	rBV2	356389	662931	26.15%	7.339%
91	12.330	3415	3418	3422	rVB	219	181	0.01%	0.002%
92	12.401	3438	3440	3445	rBV	217	199	0.01%	0.002%
93	12.487	3465	3467	3469	rBV	254	134	0.01%	0.001%
94	12.774	3547	3556	3561	rVB3	887	1468	0.06%	0.016%
95	13.195	3684	3687	3688	rBV	407	243	0.01%	0.003%
96	13.835	3877	3886	3902	rBV2	22225	36272	1.43%	0.402%
97	14.221	4004	4006	4008	rBV	288	158	0.01%	0.002%
98	14.288	4025	4027	4031	rVB	425	287	0.01%	0.003%
99	14.330	4031	4040	4052	rBV5	5459	8502	0.34%	0.094%
100	14.642	4134	4137	4139	rBV	336	251	0.01%	0.003%




Sum of corrected areas: 9033411

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052884.D
Acq On : 31 Jan 2023 17:17
Operator : JC/MD
Sample : 01314-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

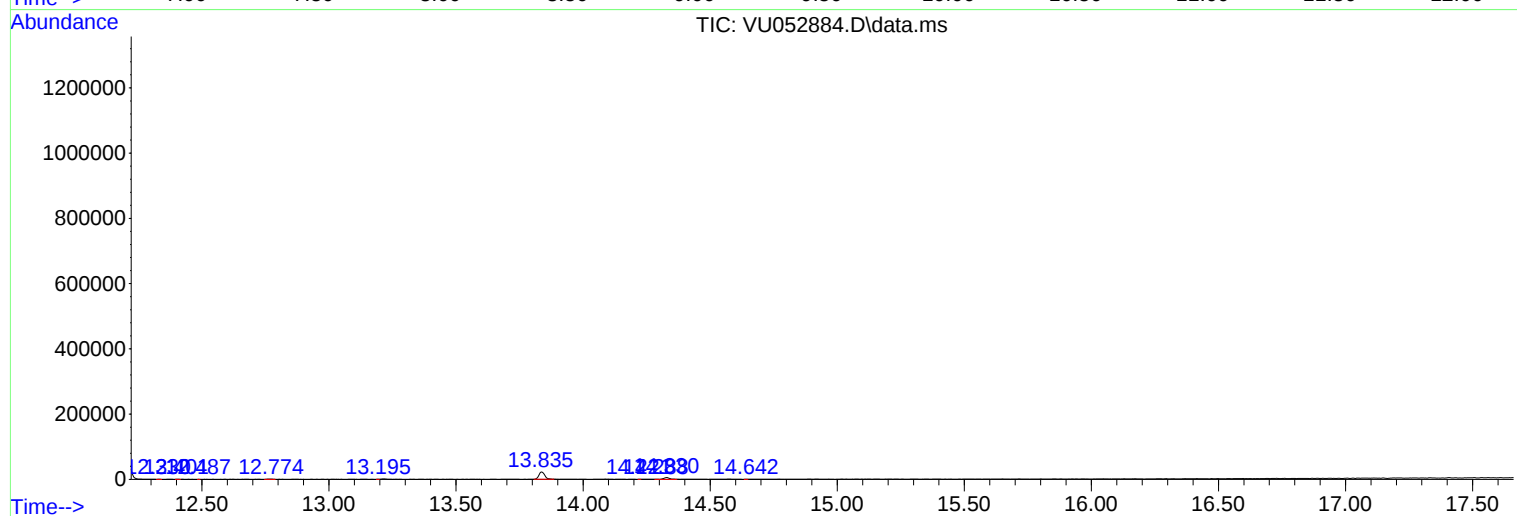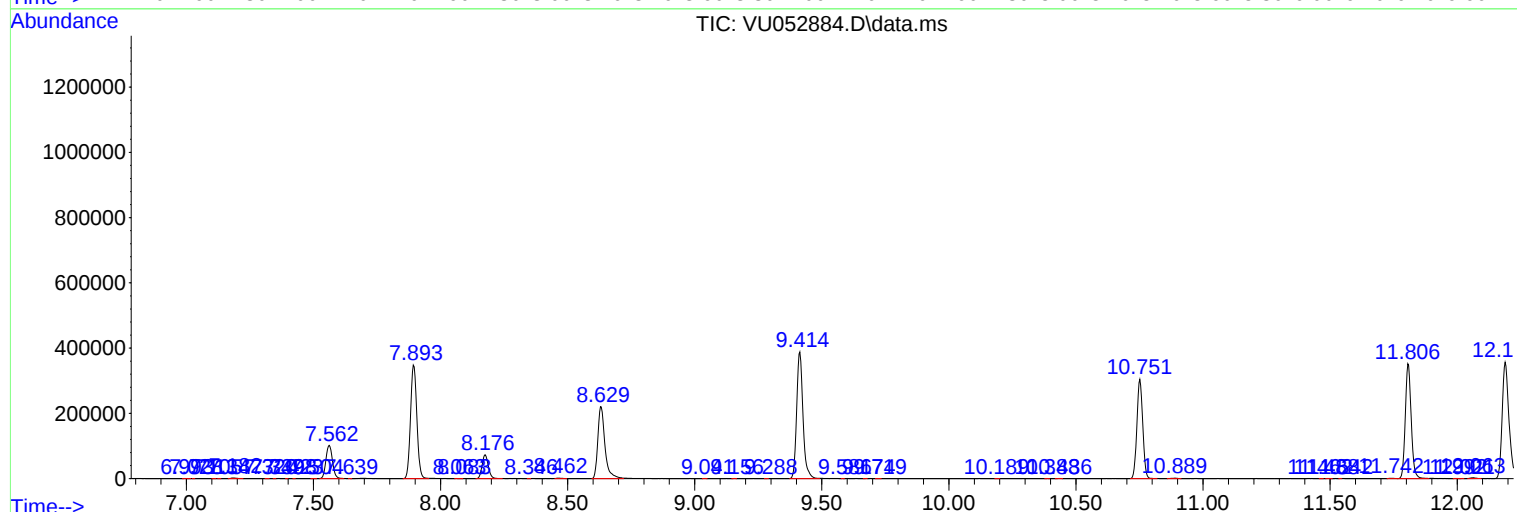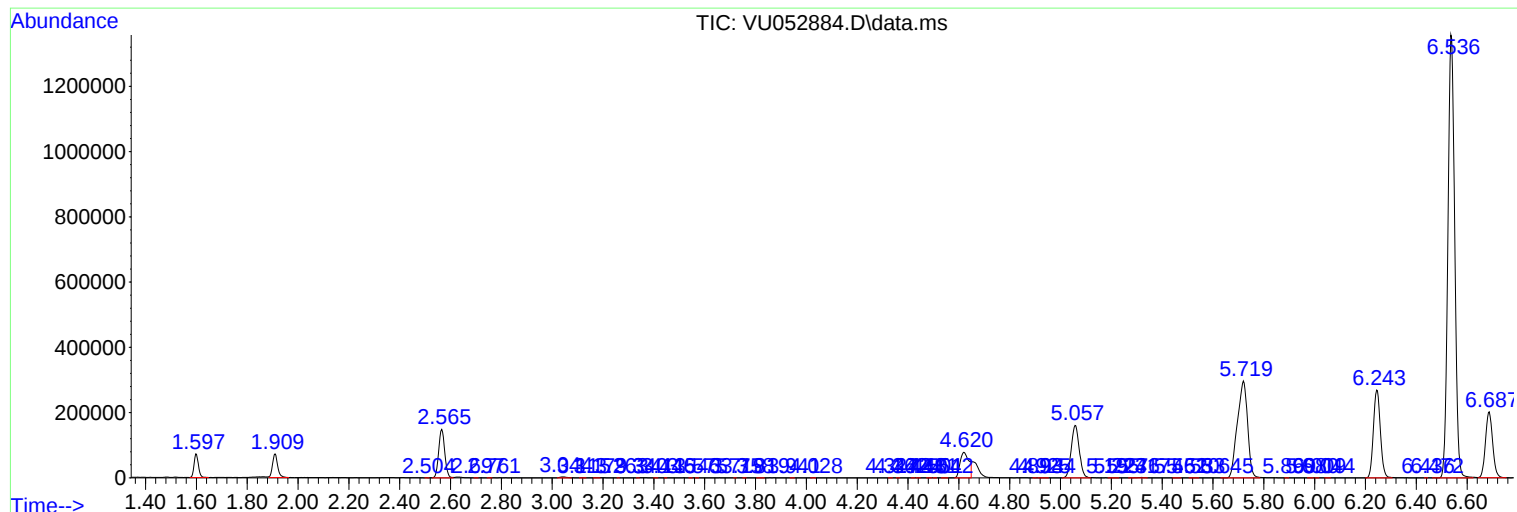

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052884.D
Acq On : 31 Jan 2023 17:17
Operator : JC/MD
Sample : 01314-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052884.D
Acq On : 31 Jan 2023 17:17
Operator : JC/MD
Sample : 01314-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------