

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052885.D
 Acq On : 31 Jan 2023 17:40
 Operator : JC/MD
 Sample : 01314-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	108810	132017	13.12%	1.843%
2	1.906	169	176	195	rVB	103491	144384	14.35%	2.015%
3	2.334	304	309	310	rBV2	438	371	0.04%	0.005%
4	2.562	368	380	401	rBV	208228	341607	33.96%	4.768%
5	2.768	442	444	447	rBV2	365	219	0.02%	0.003%
6	2.861	471	473	478	rBV	245	168	0.02%	0.002%
7	3.047	518	531	541	rBV3	3744	6855	0.68%	0.096%
8	3.292	603	607	610	rBV	142	159	0.02%	0.002%
9	3.449	646	656	658	rBV	301	444	0.04%	0.006%
10	3.539	682	684	689	rBB	170	169	0.02%	0.002%
11	3.697	731	733	737	rVB2	262	196	0.02%	0.003%
12	3.723	738	741	746	rBB	156	177	0.02%	0.002%
13	3.748	746	749	752	rBV	237	212	0.02%	0.003%
14	3.809	766	768	770	rVB	283	134	0.01%	0.002%
15	3.842	773	778	783	rBV	193	301	0.03%	0.004%
16	3.928	802	805	807	rBV	274	155	0.02%	0.002%
17	3.980	818	821	823	rBV	185	140	0.01%	0.002%
18	4.031	832	837	839	rBV	334	338	0.03%	0.005%
19	4.108	857	861	862	rBV	281	193	0.02%	0.003%
20	4.160	872	877	879	rBV	162	189	0.02%	0.003%
21	4.208	890	892	897	rBB	170	165	0.02%	0.002%
22	4.311	921	924	930	rVB2	195	212	0.02%	0.003%
23	4.375	942	944	949	rVB	202	190	0.02%	0.003%
24	4.436	959	963	965	rBB2	235	176	0.02%	0.002%
25	4.478	974	976	978	rBV	327	176	0.02%	0.002%
26	4.562	999	1002	1004	rBV	181	146	0.01%	0.002%
27	4.620	1008	1020	1050	rBV	74003	186748	18.56%	2.607%
28	4.909	1107	1110	1112	rBV2	248	180	0.02%	0.003%
29	5.057	1140	1156	1183	rBV	191054	417847	41.54%	5.832%
30	5.170	1187	1191	1192	rBV	473	287	0.03%	0.004%
31	5.292	1226	1229	1233	rVV2	317	294	0.03%	0.004%
32	5.443	1273	1276	1279	rBB	205	147	0.01%	0.002%
33	5.539	1302	1306	1310	rBB2	344	298	0.03%	0.004%
34	5.581	1315	1319	1322	rBV	170	194	0.02%	0.003%
35	5.613	1326	1329	1332	rBB2	294	228	0.02%	0.003%
36	5.719	1340	1362	1386	rBV2	367021	1006006	100.00%	14.041%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052885.D
 Acq On : 31 Jan 2023 17:40
 Operator : JC/MD
 Sample : 01314-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	5.870	1406	1409	1414	rVB2	241	181	0.02%	0.003%
38	5.893	1414	1416	1418	rBV2	296	196	0.02%	0.003%
39	5.980	1441	1443	1447	rVB	264	173	0.02%	0.002%
40	6.044	1460	1463	1466	rVB2	211	150	0.01%	0.002%
41	6.070	1469	1471	1475	rBV	142	151	0.02%	0.002%
42	6.108	1480	1483	1486	rBV	264	228	0.02%	0.003%
43	6.182	1504	1506	1511	rBV	161	178	0.02%	0.002%
44	6.243	1511	1525	1547	rBV	283501	534591	53.14%	7.462%
45	6.369	1563	1564	1567	rVB2	292	143	0.01%	0.002%
46	6.388	1567	1570	1573	rVB2	211	179	0.02%	0.002%
47	6.491	1599	1602	1606	rVV2	263	196	0.02%	0.003%
48	6.536	1606	1616	1627	rVV6	4716	9163	0.91%	0.128%
49	6.620	1636	1642	1643	rBV	204	209	0.02%	0.003%
50	6.687	1648	1663	1682	rVV	227051	448062	44.54%	6.254%
51	6.813	1696	1702	1705	rBV3	347	402	0.04%	0.006%
52	6.960	1743	1748	1749	rBV	290	181	0.02%	0.003%
53	7.067	1777	1781	1784	rVV2	190	142	0.01%	0.002%
54	7.186	1810	1818	1819	rBV3	1710	1797	0.18%	0.025%
55	7.237	1831	1834	1838	rVB	338	253	0.03%	0.004%
56	7.259	1839	1841	1843	rBV	290	200	0.02%	0.003%
57	7.343	1865	1867	1870	rBV	215	157	0.02%	0.002%
58	7.407	1883	1887	1891	rBV	170	221	0.02%	0.003%
59	7.562	1922	1935	1965	rVB	120662	209279	20.80%	2.921%
60	7.690	1968	1975	1982	rBV4	989	1519	0.15%	0.021%
61	7.893	2025	2038	2060	rBV	448578	761523	75.70%	10.629%
62	8.176	2112	2126	2143	rBV	83472	145351	14.45%	2.029%
63	8.259	2149	2152	2153	rBV2	271	152	0.02%	0.002%
64	8.285	2158	2160	2162	rBV2	196	134	0.01%	0.002%
65	8.632	2256	2268	2296	rBV2	215173	419256	41.68%	5.852%
66	8.822	2321	2327	2334	rVB4	534	661	0.07%	0.009%
67	8.851	2334	2336	2339	rBV	243	178	0.02%	0.002%
68	9.189	2437	2441	2444	rBB	341	257	0.03%	0.004%
69	9.221	2447	2451	2454	rBV	288	297	0.03%	0.004%
70	9.337	2481	2487	2489	rBV	227	269	0.03%	0.004%
71	9.414	2498	2511	2527	rBV	396864	653427	64.95%	9.120%
72	9.591	2563	2566	2570	rVB2	397	297	0.03%	0.004%
73	9.613	2570	2573	2577	rVB	257	187	0.02%	0.003%
74	9.645	2578	2583	2587	rBV	227	310	0.03%	0.004%
75	9.703	2594	2601	2606	rBB2	332	439	0.04%	0.006%
76	9.729	2606	2609	2612	rBV	244	191	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052885.D
 Acq On : 31 Jan 2023 17:40
 Operator : JC/MD
 Sample : 01314-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	9.793	2624	2629	2633	rVB	271	260	0.03%	0.004%
78	9.909	2662	2665	2668	rBV	182	135	0.01%	0.002%
79	9.931	2668	2672	2678	rVV2	306	320	0.03%	0.004%
80	9.960	2678	2681	2684	rVB	246	181	0.02%	0.003%
81	10.054	2707	2710	2714	rBV	255	133	0.01%	0.002%
82	10.115	2726	2729	2733	rVB	282	178	0.02%	0.002%
83	10.144	2734	2738	2743	rVB2	276	309	0.03%	0.004%
84	10.173	2743	2747	2751	rBV	274	313	0.03%	0.004%
85	10.652	2889	2896	2898	rBV	385	434	0.04%	0.006%
86	10.751	2915	2927	2948	rBV	311607	497533	49.46%	6.944%
87	10.883	2963	2968	2976	rVB4	611	915	0.09%	0.013%
88	10.967	2989	2994	2996	rBV	242	209	0.02%	0.003%
89	11.227	3071	3075	3077	rBV	223	144	0.01%	0.002%
90	11.459	3144	3147	3152	rVB2	310	253	0.03%	0.004%
91	11.491	3155	3157	3161	rVB	279	144	0.01%	0.002%
92	11.806	3243	3255	3274	rBV	350257	563859	56.05%	7.870%
93	12.189	3361	3374	3393	rBV	398274	637974	63.42%	8.904%
94	12.381	3431	3434	3436	rBV	214	140	0.01%	0.002%
95	12.764	3549	3553	3558	rBV2	487	543	0.05%	0.008%
96	13.008	3625	3629	3633	rBV2	441	311	0.03%	0.004%
97	13.529	3788	3791	3793	rBV2	424	253	0.03%	0.004%
98	13.684	3836	3839	3842	rBV	352	198	0.02%	0.003%
99	13.838	3877	3887	3899	rBV2	14100	22508	2.24%	0.314%
100	14.327	4032	4039	4050	rVB5	3440	4783	0.48%	0.067%




Sum of corrected areas: 7164632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052885.D
Acq On : 31 Jan 2023 17:40
Operator : JC/MD
Sample : 01314-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

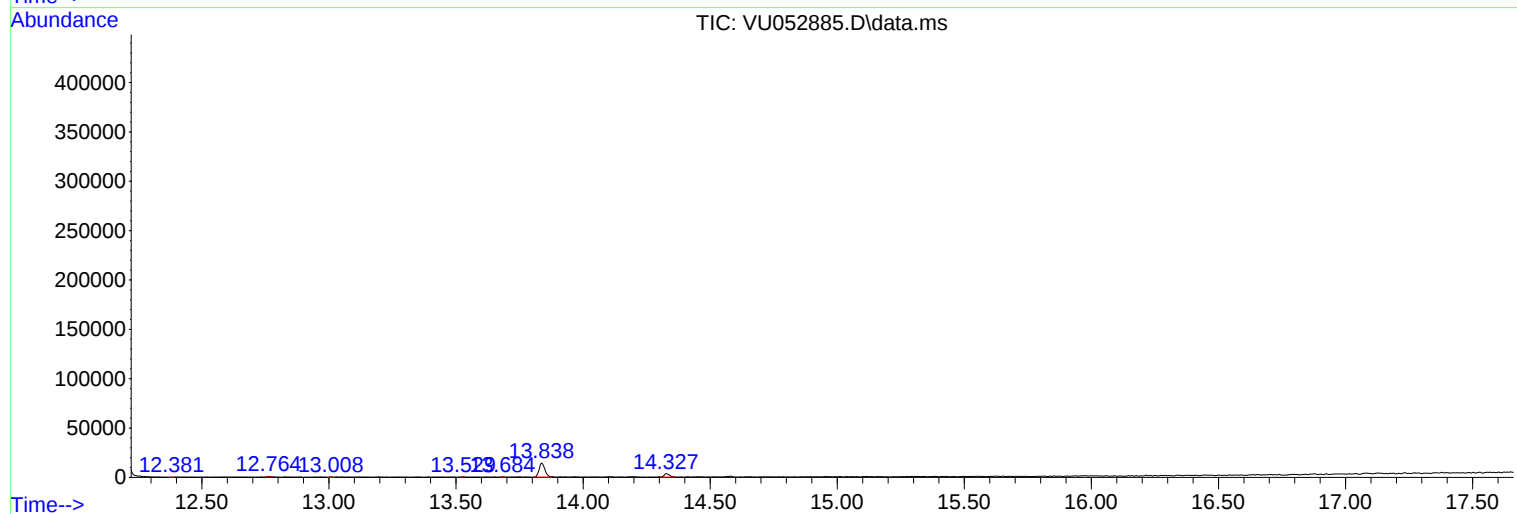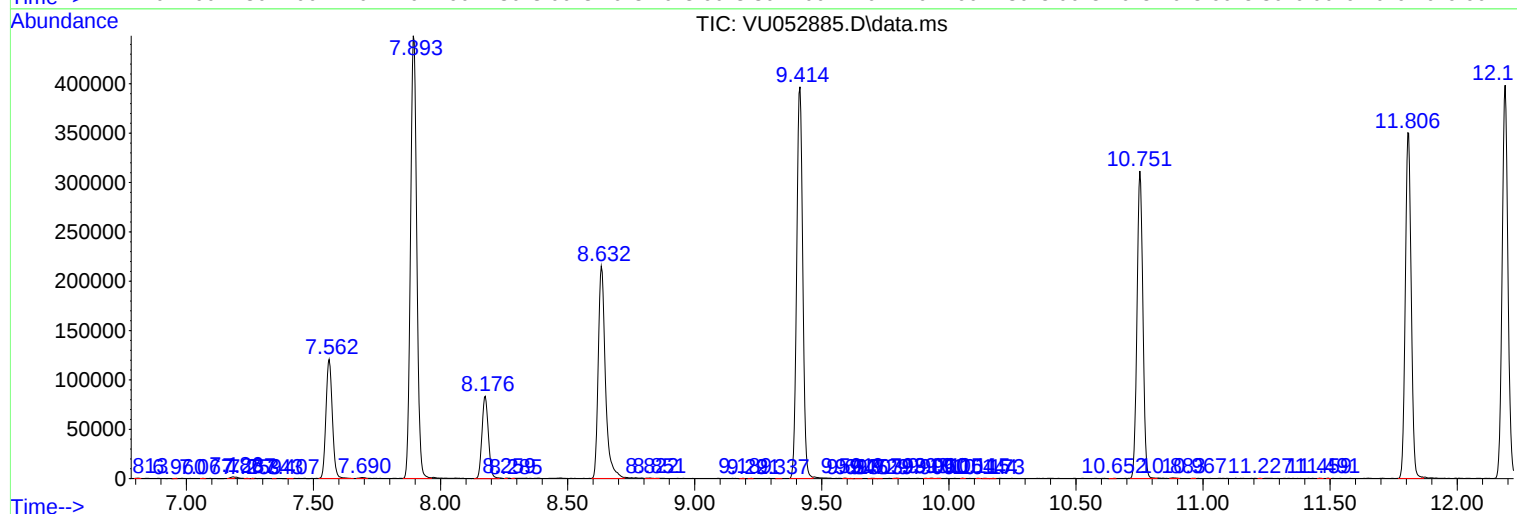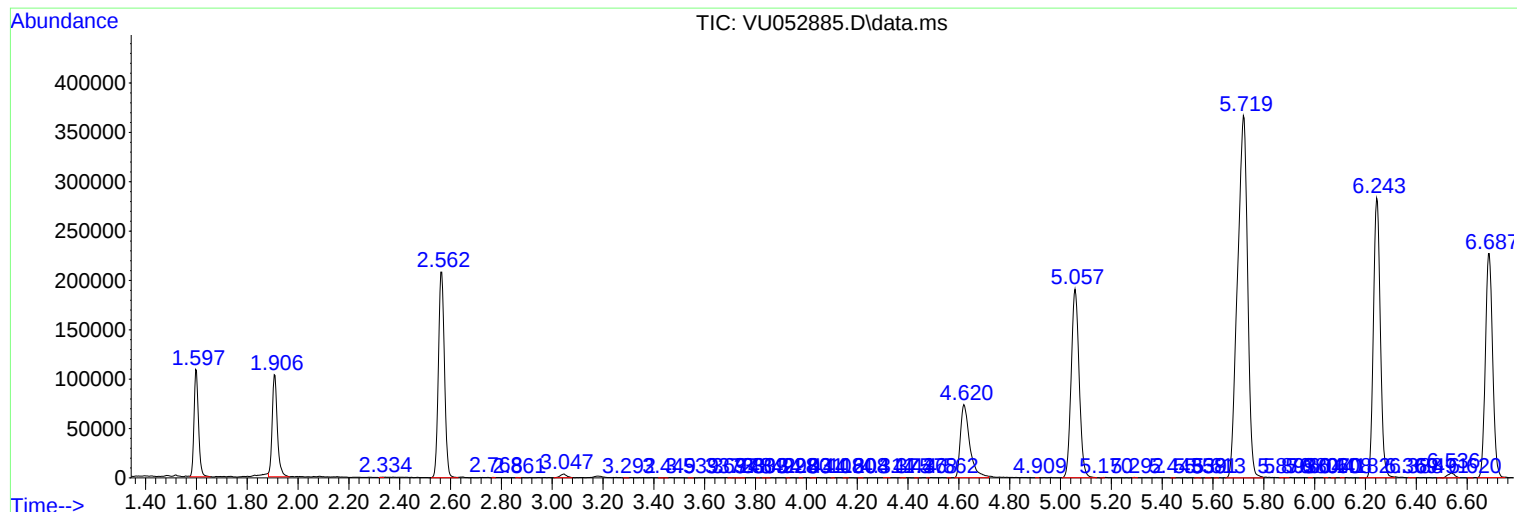

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052885.D
Acq On : 31 Jan 2023 17:40
Operator : JC/MD
Sample : 01314-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052885.D
Acq On : 31 Jan 2023 17:40
Operator : JC/MD
Sample : 01314-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc