

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052889.D
 Acq On : 31 Jan 2023 19:14
 Operator : JC/MD
 Sample : 01381-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M

Title : VOC Analysis

Signal : TIC: VU052889.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	113269	137715	13.83%	1.695%
2	1.909	170	177	206	rVB	104693	150678	15.13%	1.854%
3	2.443	339	343	346	rBV3	409	333	0.03%	0.004%
4	2.481	353	355	357	rBV	340	165	0.02%	0.002%
5	2.514	361	365	366	rBV	280	196	0.02%	0.002%
6	2.565	368	381	398	rVV	212563	345337	34.67%	4.250%
7	2.793	449	452	456	rBV2	340	298	0.03%	0.004%
8	2.883	476	480	482	rBV	302	207	0.02%	0.003%
9	2.977	506	509	512	rBV2	324	228	0.02%	0.003%
10	3.041	524	529	535	rVB2	764	985	0.10%	0.012%
11	3.192	566	576	579	rBV3	720	1252	0.13%	0.015%
12	3.359	625	628	634	rBV2	454	384	0.04%	0.005%
13	3.517	672	677	679	rBV	181	207	0.02%	0.003%
14	3.665	721	723	725	rBV	285	170	0.02%	0.002%
15	3.774	755	757	761	rVV	252	160	0.02%	0.002%
16	3.797	761	764	768	rVB	242	221	0.02%	0.003%
17	4.015	828	832	837	rBB2	269	288	0.03%	0.004%
18	4.195	885	888	891	rVB2	283	198	0.02%	0.002%
19	4.243	900	903	907	rVB2	305	228	0.02%	0.003%
20	4.292	913	918	921	rBB	215	218	0.02%	0.003%
21	4.314	922	925	929	rBB	188	164	0.02%	0.002%
22	4.337	929	932	935	rBV	222	196	0.02%	0.002%
23	4.378	941	945	948	rBB	211	189	0.02%	0.002%
24	4.420	954	958	960	rBV	308	247	0.02%	0.003%
25	4.488	976	979	985	rBB	169	171	0.02%	0.002%
26	4.520	986	989	992	rBB	197	159	0.02%	0.002%
27	4.555	996	1000	1002	rBV2	252	213	0.02%	0.003%
28	4.623	1008	1021	1052	rBV3	68941	242126	24.31%	2.980%
29	4.925	1111	1115	1117	rBV	220	168	0.02%	0.002%
30	5.057	1140	1156	1176	rBV2	186653	407563	40.92%	5.016%
31	5.214	1202	1205	1208	rVB3	438	284	0.03%	0.003%
32	5.247	1212	1215	1221	rBV	268	288	0.03%	0.004%
33	5.417	1265	1268	1271	rBV2	286	226	0.02%	0.003%
34	5.449	1274	1278	1281	rVB	211	188	0.02%	0.002%
35	5.581	1315	1319	1323	rVB2	261	256	0.03%	0.003%
36	5.719	1341	1362	1385	rBV2	362770	996059	100.00%	12.258%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052889.D
 Acq On : 31 Jan 2023 19:14
 Operator : JC/MD
 Sample : 01381-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	5.883	1409	1413	1415	rBV2	173	153	0.02%	0.002%
38	5.948	1429	1433	1434	rBV	233	181	0.02%	0.002%
39	6.021	1454	1456	1460	rBV2	289	205	0.02%	0.003%
40	6.070	1468	1471	1475	rBB	194	187	0.02%	0.002%
41	6.112	1480	1484	1485	rBV2	242	159	0.02%	0.002%
42	6.169	1499	1502	1505	rVB2	312	225	0.02%	0.003%
43	6.243	1509	1525	1545	rBV	293598	554809	55.70%	6.828%
44	6.394	1569	1572	1575	rVB2	322	227	0.02%	0.003%
45	6.411	1575	1577	1579	rBV	243	154	0.02%	0.002%
46	6.456	1589	1591	1594	rBV	248	168	0.02%	0.002%
47	6.536	1603	1616	1637	rBV	307105	579827	58.21%	7.136%
48	6.684	1649	1662	1686	rBV	232312	451584	45.34%	5.557%
49	6.803	1695	1699	1700	rBV	627	339	0.03%	0.004%
50	6.838	1707	1710	1714	rVV2	239	194	0.02%	0.002%
51	6.874	1718	1721	1723	rBB	286	162	0.02%	0.002%
52	6.909	1729	1732	1736	rBB	276	194	0.02%	0.002%
53	7.076	1780	1784	1785	rBV	230	176	0.02%	0.002%
54	7.189	1810	1819	1831	rBV4	1506	2881	0.29%	0.035%
55	7.256	1837	1840	1843	rVB2	321	249	0.02%	0.003%
56	7.372	1873	1876	1880	rVB2	303	255	0.03%	0.003%
57	7.427	1890	1893	1895	rBV	204	155	0.02%	0.002%
58	7.472	1902	1907	1909	rBV	221	236	0.02%	0.003%
59	7.562	1922	1935	1954	rBV2	119374	205974	20.68%	2.535%
60	7.677	1967	1971	1972	rBV	458	313	0.03%	0.004%
61	7.790	2002	2006	2007	rBV2	569	362	0.04%	0.004%
62	7.893	2023	2038	2057	rBV	445165	763552	76.66%	9.397%
63	8.176	2114	2126	2146	rBV2	83589	140140	14.07%	1.725%
64	8.275	2153	2157	2158	rBV	379	208	0.02%	0.003%
65	8.359	2180	2183	2185	rBV	469	341	0.03%	0.004%
66	8.468	2209	2217	2218	rBV2	1515	1434	0.14%	0.018%
67	8.632	2256	2268	2304	rBV2	202249	409266	41.09%	5.037%
68	9.089	2408	2410	2413	rBV	396	307	0.03%	0.004%
69	9.144	2425	2427	2435	rVB	342	289	0.03%	0.004%
70	9.414	2498	2511	2538	rBV	415417	747443	75.04%	9.198%
71	9.552	2551	2554	2556	rBV2	315	257	0.03%	0.003%
72	9.607	2569	2571	2573	rBV	264	158	0.02%	0.002%
73	9.803	2626	2632	2633	rBV	240	259	0.03%	0.003%
74	9.912	2662	2666	2672	rBB	244	317	0.03%	0.004%
75	9.970	2676	2684	2687	rBV	196	315	0.03%	0.004%
76	10.179	2743	2749	2751	rBV	252	313	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052889.D
 Acq On : 31 Jan 2023 19:14
 Operator : JC/MD
 Sample : 01381-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.333	2794	2797	2803	rBV	197	304	0.03%	0.004%
78	10.751	2915	2927	2947	rBV	303445	489590	49.15%	6.025%
79	10.886	2964	2969	2970	rBV	1004	793	0.08%	0.010%
80	11.086	3026	3031	3039	rVB2	241	247	0.02%	0.003%
81	11.317	3099	3103	3105	rBV	212	155	0.02%	0.002%
82	11.648	3201	3206	3216	rVB2	261	321	0.03%	0.004%
83	11.742	3228	3235	3243	rBV4	3812	5618	0.56%	0.069%
84	11.806	3243	3255	3277	rBV	377051	623155	62.56%	7.669%
85	11.992	3311	3313	3318	rBV	217	165	0.02%	0.002%
86	12.057	3325	3333	3349	rBV3	10047	16591	1.67%	0.204%
87	12.188	3361	3374	3395	rBV2	420268	791438	79.46%	9.740%
88	12.774	3548	3556	3562	rVB2	887	1286	0.13%	0.016%
89	12.909	3594	3598	3601	rVB	285	212	0.02%	0.003%
90	13.301	3718	3720	3723	rBV2	297	176	0.02%	0.002%
91	13.661	3828	3832	3835	rBV	239	152	0.02%	0.002%
92	13.680	3835	3838	3840	rBV	317	180	0.02%	0.002%
93	13.835	3878	3886	3902	rVB2	22264	35652	3.58%	0.439%
94	13.954	3921	3923	3924	rBV	326	161	0.02%	0.002%
95	14.095	3966	3967	3973	rVB2	349	187	0.02%	0.002%
96	14.330	4032	4040	4049	rBV4	3957	6470	0.65%	0.080%
97	14.397	4058	4061	4062	rBV	275	160	0.02%	0.002%
98	14.436	4068	4073	4078	rBV2	390	435	0.04%	0.005%
99	14.680	4147	4149	4150	rBV	323	156	0.02%	0.002%
100	15.175	4300	4303	4304	rBV2	457	284	0.03%	0.003%




Sum of corrected areas: 8125821

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052889.D
Acq On : 31 Jan 2023 19:14
Operator : JC/MD
Sample : 01381-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

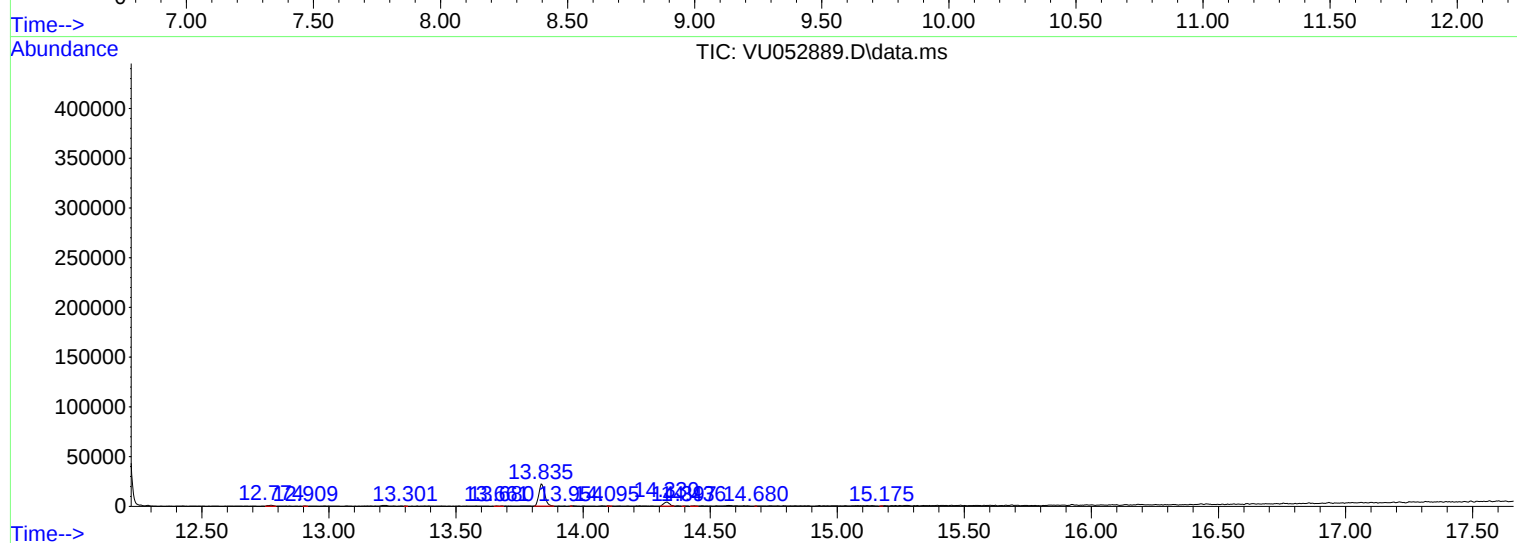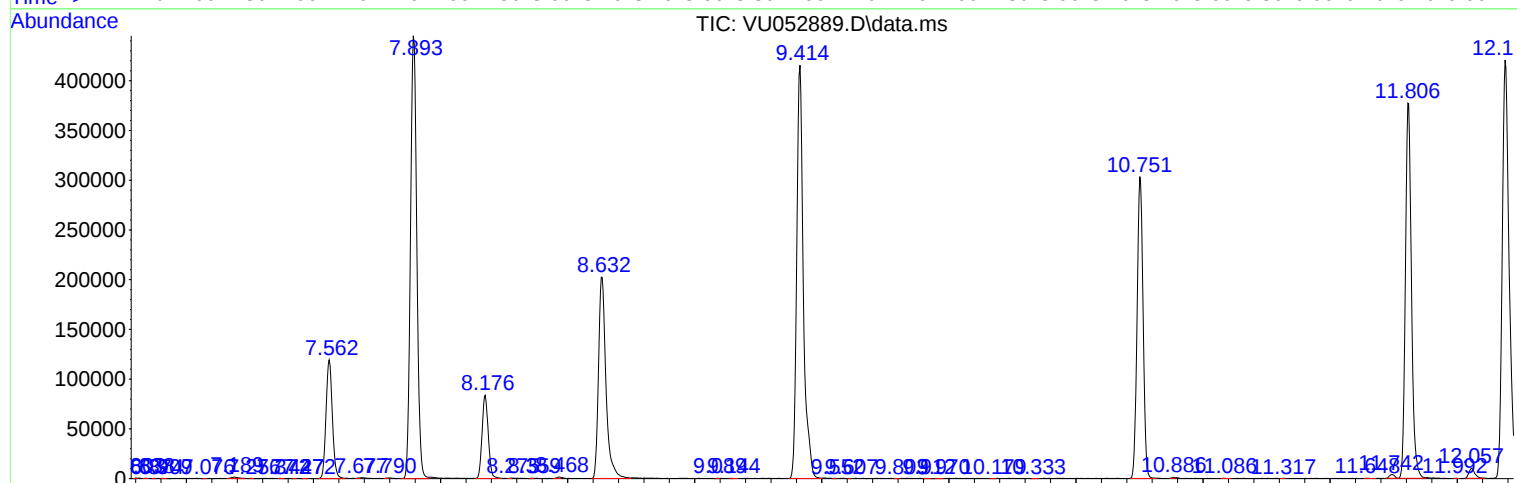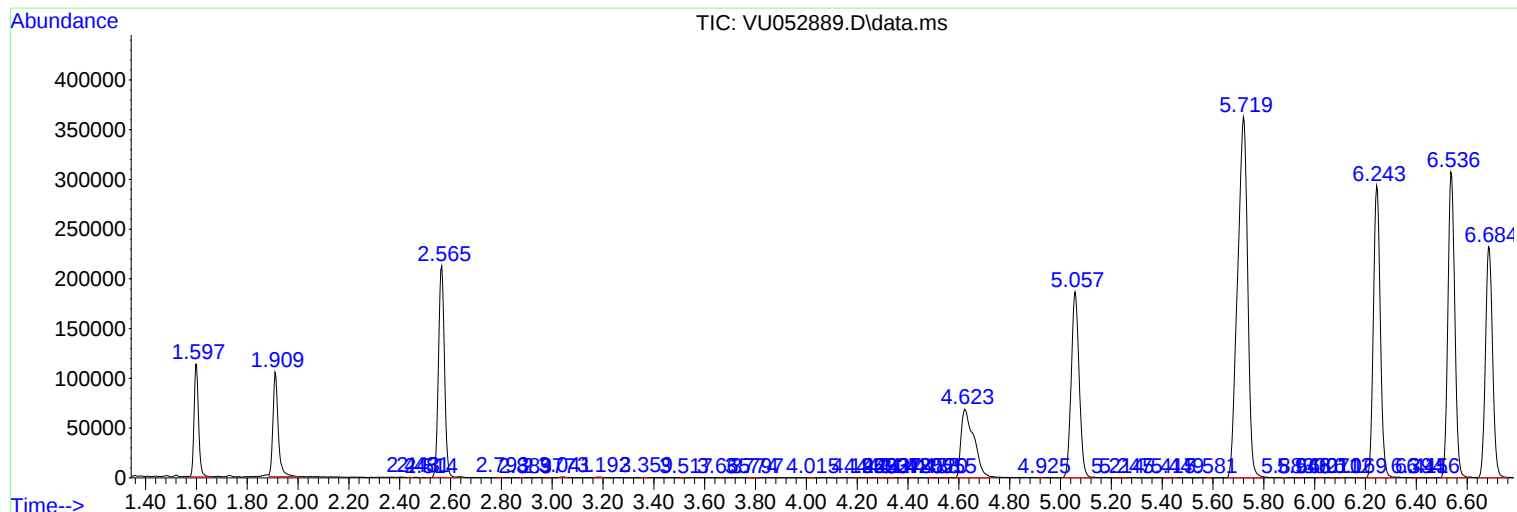

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052889.D
Acq On : 31 Jan 2023 19:14
Operator : JC/MD
Sample : 01381-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052889.D
Acq On : 31 Jan 2023 19:14
Operator : JC/MD
Sample : 01381-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------