

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052891.D
 Acq On : 31 Jan 2023 20:01
 Operator : JC/MD
 Sample : 01381-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	72	81	95	rBV2	123381	154623	0.67%	0.234%
2	1.906	169	176	196	rVB	102608	145947	0.64%	0.221%
3	2.482	352	355	358	rVB2	294	180	0.00%	0.000%
4	2.514	362	365	367	rBV2	379	197	0.00%	0.000%
5	2.565	368	381	396	rBV2	219660	369852	1.61%	0.560%
6	2.675	412	415	416	rBV2	762	433	0.00%	0.001%
7	2.716	425	428	429	rBV	414	216	0.00%	0.000%
8	2.794	448	452	457	rVV2	358	344	0.00%	0.001%
9	2.874	475	477	481	rVB2	361	250	0.00%	0.000%
10	3.041	524	529	534	rBV	788	864	0.00%	0.001%
11	3.125	551	555	559	rVB2	360	392	0.00%	0.001%
12	3.173	565	570	573	rBV2	881	964	0.00%	0.001%
13	3.282	601	604	609	rBV2	227	183	0.00%	0.000%
14	3.350	613	625	643	rVV4	33428	69082	0.30%	0.105%
15	3.443	652	654	657	rVB	286	175	0.00%	0.000%
16	3.498	666	671	673	rBV	203	187	0.00%	0.000%
17	3.568	689	693	696	rBV	183	215	0.00%	0.000%
18	3.610	703	706	709	rBB	217	172	0.00%	0.000%
19	3.864	781	785	788	rBV2	257	225	0.00%	0.000%
20	4.035	836	838	844	rBV	255	229	0.00%	0.000%
21	4.089	851	855	858	rBB	321	247	0.00%	0.000%
22	4.128	862	867	870	rBV	158	200	0.00%	0.000%
23	4.289	914	917	921	rVB2	386	304	0.00%	0.000%
24	4.311	921	924	927	rBV	198	172	0.00%	0.000%
25	4.427	956	960	964	rBV	241	263	0.00%	0.000%
26	4.514	984	987	988	rBV	378	196	0.00%	0.000%
27	4.658	1008	1032	1069	rBV	2703636	6164232	26.90%	9.327%
28	5.057	1140	1156	1181	rVB	183868	404240	1.76%	0.612%
29	5.192	1192	1198	1199	rBV2	547	487	0.00%	0.001%
30	5.240	1210	1213	1217	rBV	291	252	0.00%	0.000%
31	5.276	1221	1224	1226	rBV2	450	266	0.00%	0.000%
32	5.372	1249	1254	1255	rBV3	1200	958	0.00%	0.001%
33	5.472	1281	1285	1287	rBV	389	268	0.00%	0.000%
34	5.517	1296	1299	1305	rBV	212	279	0.00%	0.000%
35	5.555	1307	1311	1313	rBV	238	187	0.00%	0.000%
36	5.719	1341	1362	1371	rBV2	365153	989894	4.32%	1.498%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052891.D
 Acq On : 31 Jan 2023 20:01
 Operator : JC/MD
 Sample : 01381-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	5.877	1408	1411	1413	rBV	342	240	0.00%	0.000%
38	5.893	1413	1416	1421	rVB2	375	285	0.00%	0.000%
39	5.932	1421	1428	1429	rBV2	2192	2121	0.01%	0.003%
40	6.076	1469	1473	1475	rVB	342	244	0.00%	0.000%
41	6.150	1493	1496	1500	rBB	222	186	0.00%	0.000%
42	6.244	1512	1525	1545	rBV	300977	565727	2.47%	0.856%
43	6.440	1584	1586	1592	rVB2	317	220	0.00%	0.000%
44	6.469	1592	1595	1597	rBV2	287	204	0.00%	0.000%
45	6.536	1598	1616	1643	rVV	313856	588691	2.57%	0.891%
46	6.684	1649	1662	1678	rBV	228987	438457	1.91%	0.663%
47	6.961	1746	1748	1751	rVB	330	186	0.00%	0.000%
48	6.989	1751	1757	1761	rBV	239	334	0.00%	0.001%
49	7.192	1810	1820	1824	rBV5	1577	2778	0.01%	0.004%
50	7.346	1861	1868	1871	rBB	181	240	0.00%	0.000%
51	7.456	1895	1902	1904	rBV	276	305	0.00%	0.000%
52	7.562	1921	1935	1959	rVV	117890	206206	0.90%	0.312%
53	7.694	1970	1976	1985	rVB2	1010	1383	0.01%	0.002%
54	7.793	2004	2007	2010	rVB3	531	389	0.00%	0.001%
55	7.838	2019	2021	2025	rVV	318	187	0.00%	0.000%
56	7.893	2025	2038	2052	rVV	450203	769525	3.36%	1.164%
57	7.967	2054	2061	2078	rVB	20263	35638	0.16%	0.054%
58	8.089	2097	2099	2102	rBV	288	228	0.00%	0.000%
59	8.176	2114	2126	2141	rBV	82941	141415	0.62%	0.214%
60	8.353	2179	2181	2183	rBV	330	211	0.00%	0.000%
61	8.404	2194	2197	2199	rBV	291	223	0.00%	0.000%
62	8.430	2203	2205	2208	rVB2	350	190	0.00%	0.000%
63	8.459	2208	2214	2218	rBV3	1068	1323	0.01%	0.002%
64	8.632	2256	2268	2300	rVV2	200502	397423	1.73%	0.601%
65	8.771	2309	2311	2316	rBV3	545	366	0.00%	0.001%
66	8.932	2355	2361	2364	rBV3	596	491	0.00%	0.001%
67	9.214	2445	2449	2452	rBV	252	275	0.00%	0.000%
68	9.446	2498	2521	2548	rBV	13823481	22915143	100.00%	34.674%
69	9.565	2550	2558	2573	rVB	245205	390924	1.71%	0.592%
70	9.877	2651	2655	2667	rVB4	684	1141	0.00%	0.002%
71	10.012	2694	2697	2700	rVB	535	411	0.00%	0.001%
72	10.038	2700	2705	2707	rBV2	283	293	0.00%	0.000%
73	10.099	2713	2724	2735	rBV	11023	16284	0.07%	0.025%
74	10.481	2834	2843	2853	rBV2	2639	3462	0.02%	0.005%
75	10.562	2861	2868	2880	rVB4	3478	5085	0.02%	0.008%
76	10.751	2915	2927	2941	rBV	302987	478941	2.09%	0.725%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052891.D
 Acq On : 31 Jan 2023 20:01
 Operator : JC/MD
 Sample : 01381-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.854	2955	2959	2964	rBV3	842	967	0.00%	0.001%
78	10.903	2964	2974	2985	rVB2	6500	11182	0.05%	0.017%
79	10.980	2992	2998	2999	rBV2	1703	1171	0.01%	0.002%
80	11.099	3027	3035	3043	rBV3	1303	1352	0.01%	0.002%
81	11.182	3059	3061	3065	rVB	422	252	0.00%	0.000%
82	11.205	3065	3068	3071	rBV	276	250	0.00%	0.000%
83	11.288	3084	3094	3105	rBV2	11004	16513	0.07%	0.025%
84	11.465	3141	3149	3157	rBV	9706	12236	0.05%	0.019%
85	11.742	3222	3235	3245	rBV	249766	392352	1.71%	0.594%
86	11.832	3245	3263	3276	rBV2	2367580	4308427	18.80%	6.519%
87	12.057	3322	3333	3338	rBV4	8467	13570	0.06%	0.021%
88	12.211	3360	3381	3413	rBV	13785150	22178031	96.78%	33.559%
89	12.674	3523	3525	3529	rVV	491	347	0.00%	0.001%
90	12.722	3536	3540	3547	rBV5	1304	1385	0.01%	0.002%
91	12.803	3557	3565	3582	rVB3	13339	19976	0.09%	0.030%
92	12.899	3592	3595	3596	rBV	392	198	0.00%	0.000%
93	13.140	3669	3670	3673	rBV2	371	223	0.00%	0.000%
94	13.214	3688	3693	3703	rVB5	2431	3322	0.01%	0.005%
95	13.279	3709	3713	3715	rBV	223	209	0.00%	0.000%
96	13.359	3735	3738	3740	rVB2	367	197	0.00%	0.000%
97	13.787	3868	3871	3873	rBV	397	240	0.00%	0.000%
98	13.835	3873	3886	3908	rVV	2027318	3125909	13.64%	4.730%
99	14.189	3994	3996	3998	rBV2	428	246	0.00%	0.000%
100	14.324	4025	4038	4064	rBV	457801	724248	3.16%	1.096%


Sum of corrected areas: 66087353

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052891.D
Acq On : 31 Jan 2023 20:01
Operator : JC/MD
Sample : 01381-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

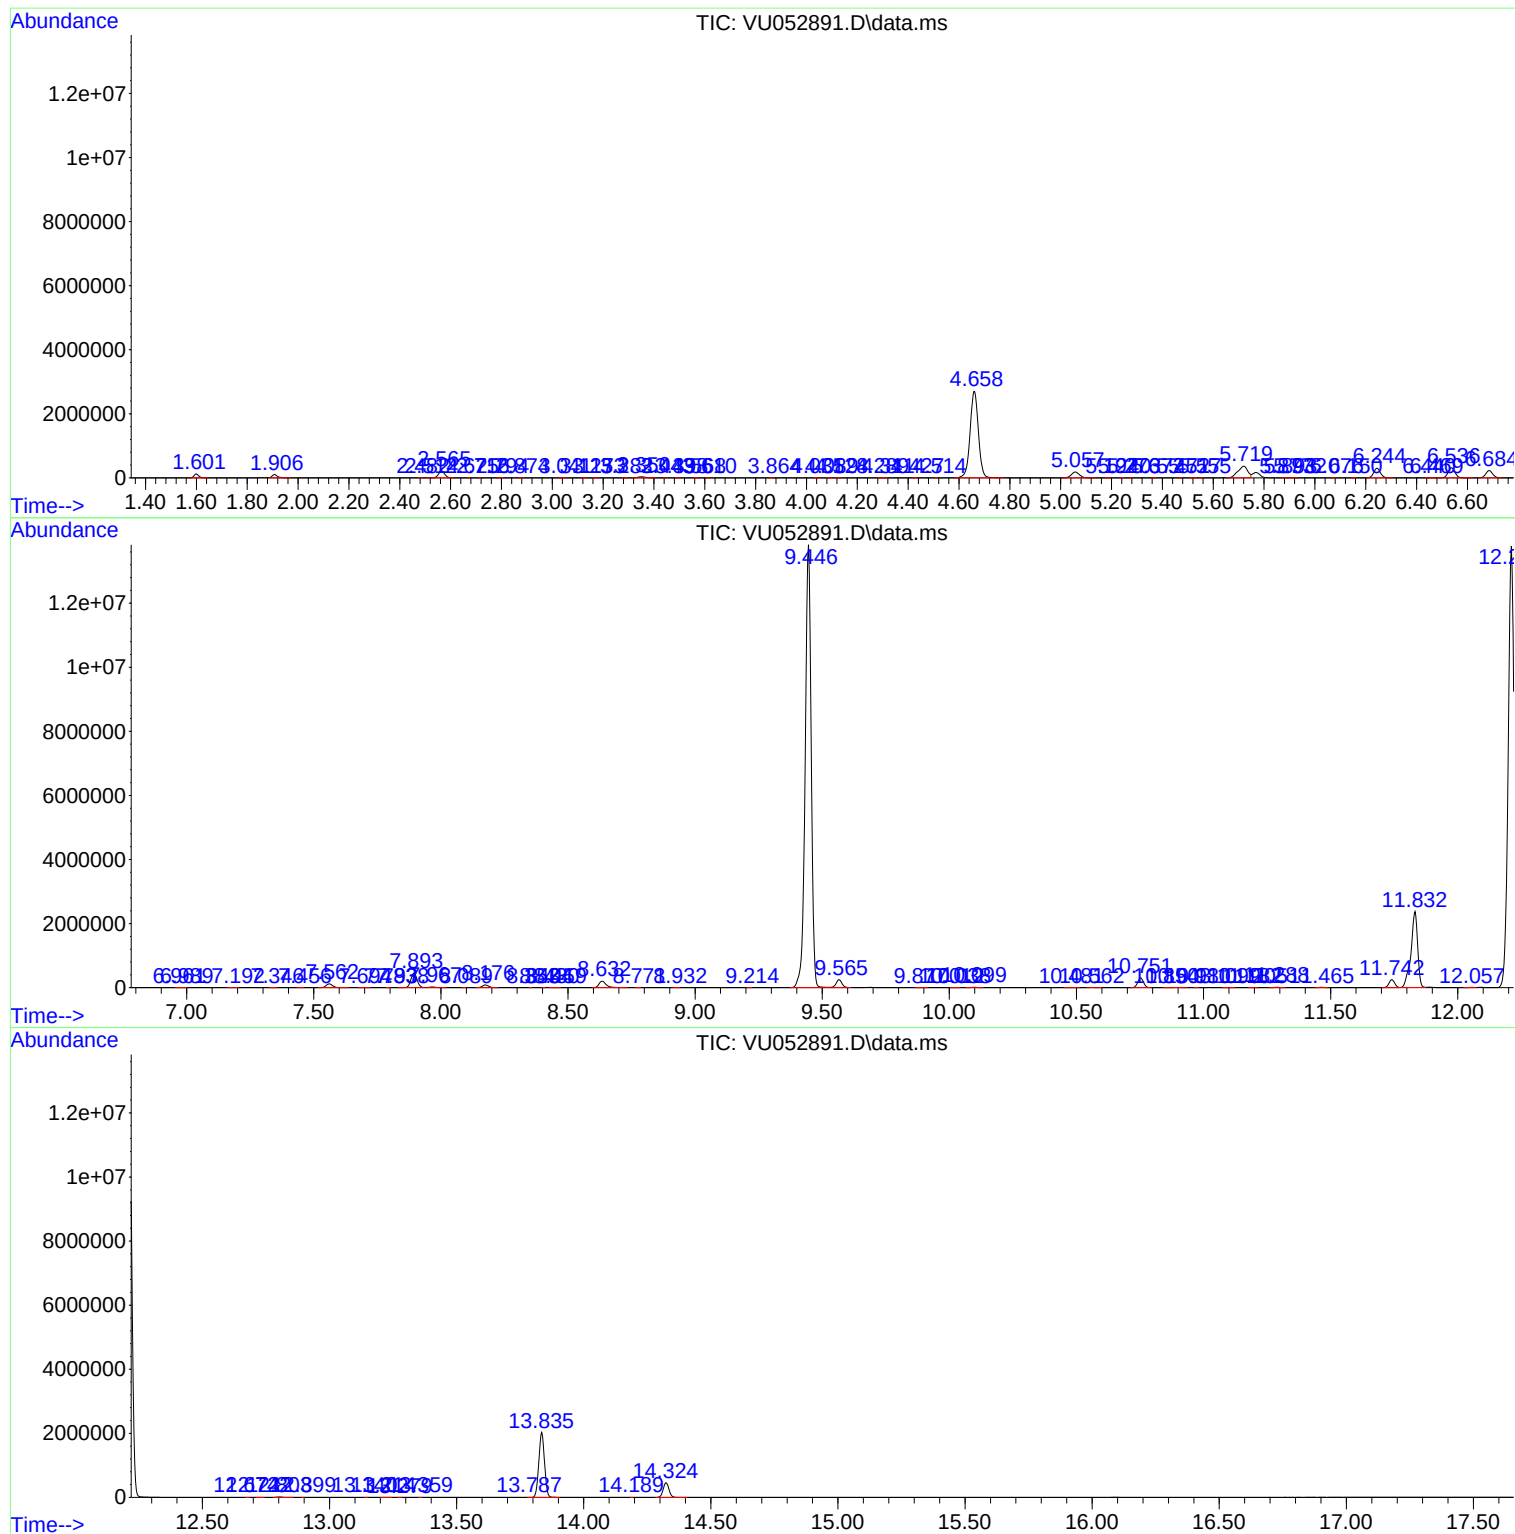

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052891.D
Acq On : 31 Jan 2023 20:01
Operator : JC/MD
Sample : 01381-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052891.D
Acq On : 31 Jan 2023 20:01
Operator : JC/MD
Sample : 01381-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------