

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052892.D
 Acq On : 31 Jan 2023 20:24
 Operator : JC/MD
 Sample : 01381-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052892.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rVB2	126438	153864	0.33%	0.115%
2	1.909	169	177	197	rVB	94456	132294	0.28%	0.099%
3	2.568	369	382	397	rBV2	219550	381240	0.81%	0.284%
4	2.684	413	418	421	rVB3	542	510	0.00%	0.000%
5	2.858	468	472	476	rBV2	179	133	0.00%	0.000%
6	2.877	476	478	485	rVV2	153	144	0.00%	0.000%
7	2.906	485	487	490	rBV2	247	164	0.00%	0.000%
8	3.041	523	529	536	rBV3	1747	2662	0.01%	0.002%
9	3.186	568	574	580	rVV4	409	610	0.00%	0.000%
10	3.215	581	583	586	rVB2	607	320	0.00%	0.000%
11	3.244	587	592	598	rBV2	247	337	0.00%	0.000%
12	3.353	611	626	643	rBV2	53893	110660	0.24%	0.083%
13	3.658	717	721	722	rBV	385	244	0.00%	0.000%
14	3.735	743	745	747	rVB	281	130	0.00%	0.000%
15	3.864	778	785	787	rVV2	362	429	0.00%	0.000%
16	3.935	802	807	811	rBV	203	238	0.00%	0.000%
17	3.977	817	820	821	rBV	275	134	0.00%	0.000%
18	4.083	850	853	856	rBV	194	181	0.00%	0.000%
19	4.147	871	873	876	rBV2	296	206	0.00%	0.000%
20	4.221	892	896	902	rBB2	308	354	0.00%	0.000%
21	4.301	917	921	926	rBB	316	338	0.00%	0.000%
22	4.362	933	940	943	rBV	242	355	0.00%	0.000%
23	4.414	954	956	959	rBV	286	189	0.00%	0.000%
24	4.661	1008	1033	1073	rBV	4525455	10200302	21.80%	7.606%
25	5.057	1142	1156	1181	rVB	182014	404026	0.86%	0.301%
26	5.166	1187	1190	1193	rBV2	663	580	0.00%	0.000%
27	5.288	1227	1228	1231	rBV2	451	284	0.00%	0.000%
28	5.382	1245	1257	1269	rBV7	3879	9157	0.02%	0.007%
29	5.446	1274	1277	1278	rBV	348	166	0.00%	0.000%
30	5.591	1314	1322	1330	rVV5	1433	2187	0.00%	0.002%
31	5.645	1336	1339	1340	rBV2	263	171	0.00%	0.000%
32	5.719	1341	1362	1371	rBV2	361639	991264	2.12%	0.739%
33	5.938	1419	1430	1438	rBV6	3329	6724	0.01%	0.005%
34	6.044	1456	1463	1466	rVB2	442	468	0.00%	0.000%
35	6.108	1477	1483	1484	rBV	254	265	0.00%	0.000%
36	6.150	1493	1496	1498	rBV	375	231	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052892.D
 Acq On : 31 Jan 2023 20:24
 Operator : JC/MD
 Sample : 01381-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.243	1511	1525	1549	rBV	302885	568167	1.21%	0.424%
38	6.443	1585	1587	1594	rBV2	270	193	0.00%	0.000%
39	6.539	1597	1617	1638	rVV	481682	905491	1.94%	0.675%
40	6.687	1648	1663	1677	rBV	223612	431840	0.92%	0.322%
41	6.886	1723	1725	1726	rBV	261	139	0.00%	0.000%
42	7.067	1778	1781	1783	rVB	345	177	0.00%	0.000%
43	7.186	1811	1818	1824	rBV3	1706	2218	0.00%	0.002%
44	7.247	1835	1837	1841	rBV	252	176	0.00%	0.000%
45	7.488	1907	1912	1915	rBB	238	149	0.00%	0.000%
46	7.510	1916	1919	1920	rBV	296	174	0.00%	0.000%
47	7.562	1923	1935	1955	rVV	118657	207385	0.44%	0.155%
48	7.684	1969	1973	1976	rBV3	743	667	0.00%	0.000%
49	7.809	2009	2012	2016	rVB3	399	321	0.00%	0.000%
50	7.848	2021	2024	2025	rBV2	421	205	0.00%	0.000%
51	7.893	2025	2038	2053	rBV	449006	771113	1.65%	0.575%
52	8.086	2095	2098	2101	rBV	280	188	0.00%	0.000%
53	8.173	2114	2125	2142	rBV	85846	144045	0.31%	0.107%
54	8.353	2179	2181	2184	rBV4	426	257	0.00%	0.000%
55	8.382	2188	2190	2194	rVB	468	278	0.00%	0.000%
56	8.629	2256	2267	2296	rBV2	208045	396947	0.85%	0.296%
57	8.835	2328	2331	2333	rVB2	356	163	0.00%	0.000%
58	8.935	2356	2362	2370	rVB4	1262	1333	0.00%	0.001%
59	9.015	2384	2387	2390	rBV	154	156	0.00%	0.000%
60	9.092	2407	2411	2414	rVB2	338	305	0.00%	0.000%
61	9.115	2415	2418	2421	rBV	167	134	0.00%	0.000%
62	9.449	2498	2522	2548	rBV	24804489	41421985	88.52%	30.885%
63	9.565	2550	2558	2581	rVB	310981	505448	1.08%	0.377%
64	10.095	2714	2723	2735	rVB2	19644	30428	0.07%	0.023%
65	10.195	2749	2754	2755	rBV2	283	268	0.00%	0.000%
66	10.404	2812	2819	2823	rBB4	524	575	0.00%	0.000%
67	10.449	2830	2833	2835	rVV	367	264	0.00%	0.000%
68	10.478	2835	2842	2856	rVV4	5498	8409	0.02%	0.006%
69	10.562	2859	2868	2879	rVB3	6170	9602	0.02%	0.007%
70	10.607	2879	2882	2885	rBV	251	153	0.00%	0.000%
71	10.751	2915	2927	2946	rBV	300844	477800	1.02%	0.356%
72	10.854	2954	2959	2964	rBV4	1250	1326	0.00%	0.001%
73	10.902	2965	2974	2990	rVB	17234	26427	0.06%	0.020%
74	10.986	2990	3000	3006	rBV5	4266	7087	0.02%	0.005%
75	11.099	3025	3035	3044	rVB4	2467	4041	0.01%	0.003%
76	11.243	3078	3080	3084	rBV	238	148	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052892.D
 Acq On : 31 Jan 2023 20:24
 Operator : JC/MD
 Sample : 01381-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	11.288	3084	3094	3108	rVV2	26883	41377	0.09%	0.031%
78	11.462	3140	3148	3155	rBV2	5961	8853	0.02%	0.007%
79	11.742	3221	3235	3245	rBV	604510	936318	2.00%	0.698%
80	11.832	3246	3263	3277	rVV	5535254	9175413	19.61%	6.841%
81	12.217	3362	3383	3424	rBV	28223130	46794933	100.00%	34.892%
82	12.725	3534	3541	3548	rVB3	2050	3026	0.01%	0.002%
83	12.767	3550	3554	3555	rVV2	759	493	0.00%	0.000%
84	12.799	3556	3564	3577	rVB2	33132	51217	0.11%	0.038%
85	12.861	3581	3583	3584	rBV2	513	221	0.00%	0.000%
86	12.967	3607	3616	3624	rBV4	3532	5005	0.01%	0.004%
87	13.025	3627	3634	3639	rBV5	1529	2016	0.00%	0.002%
88	13.143	3661	3671	3683	rVB3	4286	8038	0.02%	0.006%
89	13.214	3683	3693	3704	rBV3	13018	19611	0.04%	0.015%
90	13.324	3723	3727	3735	rBV6	1220	1455	0.00%	0.001%
91	13.410	3749	3754	3759	rBV2	241	247	0.00%	0.000%
92	13.446	3759	3765	3766	rBV4	1482	1271	0.00%	0.001%
93	13.552	3796	3798	3800	rBV	283	175	0.00%	0.000%
94	13.568	3800	3803	3804	rBV	481	292	0.00%	0.000%
95	13.687	3837	3840	3842	rBV	373	170	0.00%	0.000%
96	13.838	3872	3887	3918	rBV	9972997	15325292	32.75%	11.427%
97	14.323	4023	4038	4061	rBV	2093113	3321751	7.10%	2.477%
98	15.410	4372	4376	4387	rVB6	2867	3741	0.01%	0.003%
99	15.944	4538	4542	4544	rBV4	4627	3824	0.01%	0.003%
100	16.085	4577	4586	4598	rBV2	52443	82900	0.18%	0.062%




Sum of corrected areas: 134115382

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052892.D
Acq On : 31 Jan 2023 20:24
Operator : JC/MD
Sample : 01381-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

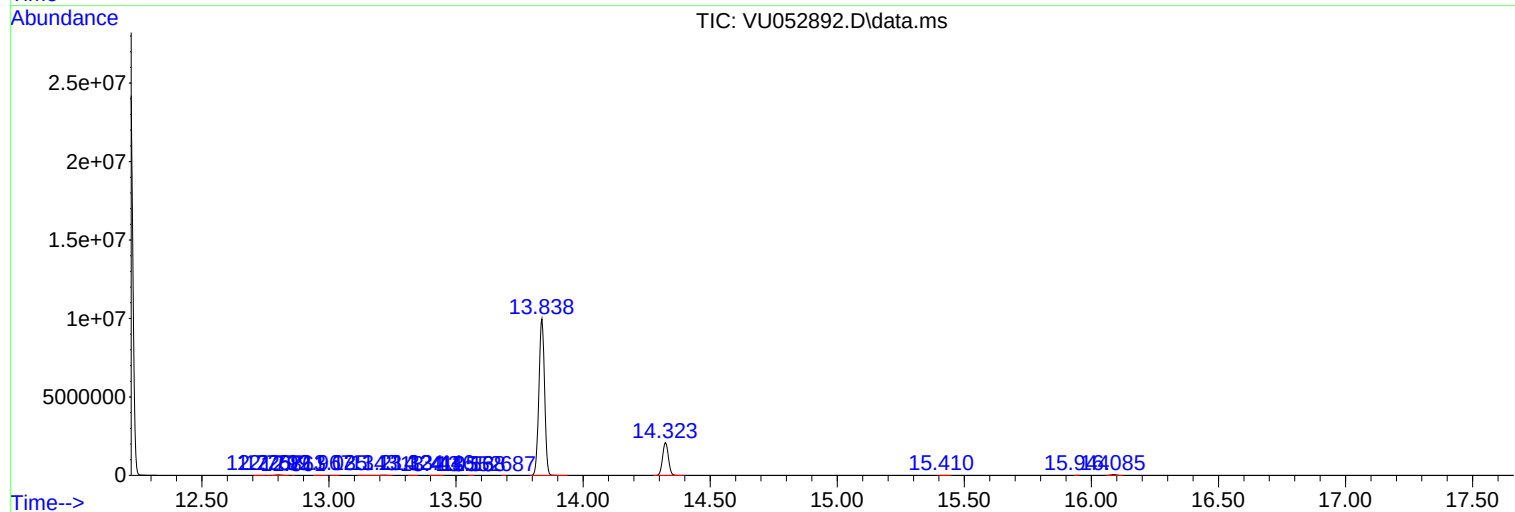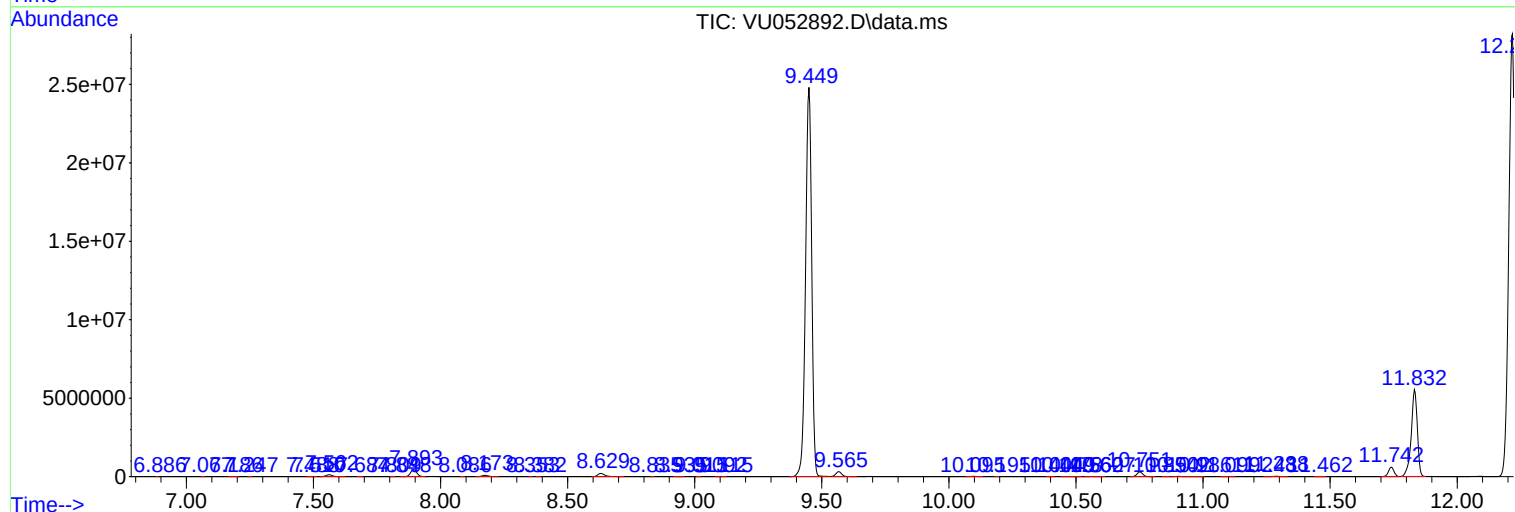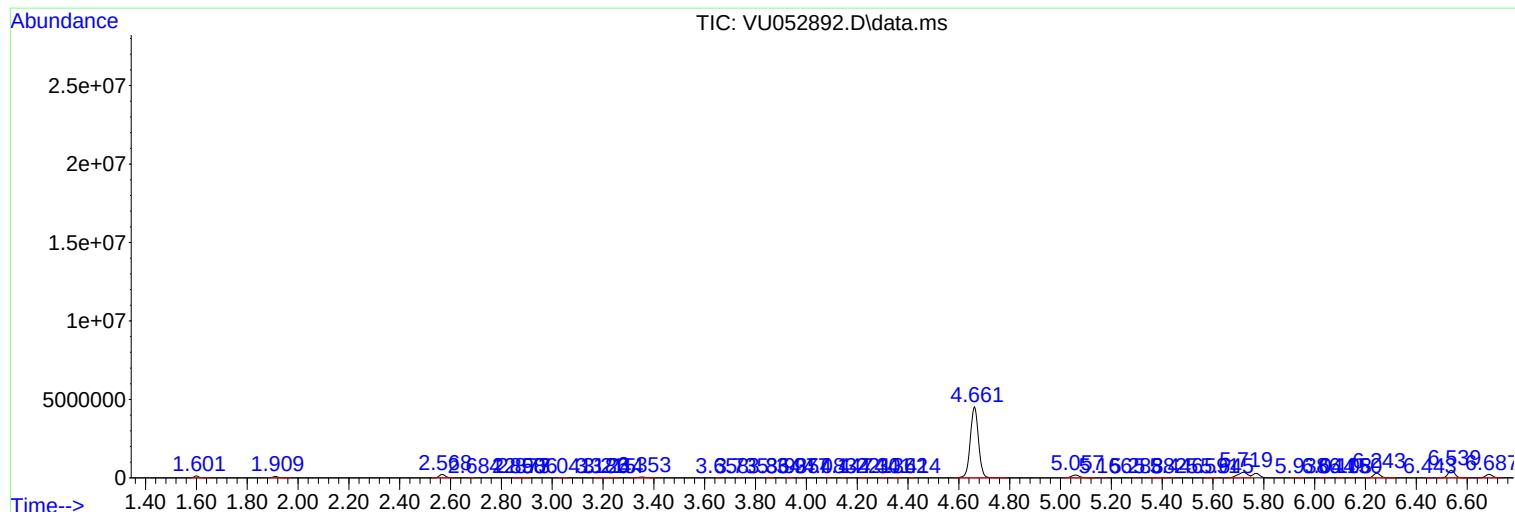

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052892.D
Acq On : 31 Jan 2023 20:24
Operator : JC/MD
Sample : 01381-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052892.D
Acq On : 31 Jan 2023 20:24
Operator : JC/MD
Sample : 01381-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------