

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052893.D
 Acq On : 31 Jan 2023 20:48
 Operator : JC/MD
 Sample : VIBLK108
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	113955	138157	13.63%	1.708%
2	1.906	169	176	196	rVB	106967	148553	14.66%	1.837%
3	2.565	369	381	397	rBV	216544	349185	34.45%	4.317%
4	2.719	427	429	434	rVB	469	284	0.03%	0.004%
5	2.909	485	488	491	rBV2	511	421	0.04%	0.005%
6	3.044	522	530	543	rVB4	2550	4654	0.46%	0.058%
7	3.179	562	572	585	rBV2	2807	5833	0.58%	0.072%
8	3.379	631	634	638	rVB2	329	269	0.03%	0.003%
9	3.404	638	642	645	rBV2	299	280	0.03%	0.003%
10	3.507	671	674	678	rBV	351	308	0.03%	0.004%
11	3.559	687	690	694	rVB	409	286	0.03%	0.004%
12	3.594	698	701	703	rBB2	360	191	0.02%	0.002%
13	3.658	719	721	726	rBV2	317	311	0.03%	0.004%
14	3.761	748	753	758	rBV2	345	439	0.04%	0.005%
15	3.842	775	778	780	rBV	157	131	0.01%	0.002%
16	3.915	795	801	804	rBB	225	255	0.03%	0.003%
17	3.938	805	808	812	rBB	457	313	0.03%	0.004%
18	3.960	812	815	818	rBB	183	141	0.01%	0.002%
19	3.996	824	826	829	rBV	201	169	0.02%	0.002%
20	4.147	871	873	876	rBV	161	129	0.01%	0.002%
21	4.266	908	910	914	rVB2	223	142	0.01%	0.002%
22	4.388	945	948	952	rVB	306	248	0.02%	0.003%
23	4.423	956	959	961	rBV	186	144	0.01%	0.002%
24	4.620	1008	1020	1055	rBV	72265	208701	20.59%	2.580%
25	4.899	1104	1107	1111	rBV2	254	246	0.02%	0.003%
26	4.989	1133	1135	1138	rBV2	264	174	0.02%	0.002%
27	5.057	1141	1156	1182	rVB	186598	412396	40.69%	5.099%
28	5.153	1183	1186	1190	rBV2	389	244	0.02%	0.003%
29	5.208	1200	1203	1204	rBV	339	214	0.02%	0.003%
30	5.263	1217	1220	1223	rBV2	174	144	0.01%	0.002%
31	5.462	1277	1282	1285	rBV	275	291	0.03%	0.004%
32	5.546	1305	1308	1310	rVB	201	137	0.01%	0.002%
33	5.642	1331	1338	1341	rBB	214	252	0.02%	0.003%
34	5.719	1341	1362	1389	rBV2	370547	1013488	100.00%	12.531%
35	5.870	1404	1409	1418	rVB2	288	421	0.04%	0.005%
36	5.967	1436	1439	1443	rVB2	296	242	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052893.D
 Acq On : 31 Jan 2023 20:48
 Operator : JC/MD
 Sample : VIBLK108
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.015	1452	1454	1458	rBV	232	163	0.02%	0.002%
38	6.041	1458	1462	1468	rVB2	478	566	0.06%	0.007%
39	6.243	1511	1525	1549	rBV	308629	579405	57.17%	7.164%
40	6.462	1590	1593	1596	rVV	222	203	0.02%	0.003%
41	6.533	1604	1615	1627	rBV9	2462	4946	0.49%	0.061%
42	6.610	1636	1639	1646	rVB2	367	388	0.04%	0.005%
43	6.684	1647	1662	1682	rBV	229666	452154	44.61%	5.590%
44	6.787	1692	1694	1695	rVB	440	142	0.01%	0.002%
45	6.809	1696	1701	1704	rBV	461	407	0.04%	0.005%
46	6.829	1704	1707	1711	rVV3	407	243	0.02%	0.003%
47	7.012	1759	1764	1765	rBV	219	193	0.02%	0.002%
48	7.105	1791	1793	1796	rVB	262	135	0.01%	0.002%
49	7.124	1796	1799	1803	rBB	142	137	0.01%	0.002%
50	7.185	1808	1818	1826	rBV5	2172	3662	0.36%	0.045%
51	7.282	1846	1848	1850	rBV	256	157	0.02%	0.002%
52	7.449	1893	1900	1903	rBV	208	325	0.03%	0.004%
53	7.562	1922	1935	1957	rBV	116993	207593	20.48%	2.567%
54	7.687	1968	1974	1975	rBV2	936	838	0.08%	0.010%
55	7.893	2025	2038	2057	rBV	459546	785053	77.46%	9.706%
56	8.070	2088	2093	2096	rVB2	373	287	0.03%	0.004%
57	8.176	2115	2126	2146	rBV2	85099	144825	14.29%	1.791%
58	8.250	2146	2149	2150	rBV	293	173	0.02%	0.002%
59	8.430	2202	2205	2208	rBV2	189	159	0.02%	0.002%
60	8.578	2248	2251	2252	rBV	257	155	0.02%	0.002%
61	8.632	2255	2268	2295	rBV2	214910	415831	41.03%	5.141%
62	8.861	2335	2339	2341	rBV	316	227	0.02%	0.003%
63	8.886	2344	2347	2351	rVB	375	289	0.03%	0.004%
64	8.912	2352	2355	2356	rBV	274	137	0.01%	0.002%
65	8.925	2357	2359	2364	rVB2	267	164	0.02%	0.002%
66	9.079	2403	2407	2409	rBV	242	201	0.02%	0.002%
67	9.147	2424	2428	2431	rBV	180	215	0.02%	0.003%
68	9.253	2457	2461	2466	rBV	283	413	0.04%	0.005%
69	9.311	2476	2479	2482	rBV2	239	216	0.02%	0.003%
70	9.414	2497	2511	2532	rBV2	423287	794269	78.37%	9.820%
71	9.558	2554	2556	2558	rBV	560	344	0.03%	0.004%
72	9.867	2650	2652	2657	rVB2	286	158	0.02%	0.002%
73	10.015	2695	2698	2704	rVB2	159	142	0.01%	0.002%
74	10.118	2728	2730	2733	rBV	264	173	0.02%	0.002%
75	10.426	2823	2826	2830	rBV	210	237	0.02%	0.003%
76	10.587	2873	2876	2880	rVB2	235	207	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
 Data File : VU052893.D
 Acq On : 31 Jan 2023 20:48
 Operator : JC/MD
 Sample : VIBLK108
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.677	2898	2904	2907	rBV2	311	365	0.04%	0.005%
78	10.751	2914	2927	2946	rBV	298197	486180	47.97%	6.011%
79	10.877	2963	2966	2969	rBV	264	185	0.02%	0.002%
80	10.893	2969	2971	2976	rVB	354	232	0.02%	0.003%
81	11.465	3142	3149	3151	rBV2	383	418	0.04%	0.005%
82	11.671	3210	3213	3217	rBV	227	222	0.02%	0.003%
83	11.742	3229	3235	3243	rBV3	2422	3537	0.35%	0.044%
84	11.809	3243	3256	3286	rVV	398221	681603	67.25%	8.427%
85	12.044	3325	3329	3331	rBV	234	219	0.02%	0.003%
86	12.057	3331	3333	3338	rVV	250	263	0.03%	0.003%
87	12.140	3356	3359	3361	rBV	373	245	0.02%	0.003%
88	12.188	3361	3374	3403	rVV2	438174	887039	87.52%	10.967%
89	12.507	3471	3473	3476	rBV2	252	157	0.02%	0.002%
90	12.796	3560	3563	3566	rBV	180	170	0.02%	0.002%
91	12.844	3574	3578	3580	rBV2	417	285	0.03%	0.004%
92	13.430	3758	3760	3763	rVB	314	139	0.01%	0.002%
93	13.539	3792	3794	3796	rBV	269	140	0.01%	0.002%
94	13.835	3875	3886	3903	rBV	155724	251205	24.79%	3.106%
95	13.941	3917	3919	3921	rBV	271	141	0.01%	0.002%
96	14.208	3999	4002	4006	rBV2	268	234	0.02%	0.003%
97	14.323	4027	4038	4052	rBV2	43612	69851	6.89%	0.864%
98	15.095	4276	4278	4282	rVB2	619	276	0.03%	0.003%
99	15.410	4373	4376	4379	rBV3	605	582	0.06%	0.007%
100	16.085	4579	4586	4601	rVB3	13864	20992	2.07%	0.260%




Sum of corrected areas: 8088005

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052893.D
Acq On : 31 Jan 2023 20:48
Operator : JC/MD
Sample : VIBLK108
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK108

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

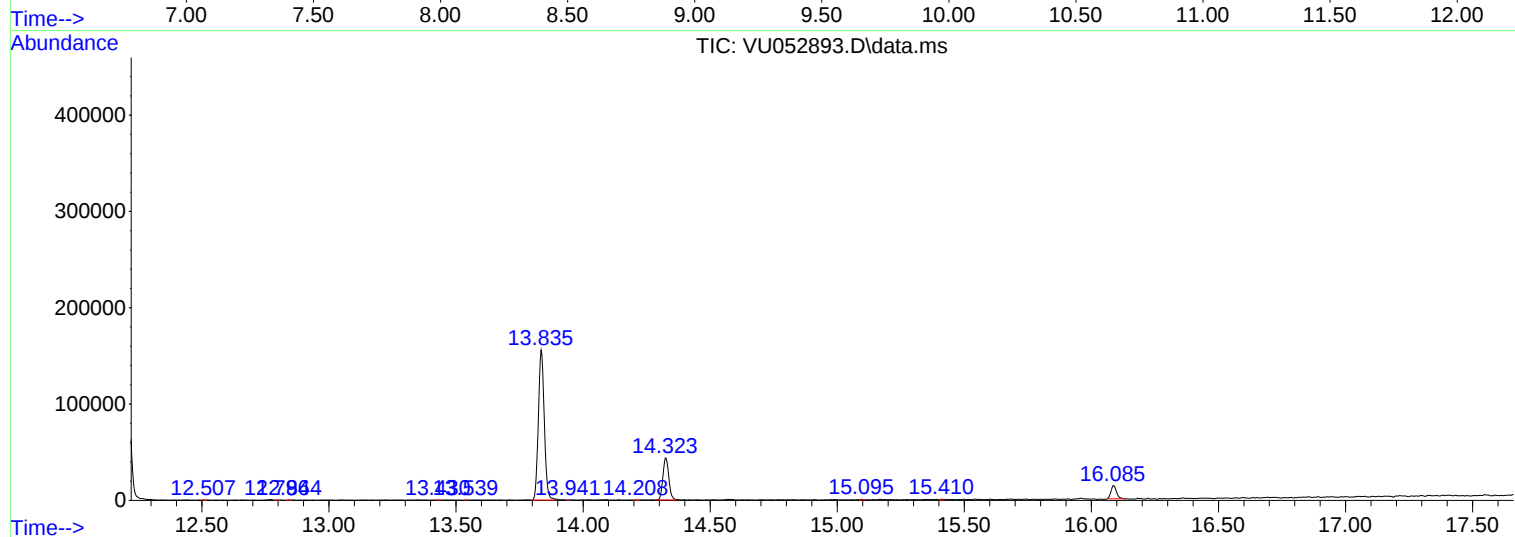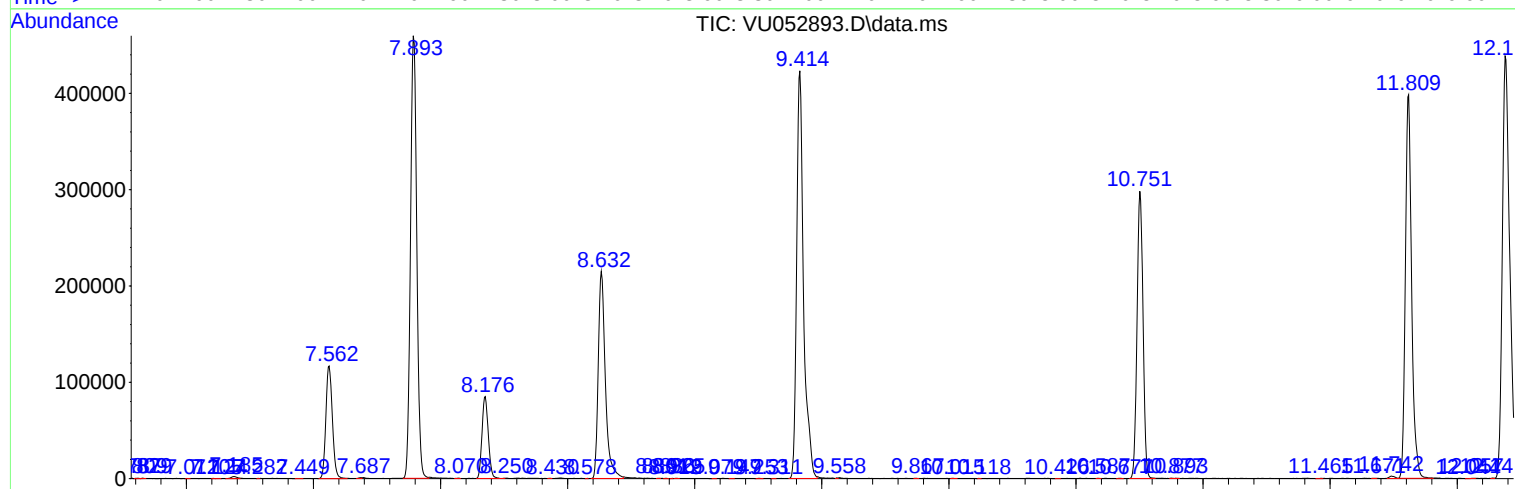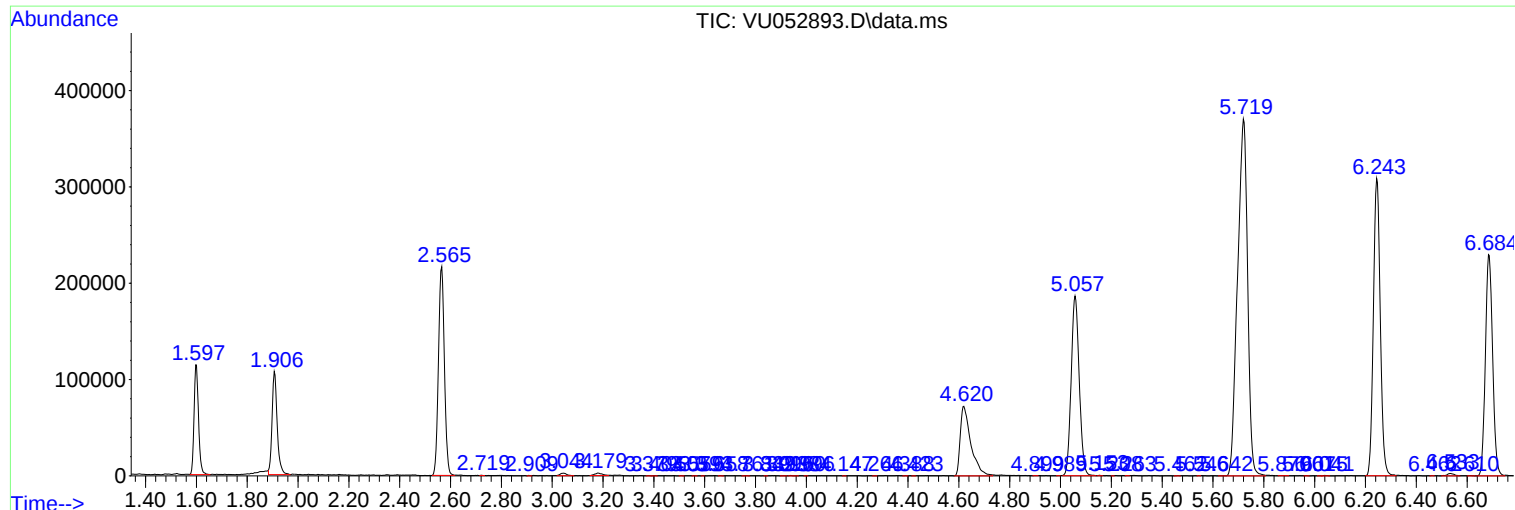

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052893.D
Acq On : 31 Jan 2023 20:48
Operator : JC/MD
Sample : VIBLK108
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK108

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013123\
Data File : VU052893.D
Acq On : 31 Jan 2023 20:48
Operator : JC/MD
Sample : VIBLK108
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK108

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------