
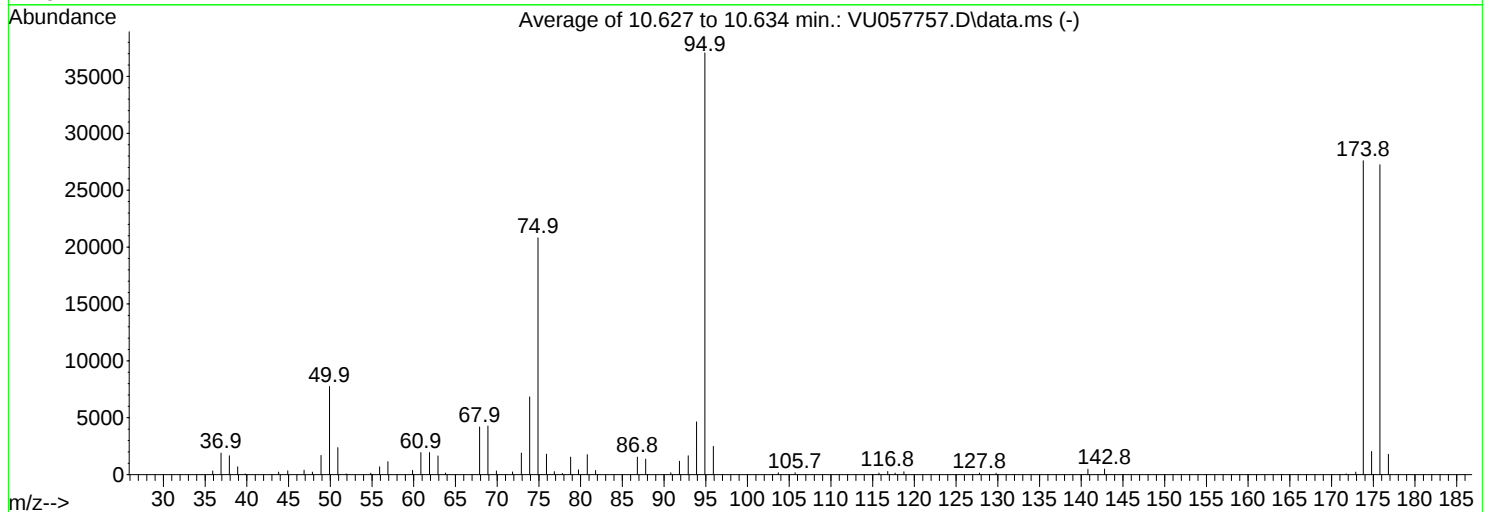


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013124\
Data File : VU057757.D
Acq On : 31 Jan 2024 08:42
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Feb 01 16:23:36 2024

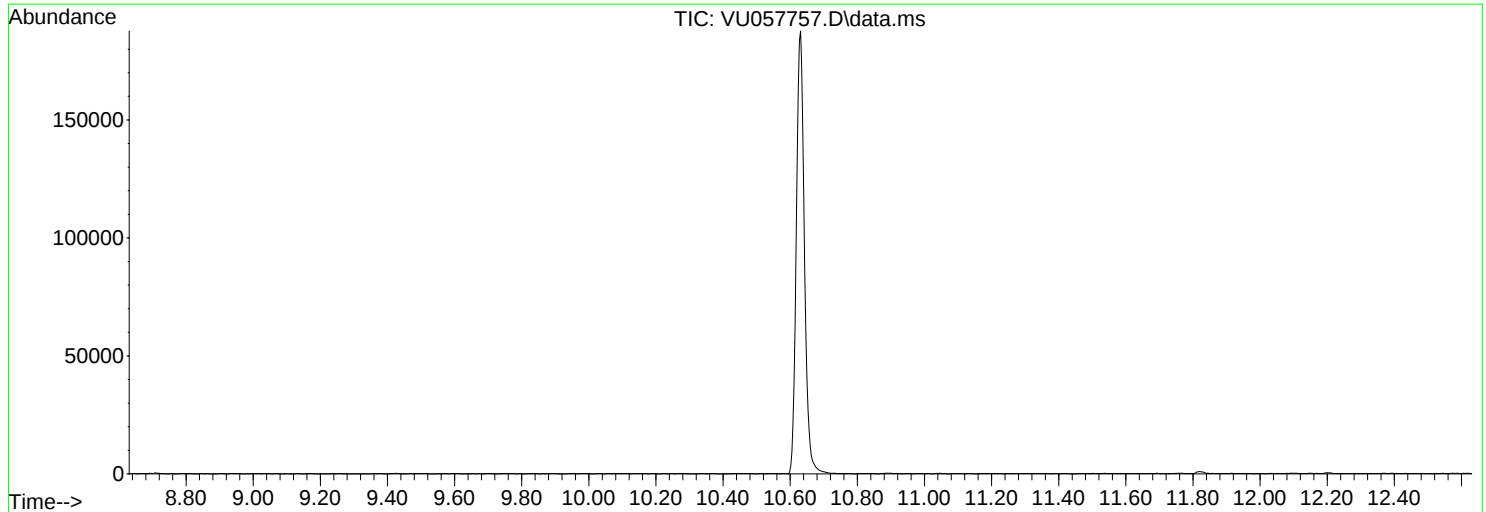

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	7746	PASS
75	95	30	60	56.1	20808	PASS
95	95	100	100	100.0	37072	PASS
96	95	5	9	6.7	2493	PASS
173	174	0.00	2	0.8	223	PASS
174	95	50	100	74.4	27597	PASS
175	174	5	9	7.4	2035	PASS
176	174	95	101	98.7	27235	PASS
177	176	5	9	6.5	1783	PASS