


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU020119\
Data File : VU029325.D
Acq On : 01 Feb 2019 09:46
Operator : JC/SP
Sample : BFB43
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB43

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR020119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Feb 01 23:50:10 2019

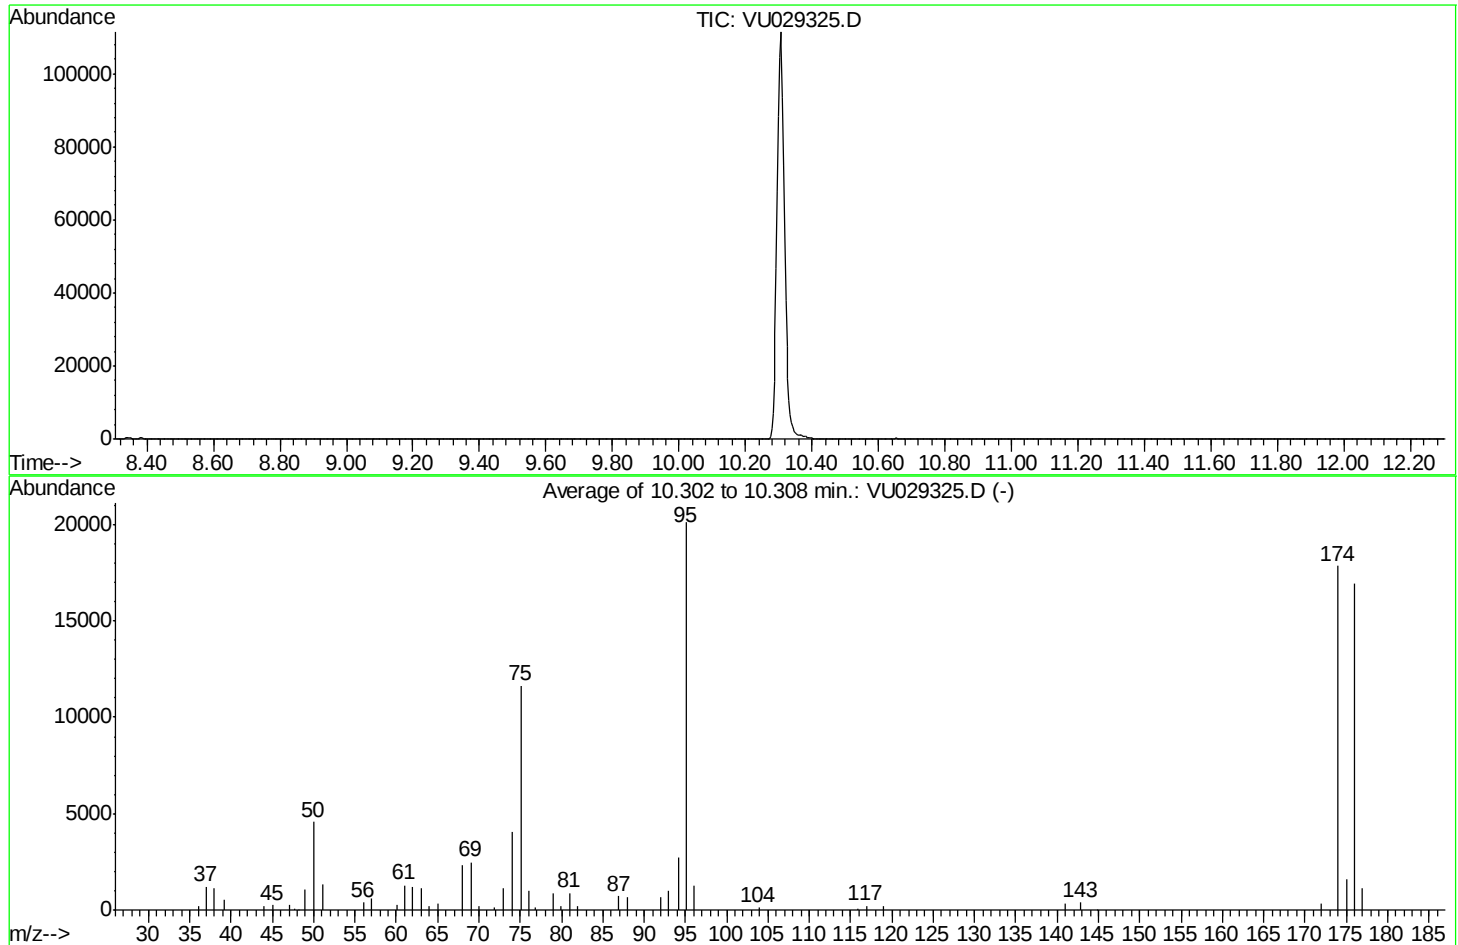

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	4571	PASS
75	95	30	80	57.9	11651	PASS
95	95	100	100	100.0	20112	PASS
96	95	5	9	6.3	1264	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.7	17834	PASS
175	174	5	9	8.9	1582	PASS
176	174	95	101	95.1	16961	PASS
177	176	5	9	6.5	1103	PASS

Scan 2827 (10.263 min): VU029325.D
BFB43

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	232.0
37.00	1127.0
38.00	1158.0
39.10	515.0
44.00	207.0
45.00	242.0
47.00	228.0
48.10	106.0
49.00	1074.0
50.00	4532.0
51.00	1367.0
56.00	376.0
57.00	568.0
60.00	270.0
61.00	1260.0
62.00	1199.0
63.00	1129.0
63.90	224.0
65.00	306.0
68.00	2334.0
69.00	2395.0
70.00	184.0
71.90	125.0
73.00	1122.0
74.10	3879.0
75.00	11477.0
76.00	1002.0
76.80	106.0
79.00	902.0
80.00	207.0
80.90	819.0
81.90	195.0
87.00	750.0
88.00	634.0
92.00	650.0
93.00	974.0
94.10	2693.0
95.10	19736.0
96.00	1294.0
103.90	123.0
116.90	207.0
119.00	154.0
141.00	274.0
142.90	379.0
172.00	287.0
174.00	17064.0
175.00	1518.0
176.00	15852.0
177.00	1079.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	232.0
37.00	1252.0
38.00	1177.0
39.10	600.0
44.00	190.0
45.00	244.0
47.00	242.0
47.70	108.0
49.00	1149.0
50.00	4722.0
51.00	1401.0
56.00	395.0
57.00	629.0
60.10	278.0
61.00	1307.0
62.00	1243.0
63.00	1142.0
63.90	207.0
65.00	313.0
68.00	2397.0
69.00	2558.0
70.00	200.0
71.90	119.0
73.00	1205.0
74.00	4162.0
75.00	11982.0
76.00	1049.0
76.90	150.0
79.00	912.0
79.90	199.0
80.90	901.0
81.90	201.0
87.00	735.0
88.00	698.0
92.00	706.0
93.00	1030.0
94.10	2776.0
95.10	20816.0
96.00	1300.0
103.90	116.0
115.90	114.0
116.90	246.0
119.00	209.0
141.00	314.0
142.90	382.0
172.00	331.0
174.00	18416.0
175.00	1641.0
176.00	17584.0
177.00	1156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	217.0
37.00	1254.0
38.00	1051.0
39.10	572.0
44.00	171.0
45.00	225.0
47.00	246.0
47.70	121.0
49.00	1066.0
50.00	4460.0
51.10	1292.0
56.00	349.0
57.00	623.0
60.10	274.0
61.00	1229.0
62.00	1177.0
63.00	1055.0
63.90	170.0
65.10	286.0
68.00	2261.0
69.00	2483.0
70.10	205.0
71.90	106.0
73.00	1137.0
74.00	4025.0
75.10	11494.0
76.00	1024.0
76.90	173.0
78.90	848.0
79.90	187.0
81.00	885.0
82.00	182.0
86.90	659.0
88.00	691.0
92.00	701.0
93.00	986.0
94.10	2633.0
95.10	19784.0
96.00	1199.0
103.90	106.0
115.90	122.0
116.90	242.0
118.90	220.0
141.00	335.0
142.90	356.0
144.90	101.0
172.00	325.0
174.00	18024.0
175.00	1588.0
176.00	17448.0
177.00	1076.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43