

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052897.D
 Acq On : 01 Feb 2023 11:54
 Operator : JC/MD
 Sample : VU0201WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK040

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M

Title : VOC Analysis

Signal : TIC: VU052897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	99627	121596	12.92%	1.834%
2	1.903	168	175	200	rVB	101791	148893	15.82%	2.246%
3	2.562	368	380	397	rBV	203806	332446	35.33%	5.014%
4	2.723	426	430	436	rBV2	240	304	0.03%	0.005%
5	2.787	446	450	464	rVB2	869	1273	0.14%	0.019%
6	2.871	473	476	479	rVB	308	224	0.02%	0.003%
7	2.893	480	483	484	rBV	254	148	0.02%	0.002%
8	3.041	520	529	539	rVV3	3465	6023	0.64%	0.091%
9	3.170	565	569	572	rBV2	355	290	0.03%	0.004%
10	3.301	608	610	614	rBV	199	178	0.02%	0.003%
11	3.485	664	667	670	rBB	190	148	0.02%	0.002%
12	3.504	670	673	676	rBV	177	175	0.02%	0.003%
13	3.633	709	713	717	rBV	168	206	0.02%	0.003%
14	3.797	761	764	767	rBV	182	172	0.02%	0.003%
15	3.938	806	808	811	rBV	301	165	0.02%	0.002%
16	3.999	824	827	829	rBV	147	130	0.01%	0.002%
17	4.028	831	836	837	rBV	153	154	0.02%	0.002%
18	4.189	882	886	888	rBB	183	133	0.01%	0.002%
19	4.211	889	893	895	rBV	298	252	0.03%	0.004%
20	4.305	917	922	923	rBV	206	193	0.02%	0.003%
21	4.620	1009	1020	1047	rBV	59567	157498	16.74%	2.375%
22	4.899	1104	1107	1111	rBV2	259	252	0.03%	0.004%
23	4.957	1121	1125	1128	rBV	384	344	0.04%	0.005%
24	4.977	1129	1131	1133	rVV2	271	141	0.01%	0.002%
25	5.057	1140	1156	1184	rVB	178543	397875	42.28%	6.001%
26	5.279	1222	1225	1226	rBV	262	170	0.02%	0.003%
27	5.340	1241	1244	1245	rVV	287	155	0.02%	0.002%
28	5.350	1245	1247	1250	rVV	286	179	0.02%	0.003%
29	5.420	1267	1269	1271	rBB	261	139	0.01%	0.002%
30	5.462	1279	1282	1285	rBB	192	139	0.01%	0.002%
31	5.510	1294	1297	1301	rBB	176	140	0.01%	0.002%
32	5.536	1302	1305	1310	rBV	172	208	0.02%	0.003%
33	5.719	1340	1362	1382	rBV2	341850	941093	100.00%	14.194%
34	5.835	1396	1398	1404	rVB	363	271	0.03%	0.004%
35	5.922	1420	1425	1427	rBB2	186	168	0.02%	0.003%
36	6.031	1456	1459	1464	rVV2	468	362	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052897.D
 Acq On : 01 Feb 2023 11:54
 Operator : JC/MD
 Sample : VU0201WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK040

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.128	1488	1489	1495	rVB	294	193	0.02%	0.003%
38	6.160	1496	1499	1502	rBV	351	247	0.03%	0.004%
39	6.243	1512	1525	1547	rBV	263975	490305	52.10%	7.395%
40	6.420	1576	1580	1585	rBB	310	320	0.03%	0.005%
41	6.507	1601	1607	1608	rBV	311	273	0.03%	0.004%
42	6.523	1608	1612	1614	rBV3	1079	865	0.09%	0.013%
43	6.600	1633	1636	1637	rBV	308	199	0.02%	0.003%
44	6.620	1640	1642	1644	rVB	293	140	0.01%	0.002%
45	6.684	1648	1662	1684	rBV	215304	424611	45.12%	6.404%
46	6.800	1692	1698	1703	rBV2	562	688	0.07%	0.010%
47	6.857	1712	1716	1722	rBV	220	297	0.03%	0.004%
48	6.915	1731	1734	1737	rBV	156	144	0.02%	0.002%
49	6.989	1754	1757	1760	rBB	195	146	0.02%	0.002%
50	7.015	1761	1765	1768	rBB	167	134	0.01%	0.002%
51	7.047	1769	1775	1777	rBV	255	213	0.02%	0.003%
52	7.108	1792	1794	1797	rBV	247	168	0.02%	0.003%
53	7.182	1810	1817	1827	rBV4	1714	2808	0.30%	0.042%
54	7.314	1854	1858	1861	rBB	167	167	0.02%	0.003%
55	7.562	1921	1935	1955	rBV	109142	192614	20.47%	2.905%
56	7.648	1958	1962	1966	rBV	215	190	0.02%	0.003%
57	7.681	1966	1972	1974	rBV3	645	524	0.06%	0.008%
58	7.800	2006	2009	2013	rBV	303	215	0.02%	0.003%
59	7.893	2024	2038	2057	rBV	422246	719404	76.44%	10.850%
60	8.054	2083	2088	2090	rBV2	266	268	0.03%	0.004%
61	8.176	2115	2126	2144	rBV	80422	133045	14.14%	2.007%
62	8.340	2174	2177	2182	rVB2	274	177	0.02%	0.003%
63	8.369	2182	2186	2189	rBV	255	253	0.03%	0.004%
64	8.462	2210	2215	2217	rBV2	300	241	0.03%	0.004%
65	8.520	2230	2233	2236	rBB	310	195	0.02%	0.003%
66	8.552	2241	2243	2245	rBV	267	148	0.02%	0.002%
67	8.636	2255	2269	2299	rBV2	179962	365029	38.79%	5.505%
68	8.819	2324	2326	2329	rVV2	187	140	0.01%	0.002%
69	9.201	2442	2445	2447	rBB	217	138	0.01%	0.002%
70	9.224	2447	2452	2453	rBV	290	217	0.02%	0.003%
71	9.234	2453	2455	2461	rVB2	247	188	0.02%	0.003%
72	9.414	2498	2511	2528	rBV	365807	595411	63.27%	8.980%
73	9.565	2555	2558	2560	rBV	546	404	0.04%	0.006%
74	9.613	2569	2573	2577	rBB	273	196	0.02%	0.003%
75	9.687	2594	2596	2598	rBV	277	182	0.02%	0.003%
76	9.771	2618	2622	2624	rBV	191	173	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052897.D
 Acq On : 01 Feb 2023 11:54
 Operator : JC/MD
 Sample : VU0201WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK040

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	9.941	2672	2675	2679	rBV	242	236	0.03%	0.004%
78	10.012	2693	2697	2701	rBV	170	222	0.02%	0.003%
79	10.111	2726	2728	2729	rBV	349	133	0.01%	0.002%
80	10.475	2838	2841	2844	rBV2	275	219	0.02%	0.003%
81	10.751	2914	2927	2950	rBV	280611	459209	48.80%	6.926%
82	10.835	2951	2953	2957	rVB	318	196	0.02%	0.003%
83	11.092	3028	3033	3036	rBV2	405	361	0.04%	0.005%
84	11.131	3041	3045	3048	rVV2	324	263	0.03%	0.004%
85	11.269	3086	3088	3094	rBV	205	206	0.02%	0.003%
86	11.471	3146	3151	3153	rBV2	259	256	0.03%	0.004%
87	11.635	3198	3202	3204	rBV	193	147	0.02%	0.002%
88	11.806	3244	3255	3274	rBV	324024	513566	54.57%	7.746%
89	12.188	3361	3374	3392	rBV	380773	598687	63.62%	9.030%
90	12.291	3402	3406	3408	rVB3	426	235	0.02%	0.004%
91	12.523	3475	3478	3480	rBV2	250	159	0.02%	0.002%
92	12.764	3548	3553	3554	rBV2	622	428	0.05%	0.006%
93	13.221	3688	3695	3701	rBV	1201	1372	0.15%	0.021%
94	13.459	3767	3769	3774	rVB2	402	223	0.02%	0.003%
95	13.603	3810	3814	3815	rBV	364	204	0.02%	0.003%
96	13.841	3881	3888	3897	rVB5	3807	5516	0.59%	0.083%
97	13.986	3929	3933	3935	rBV3	486	350	0.04%	0.005%
98	14.089	3957	3965	3973	rBV3	2481	3935	0.42%	0.059%
99	14.729	4161	4164	4165	rBV2	373	198	0.02%	0.003%
100	15.712	4467	4470	4473	rBV3	566	449	0.05%	0.007%




Sum of corrected areas: 6630277

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052897.D
Acq On : 01 Feb 2023 11:54
Operator : JC/MD
Sample : VU0201WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK040

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

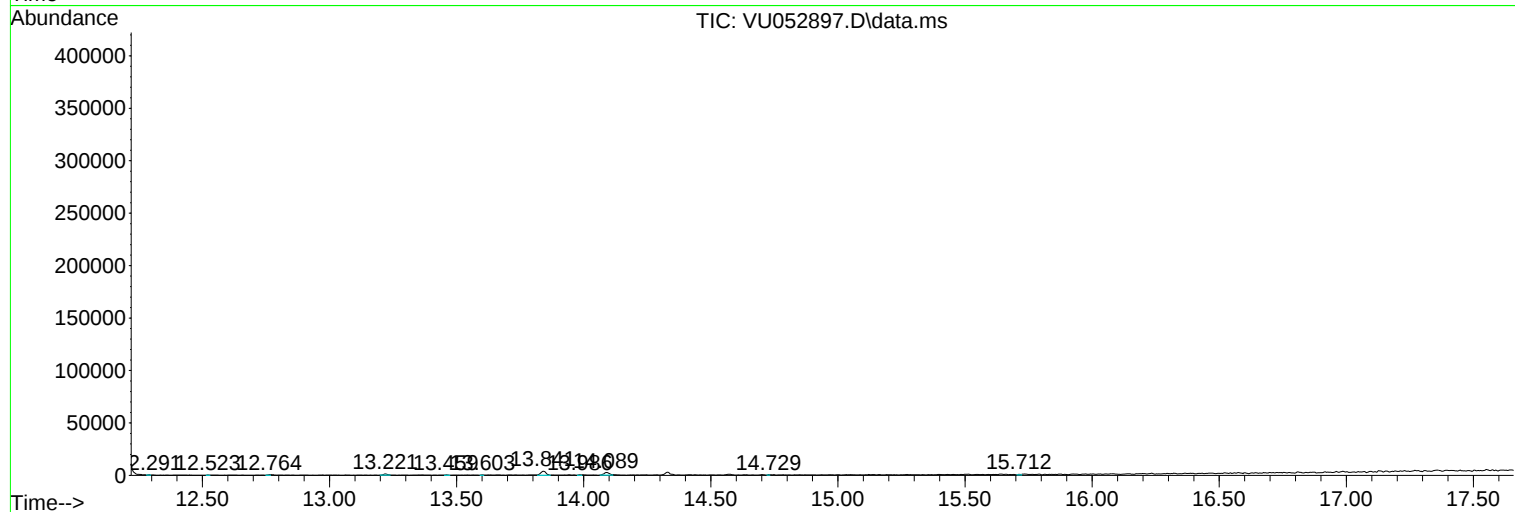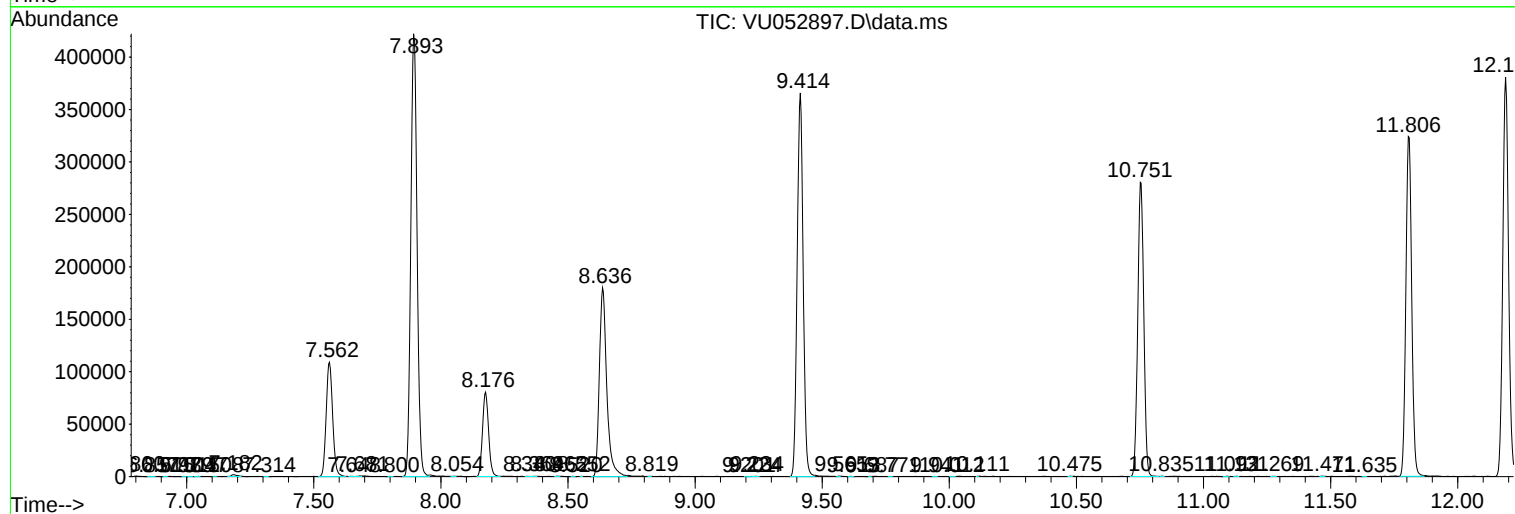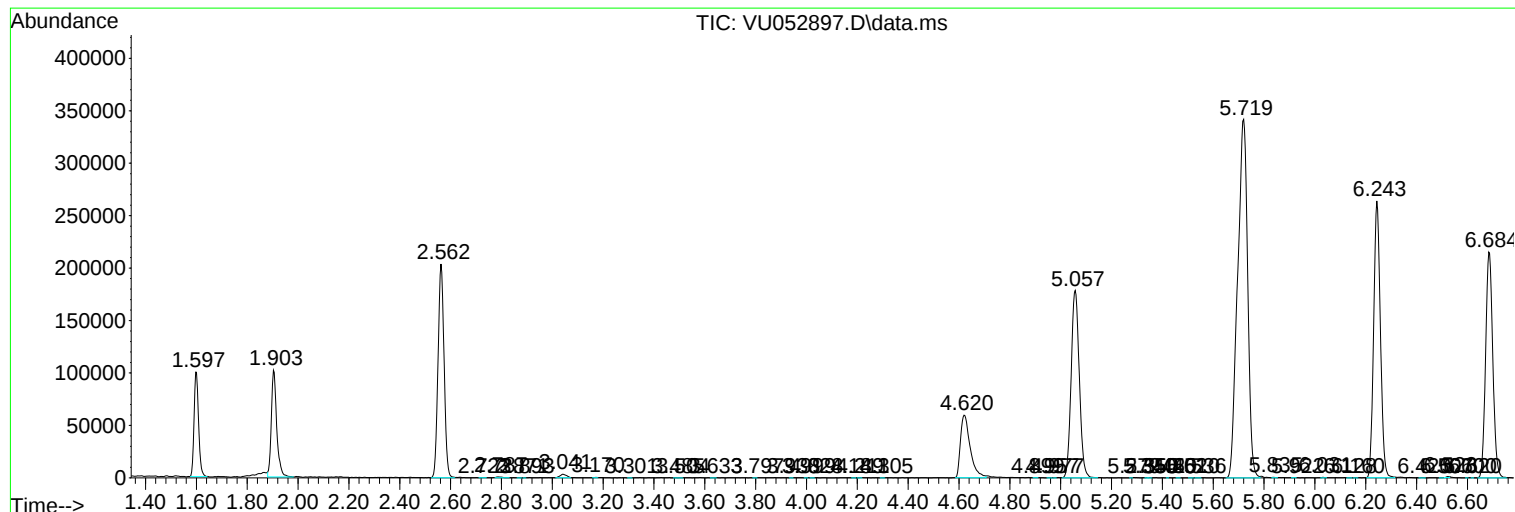

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052897.D
Acq On : 01 Feb 2023 11:54
Operator : JC/MD
Sample : VU0201WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK040

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052897.D
Acq On : 01 Feb 2023 11:54
Operator : JC/MD
Sample : VU0201WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK040

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------