

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052898.D
 Acq On : 01 Feb 2023 12:25
 Operator : JC/MD
 Sample : 01381-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	102927	127612	13.16%	1.912%
2	1.903	168	175	193	rVB	104592	159912	16.49%	2.396%
3	2.562	365	380	394	rBV	209147	343837	35.46%	5.153%
4	2.723	427	430	437	rBV2	231	241	0.02%	0.004%
5	2.787	443	450	458	rBV2	826	1342	0.14%	0.020%
6	3.044	520	530	542	rVB5	2872	5442	0.56%	0.082%
7	3.099	543	547	550	rBB	243	177	0.02%	0.003%
8	3.160	563	566	567	rBV	284	173	0.02%	0.003%
9	3.176	568	571	573	rBV	409	333	0.03%	0.005%
10	3.215	580	583	586	rVB	473	330	0.03%	0.005%
11	3.240	586	591	593	rBV	189	212	0.02%	0.003%
12	3.295	605	608	613	rBV2	250	252	0.03%	0.004%
13	3.314	613	614	616	rVB2	398	144	0.01%	0.002%
14	3.353	622	626	628	rBB	251	148	0.02%	0.002%
15	3.395	637	639	642	rBV	212	166	0.02%	0.002%
16	3.420	646	647	653	rVB	245	181	0.02%	0.003%
17	3.449	653	656	660	rBV	182	193	0.02%	0.003%
18	3.755	748	751	754	rBB	234	183	0.02%	0.003%
19	3.916	797	801	802	rBV	295	181	0.02%	0.003%
20	3.964	813	816	819	rBV	135	141	0.01%	0.002%
21	4.105	855	860	863	rBV	213	246	0.03%	0.004%
22	4.173	878	881	884	rBB	262	153	0.02%	0.002%
23	4.321	924	927	930	rBV	172	163	0.02%	0.002%
24	4.385	945	947	952	rBB	229	170	0.02%	0.003%
25	4.414	952	956	958	rBV2	238	178	0.02%	0.003%
26	4.481	973	977	980	rBB2	303	242	0.02%	0.004%
27	4.623	1008	1021	1047	rBV2	52132	139692	14.41%	2.093%
28	5.057	1140	1156	1179	rBV	183207	402920	41.55%	6.038%
29	5.176	1189	1193	1196	rBV2	272	218	0.02%	0.003%
30	5.272	1220	1223	1225	rBV	267	196	0.02%	0.003%
31	5.517	1296	1299	1302	rBV	164	160	0.02%	0.002%
32	5.626	1331	1333	1335	rBV2	264	142	0.01%	0.002%
33	5.639	1335	1337	1341	rVB	253	166	0.02%	0.002%
34	5.719	1341	1362	1384	rBV2	357756	969631	100.00%	14.531%
35	5.886	1411	1414	1416	rVB2	281	161	0.02%	0.002%
36	5.970	1437	1440	1443	rBV2	475	314	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052898.D
 Acq On : 01 Feb 2023 12:25
 Operator : JC/MD
 Sample : 01381-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.041	1460	1462	1465	rVB	323	190	0.02%	0.003%
38	6.095	1476	1479	1482	rVB2	285	191	0.02%	0.003%
39	6.115	1482	1485	1487	rBV2	241	159	0.02%	0.002%
40	6.189	1504	1508	1510	rBV	177	157	0.02%	0.002%
41	6.243	1511	1525	1551	rVV	241275	456209	47.05%	6.837%
42	6.391	1566	1571	1575	rBB2	374	304	0.03%	0.005%
43	6.530	1605	1614	1615	rBV3	985	1068	0.11%	0.016%
44	6.581	1628	1630	1632	rBV	297	176	0.02%	0.003%
45	6.604	1634	1637	1641	rVB2	458	336	0.03%	0.005%
46	6.687	1648	1663	1682	rBV	222605	430530	44.40%	6.452%
47	6.800	1692	1698	1703	rBV2	503	563	0.06%	0.008%
48	7.034	1768	1771	1776	rBB	149	171	0.02%	0.003%
49	7.070	1777	1782	1786	rBB	379	303	0.03%	0.005%
50	7.189	1810	1819	1830	rBV5	1845	3454	0.36%	0.052%
51	7.250	1836	1838	1841	rBV	241	163	0.02%	0.002%
52	7.382	1876	1879	1883	rBB	184	173	0.02%	0.003%
53	7.436	1894	1896	1900	rBB	176	148	0.02%	0.002%
54	7.465	1901	1905	1906	rBV	194	163	0.02%	0.002%
55	7.517	1917	1921	1923	rBV	171	160	0.02%	0.002%
56	7.562	1923	1935	1952	rVV	112942	199011	20.52%	2.982%
57	7.697	1972	1977	1987	rVB4	1005	1354	0.14%	0.020%
58	7.806	2007	2011	2012	rBV2	272	196	0.02%	0.003%
59	7.896	2025	2039	2058	rBV	431398	744833	76.82%	11.162%
60	8.050	2083	2087	2091	rVB2	425	422	0.04%	0.006%
61	8.099	2100	2102	2105	rBV3	277	164	0.02%	0.002%
62	8.176	2113	2126	2141	rBV	79520	135178	13.94%	2.026%
63	8.288	2156	2161	2162	rBV	401	261	0.03%	0.004%
64	8.365	2181	2185	2190	rVB	360	360	0.04%	0.005%
65	8.401	2191	2196	2200	rBB2	251	287	0.03%	0.004%
66	8.423	2200	2203	2205	rBV	202	152	0.02%	0.002%
67	8.462	2212	2215	2217	rBV2	717	446	0.05%	0.007%
68	8.546	2235	2241	2247	rVB4	1157	1729	0.18%	0.026%
69	8.584	2250	2253	2257	rBB	257	162	0.02%	0.002%
70	8.642	2258	2271	2298	rBV2	156420	332772	34.32%	4.987%
71	9.047	2394	2397	2400	rBB	267	184	0.02%	0.003%
72	9.266	2463	2465	2470	rBV	183	222	0.02%	0.003%
73	9.304	2474	2477	2484	rBV	175	264	0.03%	0.004%
74	9.337	2484	2487	2490	rVB	313	184	0.02%	0.003%
75	9.359	2490	2494	2496	rBV	143	145	0.01%	0.002%
76	9.414	2498	2511	2533	rBV	332376	580976	59.92%	8.707%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052898.D
 Acq On : 01 Feb 2023 12:25
 Operator : JC/MD
 Sample : 01381-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	9.523	2542	2545	2548	rBV	285	160	0.02%	0.002%
78	9.552	2551	2554	2555	rBV	341	200	0.02%	0.003%
79	9.690	2590	2597	2605	rBV2	1010	1478	0.15%	0.022%
80	9.790	2623	2628	2631	rBV	217	247	0.03%	0.004%
81	9.835	2637	2642	2643	rBV	209	216	0.02%	0.003%
82	9.928	2667	2671	2672	rBV	236	179	0.02%	0.003%
83	10.099	2719	2724	2725	rBV	465	323	0.03%	0.005%
84	10.378	2808	2811	2818	rBV	238	335	0.03%	0.005%
85	10.754	2916	2928	2947	rBV	281958	451332	46.55%	6.764%
86	10.890	2964	2970	2979	rVB4	1224	1437	0.15%	0.022%
87	11.066	3022	3025	3027	rBV	265	213	0.02%	0.003%
88	11.742	3231	3235	3241	rVB4	742	839	0.09%	0.013%
89	11.809	3243	3256	3274	rBV	314353	501471	51.72%	7.515%
90	12.066	3330	3336	3344	rBV3	824	1208	0.12%	0.018%
91	12.188	3362	3374	3396	rBV	393894	653844	67.43%	9.799%
92	12.758	3548	3551	3554	rBV	637	553	0.06%	0.008%
93	13.217	3691	3694	3698	rBV3	479	425	0.04%	0.006%
94	13.584	3806	3808	3815	rBV2	299	306	0.03%	0.005%
95	13.812	3877	3879	3881	rBV	265	153	0.02%	0.002%
96	13.844	3881	3889	3897	rVB4	2917	4378	0.45%	0.066%
97	14.089	3958	3965	3977	rBV5	1613	2660	0.27%	0.040%
98	14.555	4104	4110	4111	rBV	442	391	0.04%	0.006%
99	14.709	4155	4158	4161	rBV	443	259	0.03%	0.004%
100	14.883	4209	4212	4214	rBV2	430	294	0.03%	0.004%


Sum of corrected areas: 6672773

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052898.D
Acq On : 01 Feb 2023 12:25
Operator : JC/MD
Sample : 01381-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

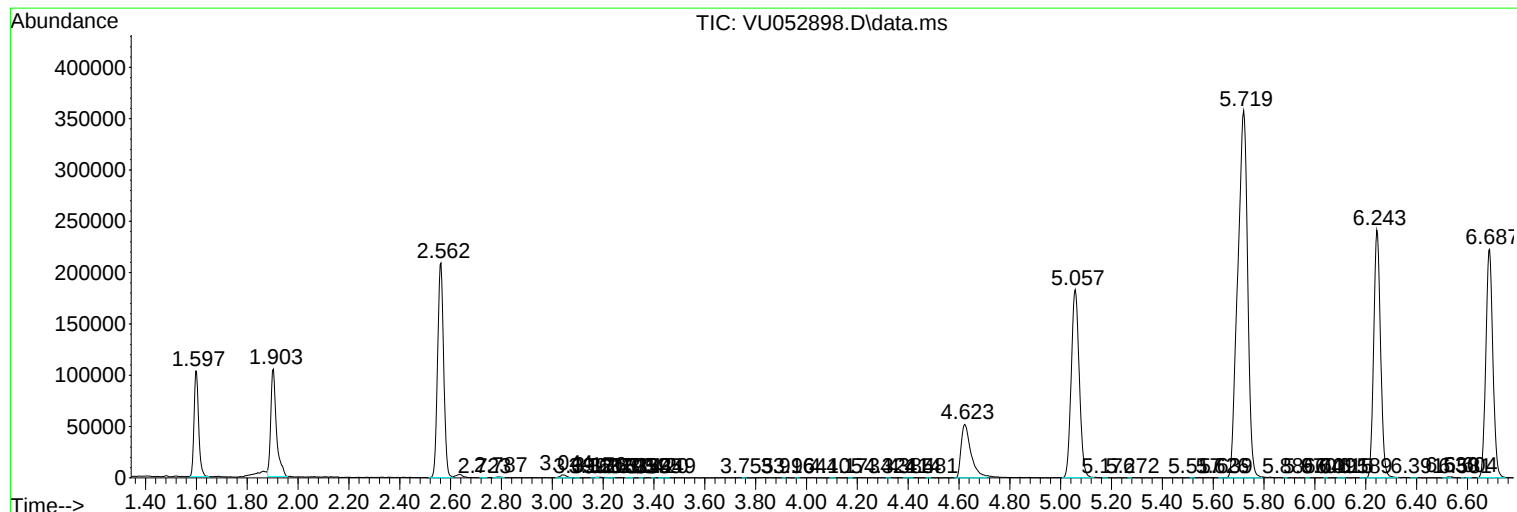

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052898.D
Acq On : 01 Feb 2023 12:25
Operator : JC/MD
Sample : 01381-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052898.D
Acq On : 01 Feb 2023 12:25
Operator : JC/MD
Sample : 01381-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc