

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052899.D
 Acq On : 01 Feb 2023 12:48
 Operator : JC/MD
 Sample : 01381-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rVB	98909	123268	13.25%	1.611%
2	1.903	169	175	195	rVB	96286	153816	16.54%	2.011%
3	2.395	325	328	332	rBV2	424	324	0.03%	0.004%
4	2.421	332	336	339	rBV2	349	356	0.04%	0.005%
5	2.559	367	379	396	rBV	197508	325250	34.97%	4.252%
6	2.671	412	414	418	rVB2	435	251	0.03%	0.003%
7	2.787	445	450	458	rVB3	457	669	0.07%	0.009%
8	2.932	491	495	497	rBV	220	228	0.02%	0.003%
9	2.967	503	506	509	rBV	322	245	0.03%	0.003%
10	3.012	515	520	521	rBV	469	250	0.03%	0.003%
11	3.041	521	529	543	rVB5	2890	6118	0.66%	0.080%
12	3.121	550	554	557	rBV	168	192	0.02%	0.003%
13	3.186	562	574	580	rBV2	642	1477	0.16%	0.019%
14	3.279	601	603	609	rBV	229	269	0.03%	0.004%
15	3.523	674	679	682	rBV	211	265	0.03%	0.003%
16	3.565	689	692	695	rBV	347	236	0.03%	0.003%
17	3.617	705	708	711	rBB	319	174	0.02%	0.002%
18	3.919	799	802	807	rBB	182	165	0.02%	0.002%
19	3.967	815	817	822	rBV	188	189	0.02%	0.002%
20	4.240	897	902	905	rBV	237	224	0.02%	0.003%
21	4.324	925	928	931	rVB2	288	220	0.02%	0.003%
22	4.414	954	956	962	rBV	171	210	0.02%	0.003%
23	4.469	968	973	975	rBB	205	190	0.02%	0.002%
24	4.527	986	991	995	rBV2	261	279	0.03%	0.004%
25	4.572	1003	1005	1009	rBB2	278	187	0.02%	0.002%
26	4.623	1009	1021	1059	rBV3	52087	206004	22.15%	2.693%
27	4.883	1099	1102	1105	rVB	272	171	0.02%	0.002%
28	4.900	1105	1107	1108	rBV	405	206	0.02%	0.003%
29	4.928	1114	1116	1118	rBV	374	214	0.02%	0.003%
30	4.941	1118	1120	1125	rVB	493	302	0.03%	0.004%
31	4.967	1125	1128	1131	rBV	183	174	0.02%	0.002%
32	5.057	1139	1156	1182	rBV	174963	388689	41.79%	5.081%
33	5.295	1227	1230	1234	rVB	417	289	0.03%	0.004%
34	5.363	1247	1251	1254	rBB	207	197	0.02%	0.003%
35	5.420	1265	1269	1272	rBV	257	221	0.02%	0.003%
36	5.469	1278	1284	1286	rBV	164	217	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052899.D
 Acq On : 01 Feb 2023 12:48
 Operator : JC/MD
 Sample : 01381-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	5.719	1339	1362	1388	rBV2	345498	930038	100.00%	12.158%
38	5.887	1410	1414	1416	rVB2	394	259	0.03%	0.003%
39	5.909	1417	1421	1422	rBV	262	170	0.02%	0.002%
40	5.951	1432	1434	1438	rVB	255	170	0.02%	0.002%
41	6.041	1459	1462	1464	rBB	288	193	0.02%	0.003%
42	6.121	1484	1487	1490	rBB	276	176	0.02%	0.002%
43	6.244	1508	1525	1547	rBV	283073	537457	57.79%	7.026%
44	6.372	1561	1565	1568	rBV2	331	237	0.03%	0.003%
45	6.408	1573	1576	1579	rBV	250	200	0.02%	0.003%
46	6.536	1602	1616	1635	rBV	325604	604869	65.04%	7.907%
47	6.684	1647	1662	1683	rBV	214179	413260	44.43%	5.402%
48	6.806	1693	1700	1704	rBV3	753	863	0.09%	0.011%
49	6.973	1748	1752	1755	rBV	223	246	0.03%	0.003%
50	7.009	1761	1763	1769	rBB	145	175	0.02%	0.002%
51	7.192	1810	1820	1825	rBV4	2074	3091	0.33%	0.040%
52	7.285	1847	1849	1852	rVB	289	179	0.02%	0.002%
53	7.436	1893	1896	1899	rBV	186	191	0.02%	0.002%
54	7.562	1923	1935	1953	rVV	109659	193229	20.78%	2.526%
55	7.687	1967	1974	1977	rBV3	767	906	0.10%	0.012%
56	7.771	1996	2000	2002	rBV	227	203	0.02%	0.003%
57	7.893	2025	2038	2055	rBV	414654	708273	76.16%	9.259%
58	8.102	2100	2103	2107	rVB	345	251	0.03%	0.003%
59	8.176	2115	2126	2143	rBV2	76959	130653	14.05%	1.708%
60	8.317	2168	2170	2172	rBV	271	174	0.02%	0.002%
61	8.465	2209	2216	2225	rBV3	1459	2239	0.24%	0.029%
62	8.555	2242	2244	2247	rVB	343	186	0.02%	0.002%
63	8.642	2257	2271	2299	rBV2	155770	336470	36.18%	4.399%
64	8.964	2368	2371	2375	rVB	294	227	0.02%	0.003%
65	9.015	2385	2387	2390	rVB2	268	169	0.02%	0.002%
66	9.157	2428	2431	2434	rBV	157	168	0.02%	0.002%
67	9.221	2449	2451	2453	rVB	369	173	0.02%	0.002%
68	9.253	2453	2461	2462	rBV	299	347	0.04%	0.005%
69	9.414	2498	2511	2533	rBV	399556	722282	77.66%	9.442%
70	9.620	2569	2575	2577	rBV	241	244	0.03%	0.003%
71	9.652	2582	2585	2590	rBV2	326	328	0.04%	0.004%
72	9.700	2599	2600	2604	rBV	228	177	0.02%	0.002%
73	9.880	2653	2656	2660	rBV	209	206	0.02%	0.003%
74	9.960	2677	2681	2687	rBV	255	316	0.03%	0.004%
75	10.095	2715	2723	2725	rBV	291	401	0.04%	0.005%
76	10.189	2747	2752	2755	rBV	353	387	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052899.D
 Acq On : 01 Feb 2023 12:48
 Operator : JC/MD
 Sample : 01381-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.231	2762	2765	2767	rVB	287	179	0.02%	0.002%
78	10.259	2768	2774	2777	rBV	205	246	0.03%	0.003%
79	10.642	2890	2893	2896	rBV	187	169	0.02%	0.002%
80	10.661	2896	2899	2903	rVV2	265	198	0.02%	0.003%
81	10.755	2915	2928	2946	rBV	277139	448334	48.21%	5.861%
82	10.890	2963	2970	2978	rBV3	1388	2025	0.22%	0.026%
83	11.240	3075	3079	3081	rBV	214	204	0.02%	0.003%
84	11.366	3117	3118	3122	rBV	247	172	0.02%	0.002%
85	11.436	3137	3140	3147	rBV2	272	247	0.03%	0.003%
86	11.536	3168	3171	3175	rBV	181	178	0.02%	0.002%
87	11.742	3229	3235	3243	rVB3	4027	5099	0.55%	0.067%
88	11.809	3243	3256	3279	rBV	370123	614153	66.04%	8.029%
89	12.063	3327	3335	3344	rBV5	2877	4946	0.53%	0.065%
90	12.189	3362	3374	3397	rBV2	406611	752486	80.91%	9.837%
91	12.304	3407	3410	3413	rBV2	400	260	0.03%	0.003%
92	12.391	3434	3437	3441	rBV	267	173	0.02%	0.002%
93	13.221	3690	3695	3698	rBV3	887	843	0.09%	0.011%
94	13.481	3774	3776	3780	rVB	353	185	0.02%	0.002%
95	13.597	3808	3812	3815	rBV	259	211	0.02%	0.003%
96	13.767	3861	3865	3870	rBV	334	264	0.03%	0.003%
97	13.838	3879	3887	3902	rVB3	9188	14279	1.54%	0.187%
98	14.192	3995	3997	4000	rBV2	336	181	0.02%	0.002%
99	14.330	4033	4040	4048	rBV4	1835	2658	0.29%	0.035%
100	14.652	4135	4140	4143	rBV2	338	322	0.03%	0.004%


Sum of corrected areas: 7649531

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052899.D
Acq On : 01 Feb 2023 12:48
Operator : JC/MD
Sample : 01381-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

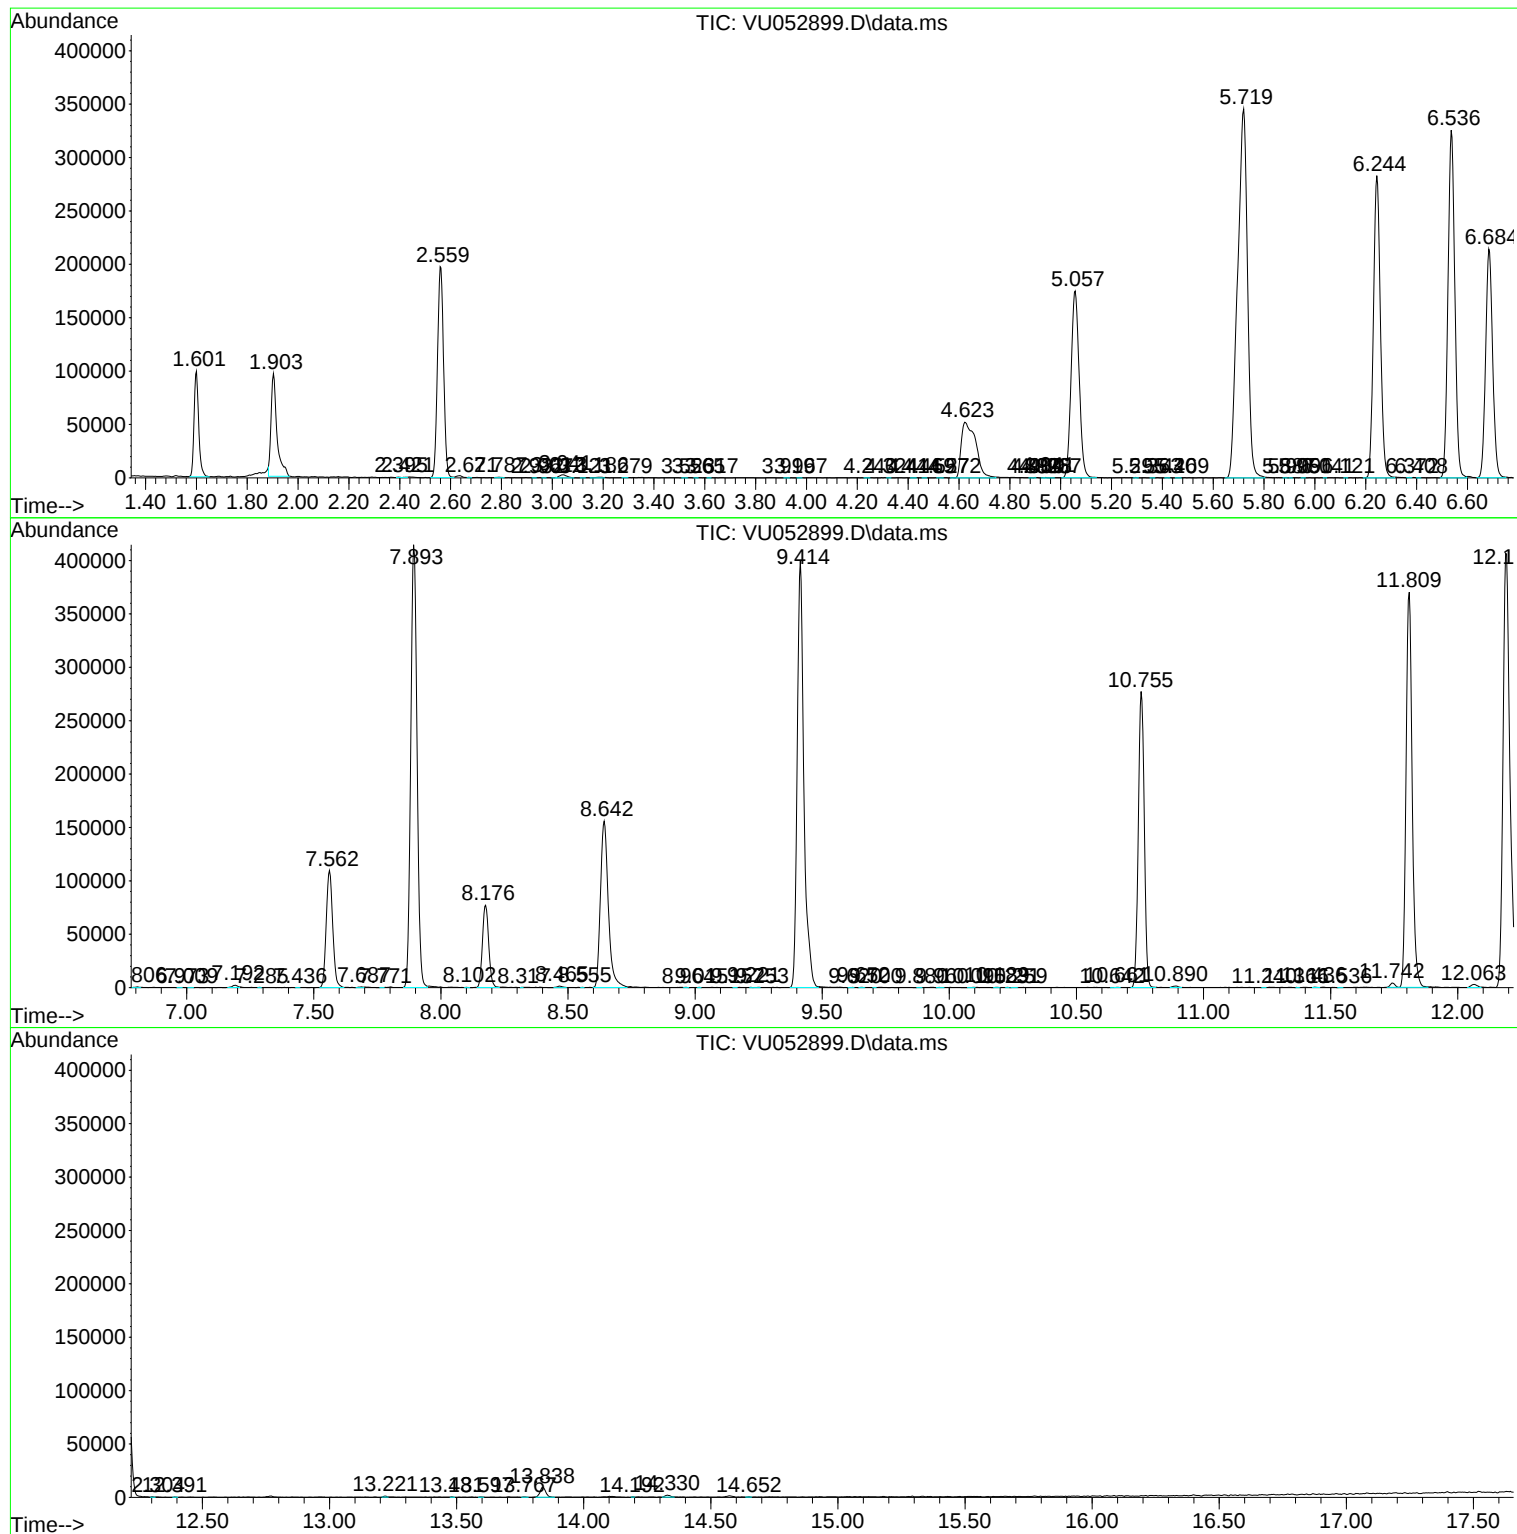

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052899.D
Acq On : 01 Feb 2023 12:48
Operator : JC/MD
Sample : 01381-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052899.D
Acq On : 01 Feb 2023 12:48
Operator : JC/MD
Sample : 01381-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------