

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052912.D
 Acq On : 01 Feb 2023 17:52
 Operator : JC/MD
 Sample : 01381-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44K1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	94609	116583	12.70%	1.733%
2	1.906	169	176	198	rVB	90686	135113	14.72%	2.008%
3	2.327	303	307	308	rBV	258	158	0.02%	0.002%
4	2.356	313	316	323	rVB3	661	470	0.05%	0.007%
5	2.478	351	354	356	rBV	353	212	0.02%	0.003%
6	2.562	368	380	396	rBV	191968	313673	34.18%	4.663%
7	3.006	515	518	522	rVB	304	216	0.02%	0.003%
8	3.041	523	529	538	rBV3	1805	3150	0.34%	0.047%
9	3.115	548	552	555	rBB	158	150	0.02%	0.002%
10	3.179	567	572	573	rBV	462	463	0.05%	0.007%
11	3.276	600	602	608	rBB	227	194	0.02%	0.003%
12	3.353	623	626	632	rBV2	283	318	0.03%	0.005%
13	3.382	633	635	640	rVB	303	226	0.02%	0.003%
14	3.542	683	685	688	rBV	181	142	0.02%	0.002%
15	3.751	746	750	753	rBB	159	148	0.02%	0.002%
16	3.838	774	777	779	rBB2	276	170	0.02%	0.003%
17	3.980	817	821	822	rBV	181	151	0.02%	0.002%
18	4.189	883	886	889	rVB2	300	233	0.03%	0.003%
19	4.350	932	936	939	rBB	141	141	0.02%	0.002%
20	4.623	1008	1021	1054	rBV	58128	153876	16.77%	2.287%
21	4.858	1093	1094	1100	rVB	252	188	0.02%	0.003%
22	4.886	1100	1103	1108	rBV	239	246	0.03%	0.004%
23	4.996	1134	1137	1140	rBV2	228	172	0.02%	0.003%
24	5.057	1140	1156	1183	rVV	175239	386452	42.11%	5.745%
25	5.285	1224	1227	1231	rVB2	316	194	0.02%	0.003%
26	5.375	1251	1255	1260	rBB	276	232	0.03%	0.003%
27	5.549	1305	1309	1312	rBV	161	191	0.02%	0.003%
28	5.719	1341	1362	1392	rBV2	336938	917676	100.00%	13.642%
29	5.851	1398	1403	1407	rBV2	303	390	0.04%	0.006%
30	6.034	1457	1460	1463	rVB	356	234	0.03%	0.003%
31	6.243	1512	1525	1550	rBV	279761	528111	57.55%	7.851%
32	6.404	1573	1575	1579	rVB	296	231	0.03%	0.003%
33	6.472	1594	1596	1601	rBB	283	182	0.02%	0.003%
34	6.494	1602	1603	1606	rBV	254	146	0.02%	0.002%
35	6.536	1606	1616	1630	rVB7	8311	16588	1.81%	0.247%
36	6.684	1647	1662	1683	rBV	204224	402559	43.87%	5.984%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052912.D
 Acq On : 01 Feb 2023 17:52
 Operator : JC/MD
 Sample : 01381-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44K1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.758	1683	1685	1691	rVV3	526	514	0.06%	0.008%
38	6.787	1691	1694	1697	rVB2	298	239	0.03%	0.004%
39	6.809	1699	1701	1704	rVB2	281	152	0.02%	0.002%
40	6.825	1704	1706	1711	rBB2	249	159	0.02%	0.002%
41	6.980	1751	1754	1758	rBB	190	149	0.02%	0.002%
42	7.009	1759	1763	1769	rBV	198	295	0.03%	0.004%
43	7.057	1772	1778	1782	rBB2	325	436	0.05%	0.006%
44	7.128	1795	1800	1803	rBB	189	201	0.02%	0.003%
45	7.182	1811	1817	1828	rBV4	1727	2950	0.32%	0.044%
46	7.378	1875	1878	1879	rBV	213	147	0.02%	0.002%
47	7.517	1917	1921	1922	rBV	207	162	0.02%	0.002%
48	7.562	1922	1935	1951	rBV	106493	186917	20.37%	2.779%
49	7.690	1970	1975	1982	rBV4	1057	1576	0.17%	0.023%
50	7.755	1992	1995	1998	rBB	167	140	0.02%	0.002%
51	7.767	1998	1999	2004	rBV	232	188	0.02%	0.003%
52	7.893	2024	2038	2055	rBV	412265	701901	76.49%	10.434%
53	8.086	2095	2098	2100	rVB	407	232	0.03%	0.003%
54	8.176	2115	2126	2144	rBV	75721	127468	13.89%	1.895%
55	8.282	2154	2159	2161	rBV2	351	309	0.03%	0.005%
56	8.301	2162	2165	2168	rVV	307	225	0.02%	0.003%
57	8.320	2168	2171	2174	rVB2	205	154	0.02%	0.002%
58	8.349	2175	2180	2182	rBV2	233	183	0.02%	0.003%
59	8.398	2192	2195	2198	rBV2	345	208	0.02%	0.003%
60	8.449	2208	2211	2212	rBV2	312	204	0.02%	0.003%
61	8.465	2213	2216	2221	rVB3	917	928	0.10%	0.014%
62	8.513	2229	2231	2234	rBV	250	173	0.02%	0.003%
63	8.636	2257	2269	2295	rBV2	174087	350645	38.21%	5.212%
64	8.780	2312	2314	2316	rVV2	398	176	0.02%	0.003%
65	8.796	2316	2319	2326	rVV2	528	497	0.05%	0.007%
66	8.838	2326	2332	2339	rVB5	768	1265	0.14%	0.019%
67	8.947	2364	2366	2370	rVB	297	185	0.02%	0.003%
68	8.986	2375	2378	2381	rBV	206	182	0.02%	0.003%
69	9.086	2406	2409	2411	rBV	198	156	0.02%	0.002%
70	9.279	2464	2469	2472	rBV	140	163	0.02%	0.002%
71	9.414	2498	2511	2530	rBV	387536	643475	70.12%	9.565%
72	9.655	2582	2586	2589	rBV	342	251	0.03%	0.004%
73	9.693	2590	2598	2601	rVV3	636	850	0.09%	0.013%
74	9.787	2620	2627	2631	rBV	250	349	0.04%	0.005%
75	9.877	2652	2655	2658	rBB	278	192	0.02%	0.003%
76	10.092	2713	2722	2725	rBV3	1144	1596	0.17%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052912.D
 Acq On : 01 Feb 2023 17:52
 Operator : JC/MD
 Sample : 01381-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44K1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.221	2758	2762	2764	rBB	236	159	0.02%	0.002%
78	10.259	2768	2774	2777	rBV	304	362	0.04%	0.005%
79	10.455	2831	2835	2841	rBV	294	387	0.04%	0.006%
80	10.516	2850	2854	2859	rBB	190	228	0.02%	0.003%
81	10.655	2892	2897	2900	rBB	185	212	0.02%	0.003%
82	10.751	2913	2927	2941	rBV	275497	444841	48.47%	6.613%
83	10.886	2962	2969	2976	rBV5	1881	2859	0.31%	0.042%
84	10.979	2994	2998	3003	rBB	229	255	0.03%	0.004%
85	11.475	3146	3152	3154	rBV	541	544	0.06%	0.008%
86	11.507	3159	3162	3165	rBV	196	181	0.02%	0.003%
87	11.742	3229	3235	3242	rBV3	1261	1587	0.17%	0.024%
88	11.809	3243	3256	3276	rBV	368094	594495	64.78%	8.837%
89	12.060	3326	3334	3345	rBV4	4795	7664	0.84%	0.114%
90	12.188	3360	3374	3400	rBV	385764	654055	71.27%	9.723%
91	12.767	3546	3554	3562	rBV3	1314	1828	0.20%	0.027%
92	13.002	3625	3627	3630	rBV	273	140	0.02%	0.002%
93	13.204	3683	3690	3692	rBV4	4088	4423	0.48%	0.066%
94	13.327	3725	3728	3731	rBV	212	167	0.02%	0.002%
95	13.458	3766	3769	3771	rBV	290	146	0.02%	0.002%
96	13.549	3795	3797	3802	rVB2	292	166	0.02%	0.002%
97	13.838	3879	3887	3897	rVV4	4193	5915	0.64%	0.088%
98	14.153	3982	3985	3987	rBV	265	164	0.02%	0.002%
99	14.262	4017	4019	4026	rVB2	305	294	0.03%	0.004%
100	14.462	4077	4081	4085	rBV3	243	243	0.03%	0.004%




Sum of corrected areas: 6727086

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052912.D
Acq On : 01 Feb 2023 17:52
Operator : JC/MD
Sample : 01381-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44K1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

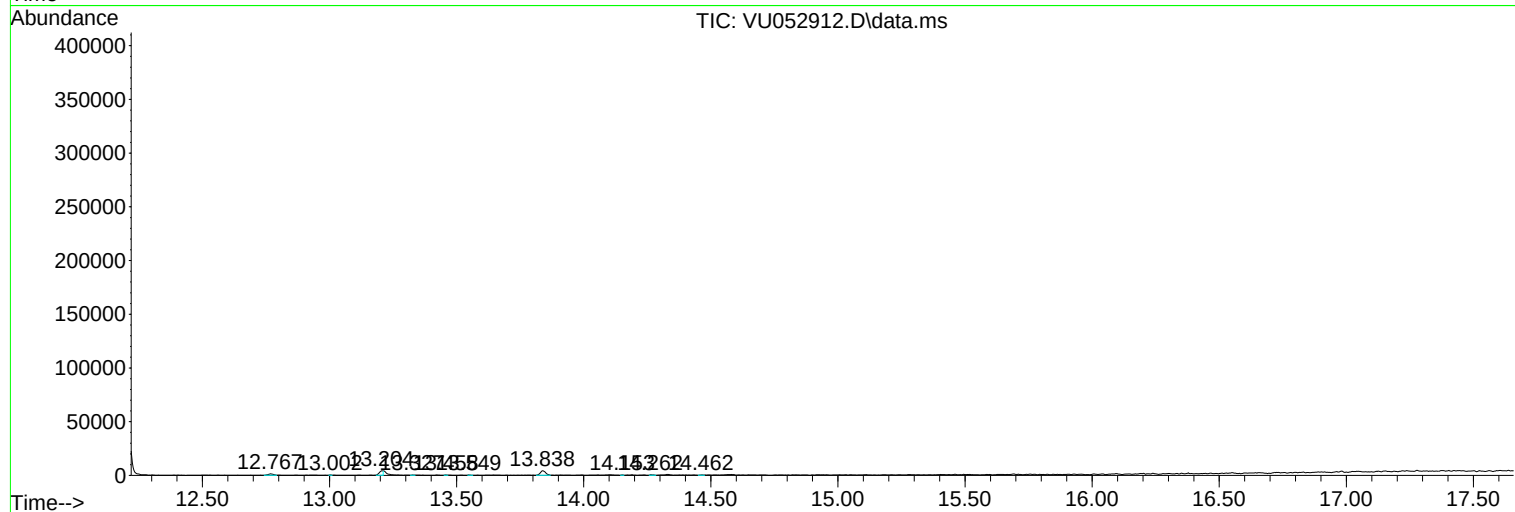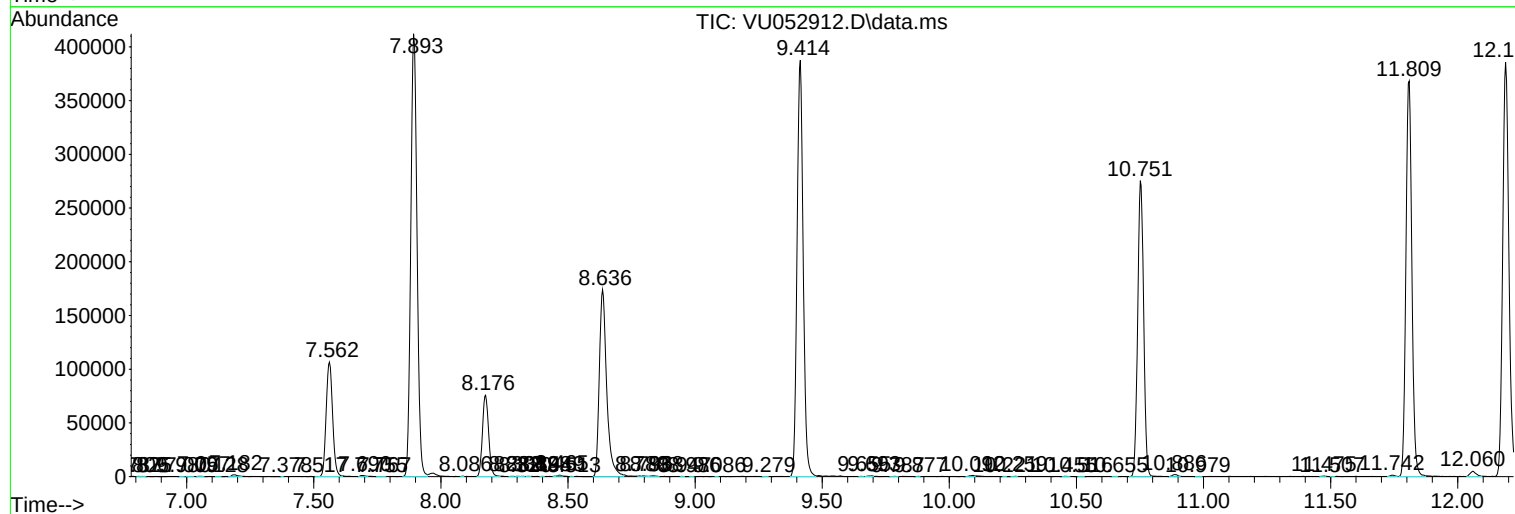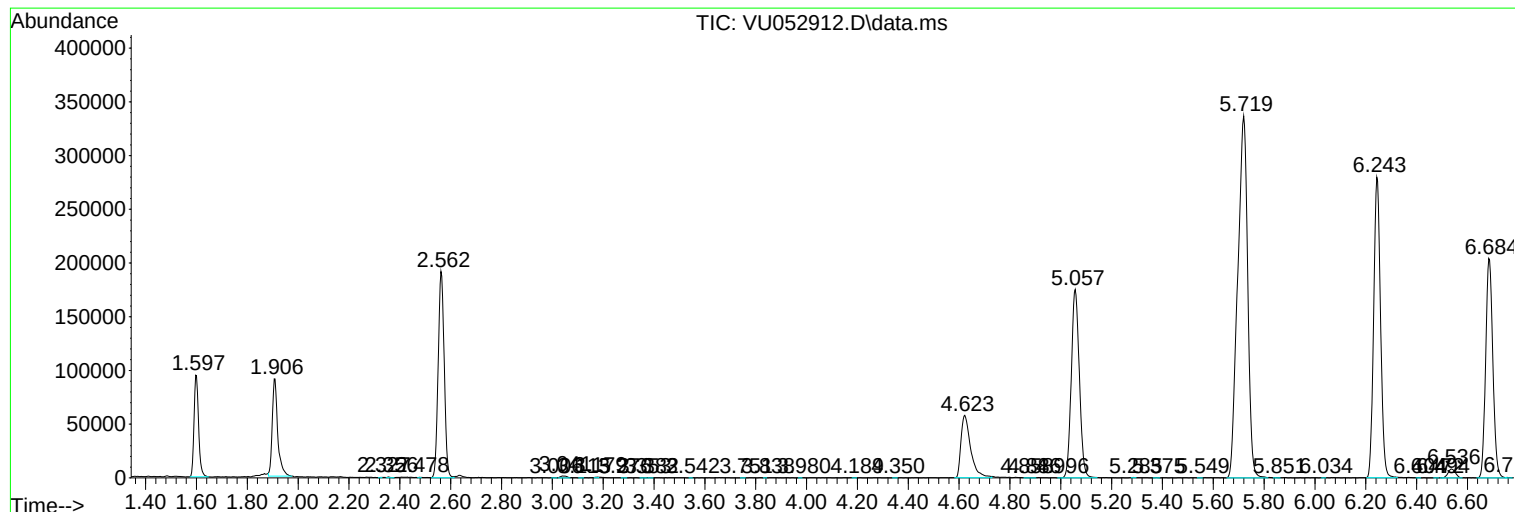

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052912.D
Acq On : 01 Feb 2023 17:52
Operator : JC/MD
Sample : 01381-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44K1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052912.D
Acq On : 01 Feb 2023 17:52
Operator : JC/MD
Sample : 01381-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44K1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------